

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062822\
 Data File : PD070587.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2022 09:04
 Operator : AR\AJ
 Sample : INDB229
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDB3242

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/30/2022
 Supervised By : Ankita Jodhani 06/30/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 00:34:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062822CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 29 02:34:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.367	3.990	30839523	257.2E6	19.288	24.197 #
27)	SA Decachlor...	8.098	9.047	65090225	339.4E6	39.817	45.637
Target Compounds							
5)	MB Aldrin	4.617	5.477	43422935	356.4E6	19.409	24.089
6)	B beta-BHC	4.331	4.822	20341353	163.2E6	19.571m	24.444
7)	B delta-BHC	4.532	5.039	44500107	323.9E6	18.980	22.218
8)	B Heptachlo...	5.059	5.860	39238605	298.4E6	19.029	23.083
10)	B trans-Chl...	5.284	6.094	39855854	318.7E6	18.623	23.272
11)	B cis-Chlor...	5.342	6.167	39508492	309.3E6	18.901	23.378
12)	B 4,4'-DDE	5.510	6.321	75184320	579.8E6	36.918	44.825
15)	B Endosulfa...	6.167	6.893	70572509	518.4E6	40.275	47.776
18)	B Endrin al...	6.337	7.016	53602047	380.5E6	35.360	41.628
19)	B Endosulfa...	6.549	7.240	68066954	461.7E6	38.199	45.004
21)	B Endrin ke...	7.040	7.707	78104020	517.2E6	39.812	45.362

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062822\
Data File : PD070587.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2022 09:04
Operator : AR\AJ
Sample : INDB229
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 00:34:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062822CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Jun 29 02:34:55 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

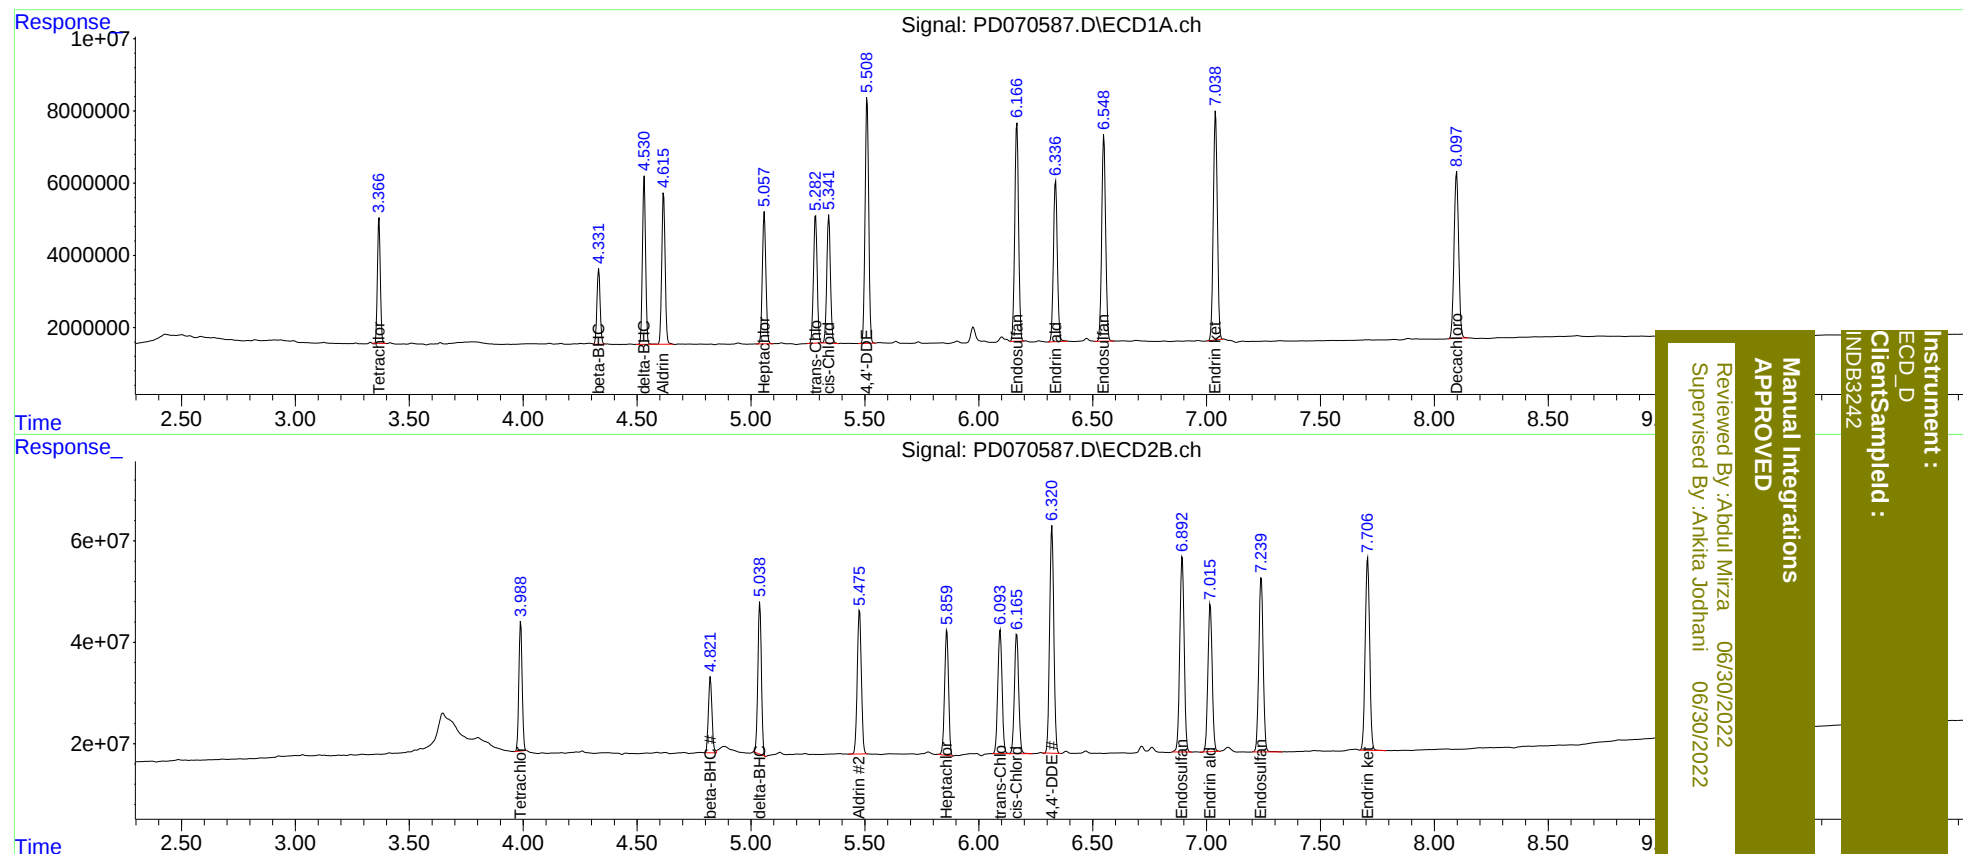

Instrument :
ECD_D
ClientSampled :
INDB3242

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/30/2022
Supervised By :Ankita Jodhani 06/30/2022