

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062824\
 Data File : PD083858.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2024 02:41
 Operator : AR\AJ
 Sample : PB161744BS
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS744

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/28/2024
 Supervised By :Ankita Jodhani 06/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 04:01:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062724CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 27 19:01:18 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	19204908	97902081	19.354	17.687
27)	SA Decachlor...	9.116	7.895	41576318	134.4E6	20.130	20.684
Target Compounds							
2)	A alpha-BHC	4.019	3.270	7362530	35807071	3.856	3.964
3)	MA gamma-BHC...	4.353	3.598	7837363	36093697	4.199	4.266
4)	MA Heptachlor	4.944	3.936	8938749	37622529	4.533	4.486
5)	MB Aldrin	5.288	4.215	8856206	37071274	4.472	4.425
6)	B beta-BHC	4.550	3.895	3614970	19148689	4.551	5.005
7)	B delta-BHC	4.796	4.124	11055646	22433130	5.360	2.492 #
8)	B Heptachlo...	5.714	4.716	9251513	35852766	4.922m	4.688
9)	A Endosulfan I	6.103	5.085	8874028	32782323	4.866	4.739
10)	B trans-Chl...	5.973	4.965	8887890	35514910	4.803	4.707
11)	B cis-Chlor...	6.052	5.029	9159147	36826388	4.814	4.830
12)	B 4,4'-DDE	6.223	5.216	17961927	66590210	9.323m	9.136m
13)	MA Dieldrin	6.379	5.348	18067327	70093144	9.017	9.146m
14)	MA Endrin	6.610	5.625	13513264	57778276	8.702	9.320
15)	B Endosulfa...	6.830	5.918	16843868	62863410	9.562	9.842
16)	A 4,4'-DDD	6.743	5.771	13102442	56928400	8.943	9.492
17)	MA 4,4'-DDT	7.059	6.022	12756185	46612562	8.616	8.159
18)	B Endrin al...	6.960	6.097	14043412	52741671	10.688	10.955
19)	B Endosulfa...	7.196	6.319	15240374	57239831	8.941	9.172
20)	A Methoxychlor	7.535	6.596	36821107	130.7E6	43.816	47.830
21)	B Endrin ke...	7.682	6.824	19166458	70095998	10.153	10.467m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062824\
Data File : PD083858.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2024 02:41
Operator : AR\AJ
Sample : PB161744BS
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 04:01:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062724CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 19:01:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

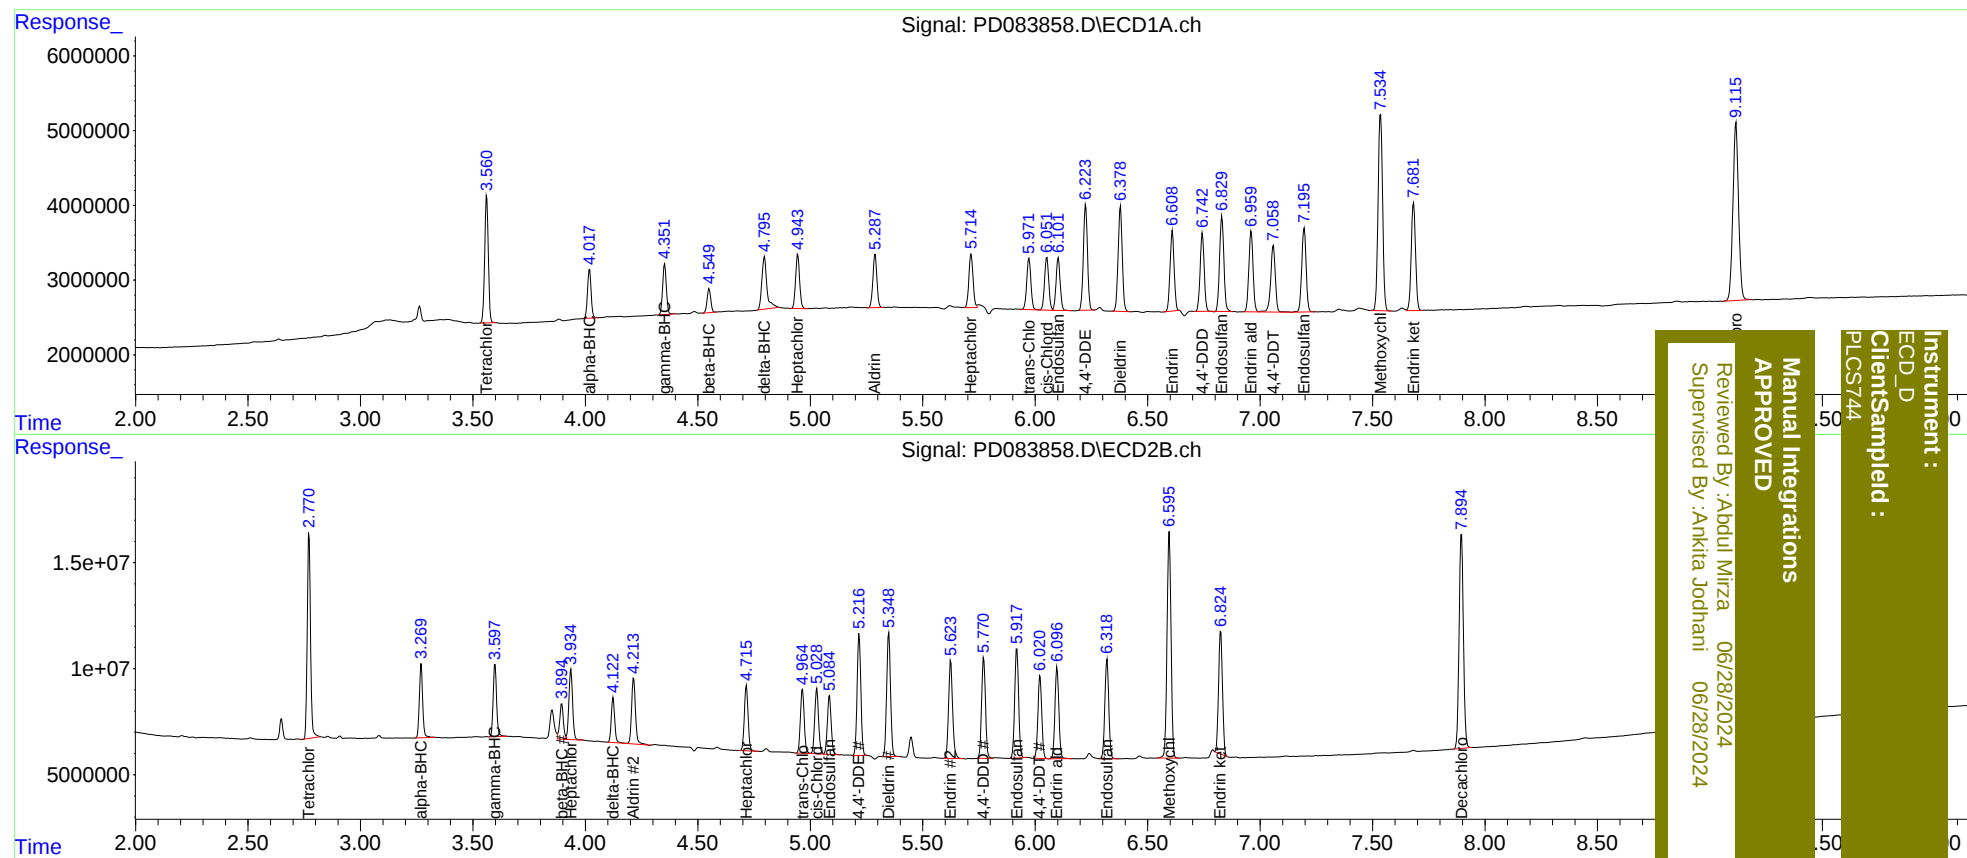

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 06/28/2024
Supervised By: Ankita Jodhani 06/28/2024

Instrument :
ECD_D
ClientSampled :
PLC5744