

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062825\
 Data File : PD089220.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2025 01:50
 Operator : AR\AJ
 Sample : Q2436-06
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-83

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 03:50:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061825.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 18 05:39:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.881	47076991	301.7E6	16.500	17.794
28)	SA Decachlor...	9.069	8.070	55441148	290.6E6	14.116	14.698
Target Compounds							
12)	B 4,4'-DDE	6.194	5.374	2345502	16189323	0.538	0.706 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062825\
Data File : PD089220.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2025 01:50
Operator : AR\AJ
Sample : Q2436-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP-83

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 03:50:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061825.M
Quant Title : GC Extractables
QLast Update : Wed Jun 18 05:39:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

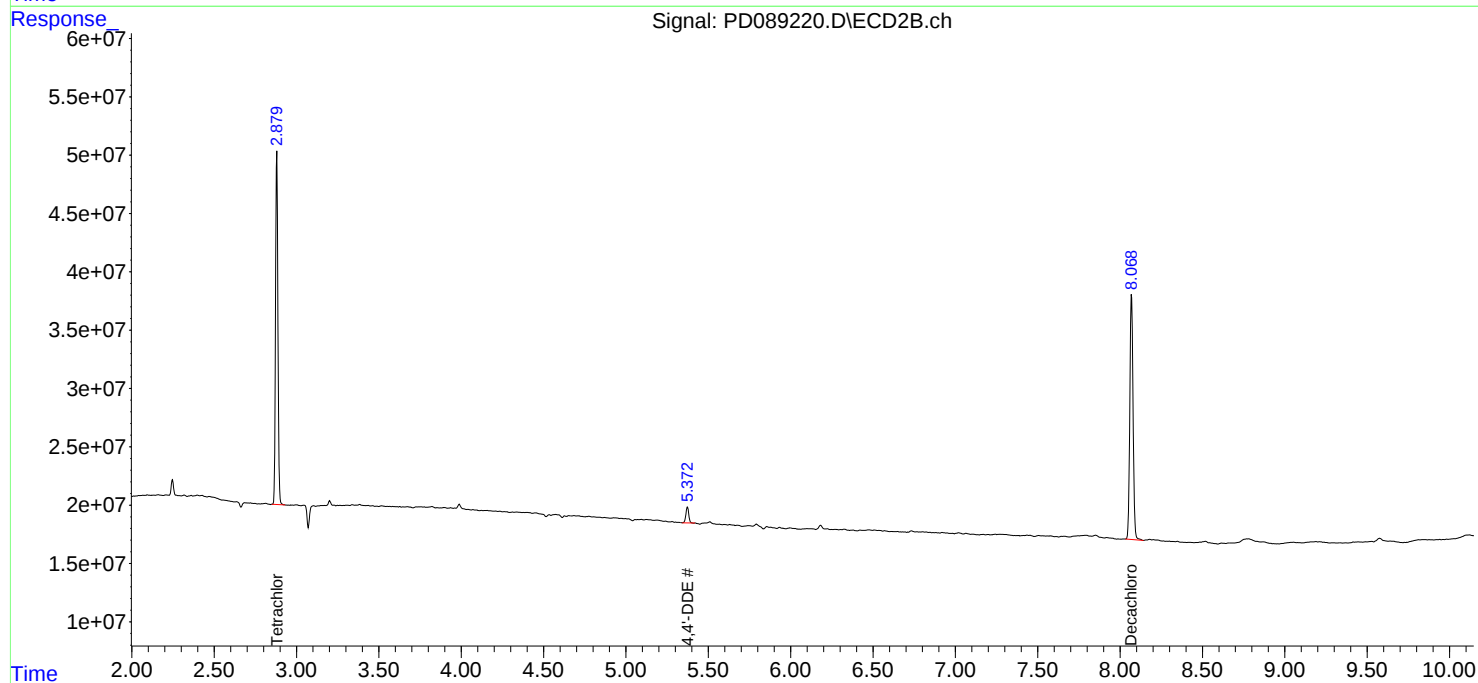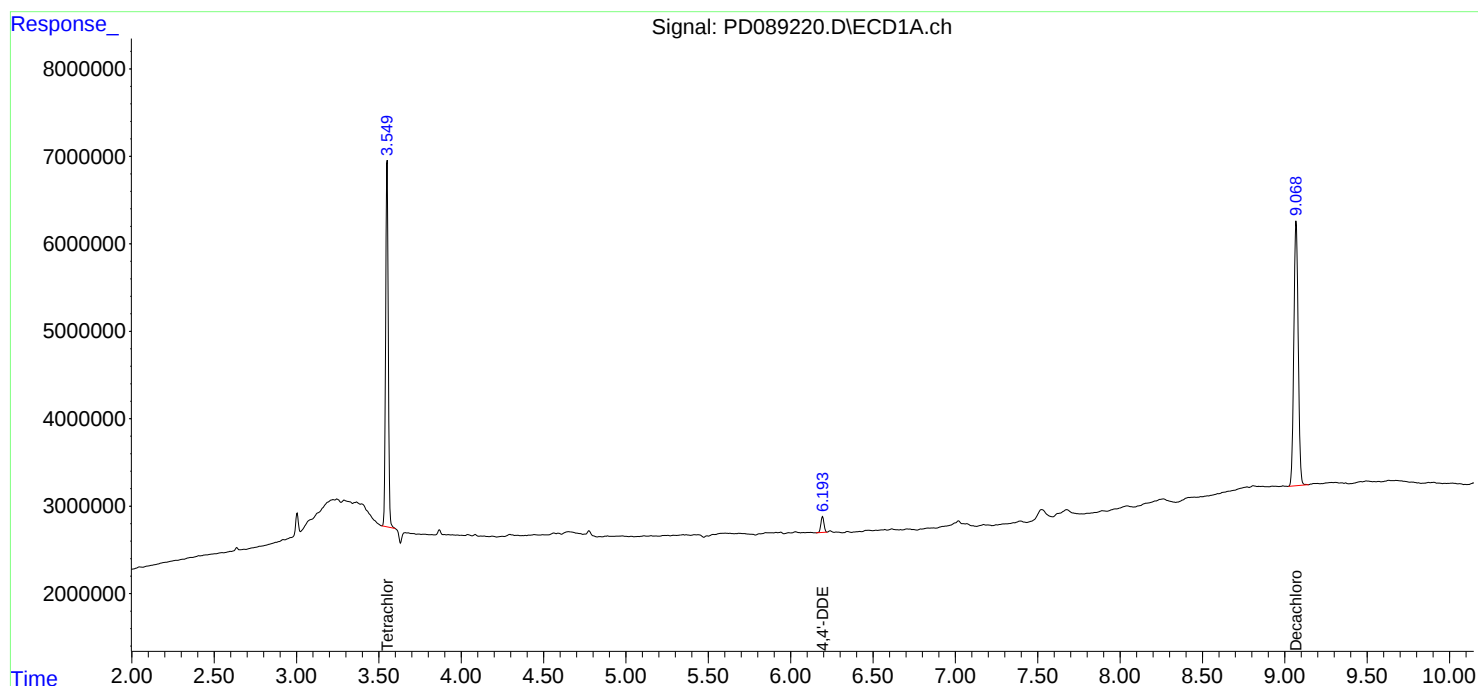


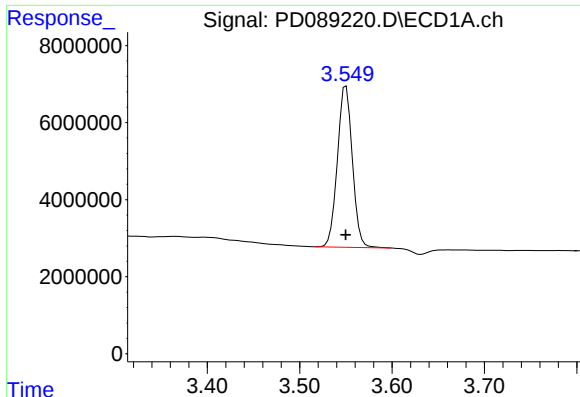

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 47076991
Conc: 16.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-83

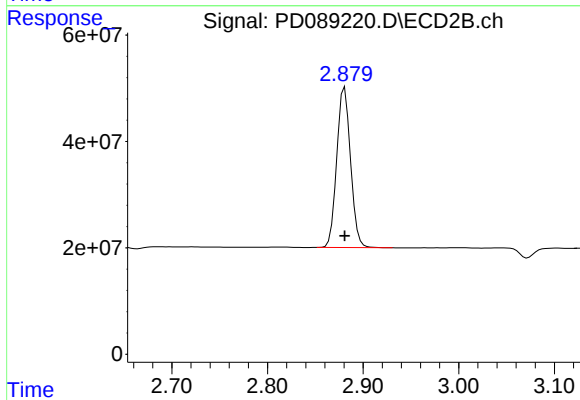


#1 Tetrachloro-m-xylene

R.T.: 2.881 min
Delta R.T.: 0.000 min
Response: 301662638
Conc: 17.79 ng/ml

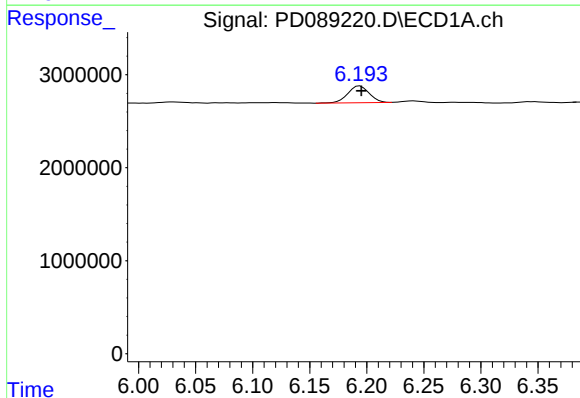


#12 4,4'-DDE

R.T.: 6.194 min
Delta R.T.: -0.001 min
Response: 2345502
Conc: 0.54 ng/ml

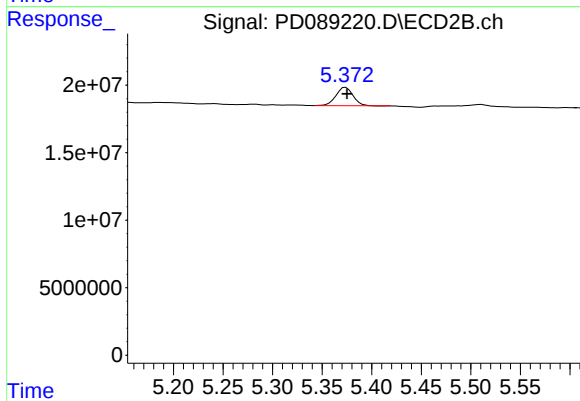

#12 4,4'-DDE


R.T.: 5.374 min
Delta R.T.: -0.001 min
Response: 16189323
Conc: 0.71 ng/ml

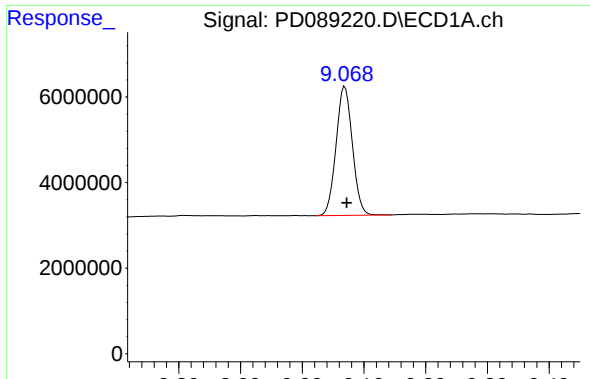

#28 Decachlorobiphenyl

R.T.: 9.069 min
Delta R.T.: -0.003 min
Response: 55441148
Conc: 14.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-83

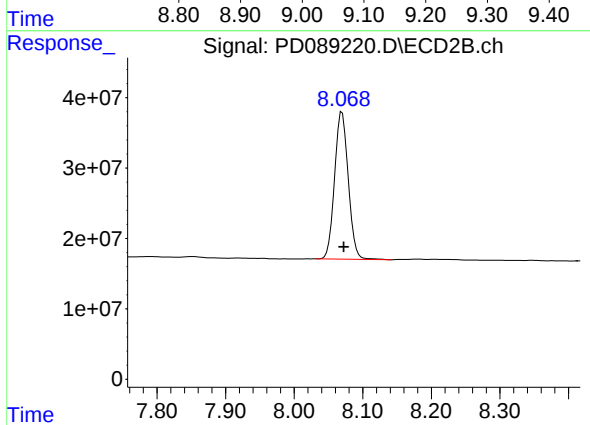

#28 Decachlorobiphenyl

R.T.: 8.070 min
Delta R.T.: -0.002 min
Response: 290585948
Conc: 14.70 ng/ml