

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062921\
 Data File : PD064002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2021 12:58
 Operator : AR\AJ
 Sample : M2872-06
 Misc : PEST GPC BLANK
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 03:58:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 21 04:24:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
27)	SA Decachlor...	0.000	9.018	0	4431447	N.D.	0.320
Target Compounds							
9)	A Endosulfan I	0.000	6.173	0	30243015	N.D.	1.527
11)	B cis-Chlor...	0.000	6.173	0	30243015	N.D.	1.502
13)	MA Dieldrin	0.000	6.433	0	2522620	N.D.	0.121
15)	B Endosulfa...	0.000	6.887	0	12035606	N.D.	0.744
16)	A 4,4'-DDD	0.000	6.793	0	62269713	N.D.	3.699
17)	MA 4,4'-DDT	0.000	7.092	0	9776216	N.D.	0.594
18)	B Endrin al...	0.000	6.986	0	15131694	N.D.	1.076
19)	B Endosulfa...	0.000	7.239	0	17103118	N.D.	1.039
20)	A Methoxychlor	0.000	7.559	0	32902746	N.D.	4.253
24)	Toxaphene-3	0.000	7.092	0	9776216	N.D.	70.959
25)	Toxaphene-4	0.000	7.092	0	9776216	N.D.	23.698
26)	Toxaphene-5	0.000	7.559	0	32902746	N.D.	192.631


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062921\
Data File : PD064002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2021 12:58
Operator : AR\AJ
Sample : M2872-06
Misc : PEST GPC BLANK
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 03:58:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

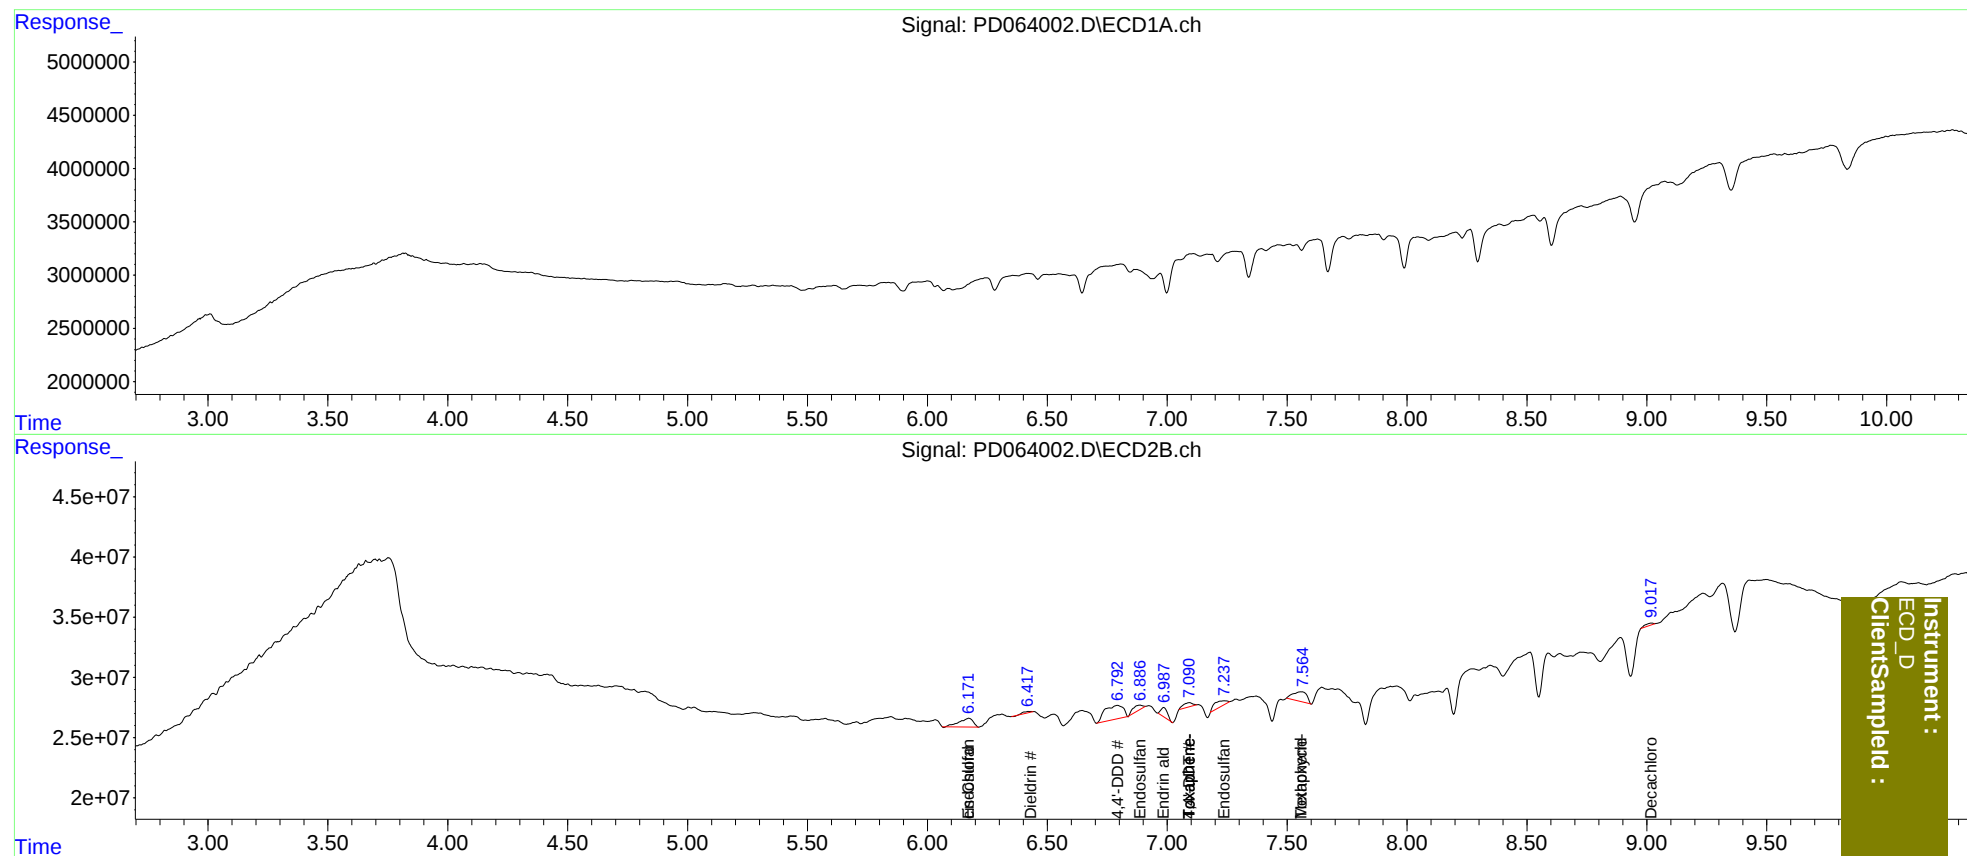


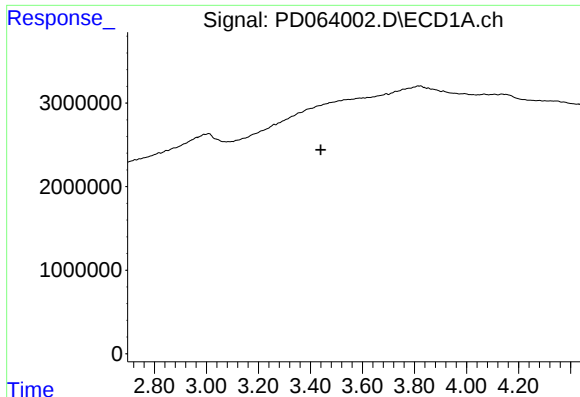

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.439 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

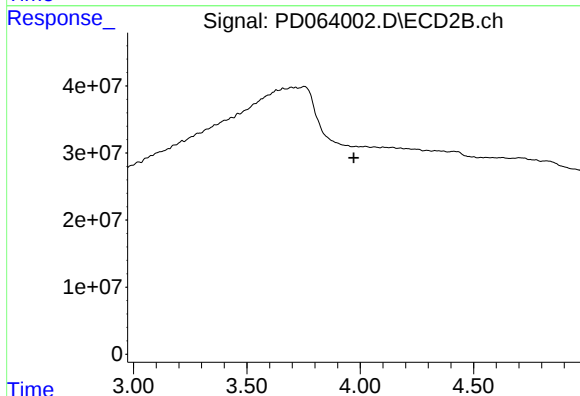


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.971 min
Response: 0
Conc: N.D.

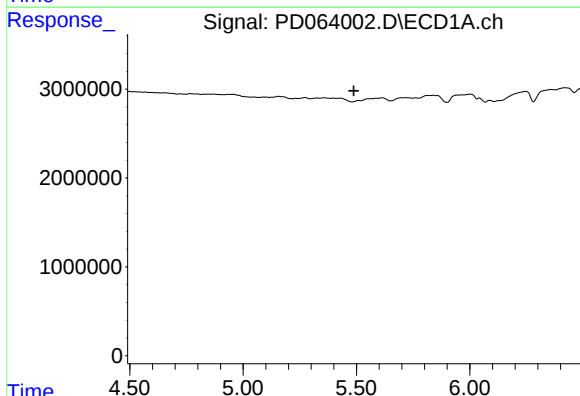


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.488 min
Response: 0
Conc: N.D.

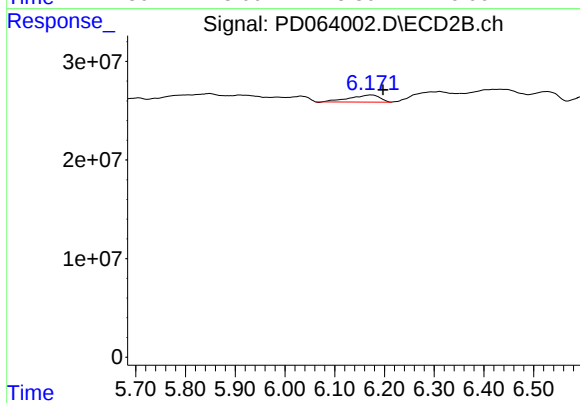

#9 Endosulfan I


R.T.: 6.173 min
Delta R.T.: -0.025 min
Response: 30243015
Conc: 1.53 ng/ml

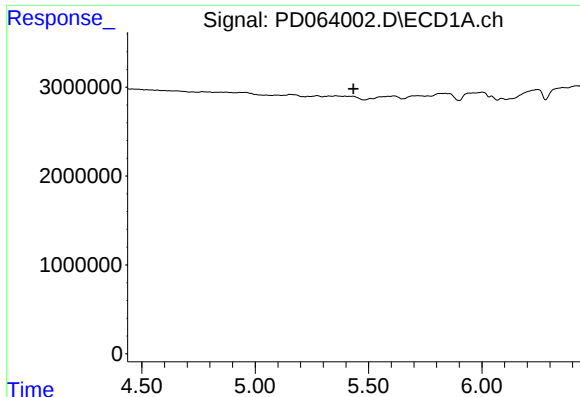

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

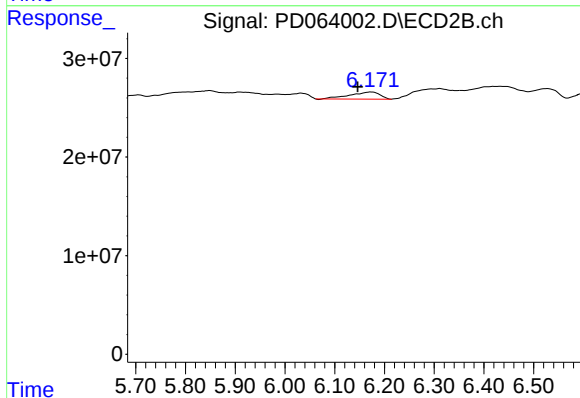


#11 cis-Chlordane

R.T.: 6.173 min
Delta R.T.: 0.026 min
Response: 30243015
Conc: 1.50 ng/ml

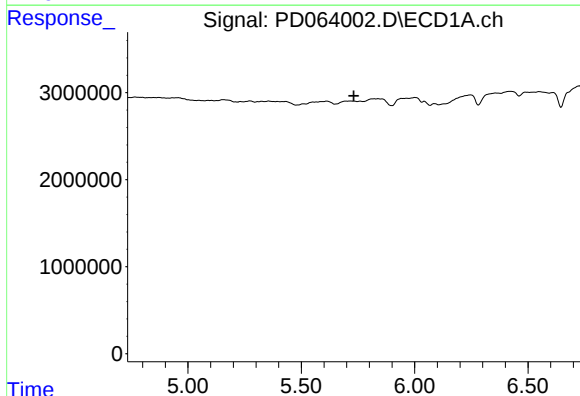


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.731 min
Response: 0
Conc: N.D.

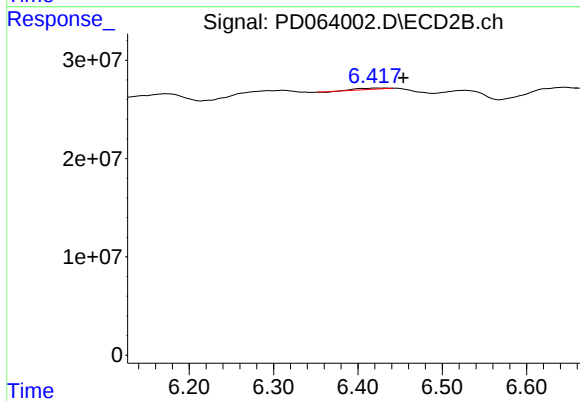

#13 Dieldrin


R.T.: 6.433 min
Delta R.T.: -0.021 min
Response: 2522620
Conc: 0.12 ng/ml

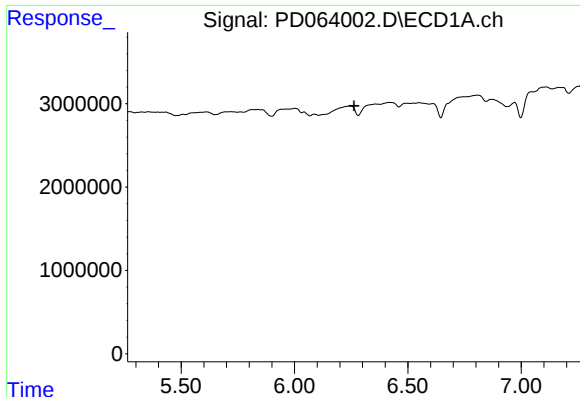

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.263 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

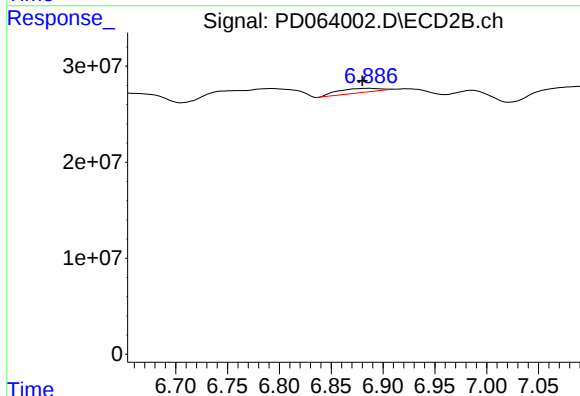


#15 Endosulfan II

R.T.: 6.887 min
Delta R.T.: 0.007 min
Response: 12035606
Conc: 0.74 ng/ml

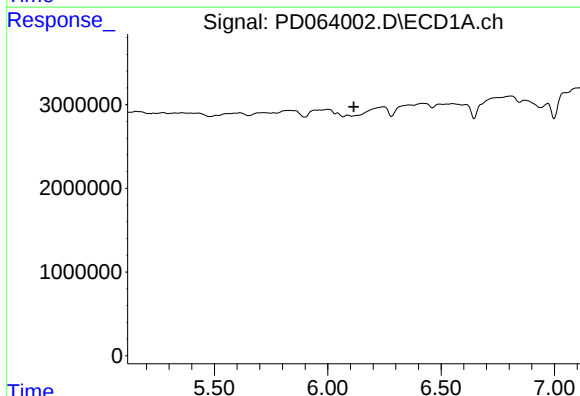


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.115 min
Response: 0
Conc: N.D.

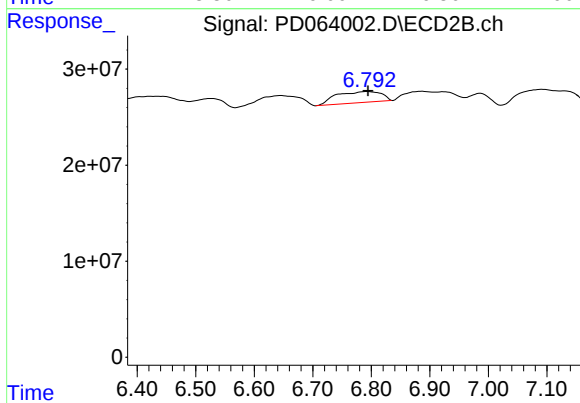

#16 4,4'-DDD


R.T.: 6.793 min
Delta R.T.: -0.001 min
Response: 62269713
Conc: 3.70 ng/ml

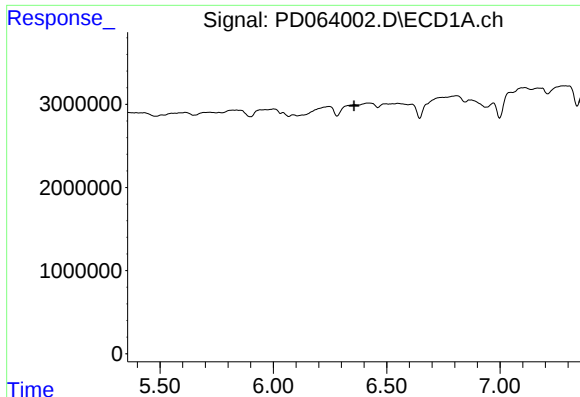

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.357 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

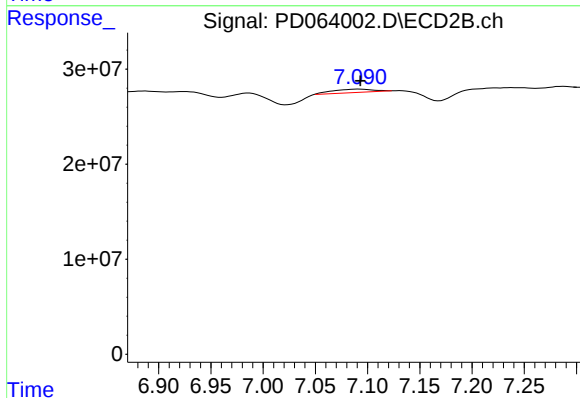


#17 4,4'-DDT

R.T.: 7.092 min
Delta R.T.: 0.000 min
Response: 9776216
Conc: 0.59 ng/ml

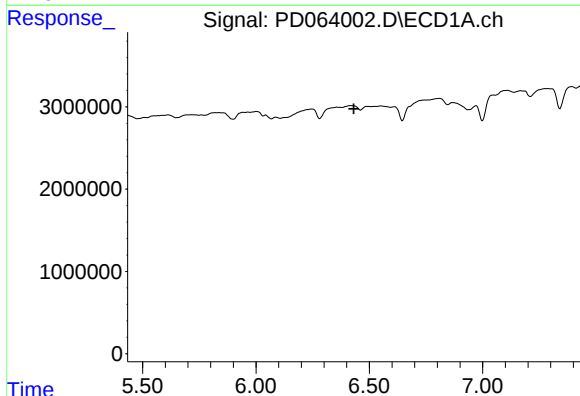


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.432 min
Response: 0
Conc: N.D.

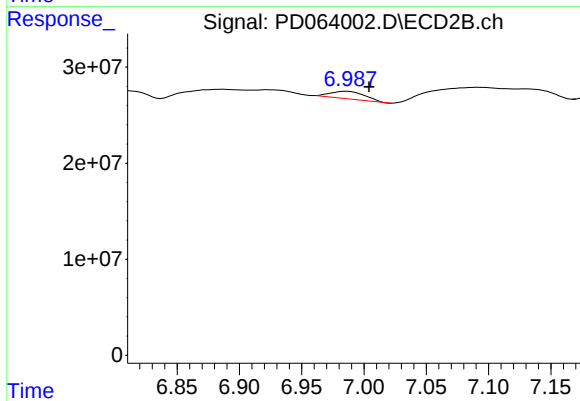

#18 Endrin aldehyde


R.T.: 6.986 min
Delta R.T.: -0.018 min
Response: 15131694
Conc: 1.08 ng/ml

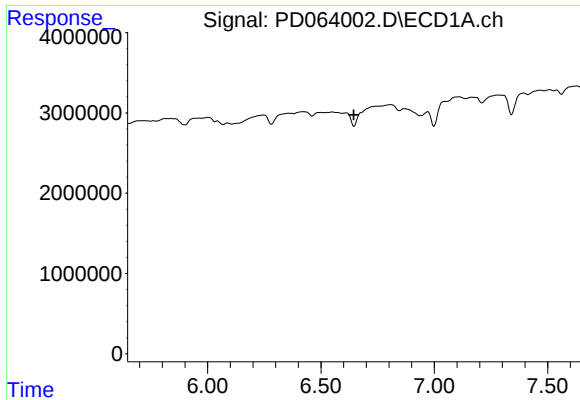

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.645 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

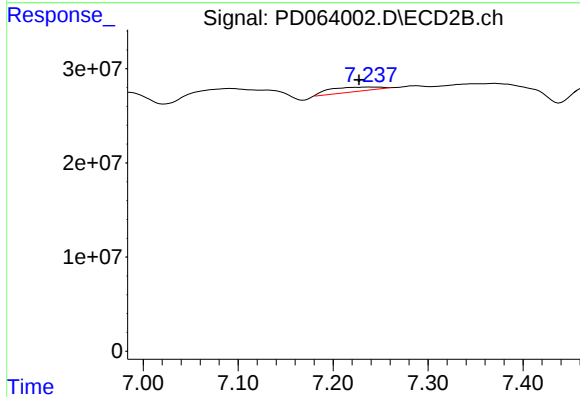


#19 Endosulfan Sulfate

R.T.: 7.239 min
Delta R.T.: 0.011 min
Response: 17103118
Conc: 1.04 ng/ml

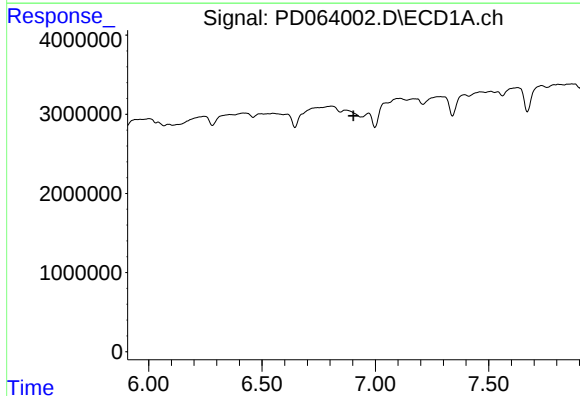


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.904 min
Response: 0
Conc: N.D.

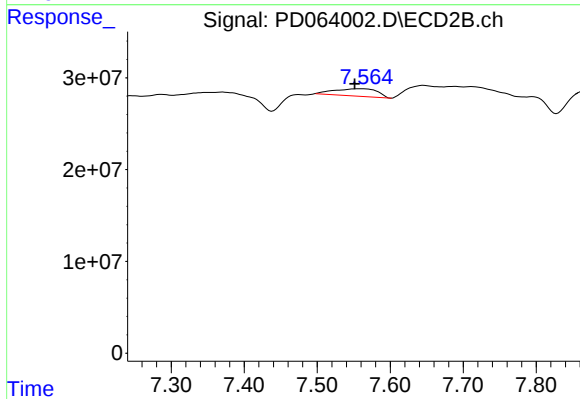

#20 Methoxychlor


R.T.: 7.559 min
Delta R.T.: 0.007 min
Response: 32902746
Conc: 4.25 ng/ml

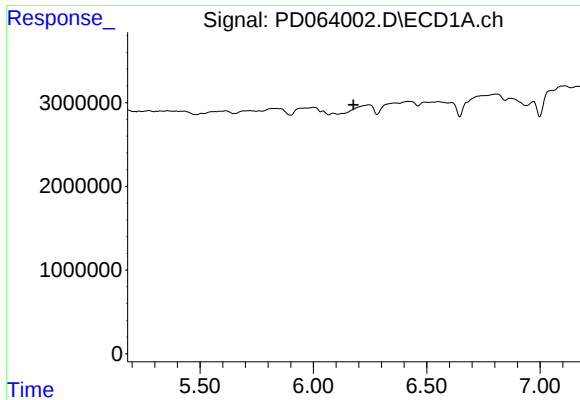

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 6.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

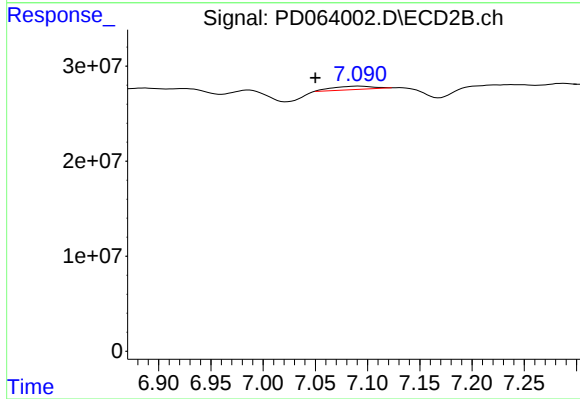


#24 Toxaphene-3

R.T.: 7.092 min
Delta R.T.: 0.042 min
Response: 9776216
Conc: 70.96 ng/ml

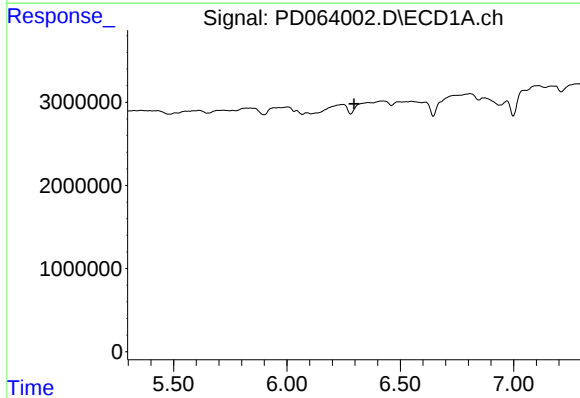


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T.: 6.297 min
Response: 0
Conc: N.D.

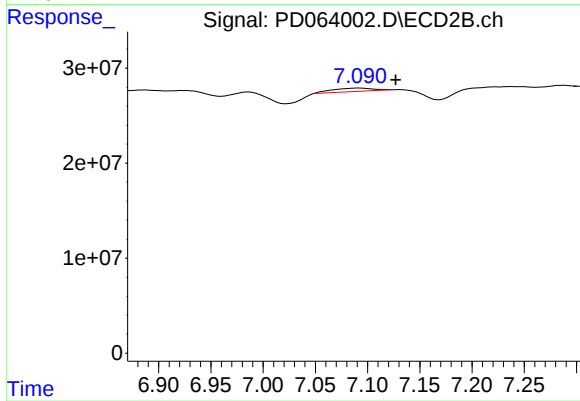

#25 Toxaphene-4


R.T.: 7.092 min
Delta R.T.: -0.035 min
Response: 9776216
Conc: 23.70 ng/ml

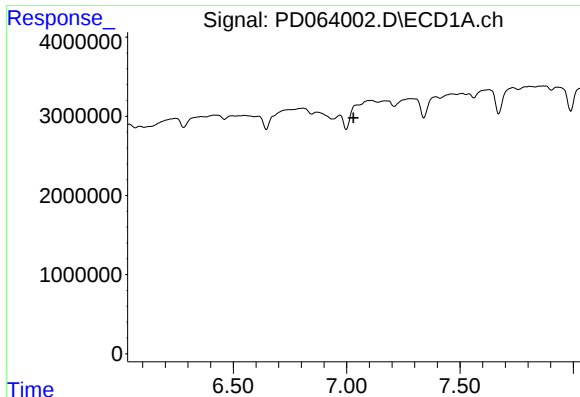

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T.: 7.030 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

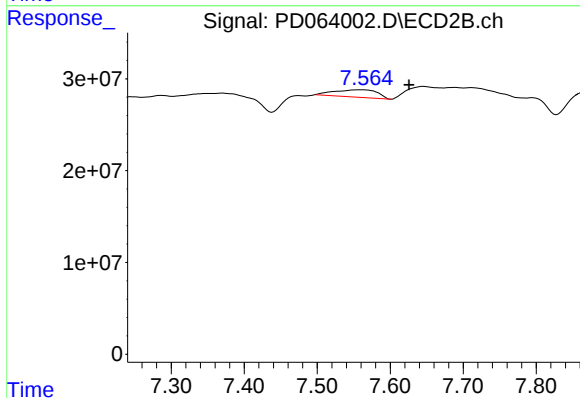


#26 Toxaphene-5

R.T.: 7.559 min
Delta R.T.: -0.067 min
Response: 32902746
Conc: 192.63 ng/ml

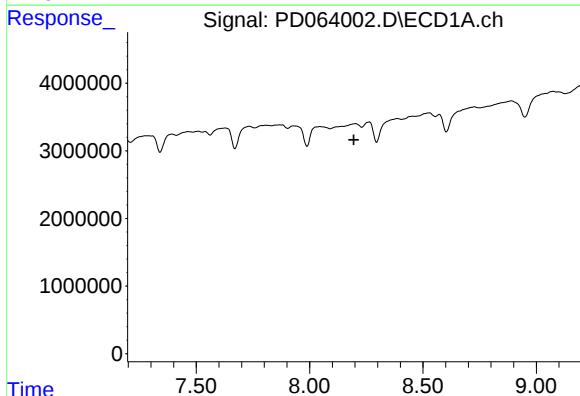

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.194 min
Response: 0
Conc: N.D.

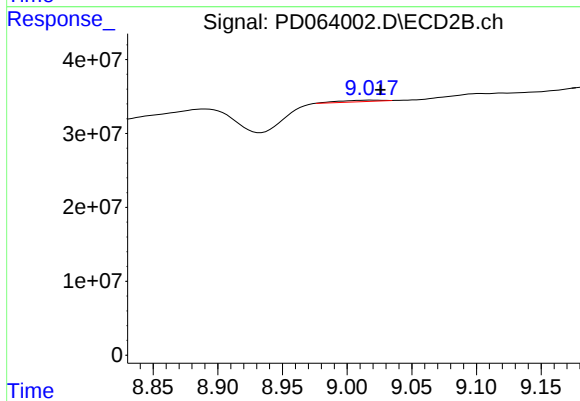

#27 Decachlorobiphenyl

R.T.: 9.018 min
Delta R.T.: -0.007 min
Response: 4431447
Conc: 0.32 ng/ml