

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062921\
 Data File : PD064004.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2021 15:32
 Operator : AR\AJ
 Sample : M2872-11
 Misc : PEST- GPC- BLANK
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 03:59:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 21 04:24:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
6) B	beta-BHC	0.000	4.835	0	134.1E6	N.D. 13.746
15) B	Endosulfa...	0.000	6.893	0	11237672	N.D. 0.695
20) A	Methoxychlor	0.000	7.577	0	4364765	N.D. 0.564
26)	Toxaphene-5	0.000	7.577	0	4364765	N.D. 25.554

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062921\
Data File : PD064004.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2021 15:32
Operator : AR\AJ
Sample : M2872-11
Misc : PEST- GPC- BLANK
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 03:59:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

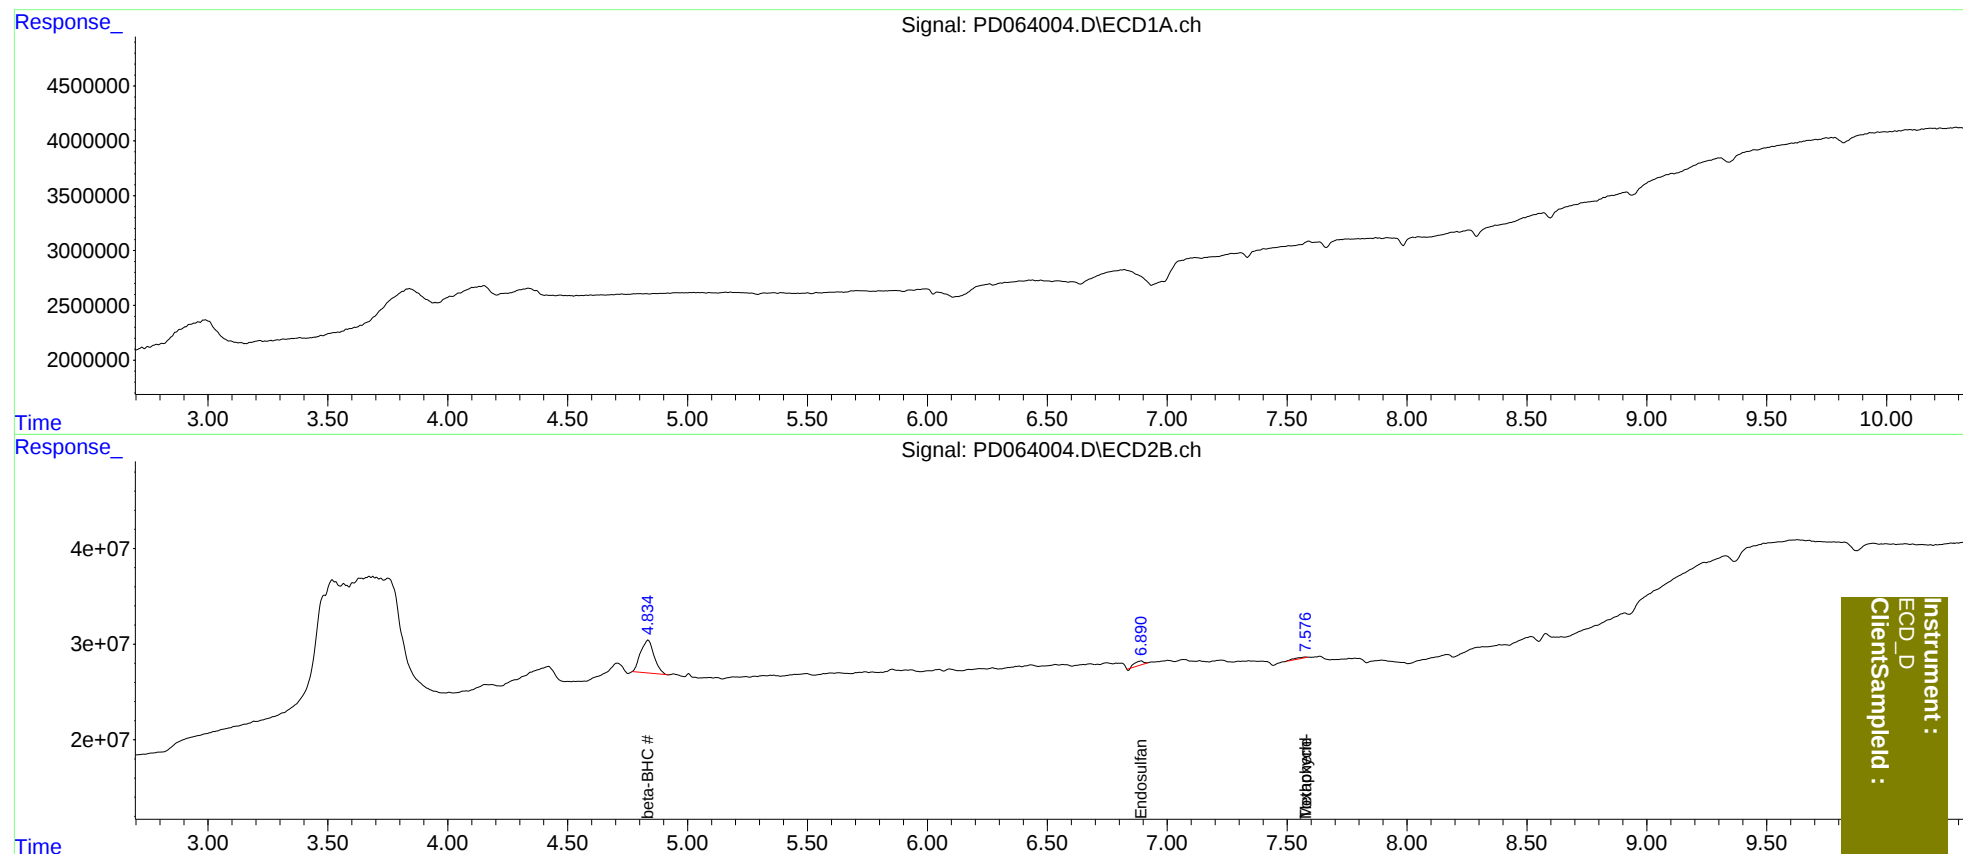


Instrument :
ECD_D
ClientSampleId :

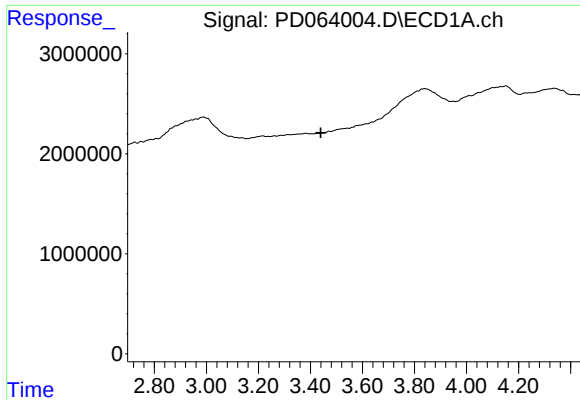

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.439 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

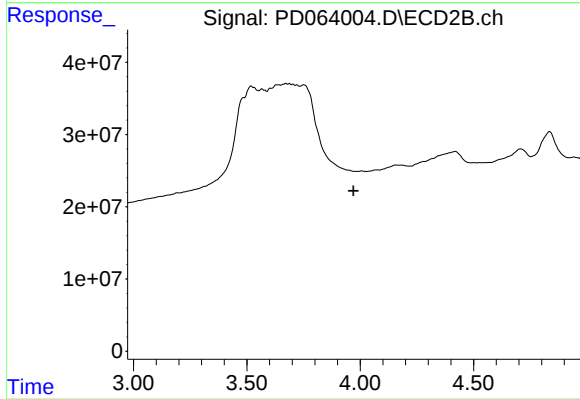


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.971 min
Response: 0
Conc: N.D.

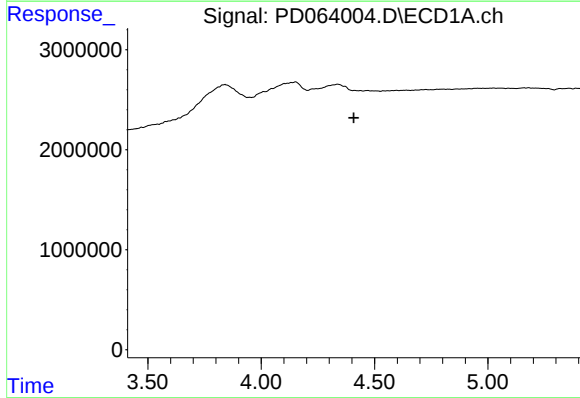


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.409 min
Response: 0
Conc: N.D.

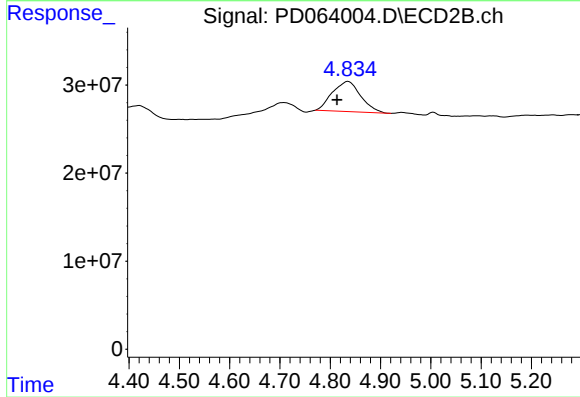

#6 beta-BHC


R.T.: 4.835 min
Delta R.T.: 0.022 min
Response: 134064139
Conc: 13.75 ng/ml

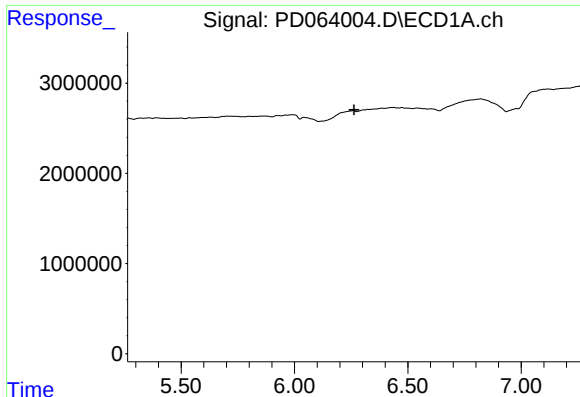

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.263 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

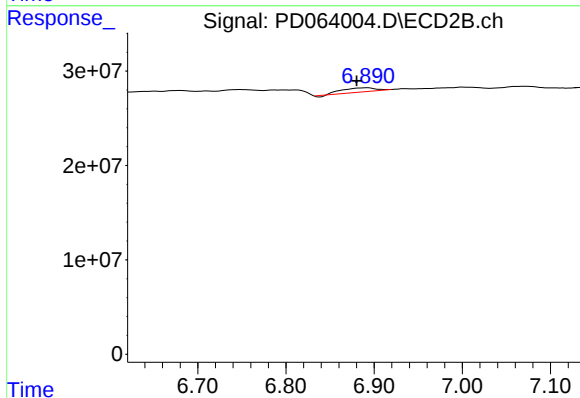


#15 Endosulfan II

R.T.: 6.893 min
Delta R.T.: 0.013 min
Response: 11237672
Conc: 0.69 ng/ml

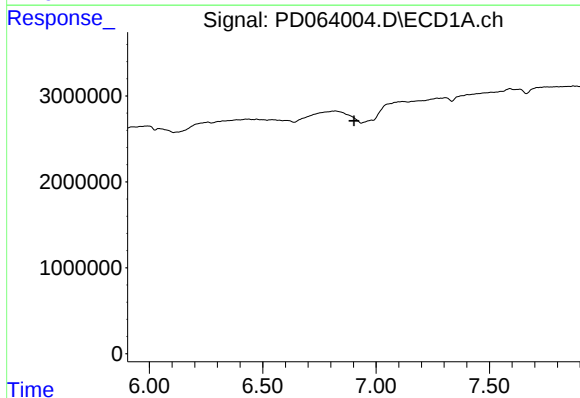


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.904 min
Response: 0
Conc: N.D.

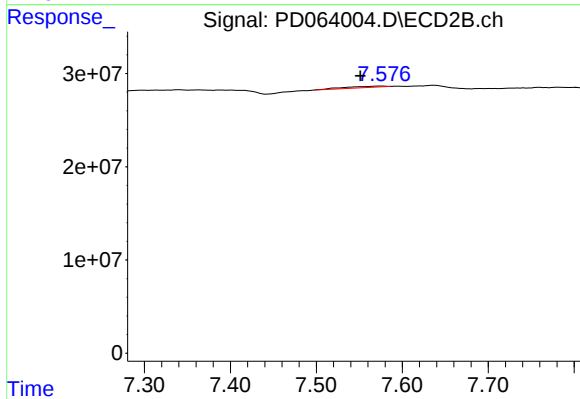

#20 Methoxychlor


R.T.: 7.577 min
Delta R.T.: 0.026 min
Response: 4364765
Conc: 0.56 ng/ml

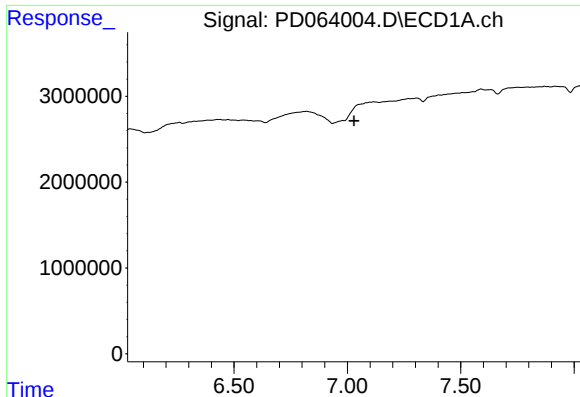

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T.: 7.030 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

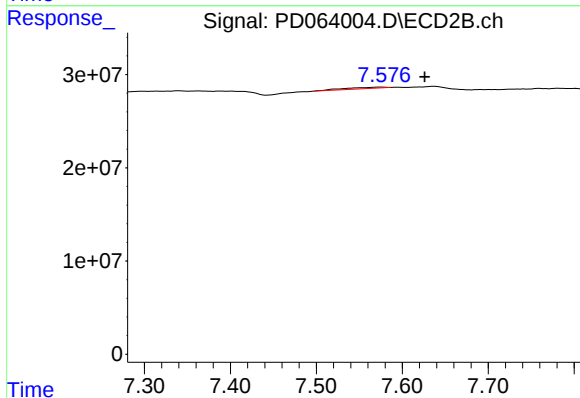


#26 Toxaphene-5

R.T.: 7.577 min
Delta R.T.: -0.049 min
Response: 4364765
Conc: 25.55 ng/ml

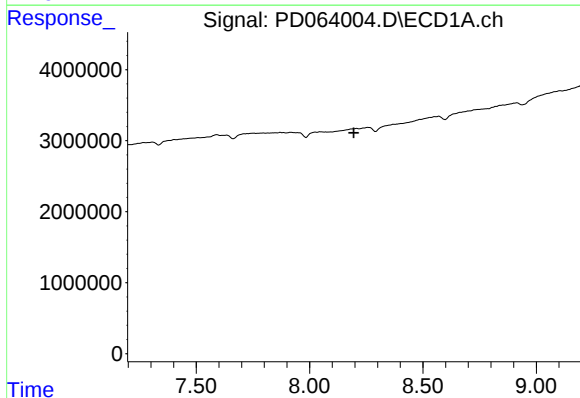

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.194 min
Response: 0
Conc: N.D.

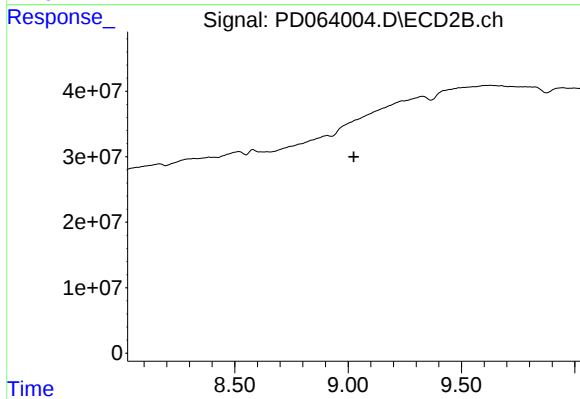

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.026 min
Response: 0
Conc: N.D.