

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062921\
Data File : PD064013.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2021 18:11
Operator : AR\AJ
Sample : M2853-03
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
C0AW1

Manual Integrations
APPROVED

Ankita
6/30/2021 2:03:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 04:01:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

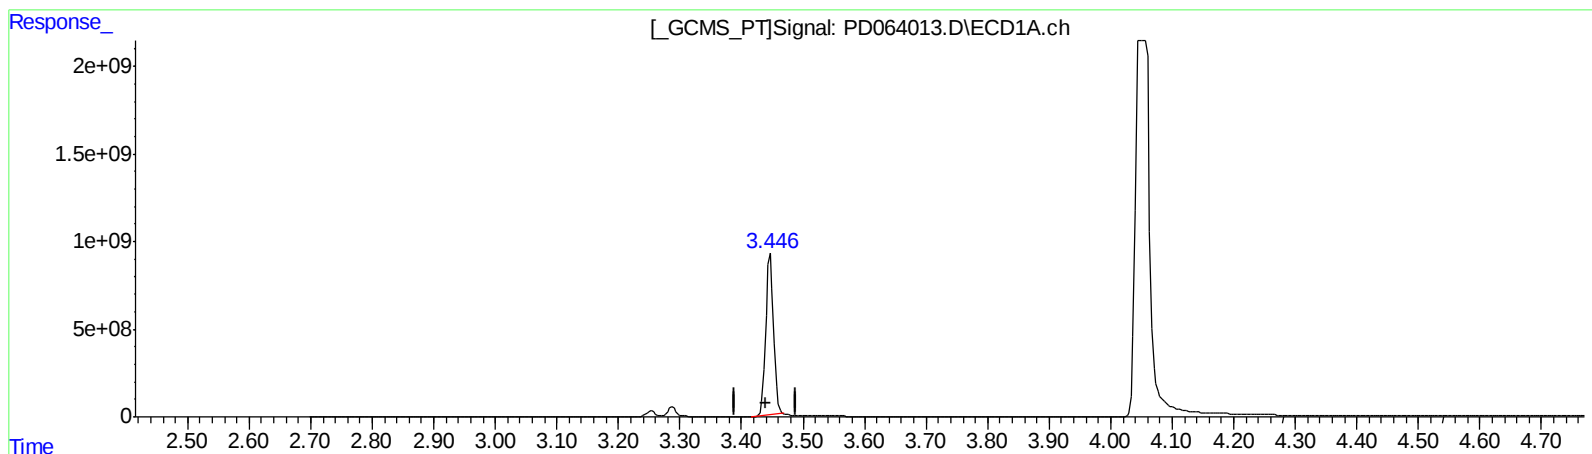

(1) Tetrachloro-m-xylene (SA)

3.447min 5167.408 ng/ml

response 8032802944

(1) Tetrachloro-m-xylene #2 (SA)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062921\
Data File : PD064013.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2021 18:11
Operator : AR\AJ
Sample : M2853-03
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
C0AW1

Manual Integrations
APPROVED

Ankita
6/30/2021 2:03:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 04:01:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

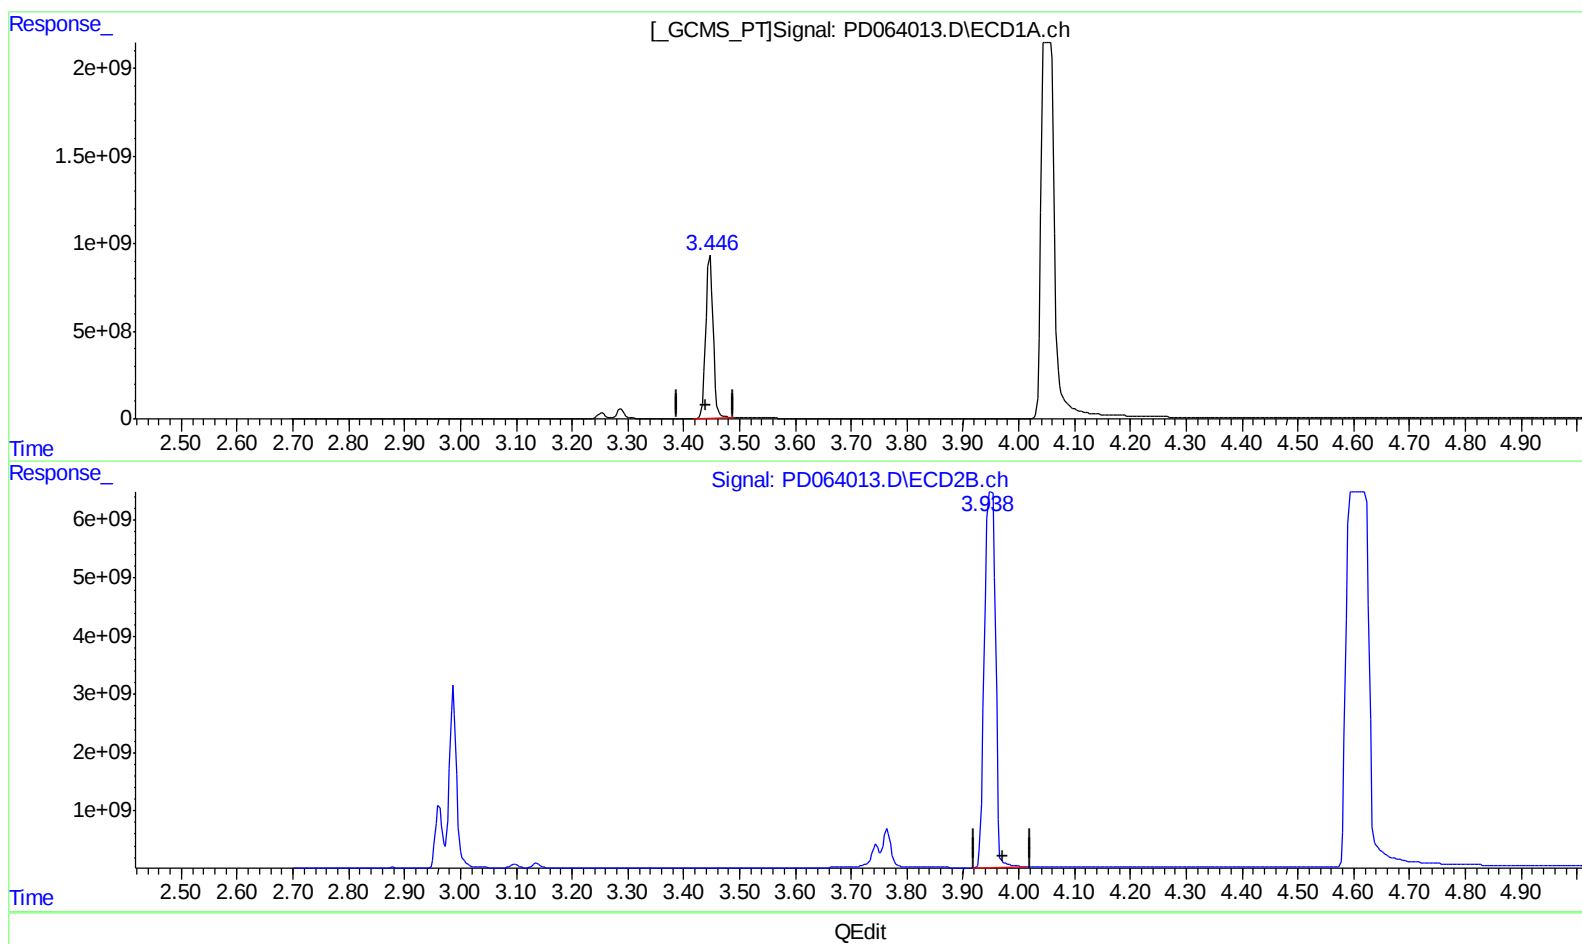

(1) Tetrachloro-m-xylene (SA)

3.446min 5380.096 ng/ml m

response 8363428812

(1) Tetrachloro-m-xylene #2 (SA)

3.938min 2494.608 ng/ml m

response 39509540857

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062921\
 Data File : PD064013.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2021 18:11
 Operator : AR\AJ
 Sample : M2853-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AW1

Manual Integrations
 APPROVED

Ankita
 6/30/2021 2:03:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 04:01:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 21 04:24:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.446	3.938f	8363.4E6	39509.5E6	5380.096m	2494.608m#
27) SA Decachlor...	8.185	9.022	61205586	582.8E6	35.359	42.027

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AJ
 07/06/21