

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD063021\
 Data File : PD064055.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2021 14:36
 Operator : AR\AJ
 Sample : INDA319
 Misc :
 ALS Vial : 13 Sample Multiplier: 1



Instrument :
 ECD_D
 LabSampleId :
 INDA319

Manual Integrations
 APPROVED

mohammad
 7/1/2021 8:29:58 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 05:18:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 21 04:24:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

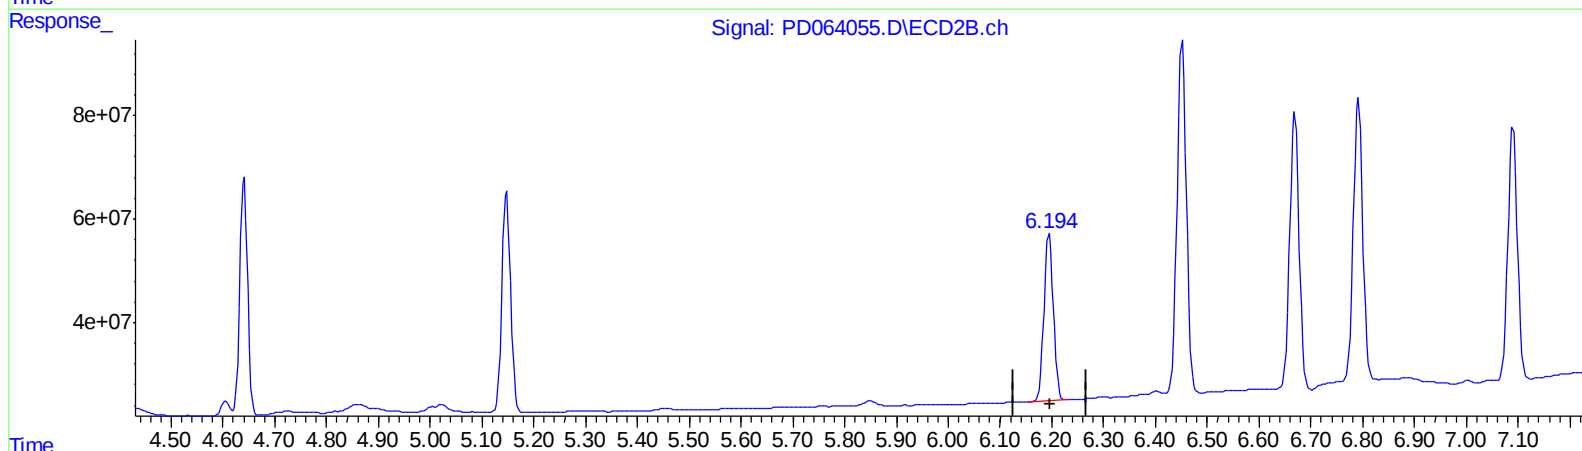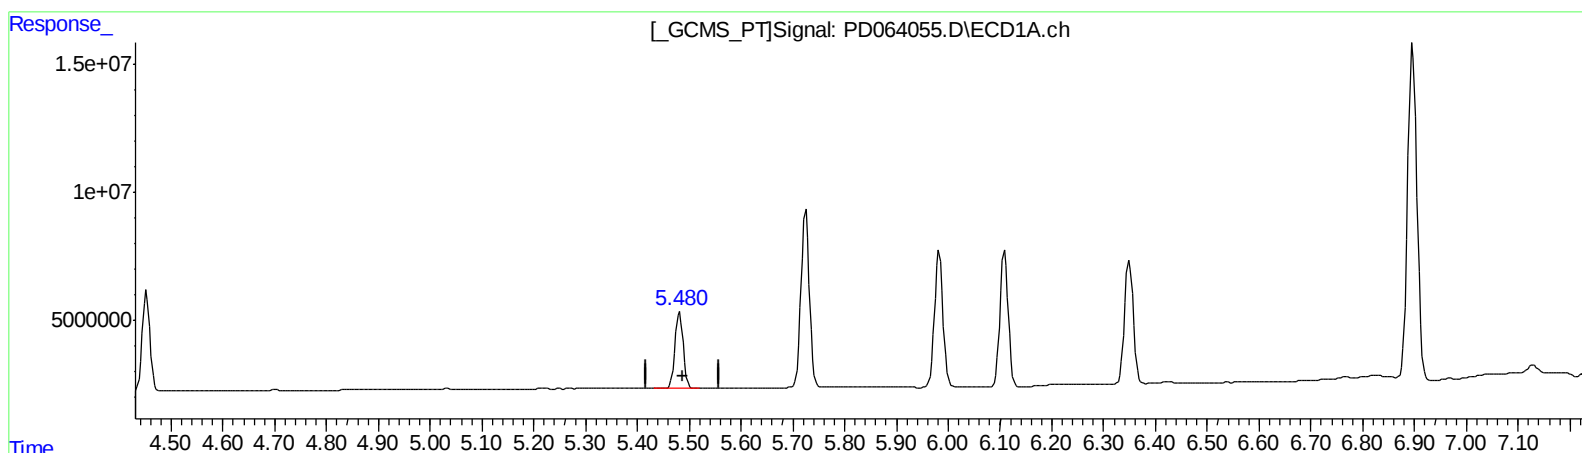

QEdit

(9) Endosulfan I (A)

5.482min 18.296 ng/ml

response 33479329

(9) Endosulfan I #2 (A)

6.194min 20.624 ng/ml m

response 408563718

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD063021\
 Data File : PD064055.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2021 14:36
 Operator : AR\AJ
 Sample : INDA319
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 LabSampleId :
 INDA319

Manual Integrations
 APPROVED

mohammad
 7/1/2021 8:29:58 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 05:18:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 21 04:24:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.434	3.969	28258764	341.6E6	18.179	21.568
27) SA Decachlor...	8.188	9.023	64206644	606.0E6	37.093	43.700
Target Compounds						
2) A alpha-BHC	3.870	4.357	42433257	530.4E6	18.141	21.349
3) MA gamma-BHC...	4.153	4.641	40809342	489.8E6	17.932	21.466
4) MA Heptachlor	4.453	5.148	39673798	493.0E6	18.172	21.162
9) A Endosulfan I	5.482	6.194	33479329	408.6E6	18.296	20.624m
13) MA Dieldrin	5.725	6.452	76577847	865.3E6	36.592	41.362
14) MA Endrin	5.983	6.669	61054590	680.0E6	33.760	38.863
16) A 4,4'-DDD	6.109	6.792	60782239	692.3E6	36.815	41.127
17) MA 4,4'-DDT	6.350	7.091	56167529	628.7E6	33.373	38.191
20) A Methoxychlor	6.897	7.549	162.1E6	1524.1E6	175.811	196.992

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Handwritten note: AJ
 07/06/21