

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD063022\
 Data File : PD070634.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2022 23:52
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4036

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/01/2022
 Supervised By : Ankita Jodhani 07/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 02:25:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD063022CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 01 02:06:38 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.487	4.127	89984936	919.8E6	39.944	40.732
27)	SA Decachlor...	8.267	9.320	164.5E6	463.5E6	79.604	79.830
Target Compounds							
2)	A alpha-BHC	3.930	4.531	130.3E6	1298.7E6	39.281	40.261
3)	MA gamma-BHC...	4.215	4.824	124.8E6	1162.9E6	39.486	40.338
4)	MA Heptachlor	4.517	5.340	125.8E6	1100.6E6	39.429	40.458
9)	A Endosulfan I	5.553	6.411	104.9E6	681.2E6	39.543	40.396
13)	MA Dieldrin	5.797	6.672	238.3E6	1365.9E6	79.086	79.966
14)	MA Endrin	6.056	6.896	203.2E6	1026.1E6	79.161	79.731
16)	A 4,4'-DDD	6.181	7.009	187.4E6	1030.6E6	78.965m	80.630m
17)	MA 4,4'-DDT	6.425	7.311	186.2E6	939.7E6	78.259	79.403
20)	A Methoxychlor	6.977	7.771	494.4E6	2114.1E6	402.464	399.733

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD063022\
Data File : PD070634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2022 23:52
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 02:25:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD063022CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 01 02:06:38 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

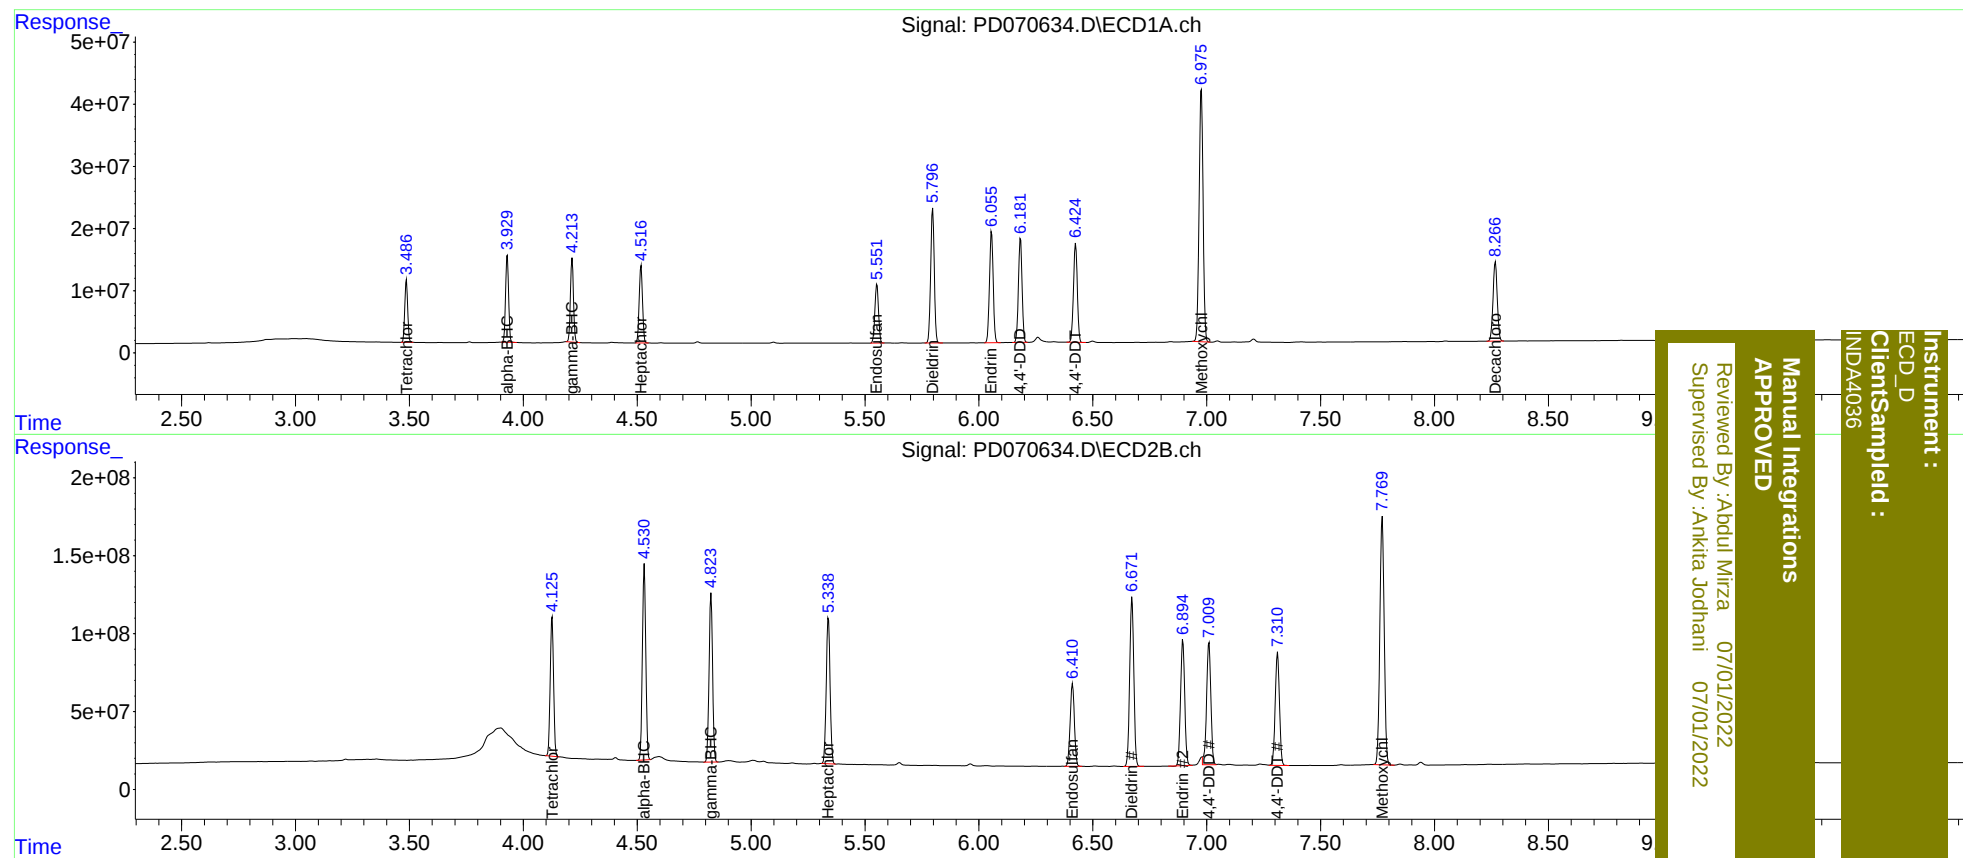

Reviewed By: Abdul Mirza 07/01/2022
Supervised By: Ankita Jodhani 07/01/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
INDA4036