

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD063022\
 Data File : PD070636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2022 00:20
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5038

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/01/2022
 Supervised By : Ankita Jodhani 07/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 02:22:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD063022CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 01 02:06:38 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.487	4.126	179.2E6	1765.2E6	79.525	78.655
27)	SA Decachlor...	8.267	9.319	326.7E6	904.4E6	157.796	155.673
Target Compounds							
2)	A alpha-BHC	3.930	4.531	269.7E6	2547.1E6	80.796	79.138
3)	MA gamma-BHC...	4.215	4.824	254.7E6	2263.6E6	80.261	78.737
4)	MA Heptachlor	4.517	5.340	258.1E6	2141.7E6	80.479	79.027
9)	A Endosulfan I	5.552	6.411	212.8E6	1328.6E6	79.923	79.041
13)	MA Dieldrin	5.797	6.673	488.8E6	2709.8E6	161.595	158.616
14)	MA Endrin	6.056	6.895	417.0E6	2050.6E6	161.907	159.165
16)	A 4,4'-DDD	6.182	7.009	384.2E6	2001.4E6	161.203	156.992m
17)	MA 4,4'-DDT	6.424	7.311	388.7E6	1884.9E6	162.198	158.866
20)	A Methoxychlor	6.976	7.771	981.8E6	4194.5E6	800.899	792.905

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD063022\
Data File : PD070636.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2022 00:20
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 02:22:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD063022CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 01 02:06:38 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

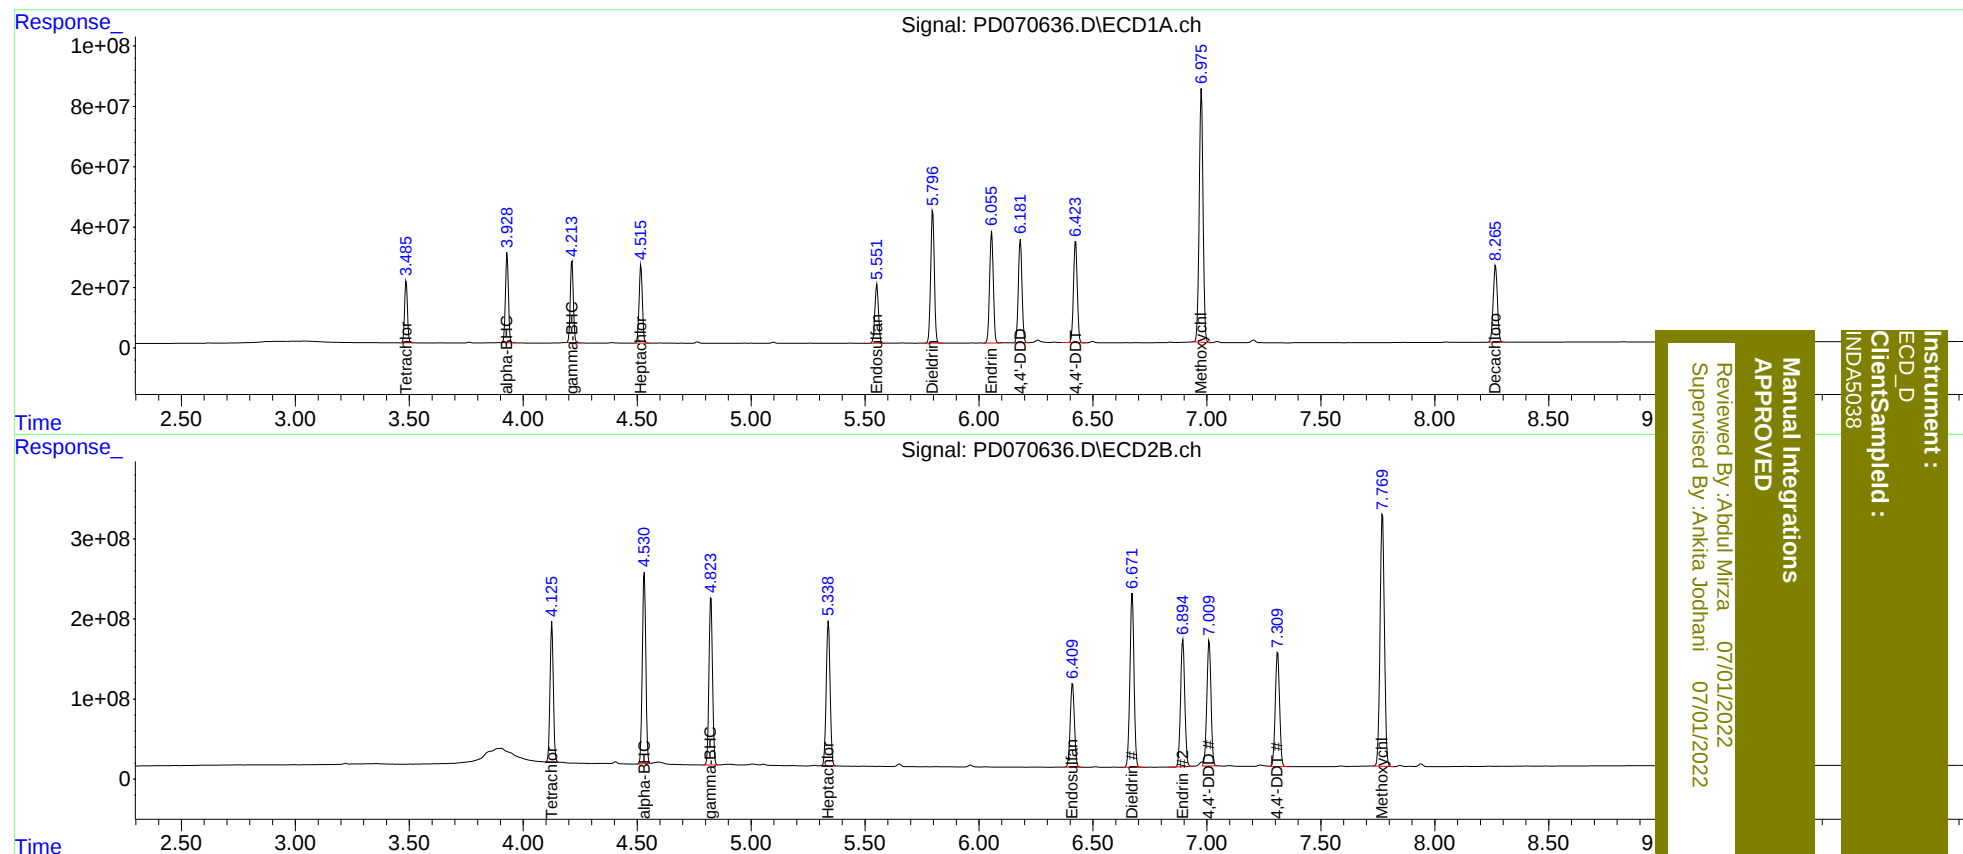

Reviewed By: Abdul Mirza 07/01/2022
Supervised By: Ankita Jodhani 07/01/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
INDA5038