

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD063022\
 Data File : PD070643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2022 01:59
 Operator : AR\AJ
 Sample : N3392-20 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
ClientSampleId :
 EXEZ5

Manual Integrations
APPROVED
 Reviewed By :Abdul Mirza 07/01/2022
 Supervised By :Ankita Jodhani 07/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 03:53:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD063022CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 01 03:19:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.486	4.126	42466050	448.7E6	18.871	19.421
27) SA Decachlor...	8.266	9.320	81602546	240.5E6	38.552	38.067
Target Compounds						
12) B 4,4'-DDE	5.663	6.509	1212985	9238511	0.434	0.530m
16) A 4,4'-DDD	6.182	7.010	14931896	107.3E6	6.466	8.154 #
17) MA 4,4'-DDT	6.421	7.309	945767	6867364	0.413m	0.573m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD063022\
 Data File : PD070643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2022 01:59
 Operator : AR\AJ
 Sample : N3392-20 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 03:53:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD063022CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 01 03:19:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

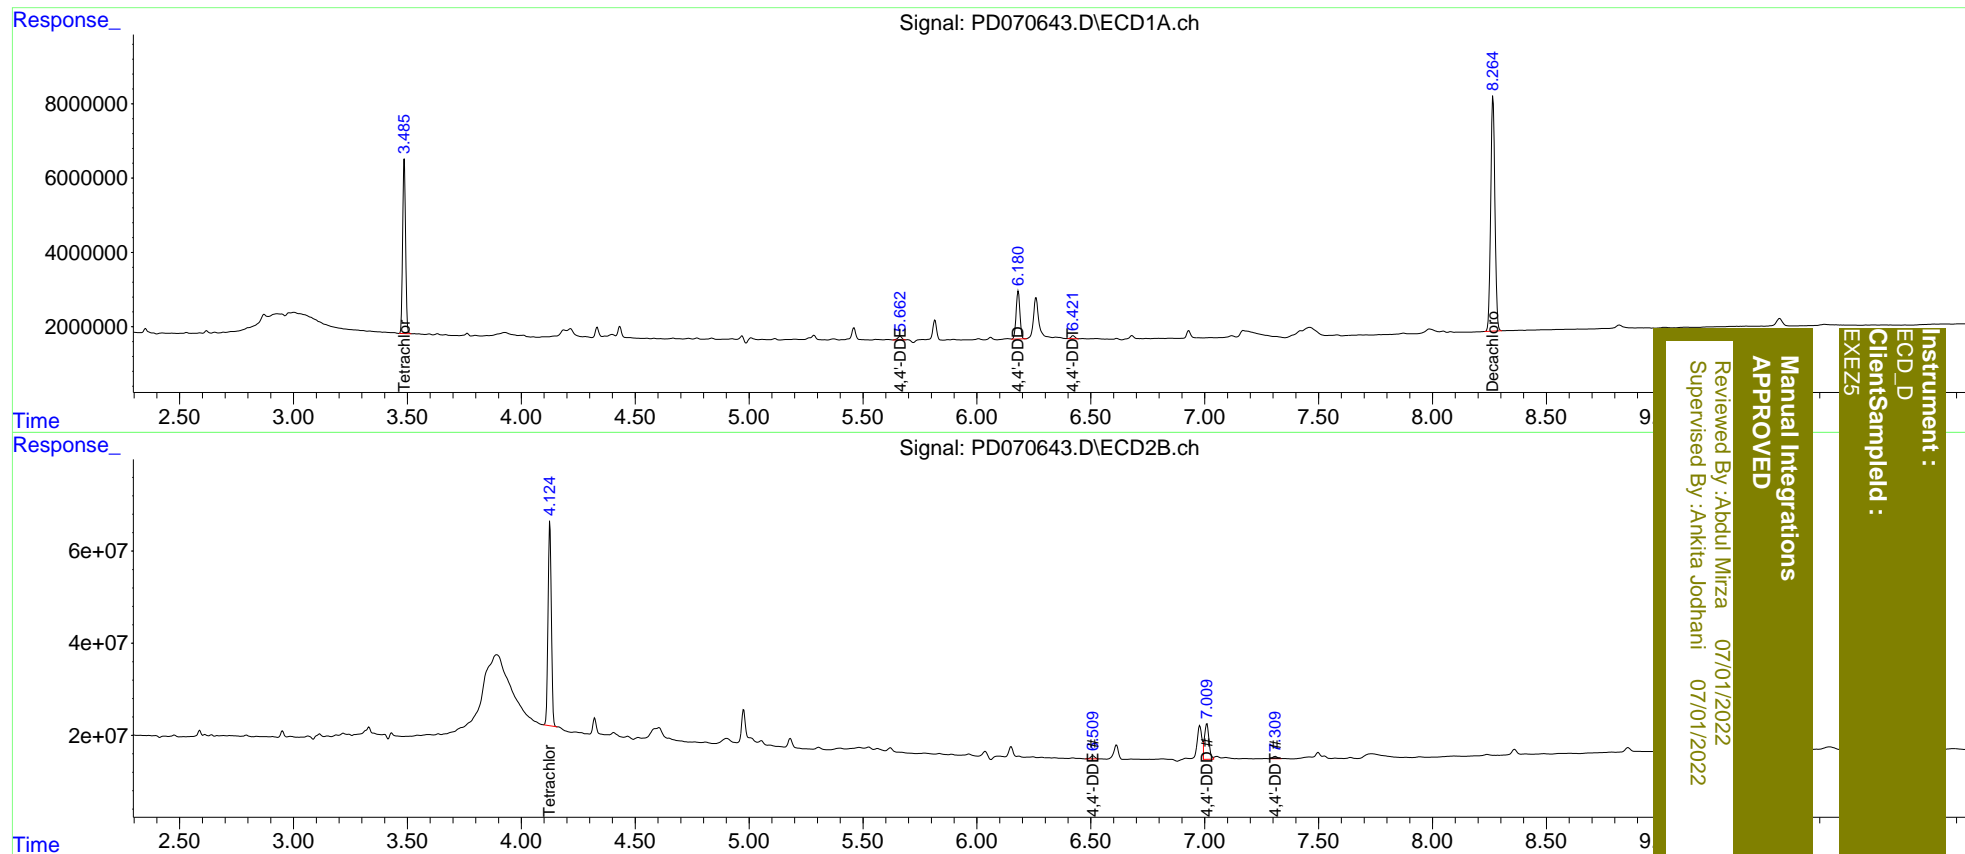

Instrument : ECD_D
 Client/Sampled : EXEZ5
 Manual Integrations
 APPROVED
 Reviewed By : Abdul Mirza 07/01/2022
 Supervised By : Ankita Jodhani 07/01/2022