

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD063022\
 Data File : PD070646.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2022 02:41
 Operator : AR\AJ
 Sample : N3392-01 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EXEX6

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/05/2022
 Supervised By : Ankita Jodhani 07/05/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 20:57:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD063022CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 01 03:19:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.487	4.126	47436504	492.7E6	21.080	21.325
2) SA Decachlor...	8.267	9.316	87465285	265.4E6	41.322	41.999m
Target Compounds						
16) A 4,4'-DDD	6.188	7.010	8340603	8941673	3.612m	0.679m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD063022\
Data File : PD070646.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2022 02:41
Operator : AR\AJ
Sample : N3392-01 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 20:57:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD063022CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 01 03:19:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

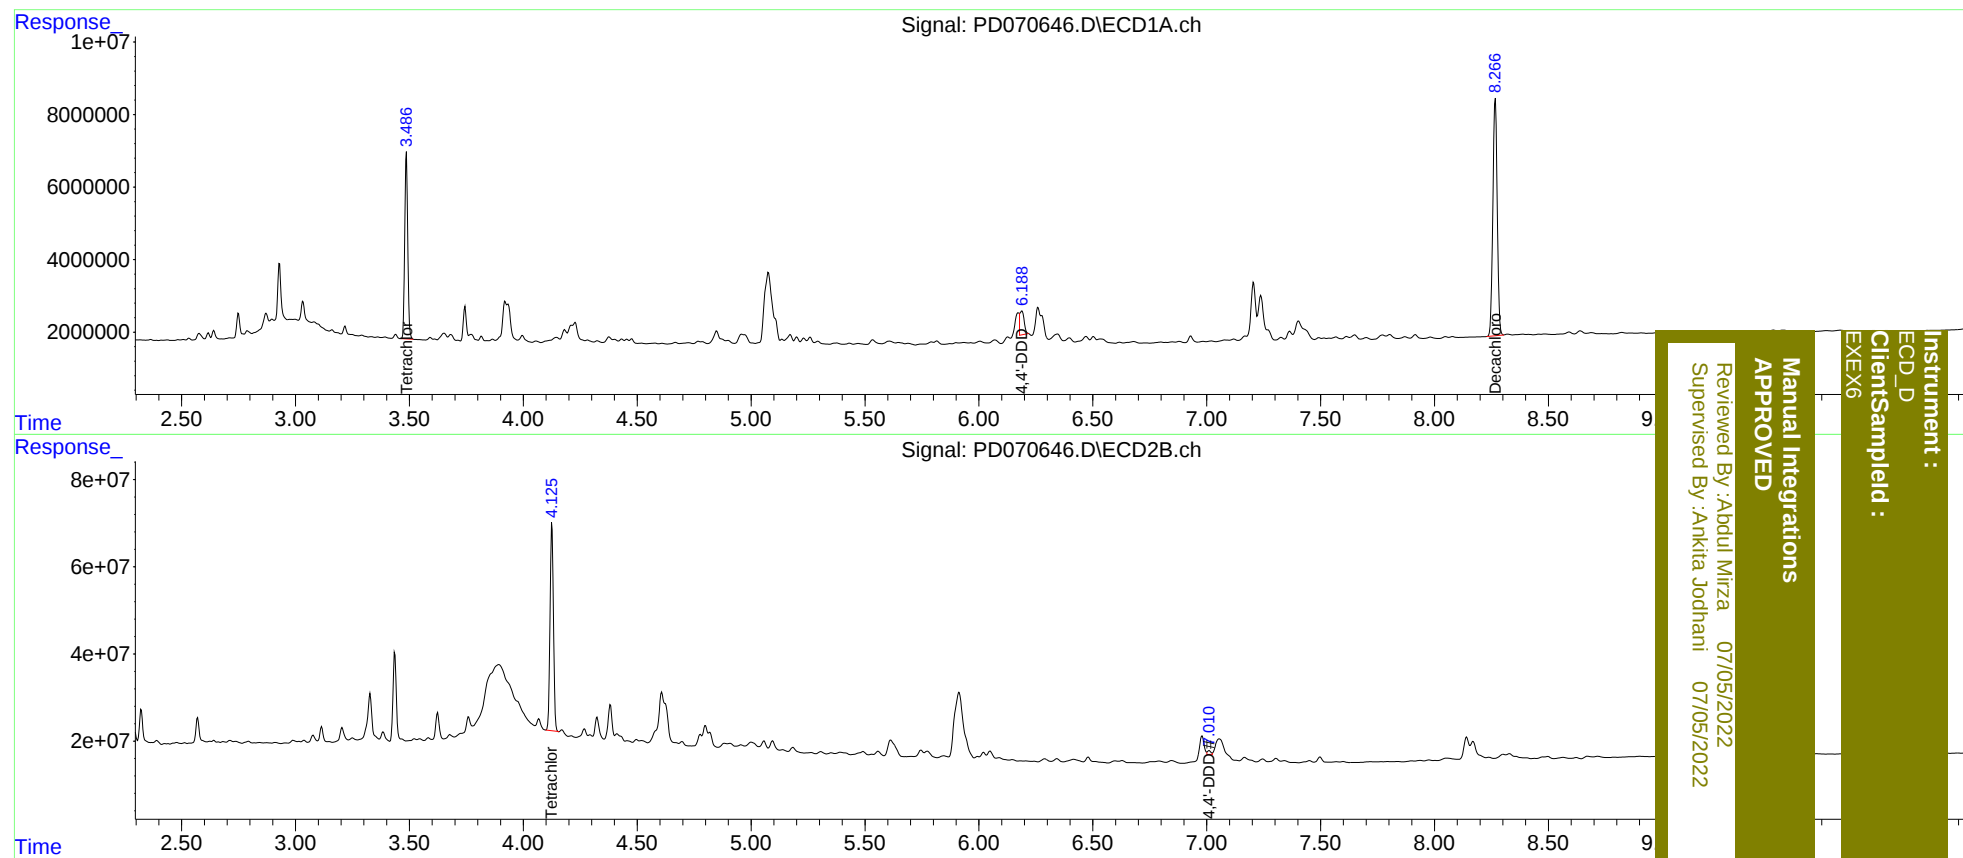

Reviewed By: Abdul Mirza 07/05/2022
Supervised By: Ankita Jodhani 07/05/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
EXEX6