

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070119\
 Data File : PD053774.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jul 2019 9:48
 Operator : SM\AJ
 Sample : K3419-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 10:24:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 22 00:19:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.983	11543358	18340446	16.332	16.758
28)	SA Decachlor...	8.011	9.026	9256619	13670680	14.238	13.517
Target Compounds							
5)	MB Aldrin	0.000	5.463	0	3507176	N.D.	2.335 #
10)	B gamma-Chl...	0.000	6.083	0	2616867	N.D.	1.662 #
11)	B alpha-Chl...	0.000	6.155	0	2942397	N.D.	1.910 #
16)	A 4,4'-DDD	0.000	6.803	0	1275626	N.D.	1.251 #
17)	MA 4,4'-DDT	6.183	7.095	3040626	2401198	4.959	2.239 #
20)	A Methoxychlor	6.711f	0.000	1700012	0	6.259	N.D. #
24)	Chlordane-2	0.000	5.463f	0	3507176	N.D.	61.702 #
25)	Chlordane-3	0.000	6.083	0	2616867	N.D.	13.170 #
26)	Chlordane-4	0.000	6.155	0	2942397	N.D.	12.545 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070119\
Data File : PD053774.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jul 2019 9:48
Operator : SM\AJ
Sample : K3419-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 10:24:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062119.M
Quant Title : GC Extractables
QLast Update : Sat Jun 22 00:19:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

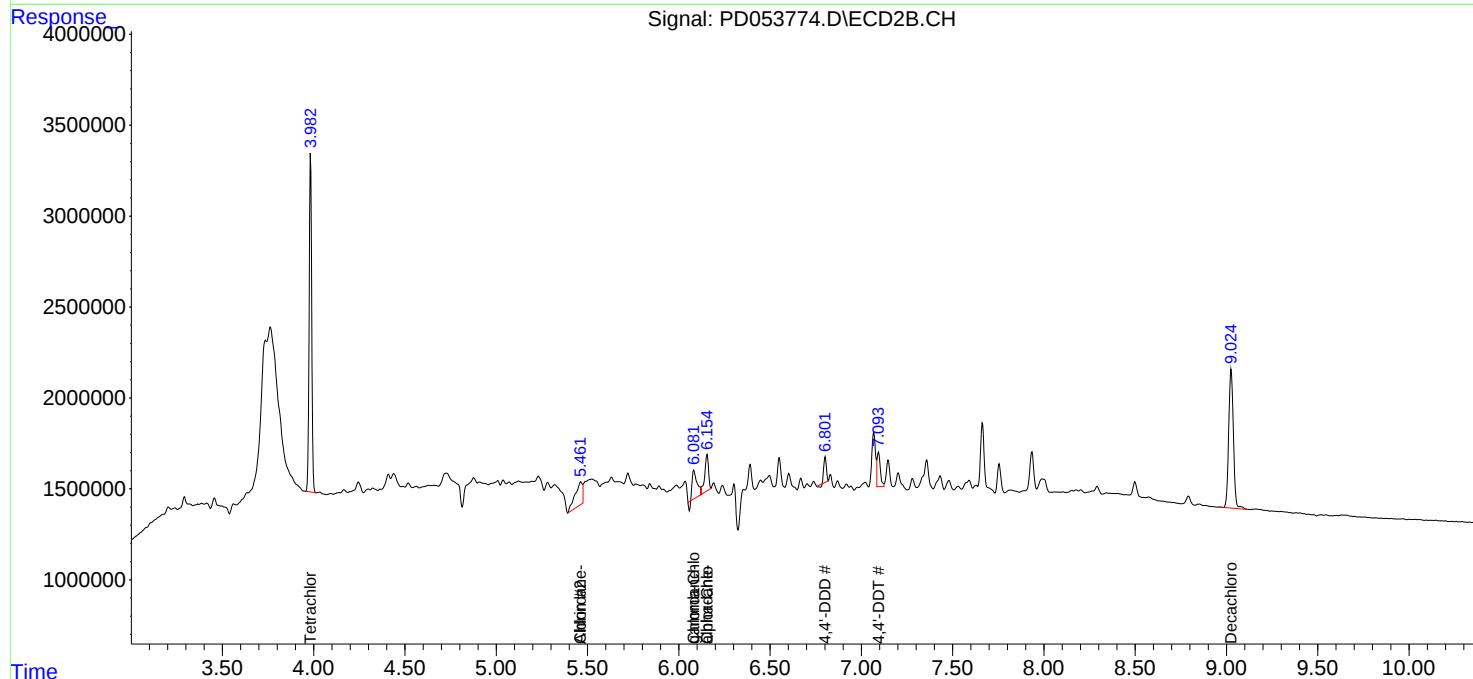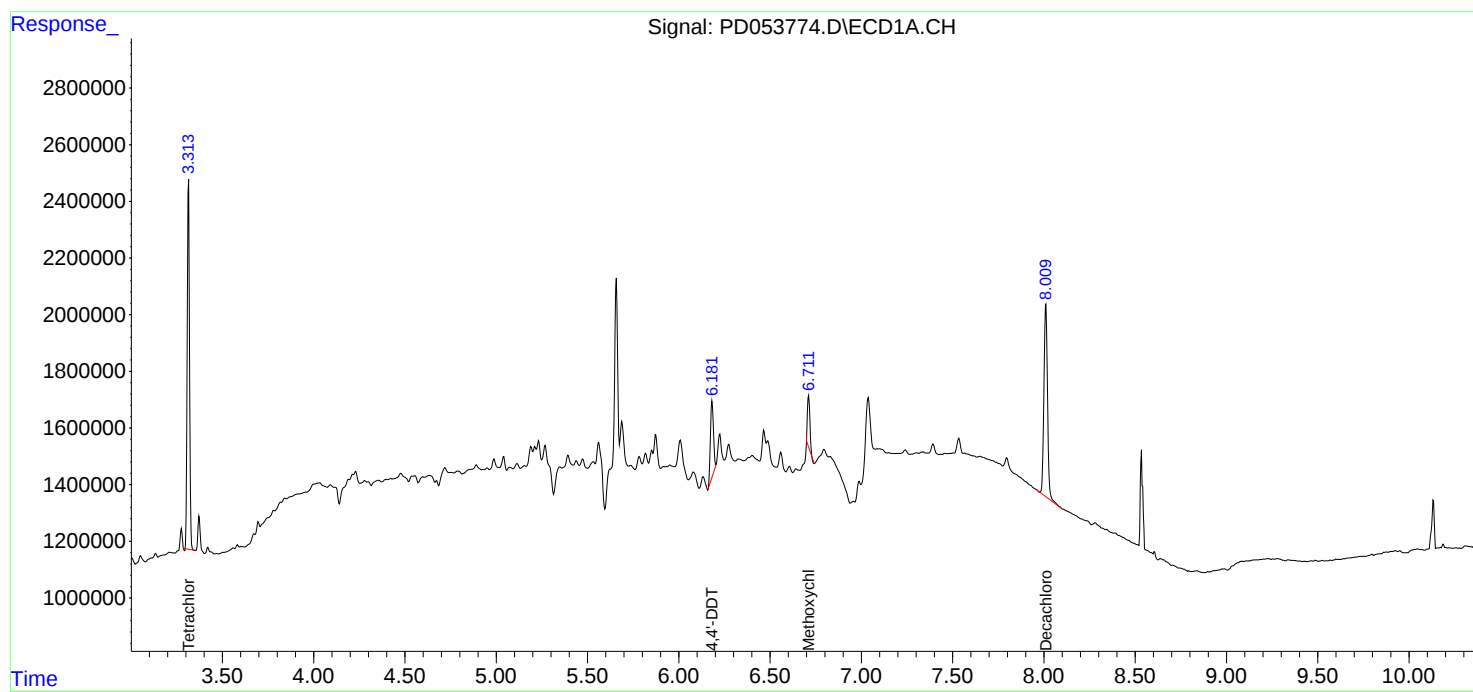


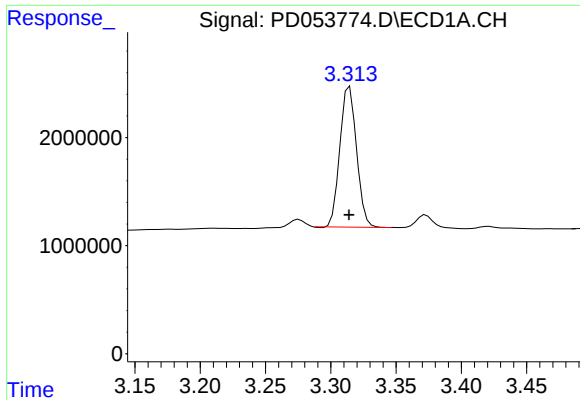

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: 0.000 min
Response: 11543358
Conc: 16.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-B

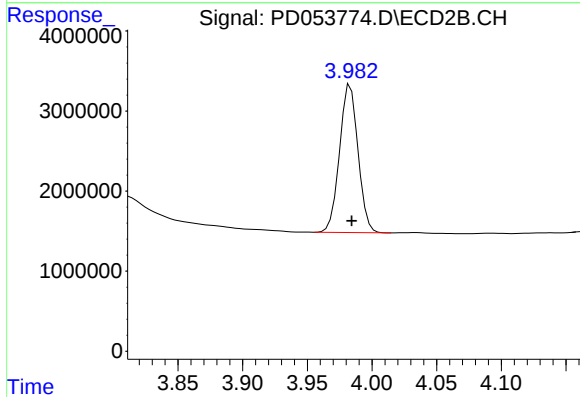


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 18340446
Conc: 16.76 ng/ml

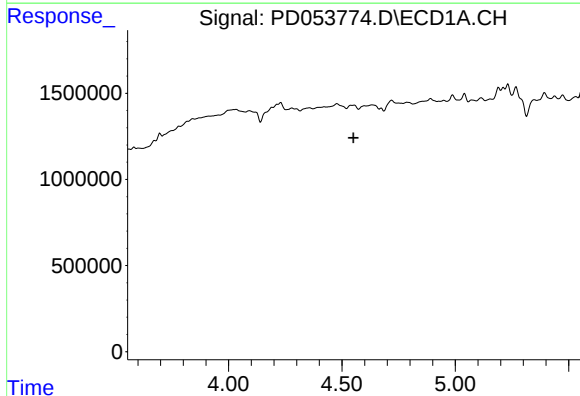


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.551 min
Response: 0
Conc: N.D.

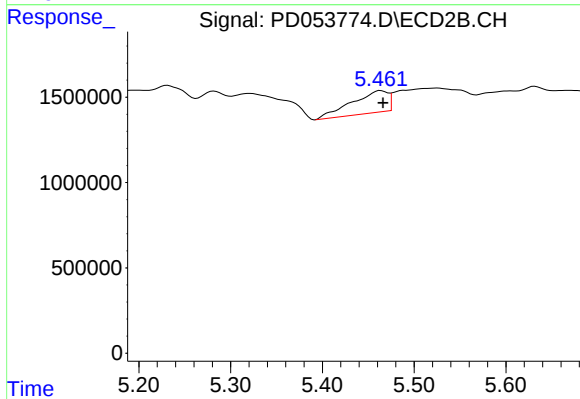

#5 Aldrin


R.T.: 5.463 min
Delta R.T.: -0.003 min
Response: 3507176
Conc: 2.33 ng/ml

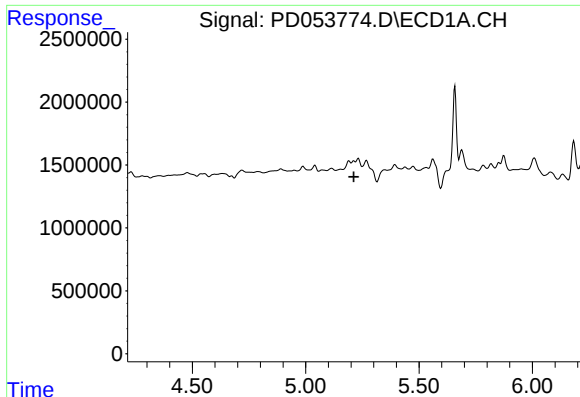

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.213 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
TP-B

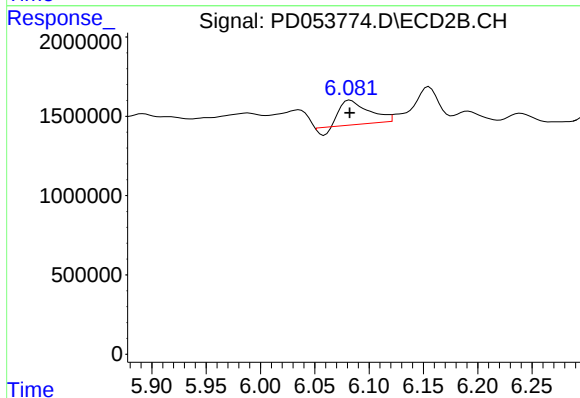


#10 gamma-Chlordane

R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 2616867
Conc: 1.66 ng/ml

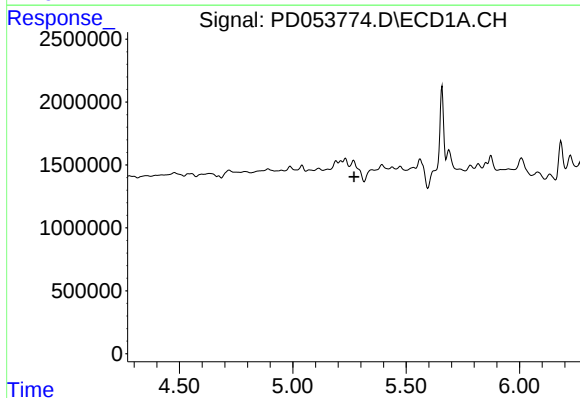


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.270 min
Response: 0
Conc: N.D.

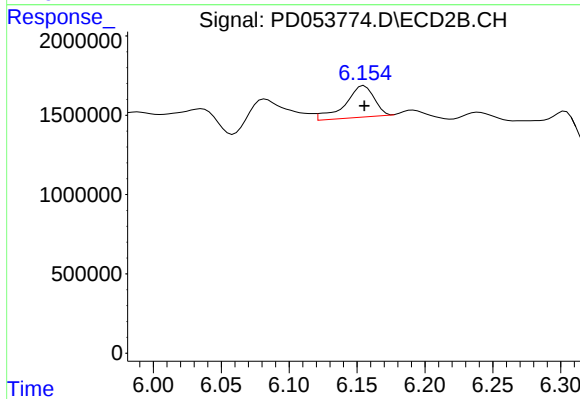

#11 alpha-Chlordane


R.T.: 6.155 min
Delta R.T.: 0.000 min
Response: 2942397
Conc: 1.91 ng/ml

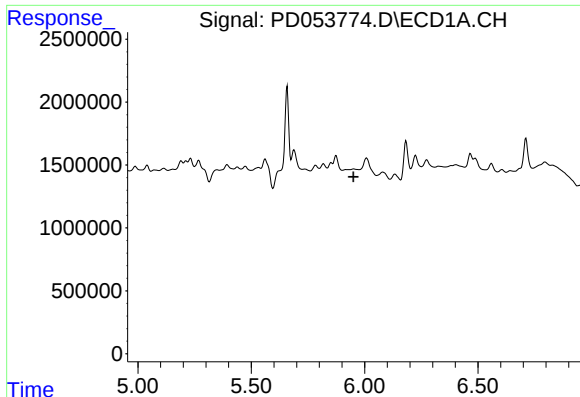

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.951 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
TP-B

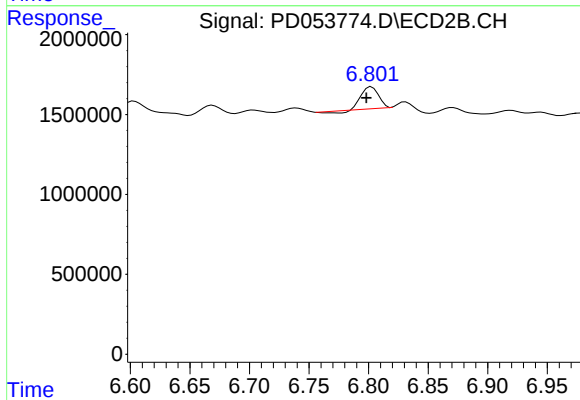


#16 4,4'-DDD

R.T.: 6.803 min
Delta R.T.: 0.004 min
Response: 1275626
Conc: 1.25 ng/ml

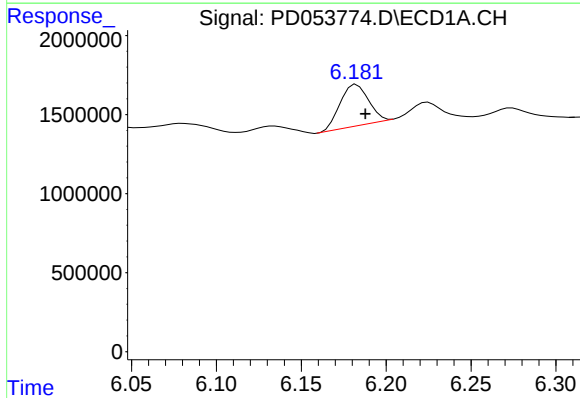


#17 4,4'-DDT

R.T.: 6.183 min
Delta R.T.: -0.005 min
Response: 3040626
Conc: 4.96 ng/ml

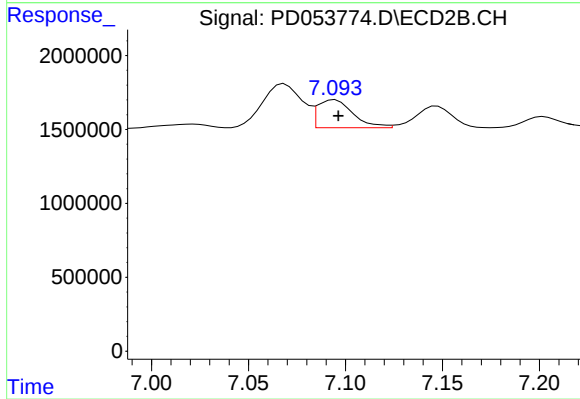

#17 4,4'-DDT


R.T.: 7.095 min
Delta R.T.: -0.002 min
Response: 2401198
Conc: 2.24 ng/ml

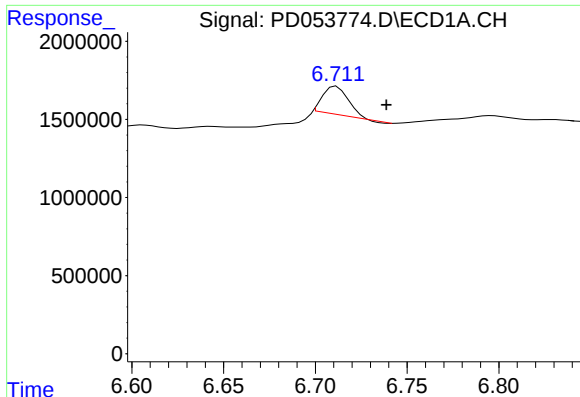

#20 Methoxychlor


R.T.: 6.711 min
Delta R.T.: -0.027 min
Response: 1700012
Conc: 6.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-B

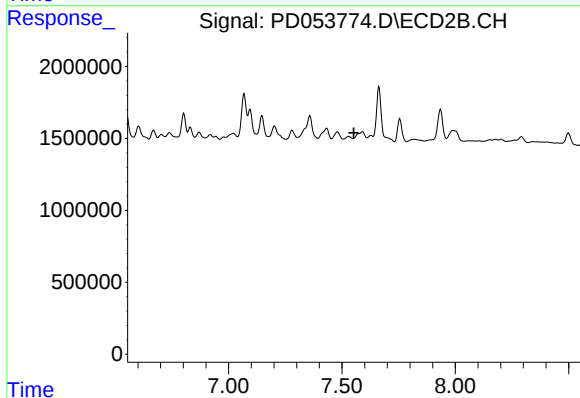


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.552 min
Response: 0
Conc: N.D.

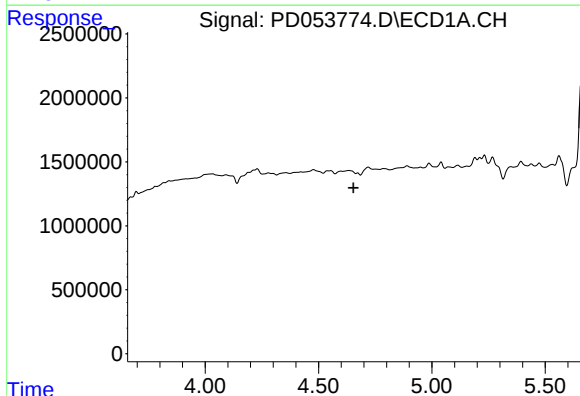


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.655 min
Response: 0
Conc: N.D.

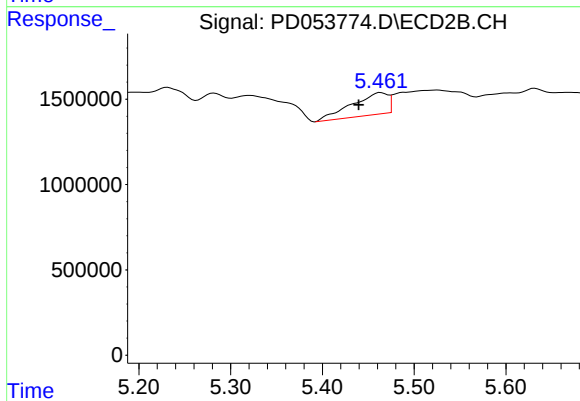

#24 Chlordane-2


R.T.: 5.463 min
Delta R.T.: 0.024 min
Response: 3507176
Conc: 61.70 ng/ml

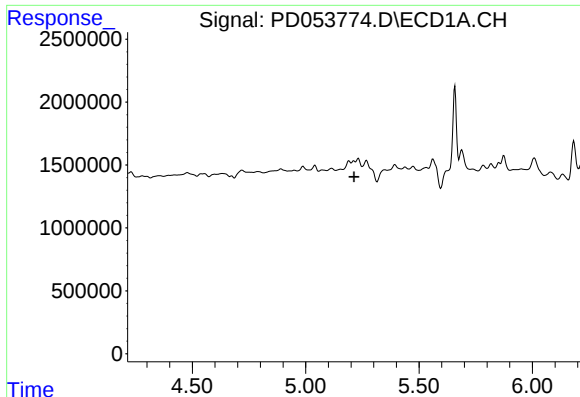

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.213 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
TP-B

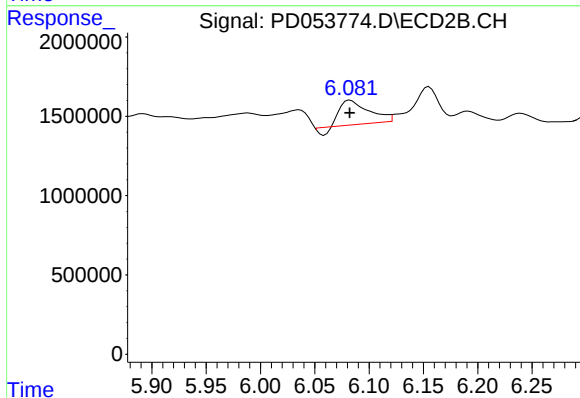


#25 Chlordane-3

R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 2616867
Conc: 13.17 ng/ml

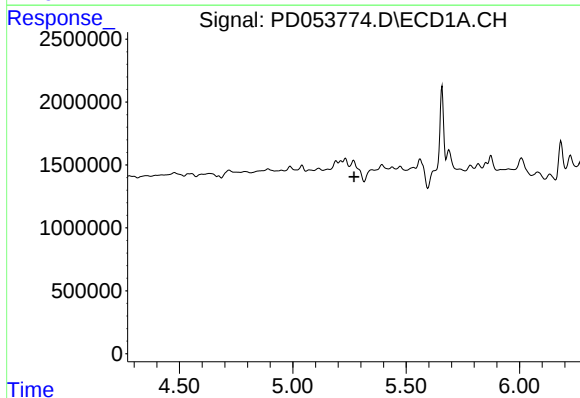


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.271 min
Response: 0
Conc: N.D.

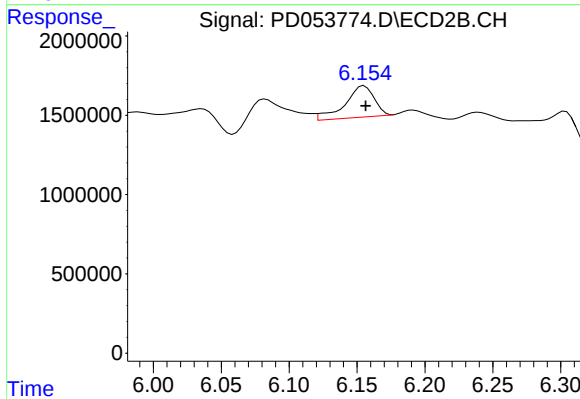

#26 Chlordane-4


R.T.: 6.155 min
Delta R.T.: -0.001 min
Response: 2942397
Conc: 12.55 ng/ml

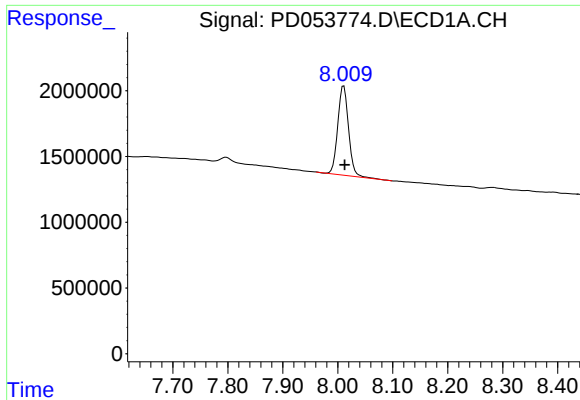

#28 Decachlorobiphenyl

R.T.: 8.011 min
Delta R.T.: -0.002 min
Response: 9256619
Conc: 14.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-B

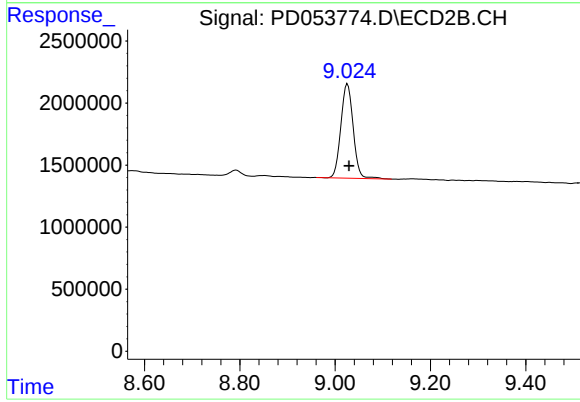

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.004 min
Response: 13670680
Conc: 13.52 ng/ml