

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070119\
 Data File : PD053778.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jul 2019 10:43
 Operator : SM\AJ
 Sample : K3419-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 11:07:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 22 00:19:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.983	4713140	7237200	6.668	6.613
28)	SA Decachlor...	8.011	9.026	4464155	6712095	6.867	6.637
Target Compounds							
8)	B Heptachlo...	0.000	5.839	0	1579958	N.D.	1.079 #
13)	MA Dieldrin	5.580f	6.451	2887483	3769231	3.241	2.503
15)	B Endosulfa...	0.000	6.870	0	1567707	N.D.	1.165 #
16)	A 4,4'-DDD	0.000	6.805	0	11618123	N.D.	11.392 #
17)	MA 4,4'-DDT	6.181	7.068f	5123525	11778459	8.357	10.984 #
19)	B Endosulfa...	6.466	7.202f	4319337	3157512	5.764	2.582 #
20)	A Methoxychlor	6.711f	0.000	3912031	0	14.402	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070119\
Data File : PD053778.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jul 2019 10:43
Operator : SM\AJ
Sample : K3419-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 11:07:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062119.M
Quant Title : GC Extractables
QLast Update : Sat Jun 22 00:19:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

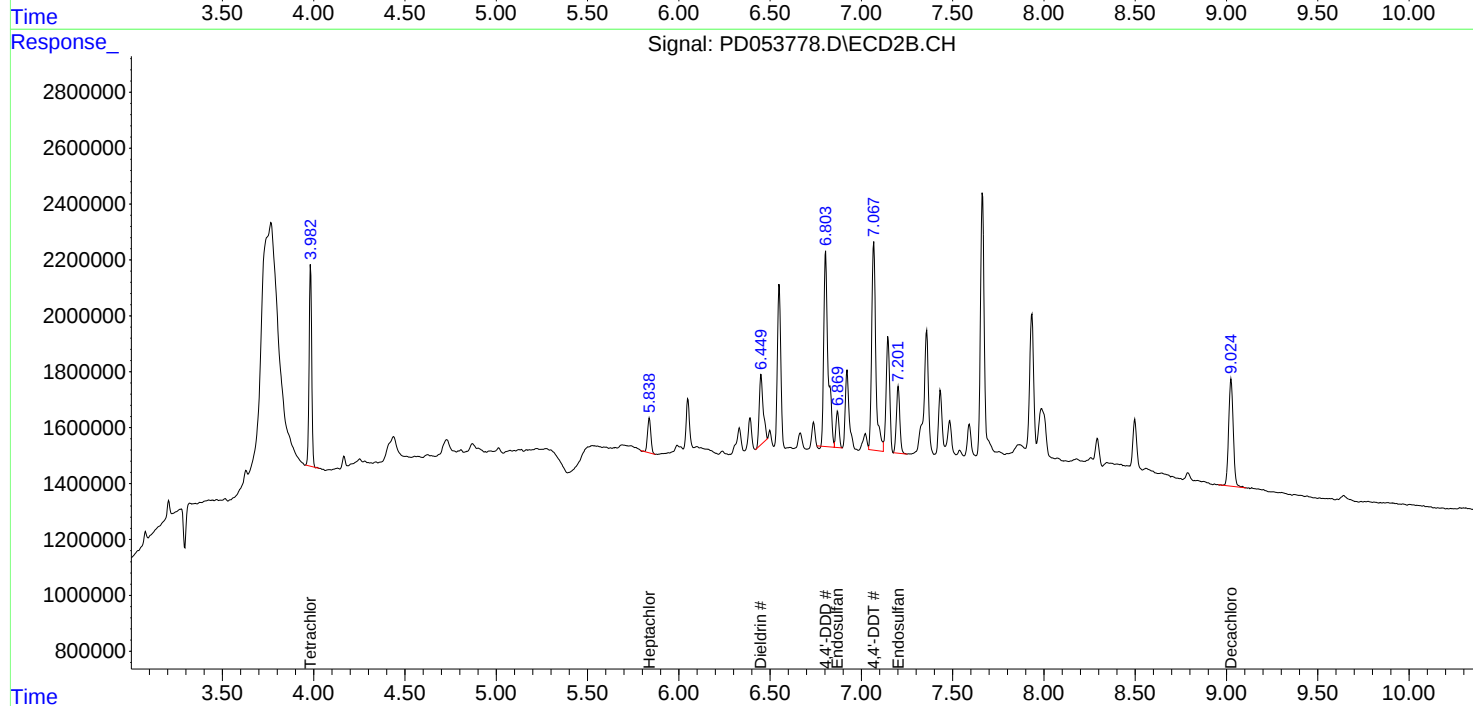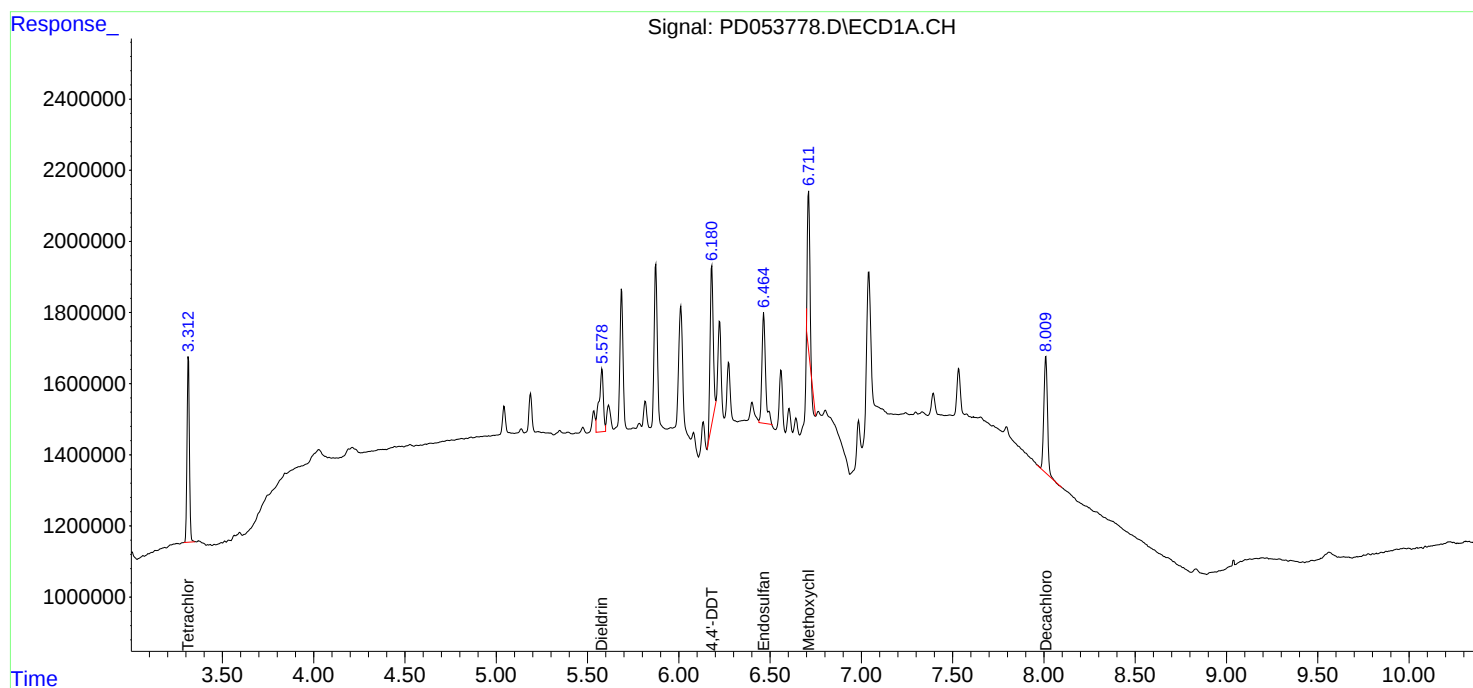


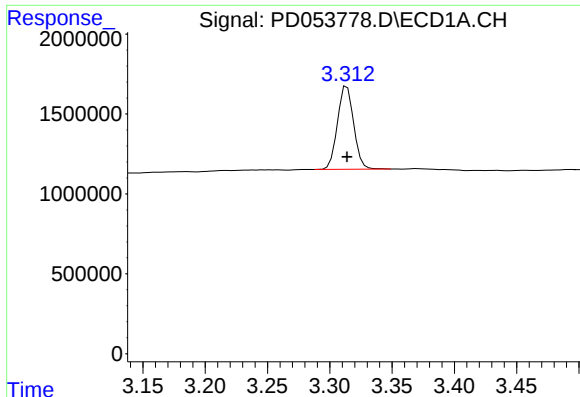

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: 0.000 min
Response: 4713140
Conc: 6.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-A

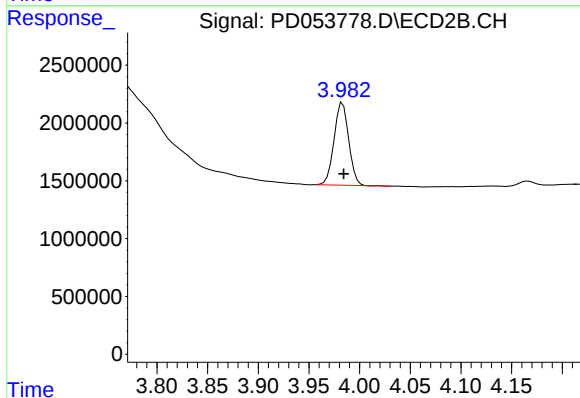


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 7237200
Conc: 6.61 ng/ml

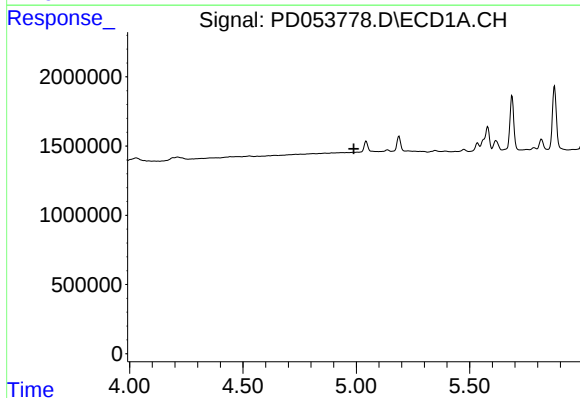


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.990 min
Response: 0
Conc: N.D.

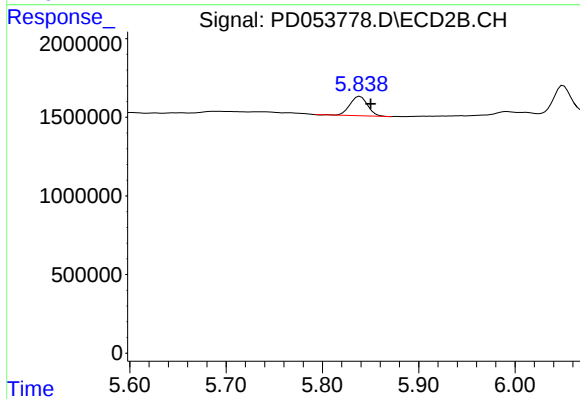

#8 Heptachlor epoxide


R.T.: 5.839 min
Delta R.T.: -0.011 min
Response: 1579958
Conc: 1.08 ng/ml

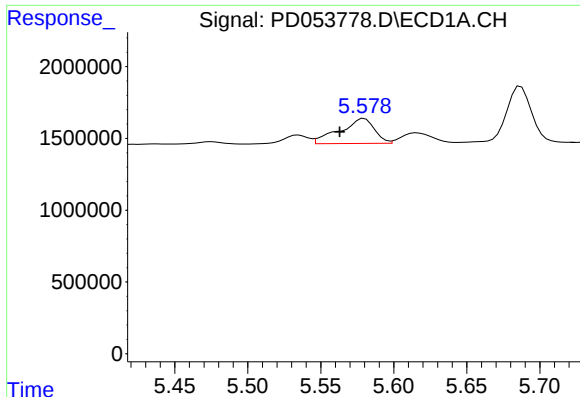

#13 Dieldrin


R.T.: 5.580 min
Delta R.T.: 0.017 min
Response: 2887483
Conc: 3.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-A

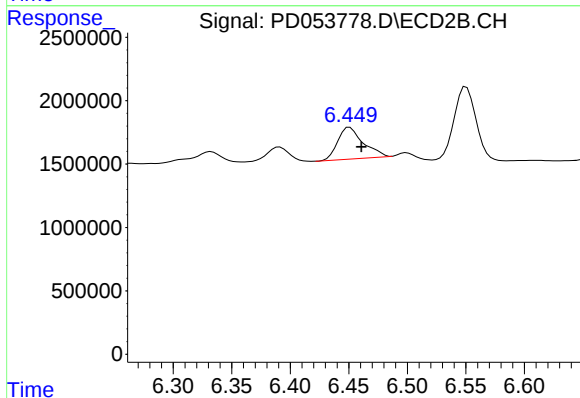


#13 Dieldrin

R.T.: 6.451 min
Delta R.T.: -0.010 min
Response: 3769231
Conc: 2.50 ng/ml

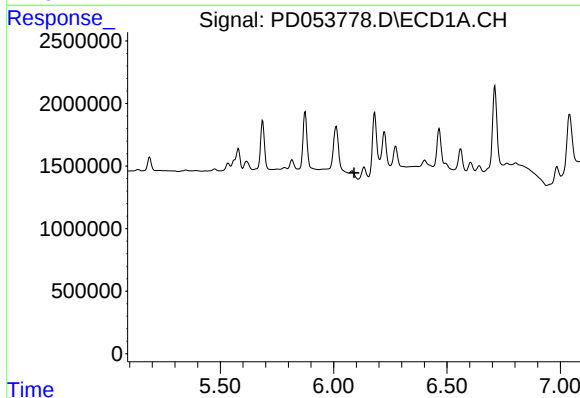


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.091 min
Response: 0
Conc: N.D.

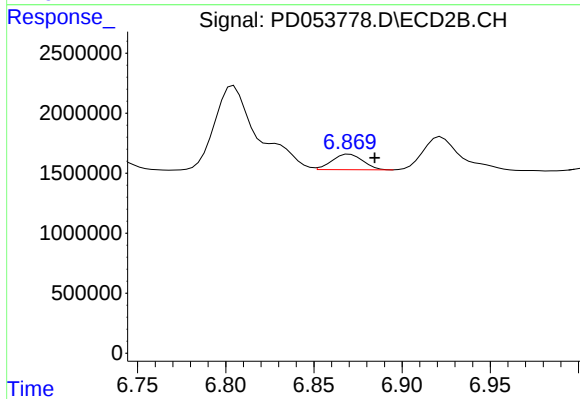

#15 Endosulfan II


R.T.: 6.870 min
Delta R.T.: -0.014 min
Response: 1567707
Conc: 1.16 ng/ml

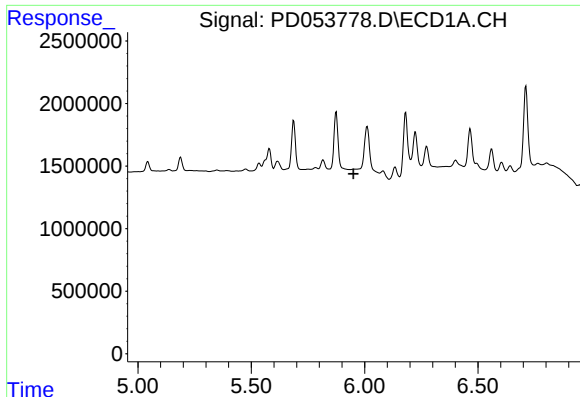

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.951 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
TP-A

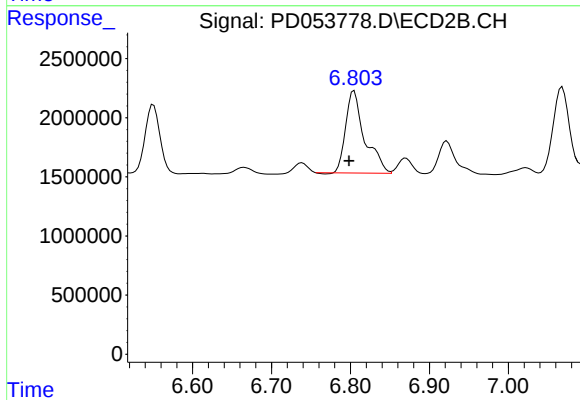


#16 4,4'-DDD

R.T.: 6.805 min
Delta R.T.: 0.006 min
Response: 11618123
Conc: 11.39 ng/ml

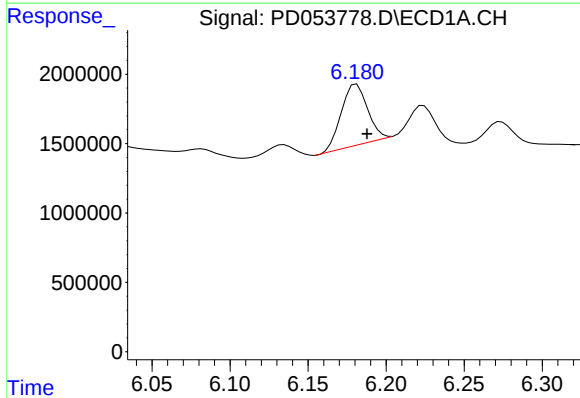


#17 4,4'-DDT

R.T.: 6.181 min
Delta R.T.: -0.007 min
Response: 5123525
Conc: 8.36 ng/ml

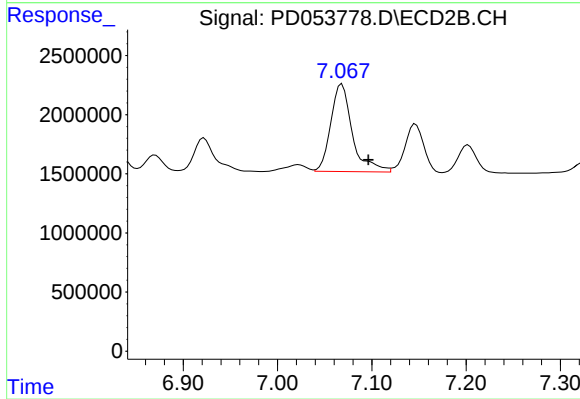

#17 4,4'-DDT


R.T.: 7.068 min
Delta R.T.: -0.028 min
Response: 11778459
Conc: 10.98 ng/ml

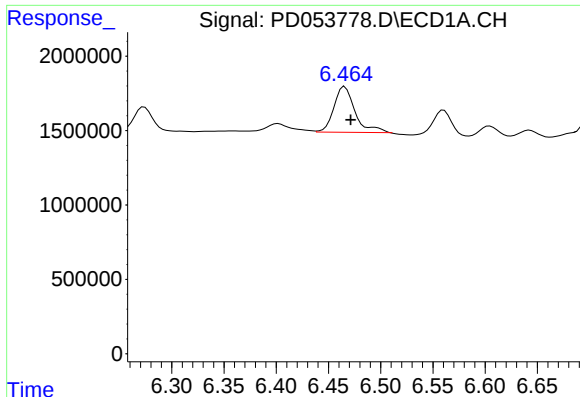

#19 Endosulfan Sulfate


R.T.: 6.466 min
Delta R.T.: -0.006 min
Response: 4319337
Conc: 5.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-A

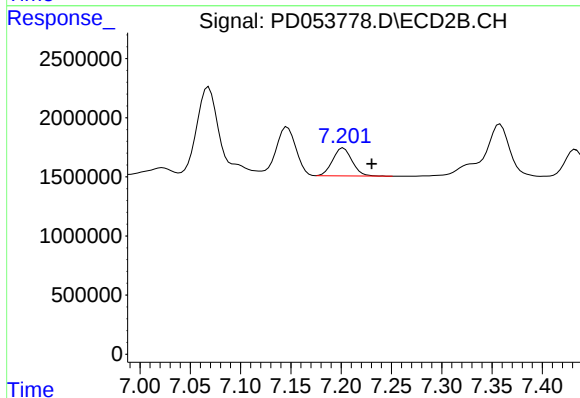


#19 Endosulfan Sulfate

R.T.: 7.202 min
Delta R.T.: -0.028 min
Response: 3157512
Conc: 2.58 ng/ml

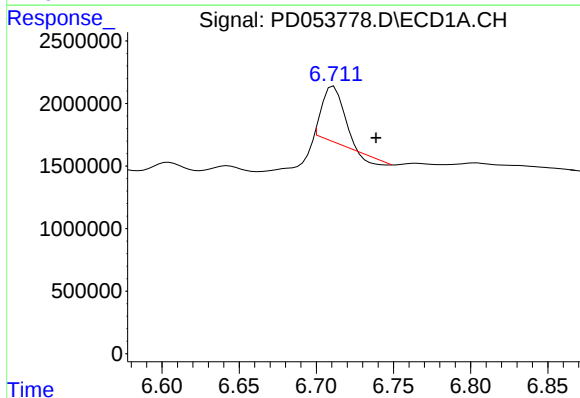


#20 Methoxychlor

R.T.: 6.711 min
Delta R.T.: -0.027 min
Response: 3912031
Conc: 14.40 ng/ml

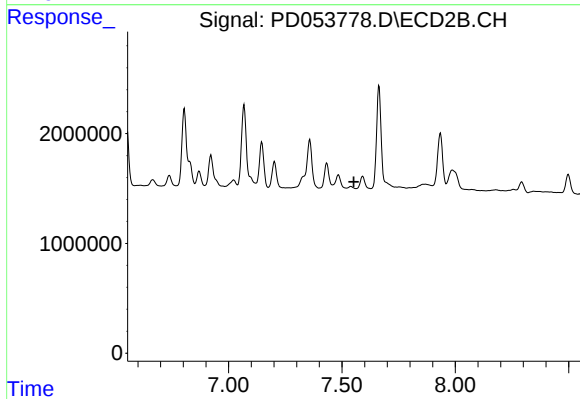

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.552 min
Response: 0
Conc: N.D.

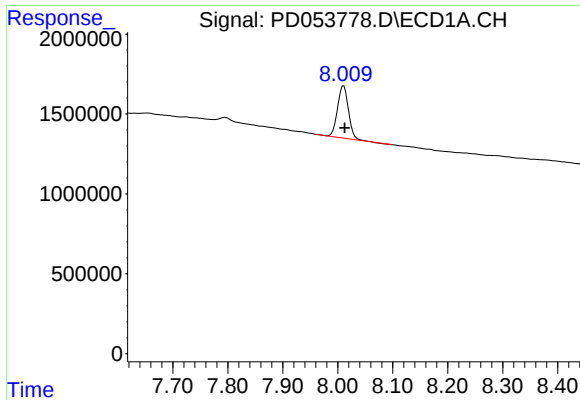

#28 Decachlorobiphenyl

R.T.: 8.011 min
Delta R.T.: -0.002 min
Response: 4464155
Conc: 6.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-A

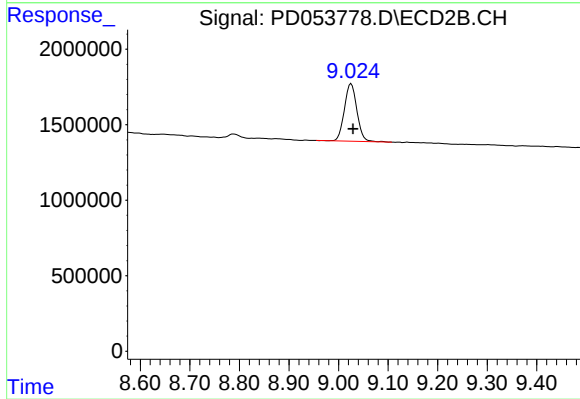

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.004 min
Response: 6712095
Conc: 6.64 ng/ml