

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070119\
 Data File : PD053801.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jul 2019 16:02
 Operator : SM\AJ
 Sample : K3160-11RE
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EO-01-062819-CRE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 01:05:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 22 00:19:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.983	4493031	6267066	6.357	5.726
28)	SA Decachlor...	8.010	9.026	4600677	7129908	7.077	7.050
Target Compounds							
12)	B 4,4'-DDE	0.000	6.308	0	1213721	N.D.	0.907 #
24)	Chlordane-2	0.000	5.434	0	1549354	N.D.	27.258 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070119\
Data File : PD053801.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jul 2019 16:02
Operator : SM\AJ
Sample : K3160-11RE
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
EO-01-062819-CRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 01:05:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062119.M
Quant Title : GC Extractables
QLast Update : Sat Jun 22 00:19:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

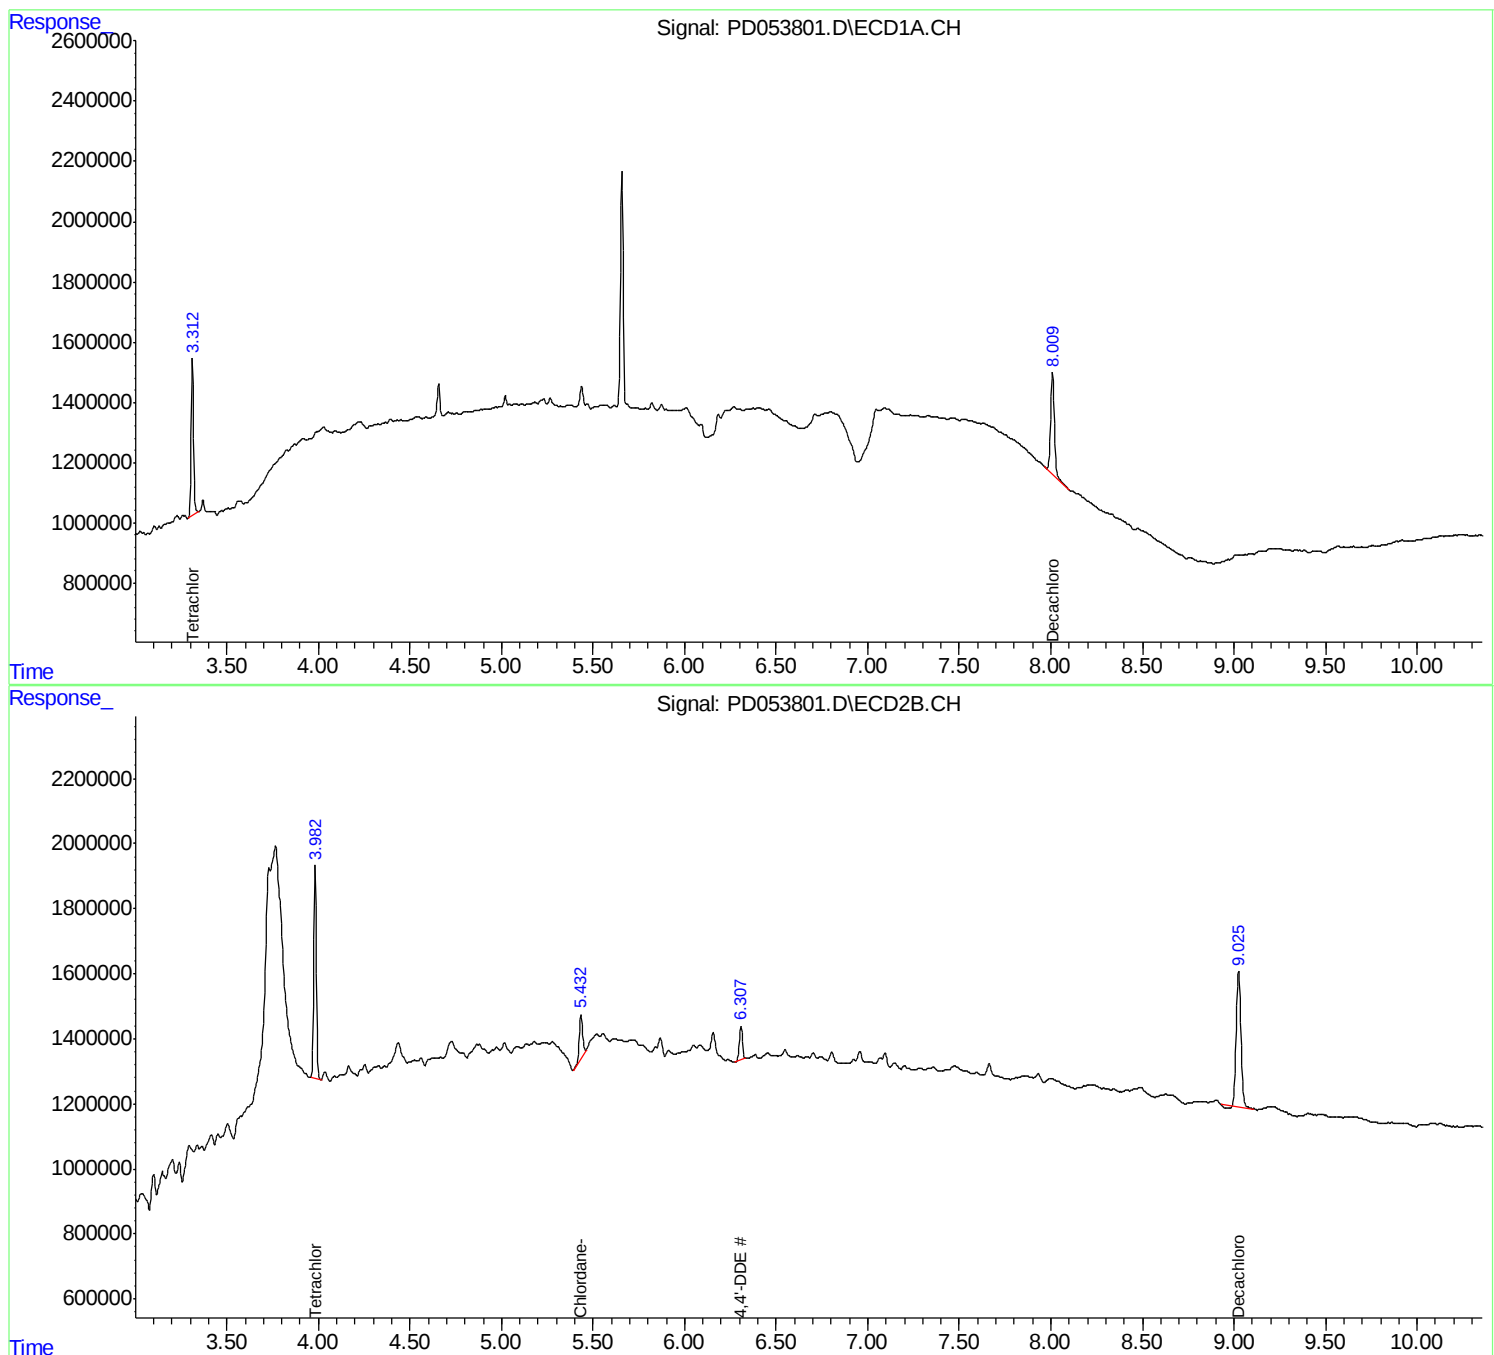


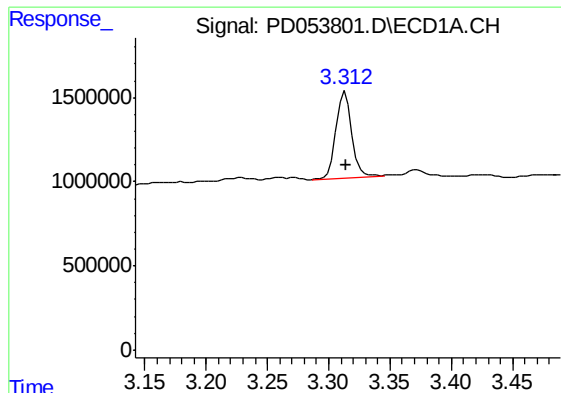

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: 0.000 min
Response: 4493031
Conc: 6.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
EO-01-062819-CRE

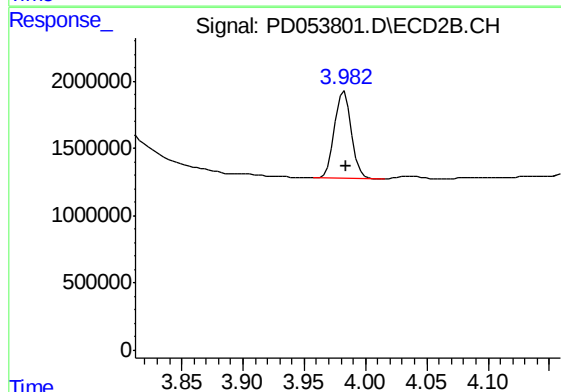


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: -0.001 min
Response: 6267066
Conc: 5.73 ng/ml

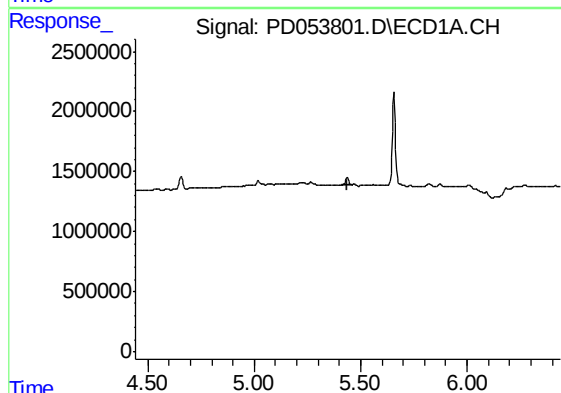


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.439 min
Response: 0
Conc: N.D.

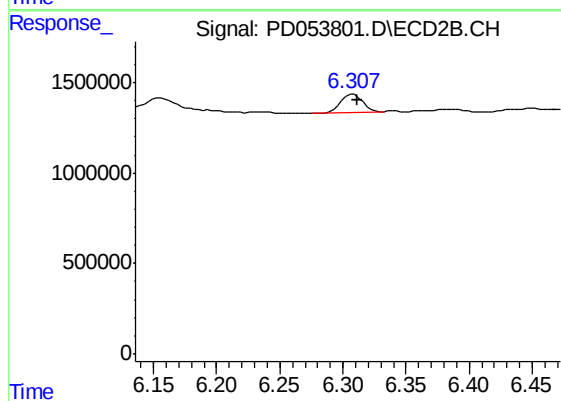

#12 4,4'-DDE


R.T.: 6.308 min
Delta R.T.: -0.003 min
Response: 1213721
Conc: 0.91 ng/ml

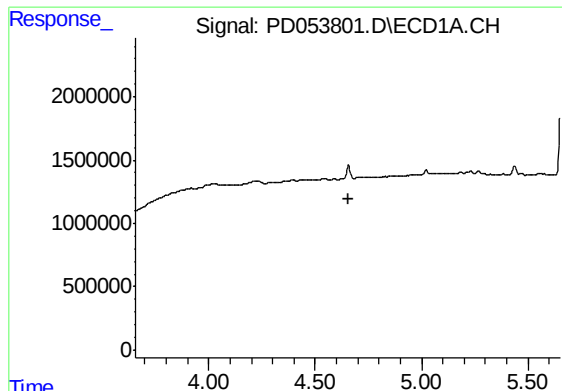

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.655 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
EO-01-062819-CRE

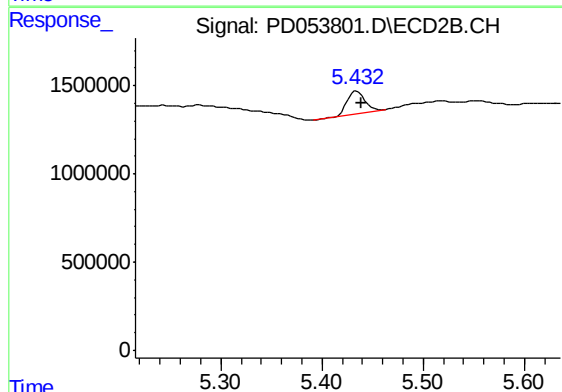


#24 Chlordane-2

R.T.: 5.434 min
Delta R.T.: -0.005 min
Response: 1549354
Conc: 27.26 ng/ml

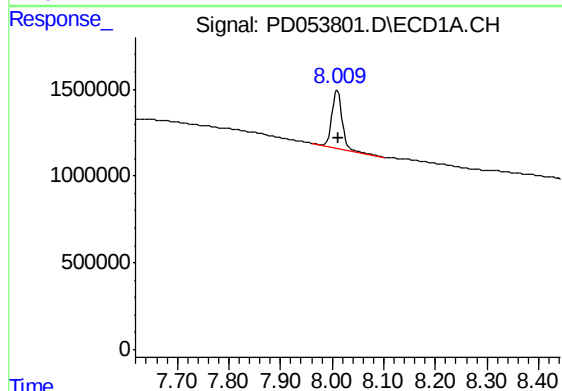

#28 Decachlorobiphenyl

R.T.: 8.010 min
Delta R.T.: -0.002 min
Response: 4600677
Conc: 7.08 ng/ml

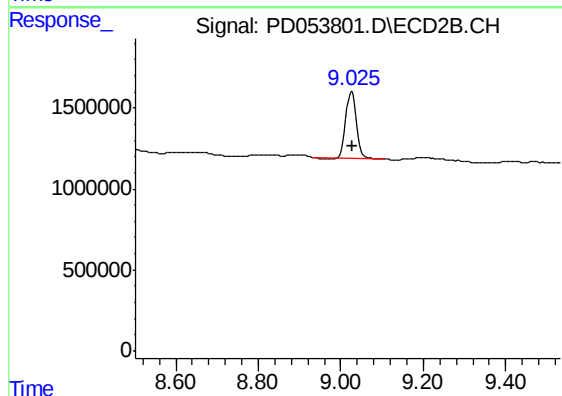

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.004 min
Response: 7129908
Conc: 7.05 ng/ml