

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070119\
 Data File : PD053785.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jul 2019 12:20
 Operator : SM\AJ
 Sample : K3561-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PST-012-B226-062419

Manual Integrations
 APPROVED

Ankita
 7/2/2019 1:17:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 01:01:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 22 00:19:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.984	14818045	21818123	20.965	19.936
28)	SA Decachlor...	8.009	9.024	9546181	14044885	14.684	13.888m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070119\
Data File : PD053785.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jul 2019 12:20
Operator : SM\AJ
Sample : K3561-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PST-012-B226-062419


Manual Integrations
APPROVED

Ankita
7/2/2019 1:17:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 01:01:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062119.M
Quant Title : GC Extractables
QLast Update : Sat Jun 22 00:19:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

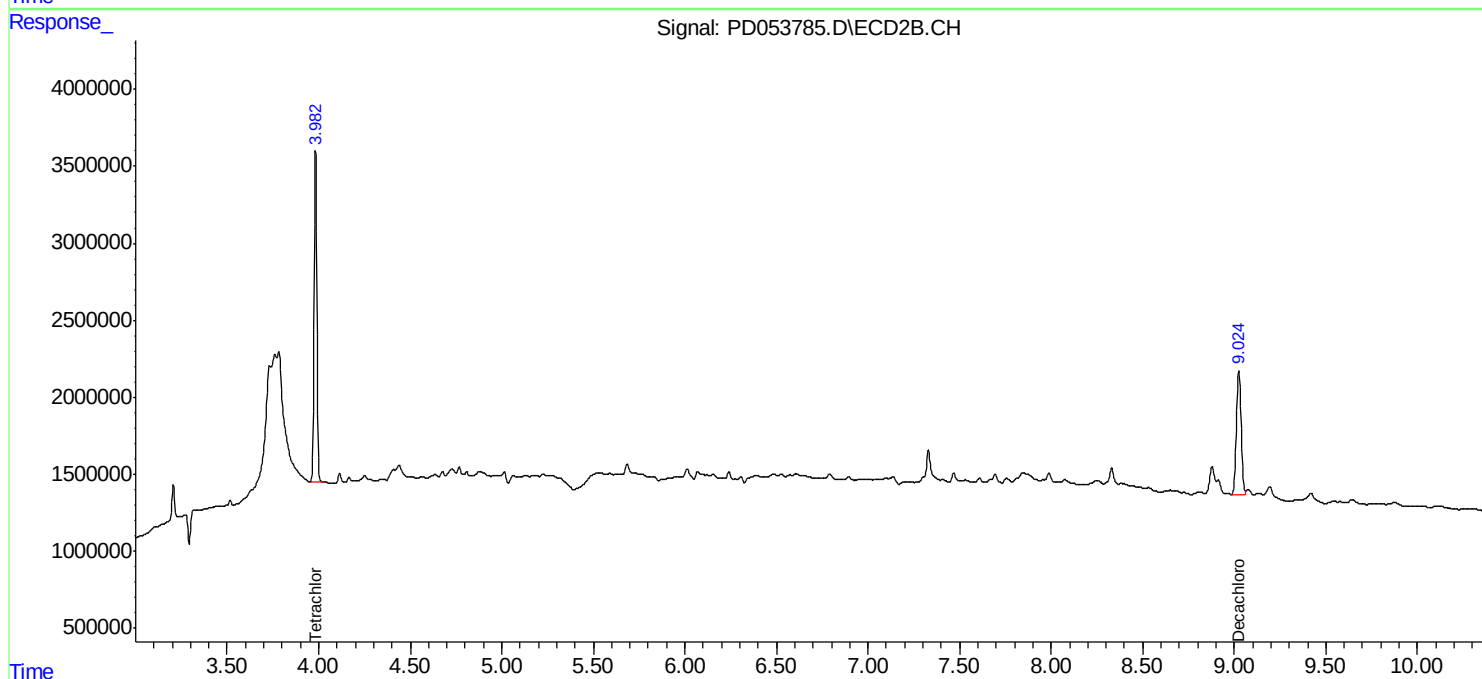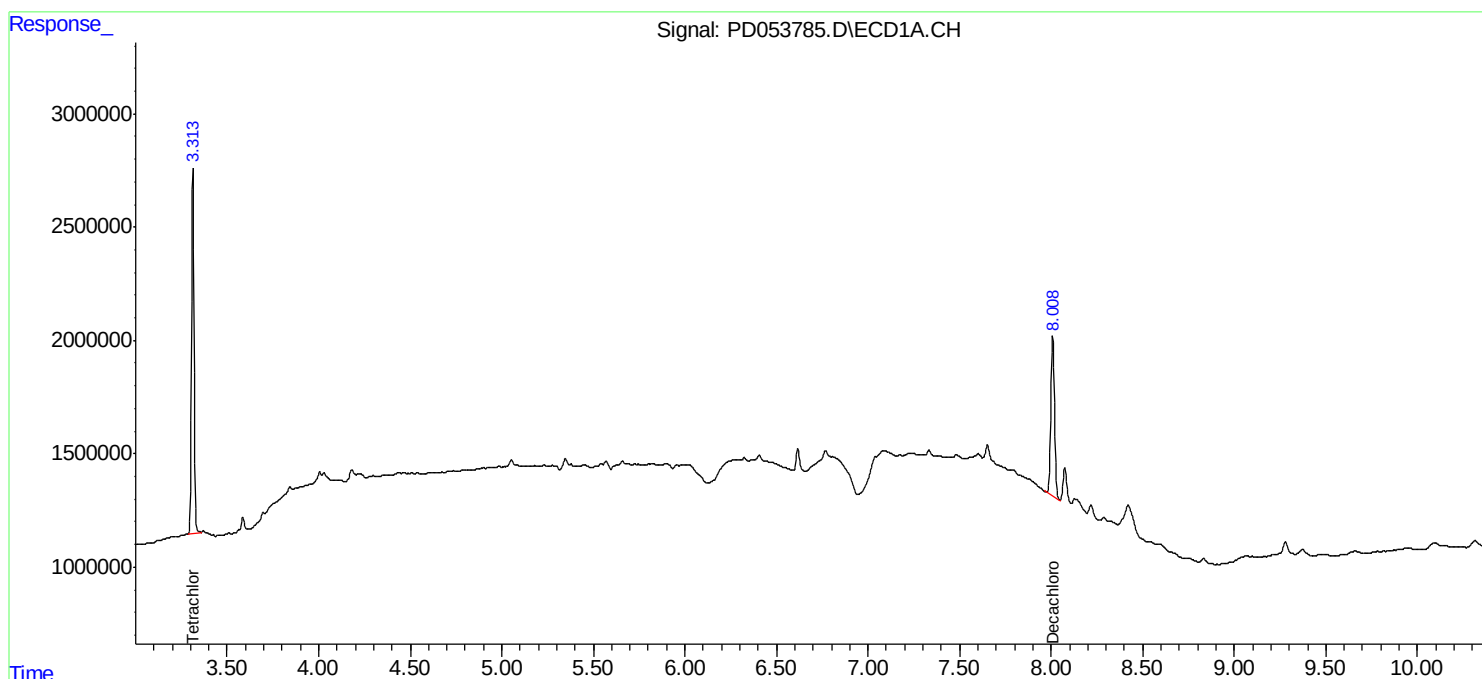

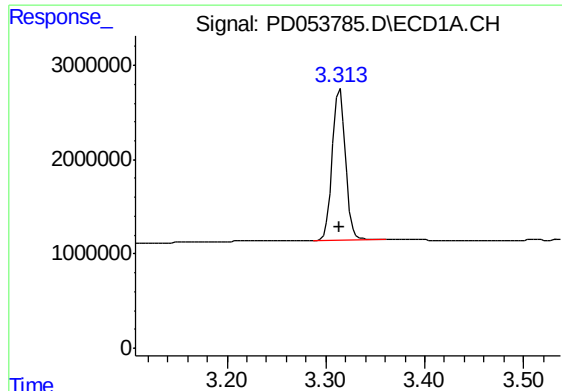


#1 Tetrachloro-m-xylene

R.T.: 3.314 min
Delta R.T.: 0.000 min
Response: 14818045
Conc: 20.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
PST-012-B226-062419


Manual Integrations
APPROVED

Ankita
7/2/2019 1:17:17 PM

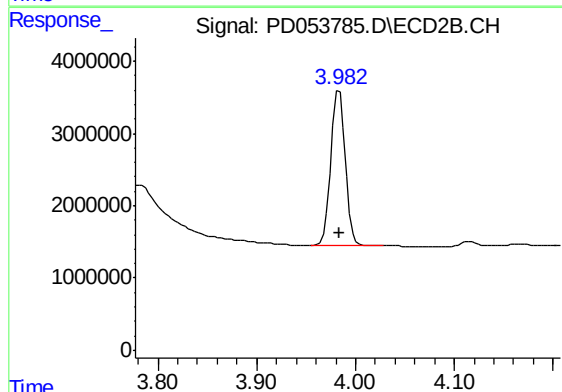


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: 0.000 min
Response: 21818123
Conc: 19.94 ng/ml

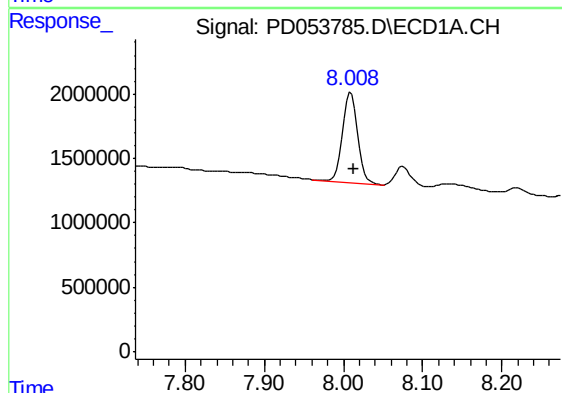

#28 Decachlorobiphenyl

R.T.: 8.009 min
Delta R.T.: -0.003 min
Response: 9546181
Conc: 14.68 ng/ml

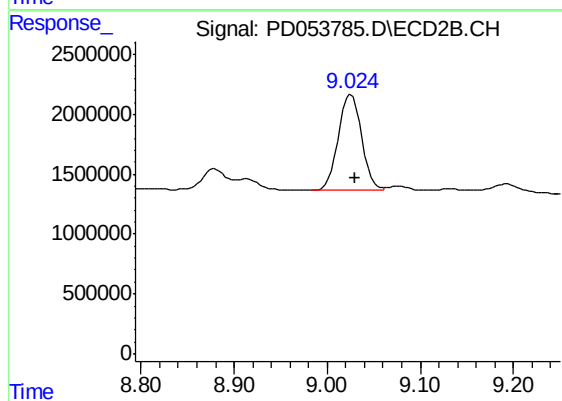

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: -0.005 min
Response: 14044885
Conc: 13.89 ng/ml m