

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070119\
 Data File : PD053800.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jul 2019 15:49
 Operator : SM\AJ
 Sample : K3561-02RE
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PST-012-B227-062419RE

Manual Integrations
 APPROVED

Ankita
 7/2/2019 1:15:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 01:05:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 22 00:19:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.983	13078504	19122900	18.504	17.473
28)	SA Decachlor...	8.010	9.024	6301611	9939943	9.693	9.829m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070119\
Data File : PD053800.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jul 2019 15:49
Operator : SM\AJ
Sample : K3561-02RE
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PST-012-B227-062419RE


Manual Integrations
APPROVED

Ankita
7/2/2019 1:15:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 01:05:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062119.M
Quant Title : GC Extractables
QLast Update : Sat Jun 22 00:19:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

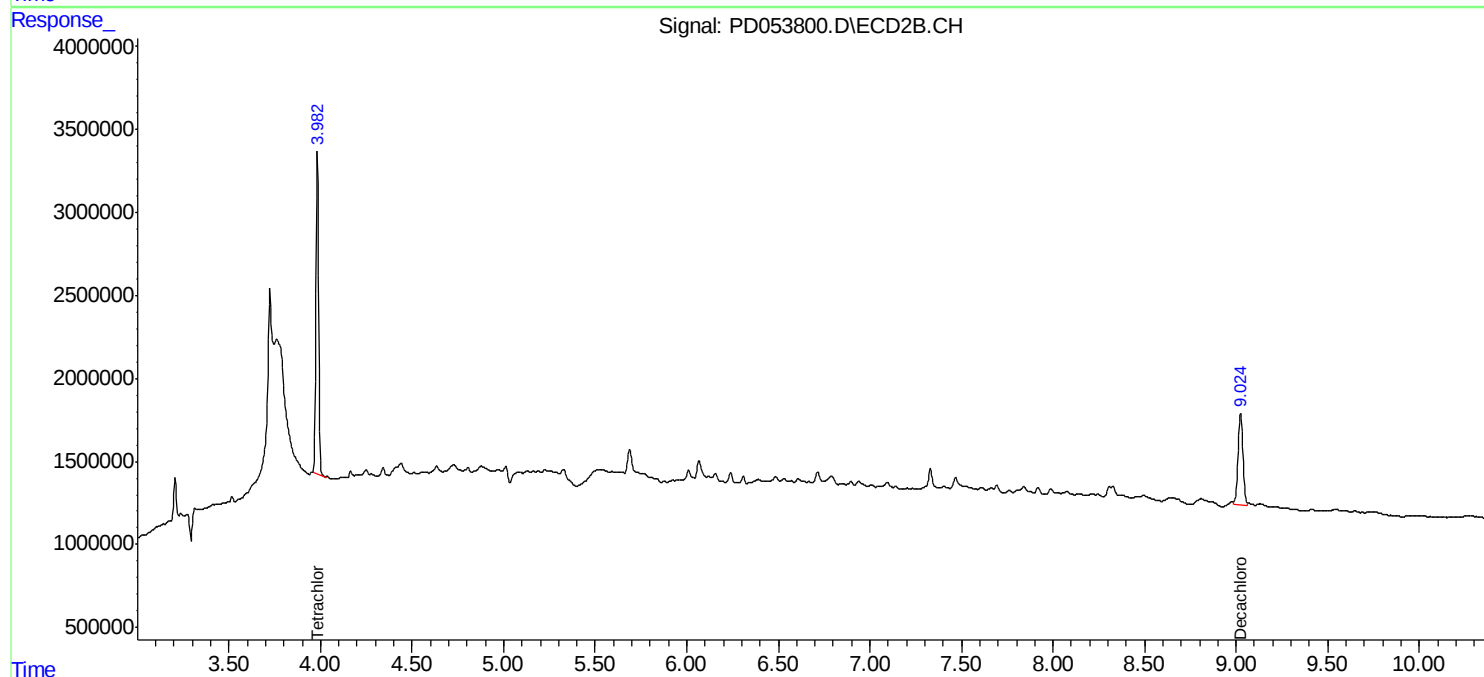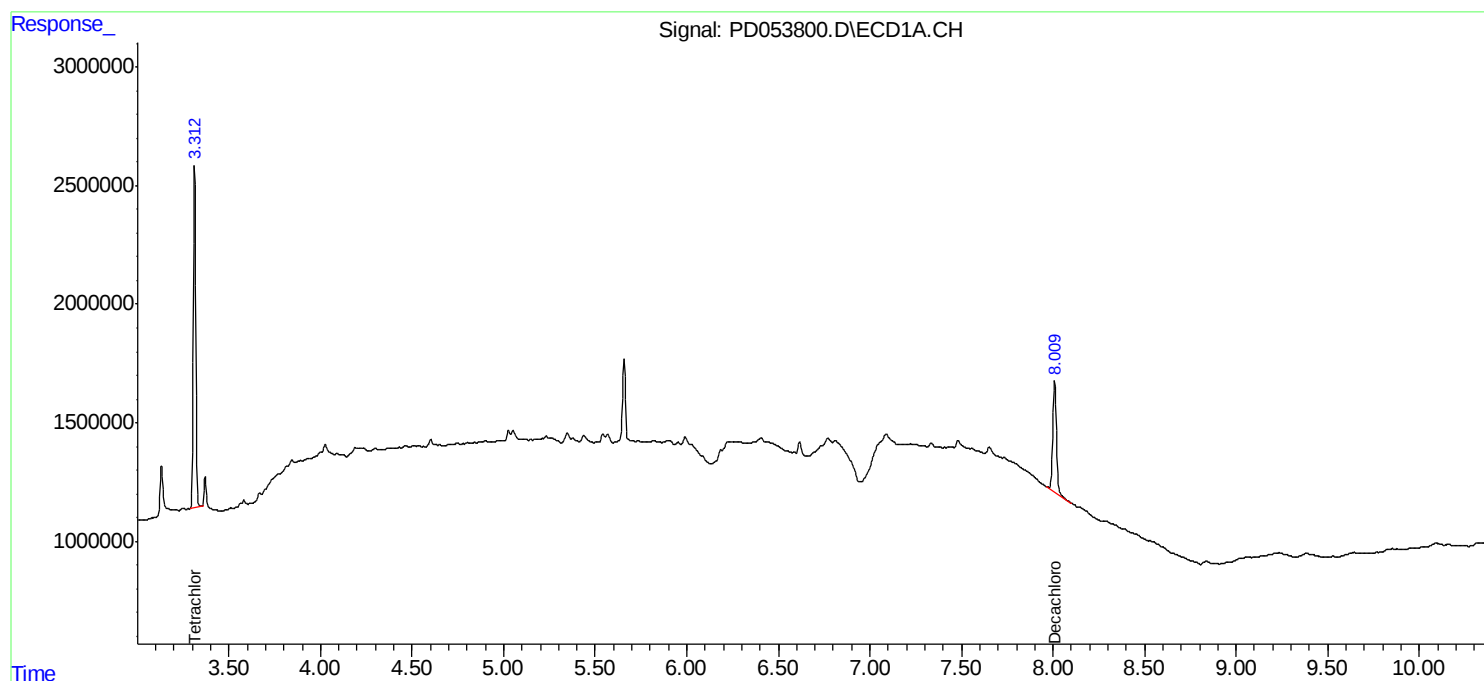

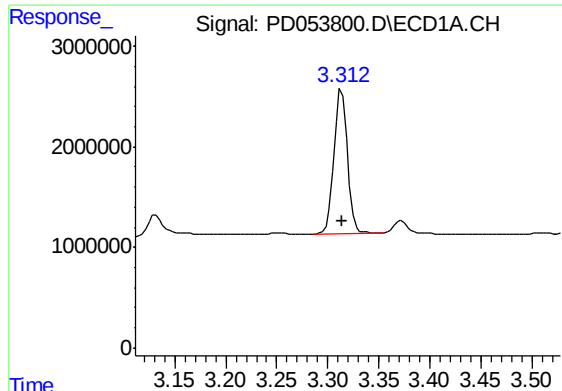


#1 Tetrachloro-m-xylene

R.T.: 3.314 min
Delta R.T.: 0.000 min
Response: 13078504
Conc: 18.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
PST-012-B227-062419RE


Manual Integrations
APPROVED

Ankita
7/2/2019 1:15:39 PM

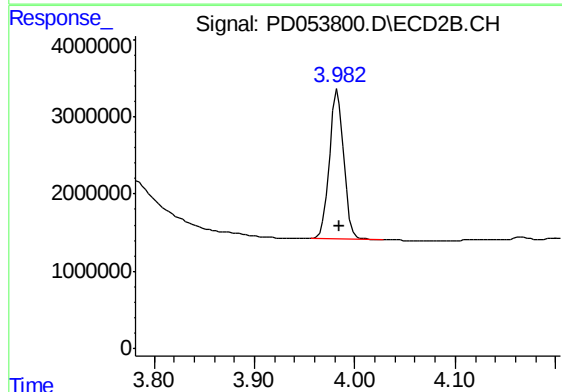


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: -0.001 min
Response: 19122900
Conc: 17.47 ng/ml

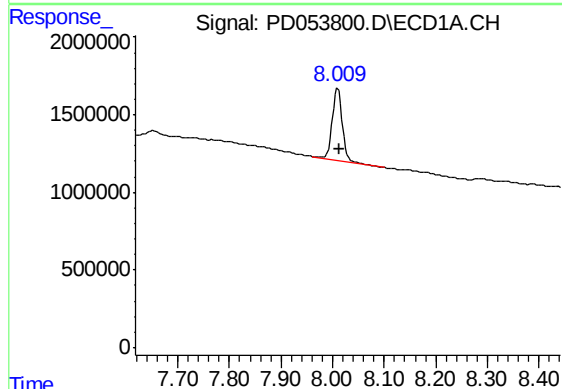

#28 Decachlorobiphenyl

R.T.: 8.010 min
Delta R.T.: -0.002 min
Response: 6301611
Conc: 9.69 ng/ml

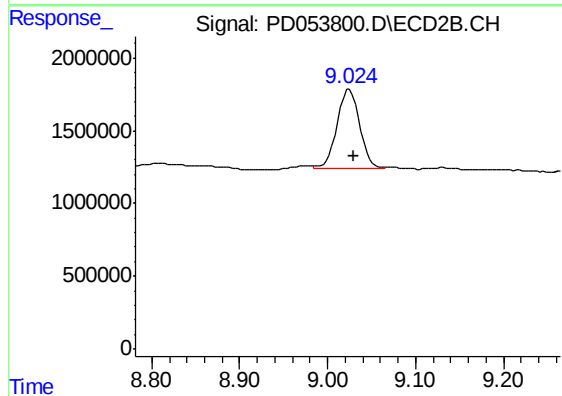

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: -0.006 min
Response: 9939943
Conc: 9.83 ng/ml m