

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070219\
 Data File : PD053805.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jul 2019 9:06
 Operator : SM\AJ
 Sample : PIBLK03
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 01:00:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062019CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 08:58:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.983	15971849	24972252	22.021	22.143
27)	SA Decachlor...	8.013	9.026	26060428	36622893	41.410	37.478


Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070219\
Data File : PD053805.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jul 2019 9:06
Operator : SM\AJ
Sample : PIBLK03
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:00:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062019CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 08:58:58 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

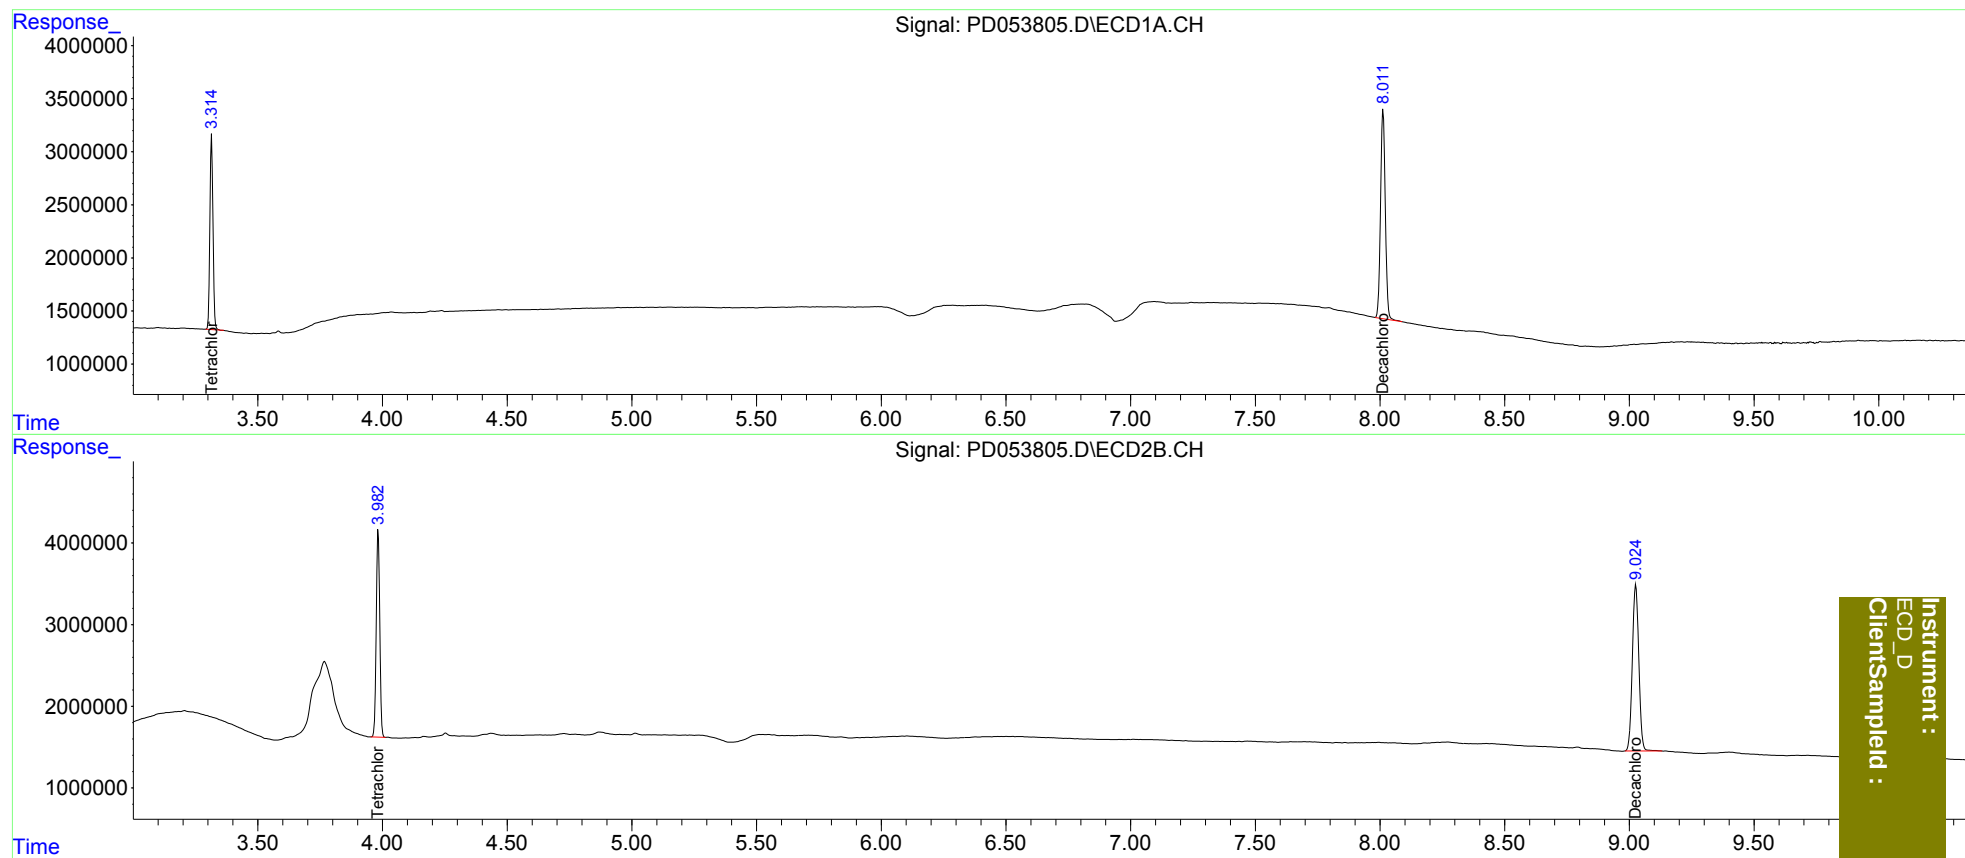


Instrument :
ECD_D
ClientSampled :

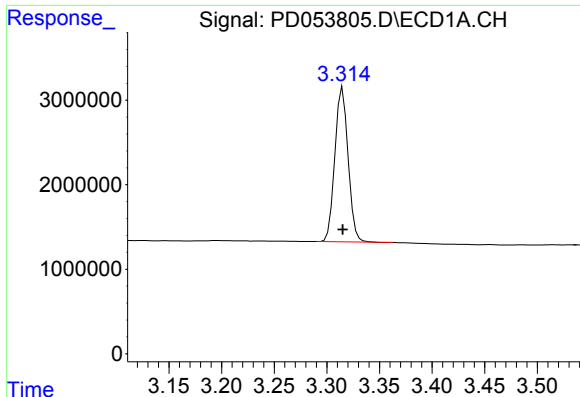

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: 0.000 min
Response: 15971849
Conc: 22.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

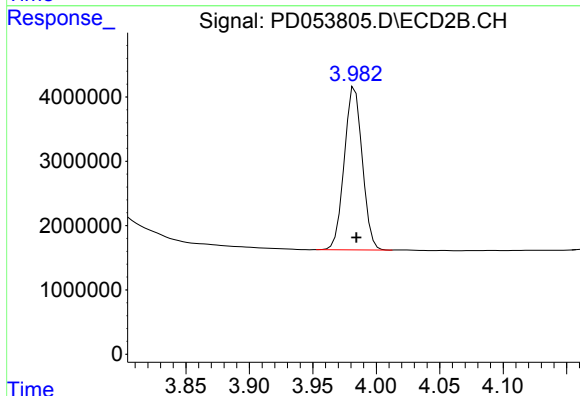


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: -0.001 min
Response: 24972252
Conc: 22.14 ng/ml

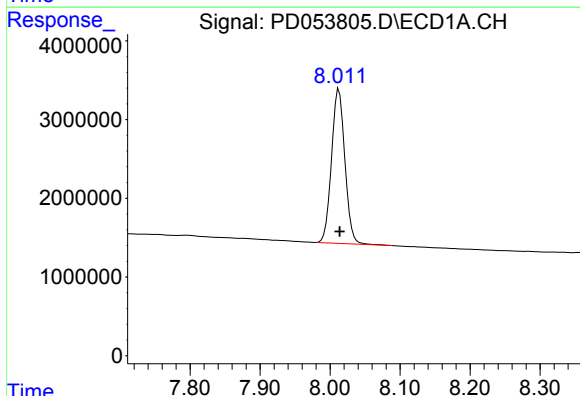

#27 Decachlorobiphenyl

R.T.: 8.013 min
Delta R.T.: -0.001 min
Response: 26060428
Conc: 41.41 ng/ml

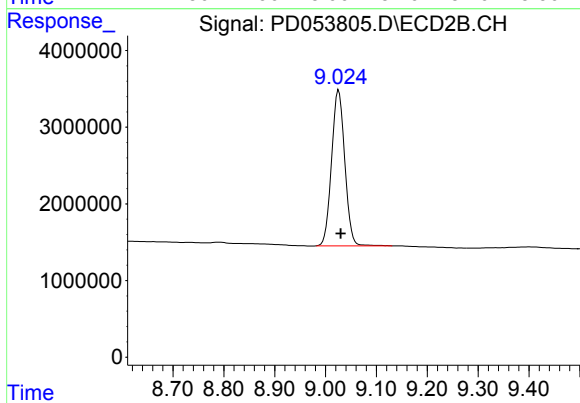

#27 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.004 min
Response: 36622893
Conc: 37.48 ng/ml