

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070220\
 Data File : PD058418.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2020 11:05
 Operator : AJ\MA
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 12:33:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 02 12:31:35 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.867	8389629	11147209	4.944	4.767
27)	SA Decachlor...	7.847	8.861	18460015	23442290	10.456	10.983
Target Compounds							
2)	A alpha-BHC	3.631	4.249	11374698	15799774	4.496	4.557
3)	MA gamma-BHC...	3.903	4.529	11875809	14569535	5.128	4.581
4)	MA Heptachlor	4.182	5.029	7956818	14178147	5.007	4.796
9)	A Endosulfan I	5.176	6.065	8954570	12188617	4.969	4.920
13)	MA Dieldrin	5.414	6.320	16836557	26141589	9.660	9.378
14)	MA Endrin	5.665	6.537	15059255	22240495	10.196	9.516
16)	A 4,4'-DDD	5.803	6.665	12293116	20830295	10.133	9.359
17)	MA 4,4'-DDT	6.036	6.962	13279353	21151701	9.334	9.190
20)	A Methoxychlor	6.584	7.421	28834913	61777860	52.302	51.660


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070220\
Data File : PD058418.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2020 11:05
Operator : AJ\MA
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 12:33:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 02 12:31:35 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

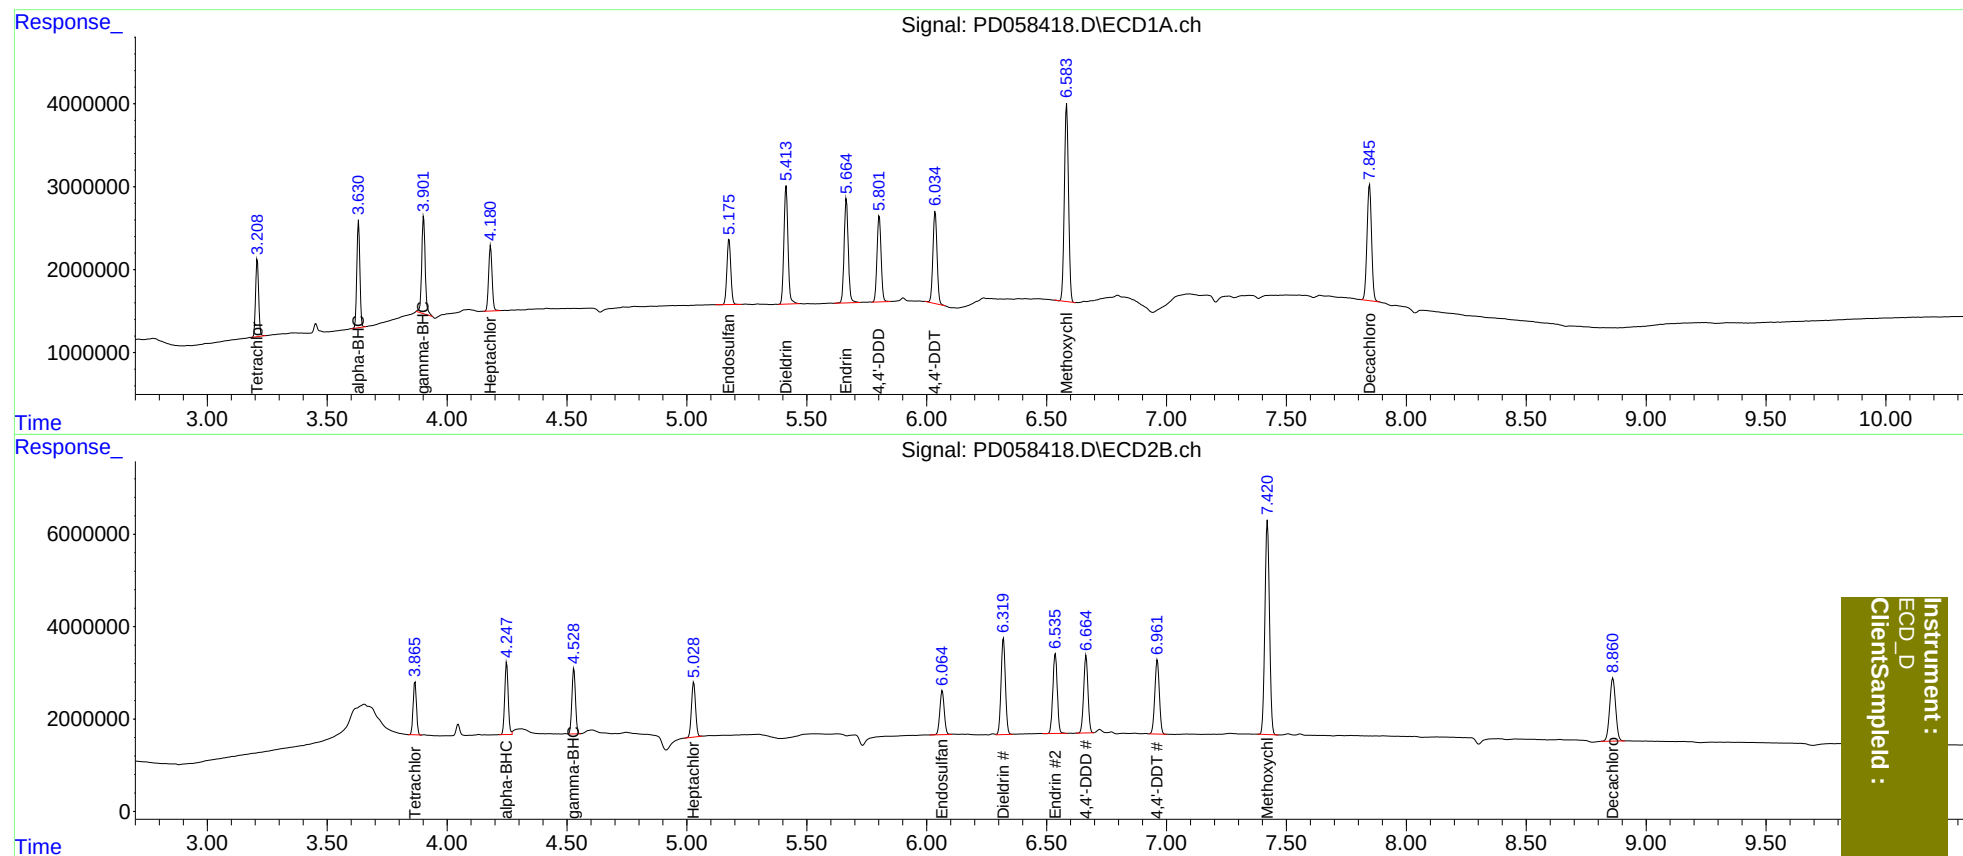


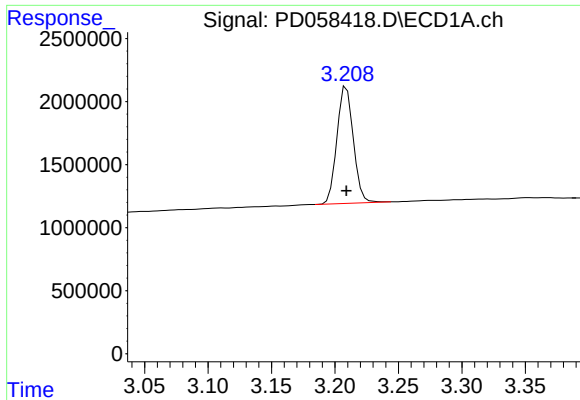

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.000 min
Response: 8389629
Conc: 4.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

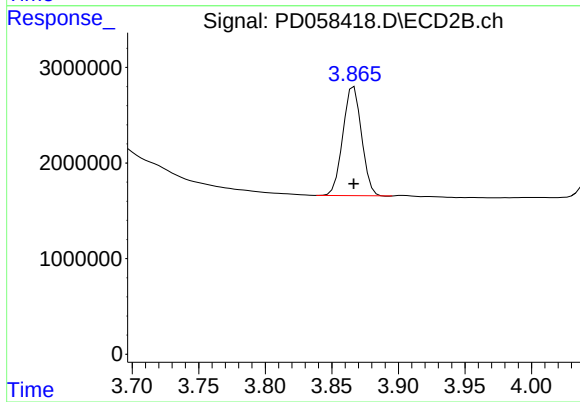


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 11147209
Conc: 4.77 ng/ml

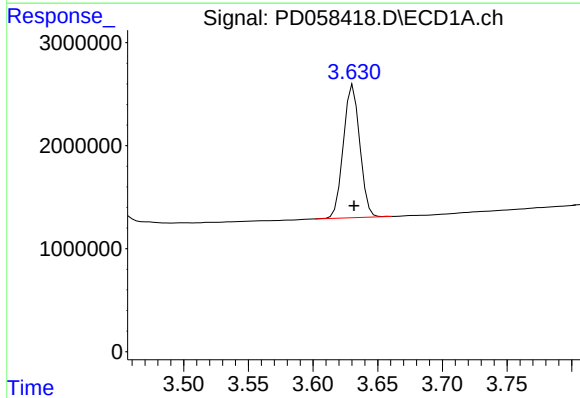


#2 alpha-BHC

R.T.: 3.631 min
Delta R.T.: 0.000 min
Response: 11374698
Conc: 4.50 ng/ml

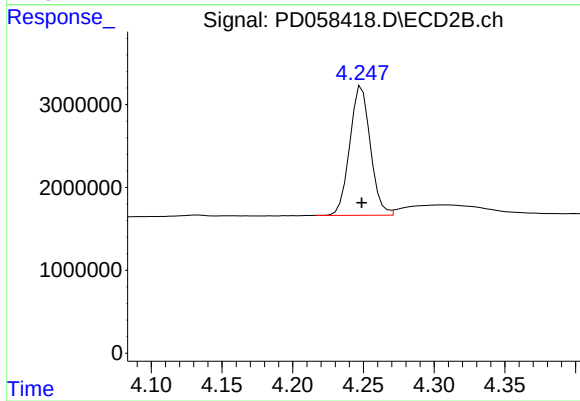

#2 alpha-BHC


R.T.: 4.249 min
Delta R.T.: 0.000 min
Response: 15799774
Conc: 4.56 ng/ml

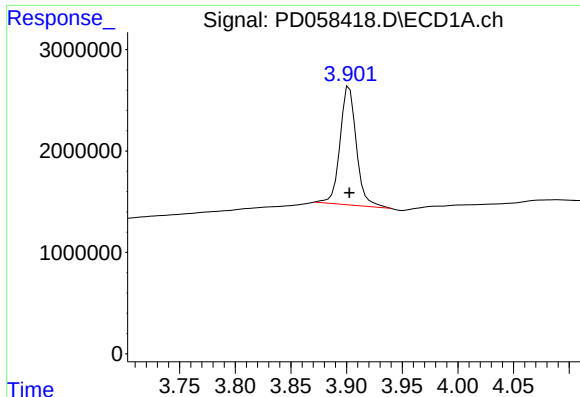

#3 gamma-BHC (Lindane)


R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 11875809
Conc: 5.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

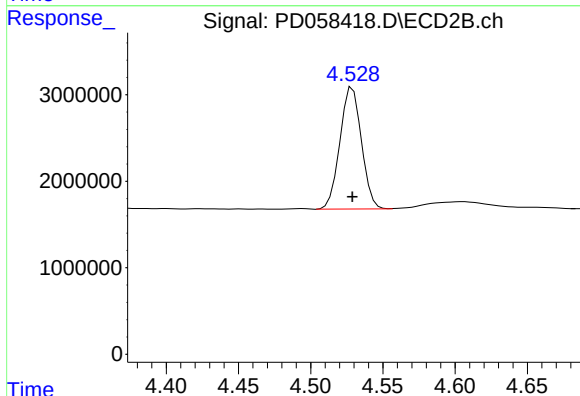


#3 gamma-BHC (Lindane)

R.T.: 4.529 min
Delta R.T.: 0.000 min
Response: 14569535
Conc: 4.58 ng/ml

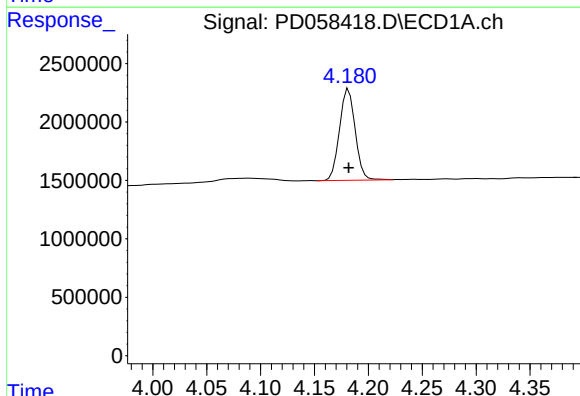


#4 Heptachlor

R.T.: 4.182 min
Delta R.T.: 0.000 min
Response: 7956818
Conc: 5.01 ng/ml

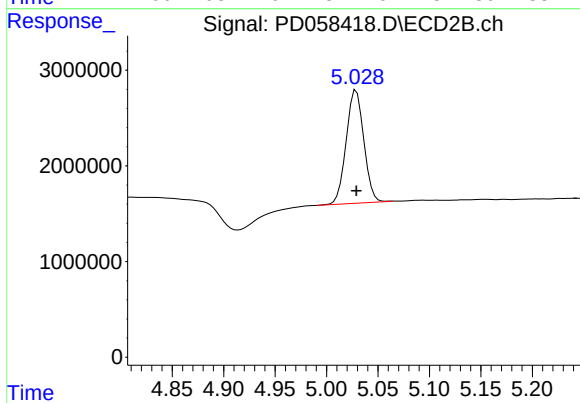

#4 Heptachlor


R.T.: 5.029 min
Delta R.T.: 0.000 min
Response: 14178147
Conc: 4.80 ng/ml

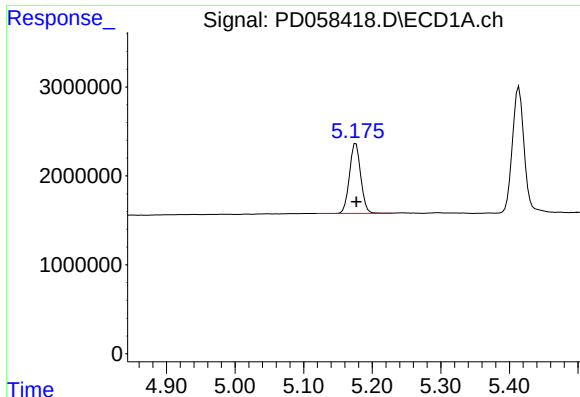

#9 Endosulfan I


R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 8954570
Conc: 4.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

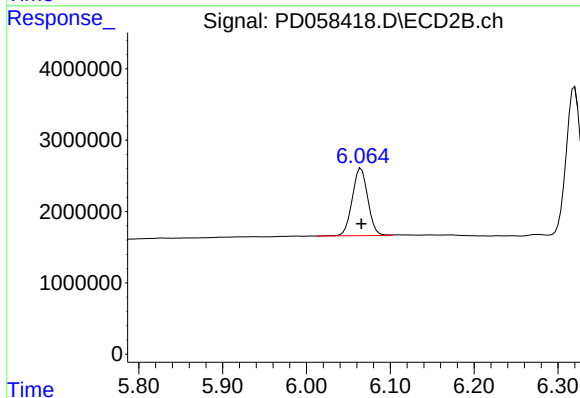


#9 Endosulfan I

R.T.: 6.065 min
Delta R.T.: 0.000 min
Response: 12188617
Conc: 4.92 ng/ml

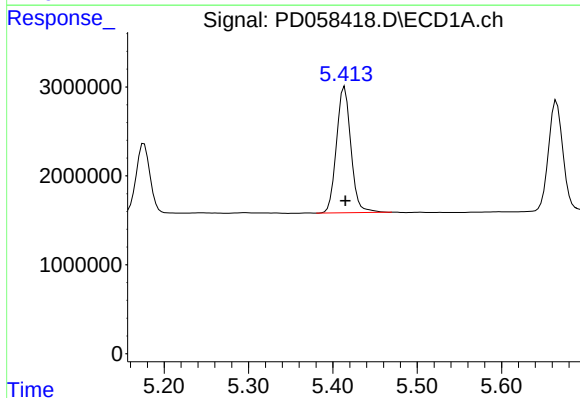


#13 Dieldrin

R.T.: 5.414 min
Delta R.T.: 0.000 min
Response: 16836557
Conc: 9.66 ng/ml

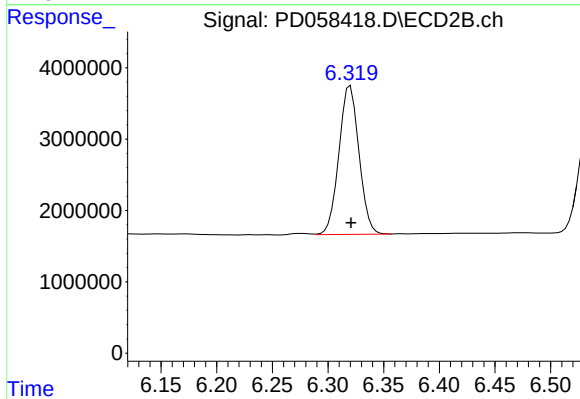

#13 Dieldrin


R.T.: 6.320 min
Delta R.T.: 0.000 min
Response: 26141589
Conc: 9.38 ng/ml

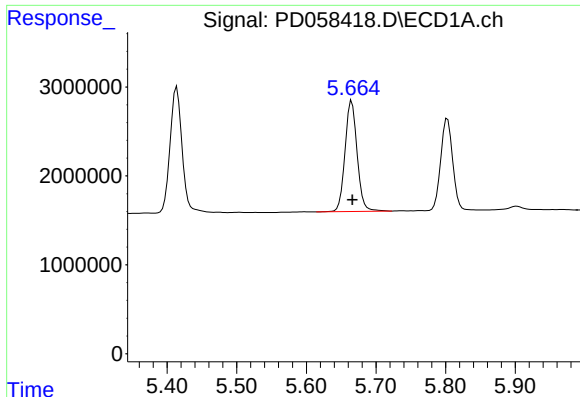

#14 Endrin


R.T.: 5.665 min
Delta R.T.: 0.000 min
Response: 15059255
Conc: 10.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

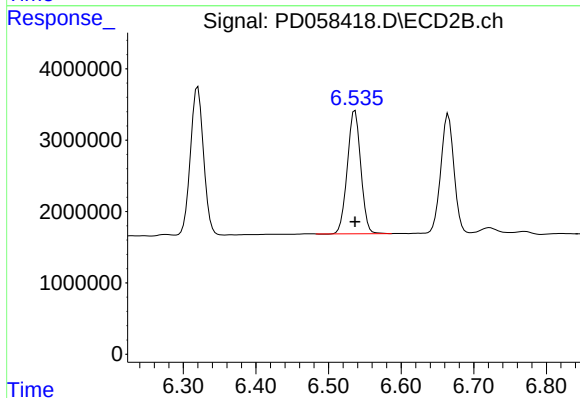


#14 Endrin

R.T.: 6.537 min
Delta R.T.: 0.000 min
Response: 22240495
Conc: 9.52 ng/ml

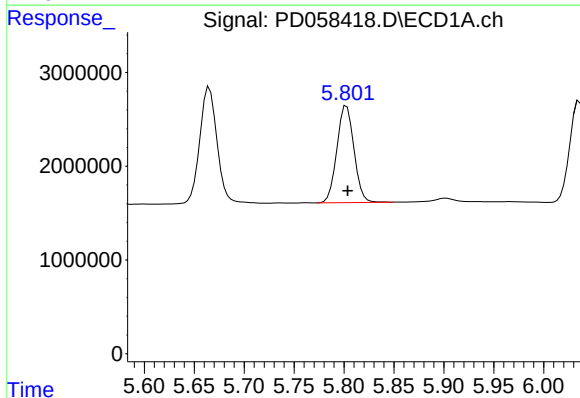


#16 4,4'-DDD

R.T.: 5.803 min
Delta R.T.: -0.001 min
Response: 12293116
Conc: 10.13 ng/ml

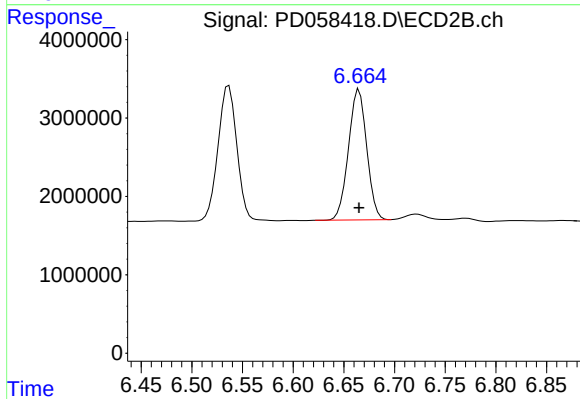

#16 4,4'-DDD


R.T.: 6.665 min
Delta R.T.: 0.000 min
Response: 20830295
Conc: 9.36 ng/ml

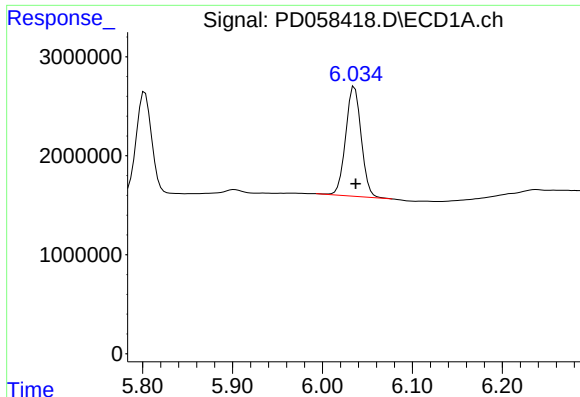

#17 4,4'-DDT


R.T.: 6.036 min
Delta R.T.: -0.001 min
Response: 13279353
Conc: 9.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

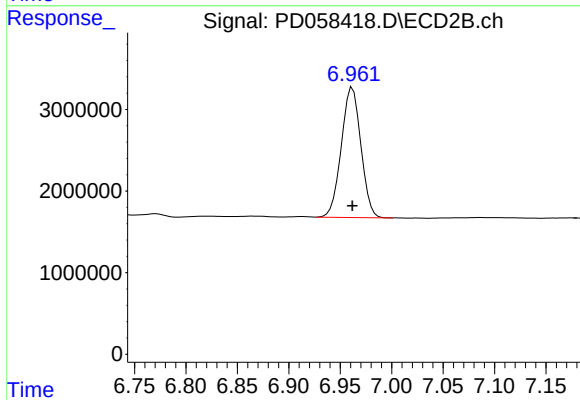


#17 4,4'-DDT

R.T.: 6.962 min
Delta R.T.: 0.000 min
Response: 21151701
Conc: 9.19 ng/ml

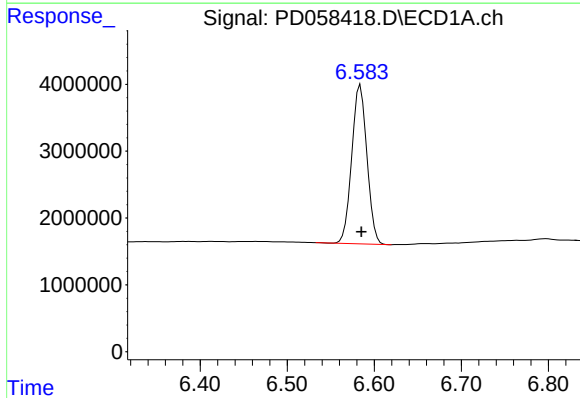


#20 Methoxychlor

R.T.: 6.584 min
Delta R.T.: 0.000 min
Response: 28834913
Conc: 52.30 ng/ml

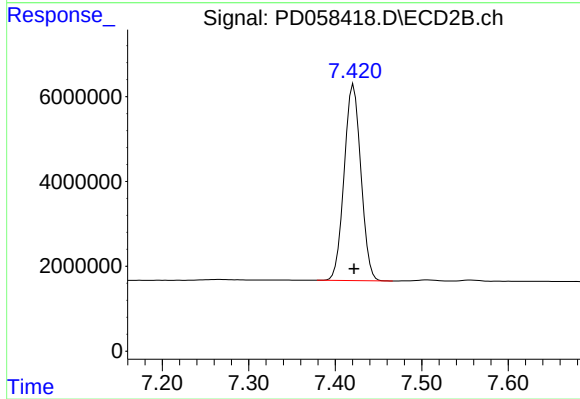

#20 Methoxychlor


R.T.: 7.421 min
Delta R.T.: 0.000 min
Response: 61777860
Conc: 51.66 ng/ml

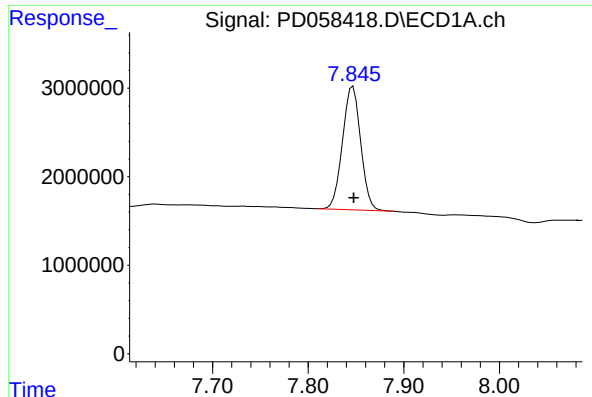

#27 Decachlorobiphenyl

R.T.: 7.847 min
Delta R.T.: 0.000 min
Response: 18460015
Conc: 10.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

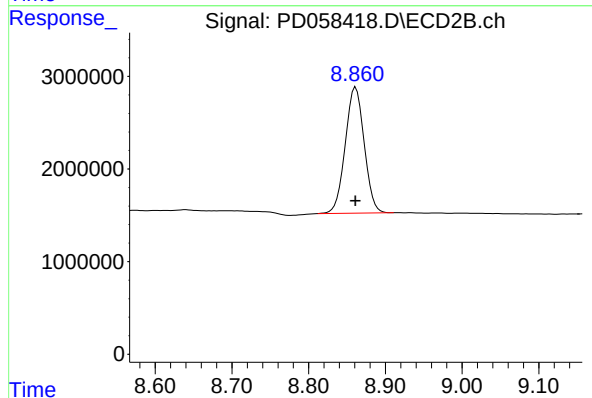

#27 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.000 min
Response: 23442290
Conc: 10.98 ng/ml