

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070220\
 Data File : PD058420.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2020 11:33
 Operator : AJ\MA
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 12:33:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 02 12:31:35 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.866	17209367	23292187	10.141	9.961
27)	SA Decachlor...	7.847	8.861	36637588	45235219	20.752	21.194
Target Compounds							
2)	A alpha-BHC	3.631	4.249	24360918	33604370	9.630	9.692
3)	MA gamma-BHC...	3.902	4.529	23312627	30878533	10.066	9.710
4)	MA Heptachlor	4.182	5.030	15959933	29209537	10.044	9.881
9)	A Endosulfan I	5.176	6.066	18178783	24965029	10.087	10.078
13)	MA Dieldrin	5.414	6.321	34720408	54766008	19.920	19.647
14)	MA Endrin	5.665	6.536	30268269	46433147	20.493	19.867
16)	A 4,4'-DDD	5.803	6.665	24619142	43668984	20.293	19.621
17)	MA 4,4'-DDT	6.036	6.961	27650559	45077671	19.436	19.584
20)	A Methoxychlor	6.585	7.421	57746407	124.3E6	104.742	103.972

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070220\
Data File : PD058420.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2020 11:33
Operator : AJ\MA
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 12:33:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 02 12:31:35 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

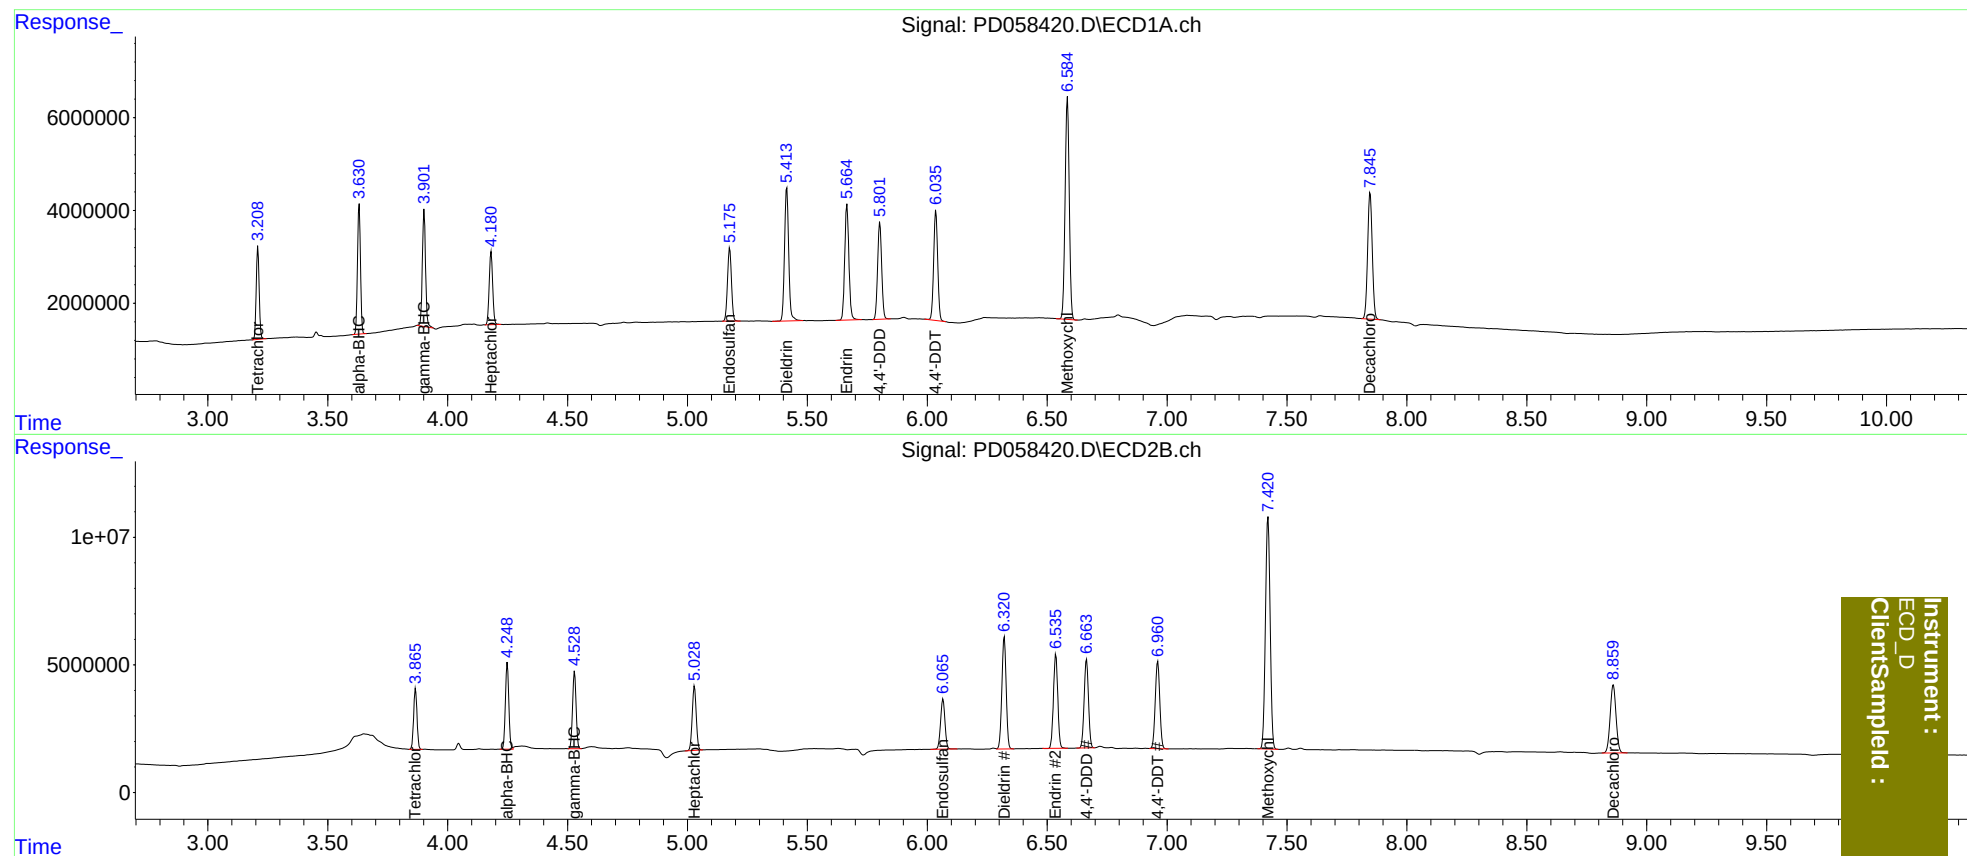


Instrument :
ECD_D
ClientSampled :

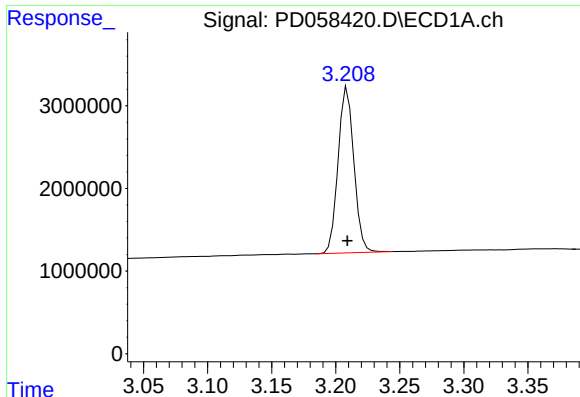

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.000 min
Response: 17209367
Conc: 10.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

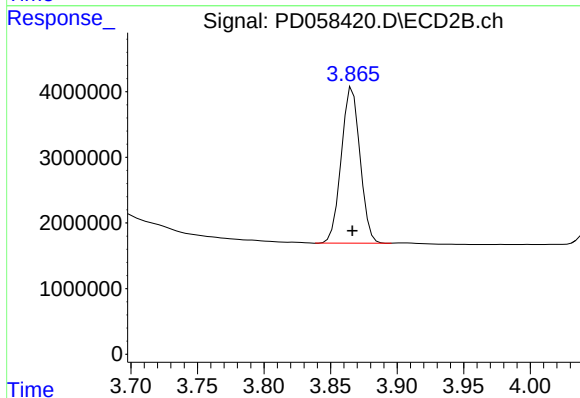


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 23292187
Conc: 9.96 ng/ml

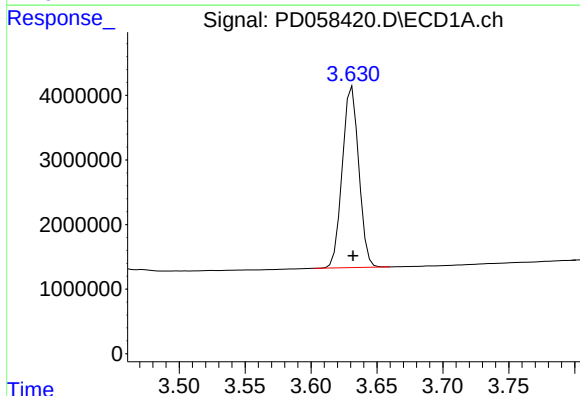


#2 alpha-BHC

R.T.: 3.631 min
Delta R.T.: 0.000 min
Response: 24360918
Conc: 9.63 ng/ml

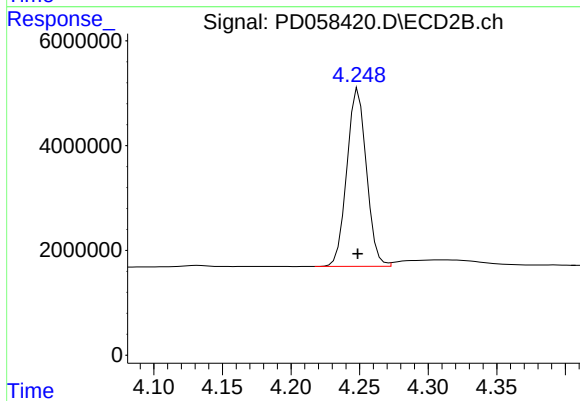

#2 alpha-BHC


R.T.: 4.249 min
Delta R.T.: 0.000 min
Response: 33604370
Conc: 9.69 ng/ml

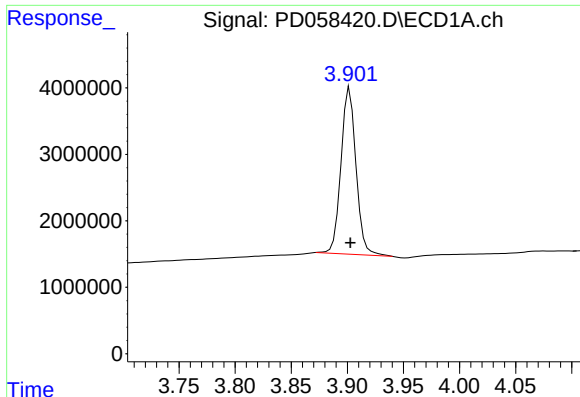

#3 gamma-BHC (Lindane)


R.T.: 3.902 min
Delta R.T.: 0.000 min
Response: 23312627
Conc: 10.07 ng/ml

Instrument :
ECD_D
ClientSampleId :

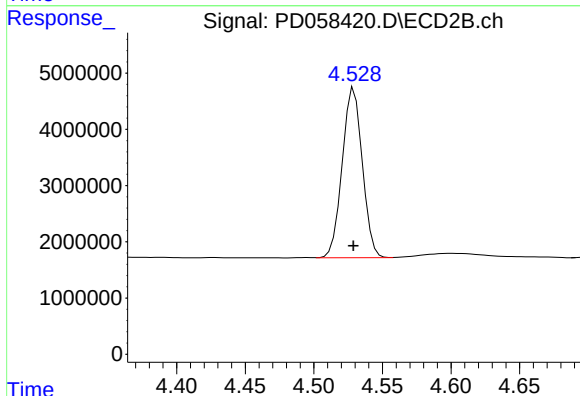


#3 gamma-BHC (Lindane)

R.T.: 4.529 min
Delta R.T.: 0.000 min
Response: 30878533
Conc: 9.71 ng/ml

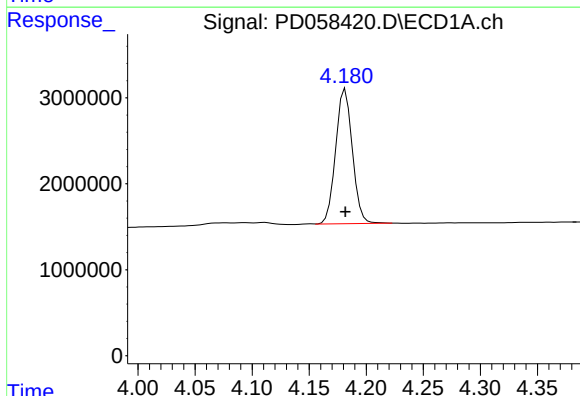


#4 Heptachlor

R.T.: 4.182 min
Delta R.T.: 0.000 min
Response: 15959933
Conc: 10.04 ng/ml

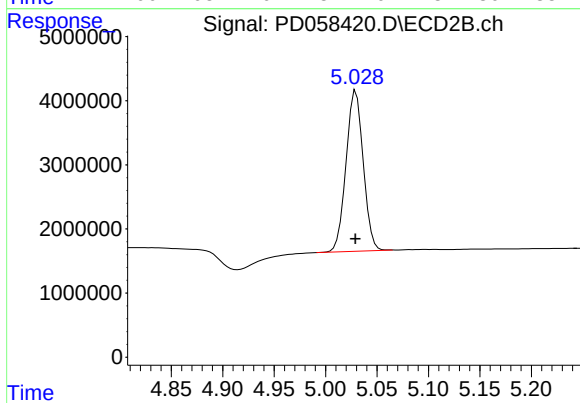

#4 Heptachlor


R.T.: 5.030 min
Delta R.T.: 0.000 min
Response: 29209537
Conc: 9.88 ng/ml

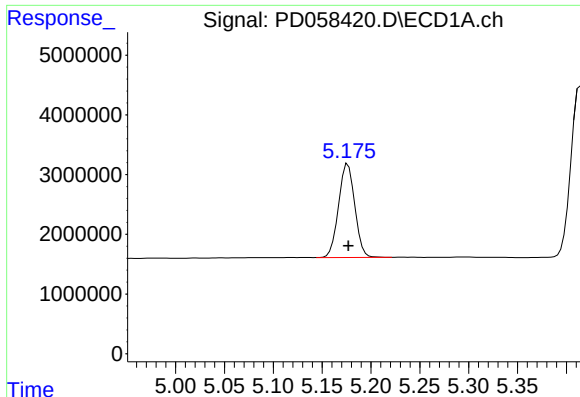

#9 Endosulfan I


R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 18178783
Conc: 10.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

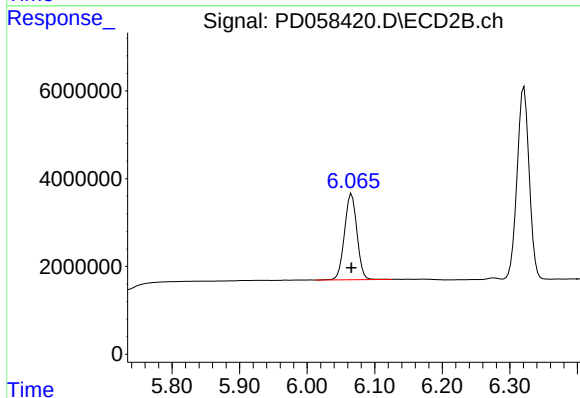


#9 Endosulfan I

R.T.: 6.066 min
Delta R.T.: 0.000 min
Response: 24965029
Conc: 10.08 ng/ml

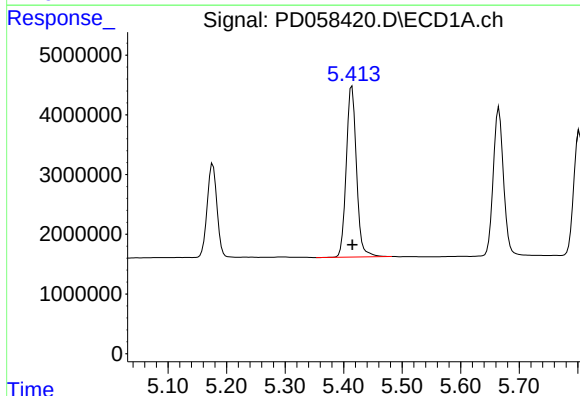


#13 Dieldrin

R.T.: 5.414 min
Delta R.T.: 0.000 min
Response: 34720408
Conc: 19.92 ng/ml

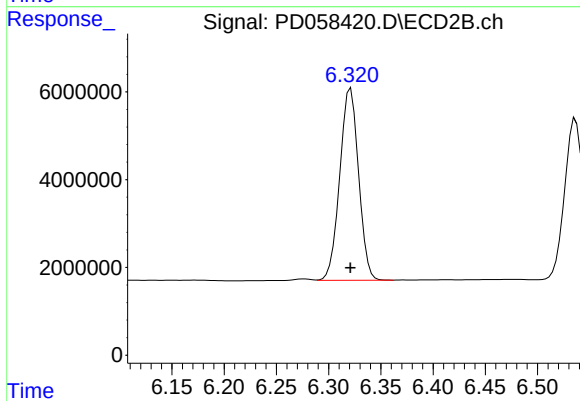

#13 Dieldrin


R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 54766008
Conc: 19.65 ng/ml

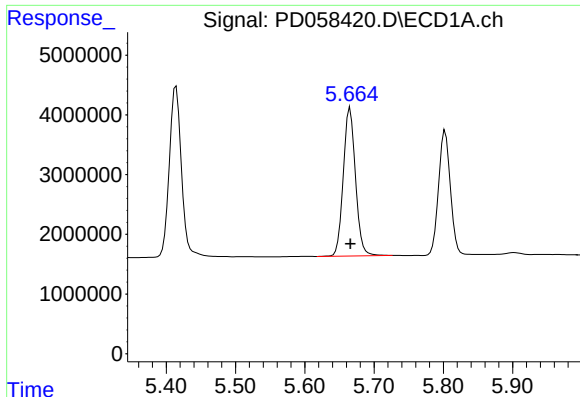

#14 Endrin


R.T.: 5.665 min
Delta R.T.: 0.000 min
Response: 30268269
Conc: 20.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

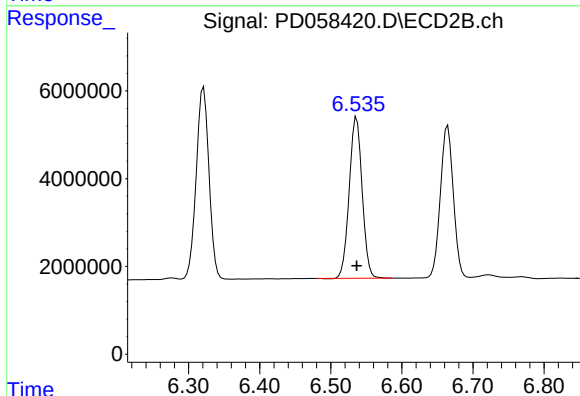


#14 Endrin

R.T.: 6.536 min
Delta R.T.: 0.000 min
Response: 46433147
Conc: 19.87 ng/ml

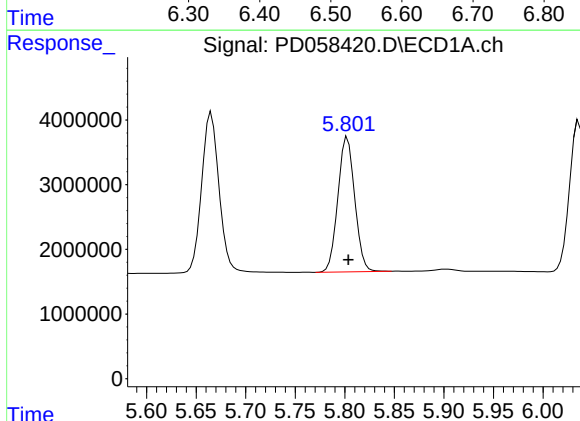


#16 4,4'-DDD

R.T.: 5.803 min
Delta R.T.: 0.000 min
Response: 24619142
Conc: 20.29 ng/ml

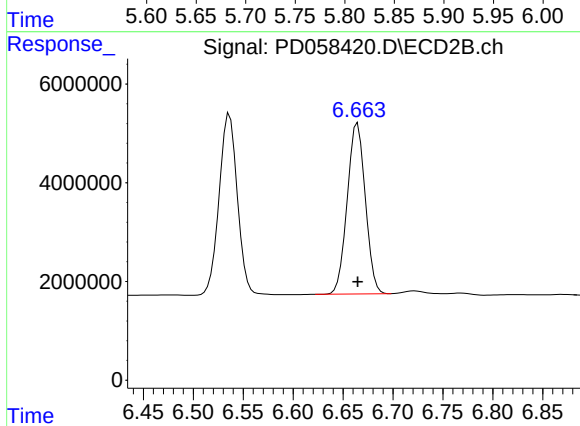

#16 4,4'-DDD


R.T.: 6.665 min
Delta R.T.: 0.000 min
Response: 43668984
Conc: 19.62 ng/ml

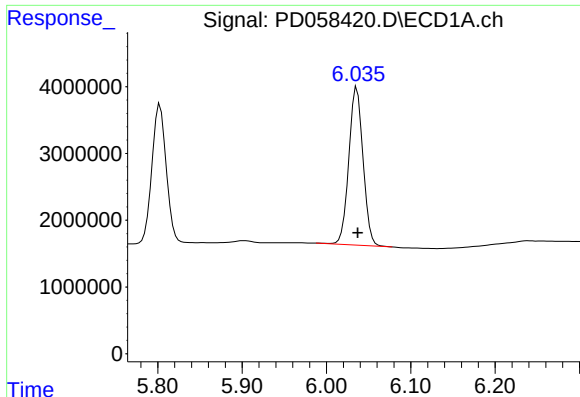

#17 4,4'-DDT


R.T.: 6.036 min
Delta R.T.: -0.001 min
Response: 27650559
Conc: 19.44 ng/ml

Instrument :
ECD_D
ClientSampleId :

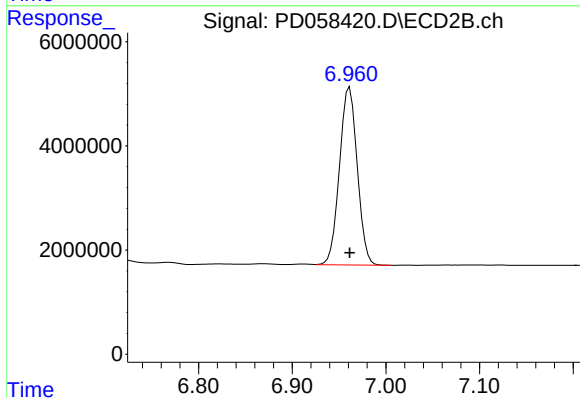


#17 4,4'-DDT

R.T.: 6.961 min
Delta R.T.: 0.000 min
Response: 45077671
Conc: 19.58 ng/ml

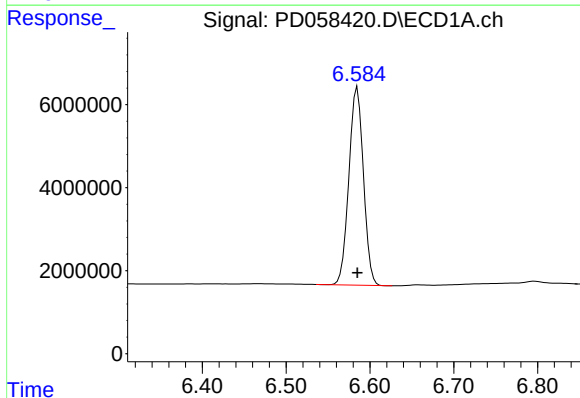


#20 Methoxychlor

R.T.: 6.585 min
Delta R.T.: 0.000 min
Response: 57746407
Conc: 104.74 ng/ml

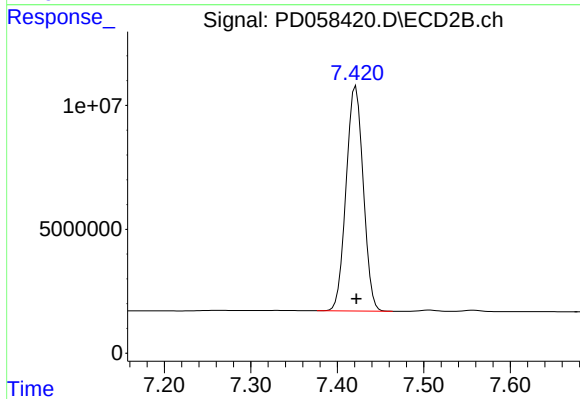

#20 Methoxychlor


R.T.: 7.421 min
Delta R.T.: 0.000 min
Response: 124336761
Conc: 103.97 ng/ml

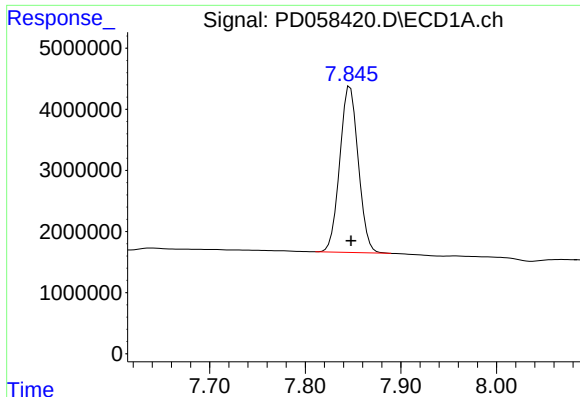

#27 Decachlorobiphenyl

R.T.: 7.847 min
Delta R.T.: 0.000 min
Response: 36637588
Conc: 20.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

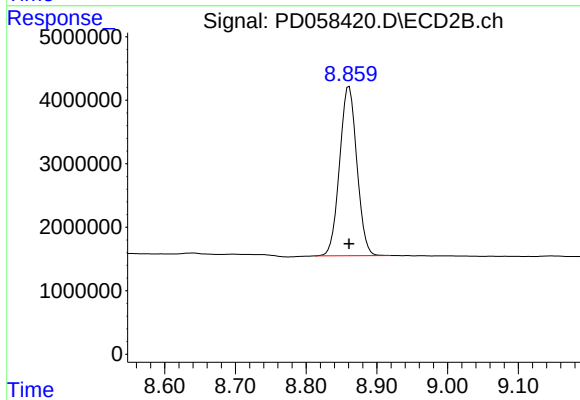

#27 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.000 min
Response: 45235219
Conc: 21.19 ng/ml