

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070220\
 Data File : PD058422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2020 12:01
 Operator : AJ\MA
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 12:34:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 02 12:31:35 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.866	33938835	46767873	20.000	20.000
27)	SA Decachlor...	7.848	8.861	70618582	85375574	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.632	4.249	50595483	69344366	20.000	20.000
3)	MA gamma-BHC...	3.903	4.529	46319309	63603937	20.000	20.000
4)	MA Heptachlor	4.182	5.029	31779744	59121968	20.000	20.000
9)	A Endosulfan I	5.177	6.066	36042199	49542495	20.000	20.000
13)	MA Dieldrin	5.415	6.321	69719143	111.5E6	40.000	40.000
14)	MA Endrin	5.666	6.536	59080582	93489404	40.000	40.000
16)	A 4,4'-DDD	5.804	6.665	48528328	89023251	40.000	40.000
17)	MA 4,4'-DDT	6.037	6.962	56906788	92068531	40.000	40.000
20)	A Methoxychlor	6.585	7.422	110.3E6	239.2E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070220\
Data File : PD058422.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2020 12:01
Operator : AJ\MA
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 12:34:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 02 12:31:35 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

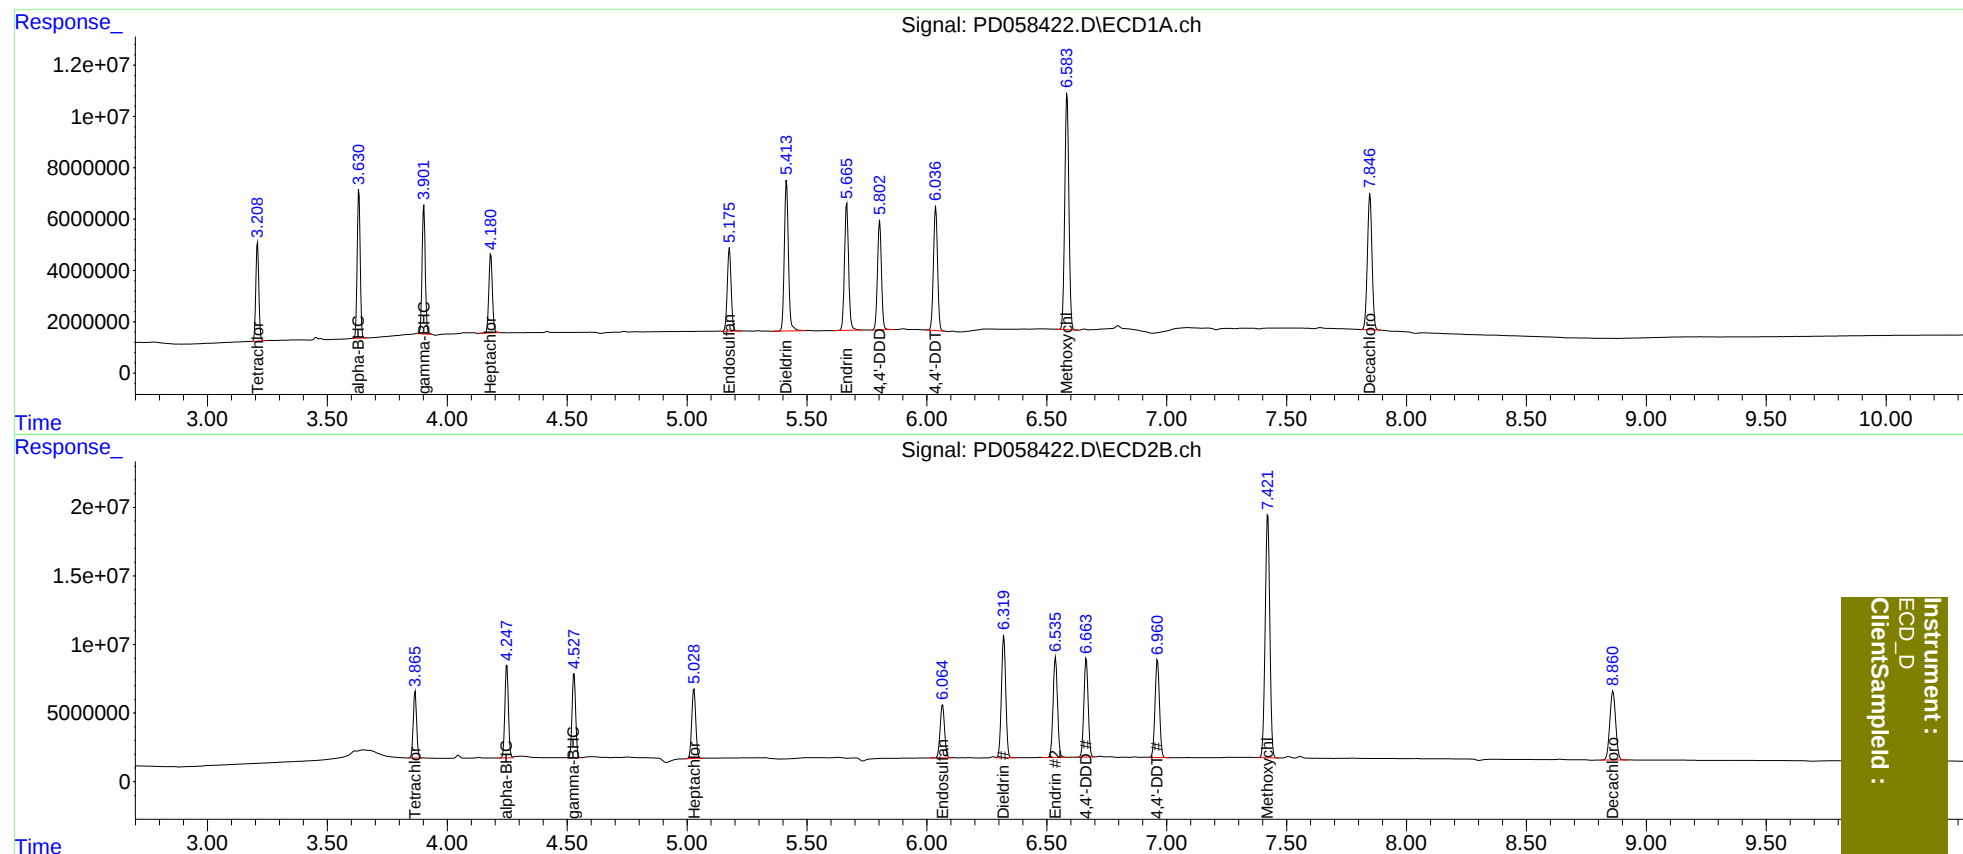


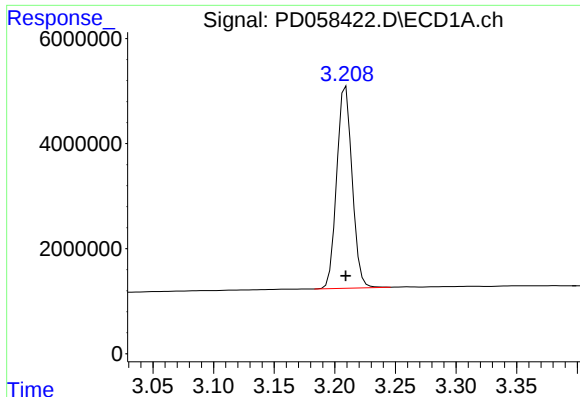

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.000 min
Response: 33938835
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

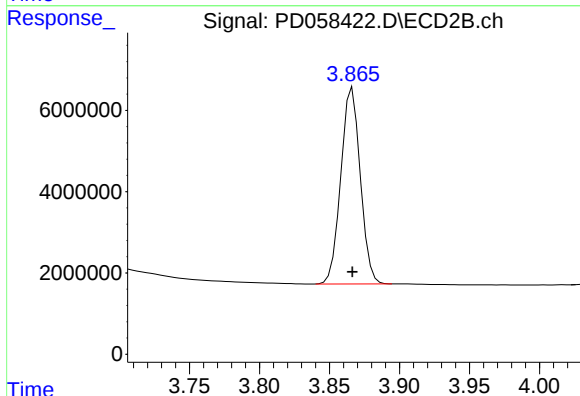


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 46767873
Conc: 20.00 ng/ml

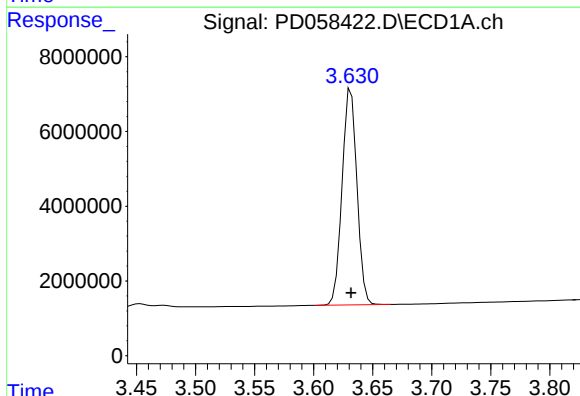


#2 alpha-BHC

R.T.: 3.632 min
Delta R.T.: 0.000 min
Response: 50595483
Conc: 20.00 ng/ml

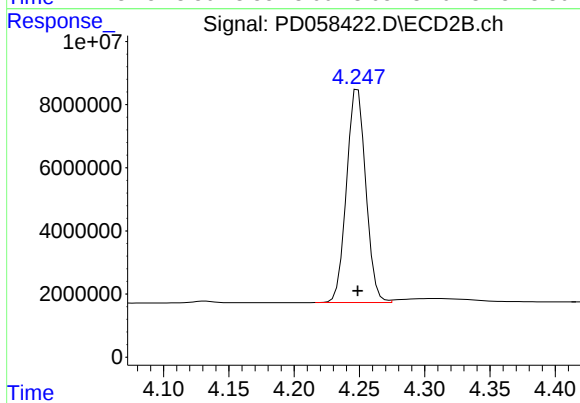

#2 alpha-BHC


R.T.: 4.249 min
Delta R.T.: 0.000 min
Response: 69344366
Conc: 20.00 ng/ml

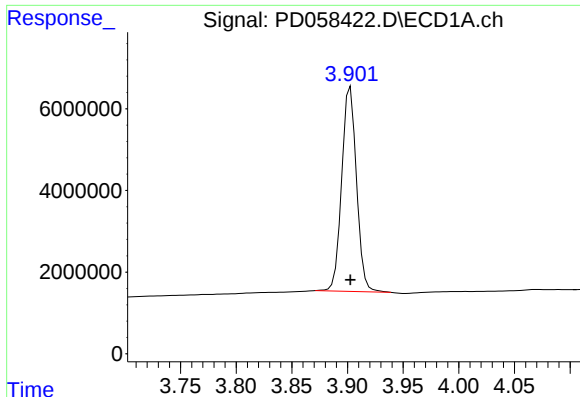

#3 gamma-BHC (Lindane)


R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 46319309
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

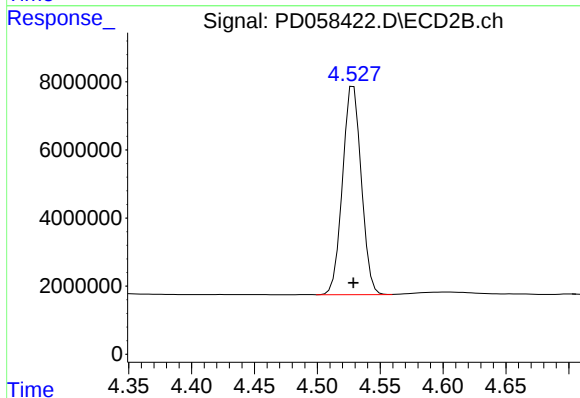


#3 gamma-BHC (Lindane)

R.T.: 4.529 min
Delta R.T.: 0.000 min
Response: 63603937
Conc: 20.00 ng/ml

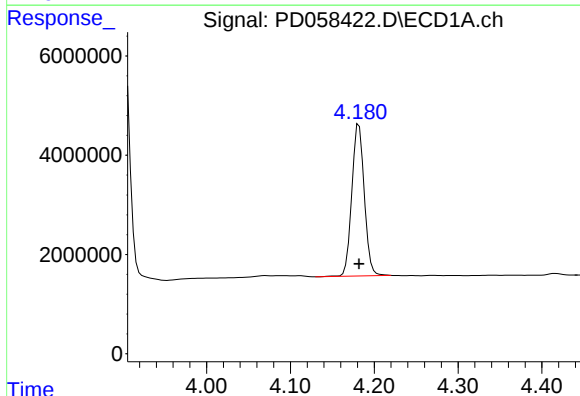


#4 Heptachlor

R.T.: 4.182 min
Delta R.T.: 0.000 min
Response: 31779744
Conc: 20.00 ng/ml

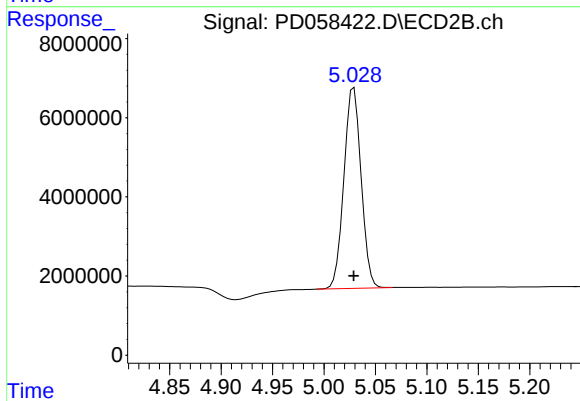

#4 Heptachlor


R.T.: 5.029 min
Delta R.T.: 0.000 min
Response: 59121968
Conc: 20.00 ng/ml

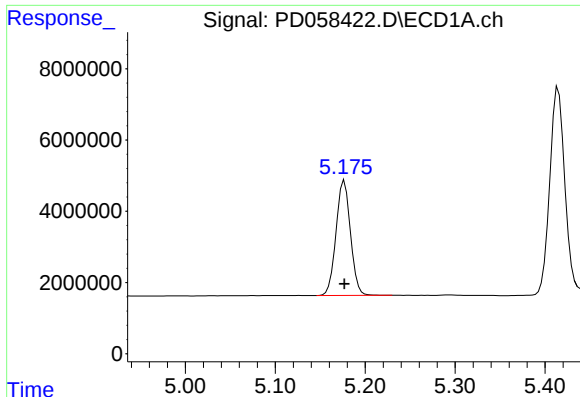

#9 Endosulfan I


R.T.: 5.177 min
Delta R.T.: 0.000 min
Response: 36042199
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

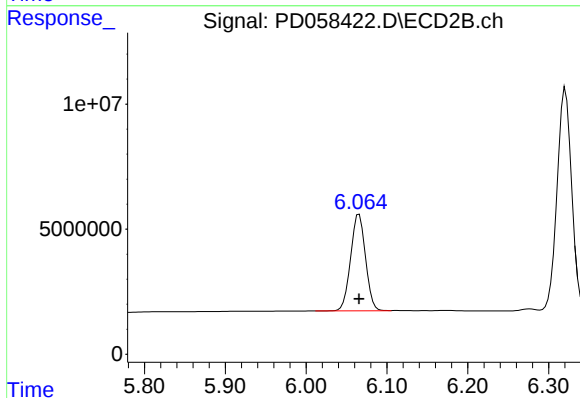


#9 Endosulfan I

R.T.: 6.066 min
Delta R.T.: 0.000 min
Response: 49542495
Conc: 20.00 ng/ml

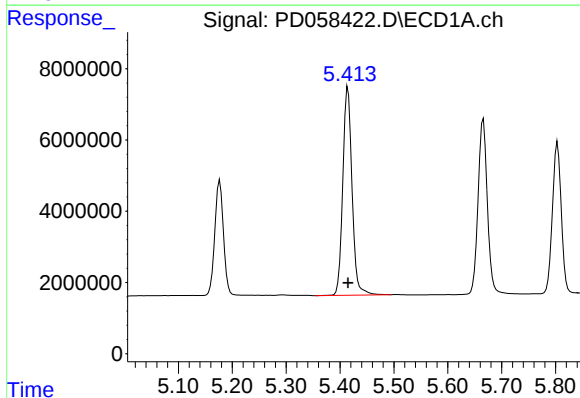


#13 Dieldrin

R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 69719143
Conc: 40.00 ng/ml

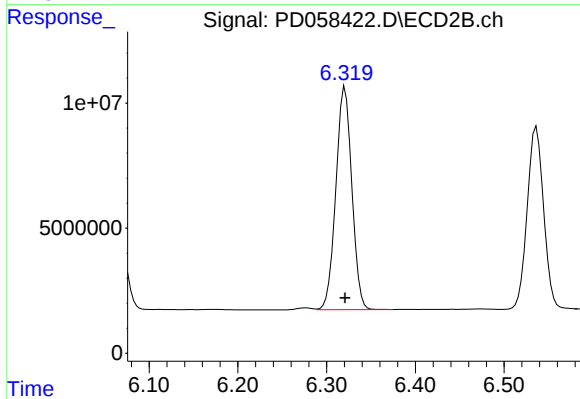

#13 Dieldrin


R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 111501297
Conc: 40.00 ng/ml

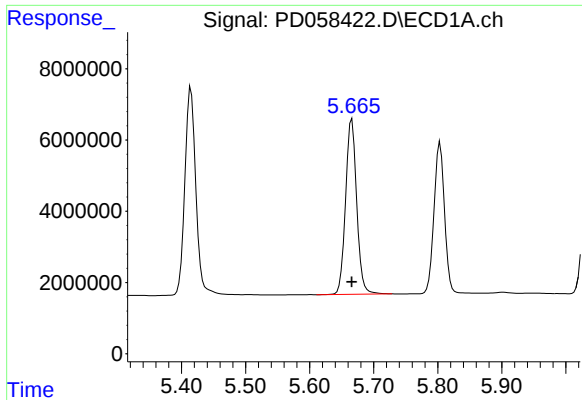

#14 Endrin


R.T.: 5.666 min
Delta R.T.: 0.000 min
Response: 59080582
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

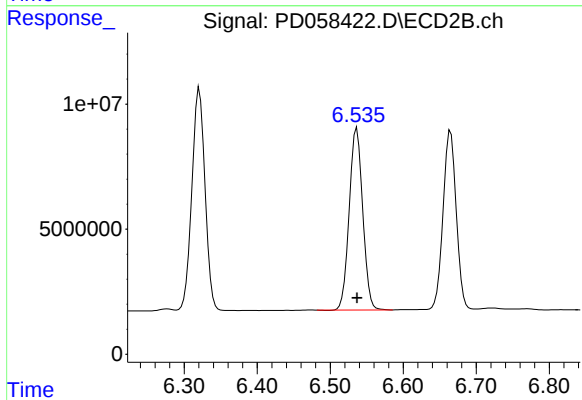


#14 Endrin

R.T.: 6.536 min
Delta R.T.: 0.000 min
Response: 93489404
Conc: 40.00 ng/ml

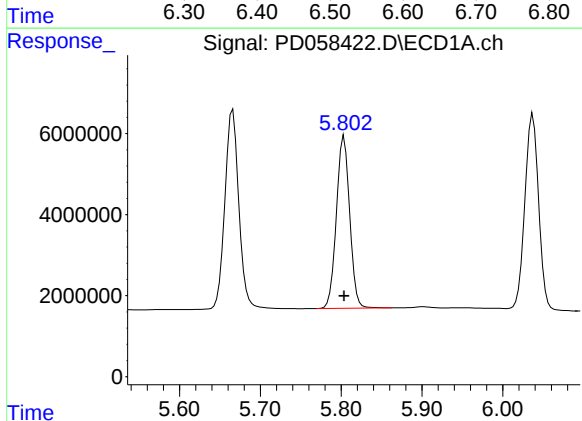


#16 4,4'-DDD

R.T.: 5.804 min
Delta R.T.: 0.000 min
Response: 48528328
Conc: 40.00 ng/ml

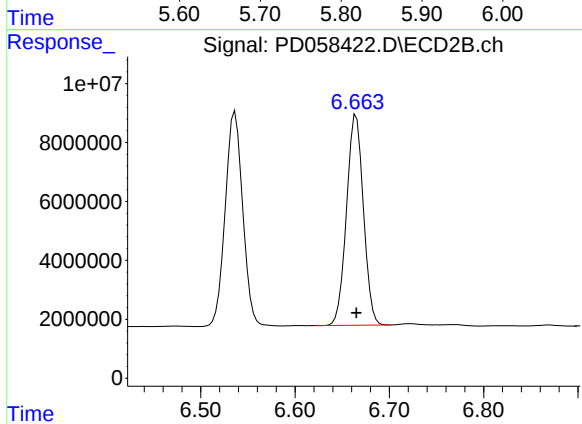

#16 4,4'-DDD


R.T.: 6.665 min
Delta R.T.: 0.000 min
Response: 89023251
Conc: 40.00 ng/ml

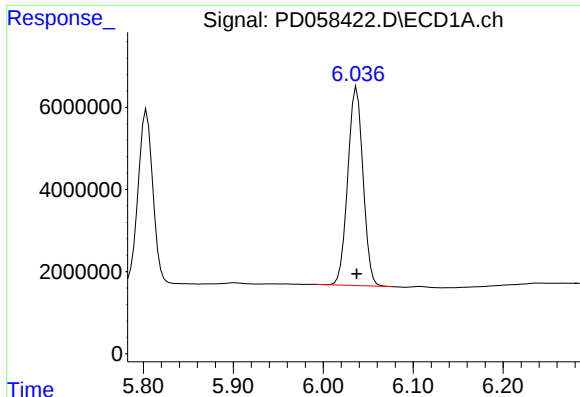

#17 4,4'-DDT


R.T.: 6.037 min
Delta R.T.: 0.000 min
Response: 56906788
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

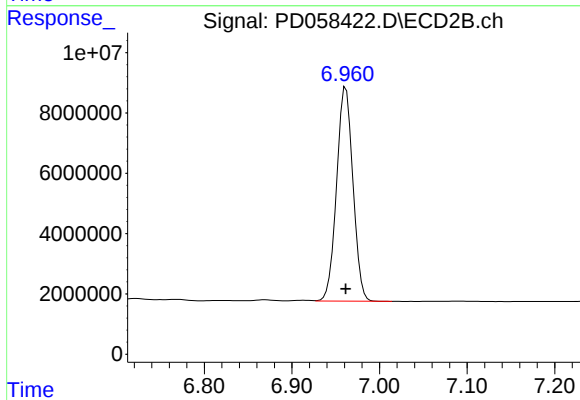


#17 4,4'-DDT

R.T.: 6.962 min
Delta R.T.: 0.000 min
Response: 92068531
Conc: 40.00 ng/ml

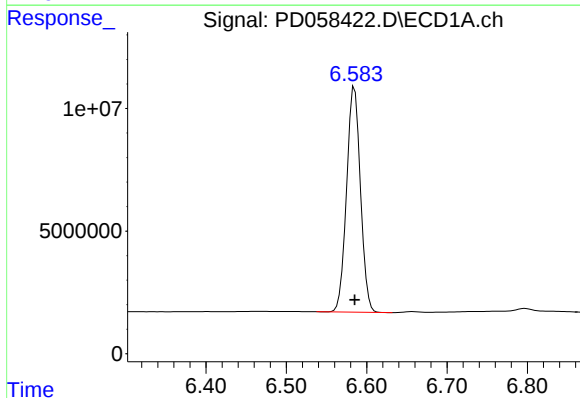


#20 Methoxychlor

R.T.: 6.585 min
Delta R.T.: 0.000 min
Response: 110263997
Conc: 200.00 ng/ml

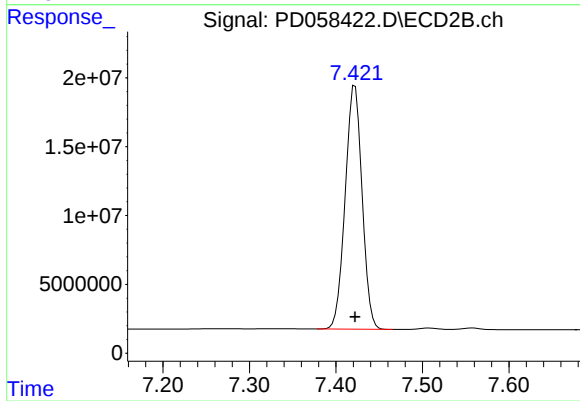

#20 Methoxychlor


R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 239172646
Conc: 200.00 ng/ml

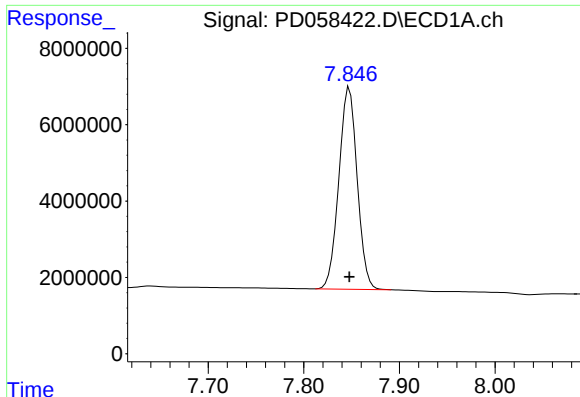

#27 Decachlorobiphenyl

R.T.: 7.848 min
Delta R.T.: 0.000 min
Response: 70618582
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

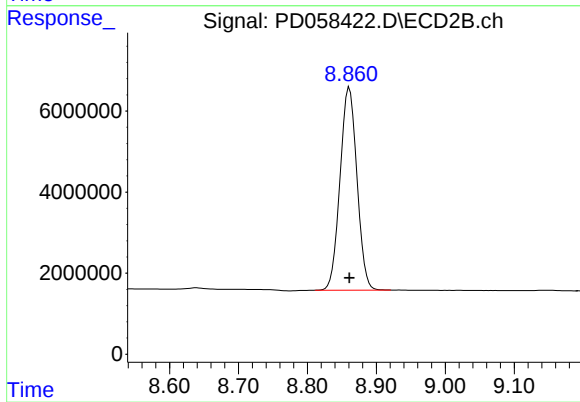

#27 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.000 min
Response: 85375574
Conc: 40.00 ng/ml