

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070220\
 Data File : PD058424.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2020 12:29
 Operator : AJ\MA
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 13:01:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 02 12:31:35 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.866	68058217	93168402	40.106	39.843
27)	SA Decachlor...	7.847	8.861	139.9E6	163.1E6	79.265	76.413
Target Compounds							
2)	A alpha-BHC	3.631	4.249	105.7E6	142.2E6	41.801	41.014
3)	MA gamma-BHC...	3.903	4.529	94777127	129.8E6	40.923	40.803
4)	MA Heptachlor	4.182	5.029	64440116	119.8E6	40.554	40.540
9)	A Endosulfan I	5.176	6.066	73106906	98779359	40.567	39.877
13)	MA Dieldrin	5.414	6.321	141.3E6	225.9E6	81.081	81.023
14)	MA Endrin	5.665	6.537	119.3E6	188.5E6	80.805	80.656
16)	A 4,4'-DDD	5.803	6.665	97123216	180.0E6	80.055	80.880
17)	MA 4,4'-DDT	6.037	6.962	120.1E6	189.1E6	84.419	82.168
20)	A Methoxychlor	6.584	7.422	215.1E6	460.5E6	390.084	385.115


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070220\
Data File : PD058424.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2020 12:29
Operator : AJ\MA
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 13:01:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 02 12:31:35 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

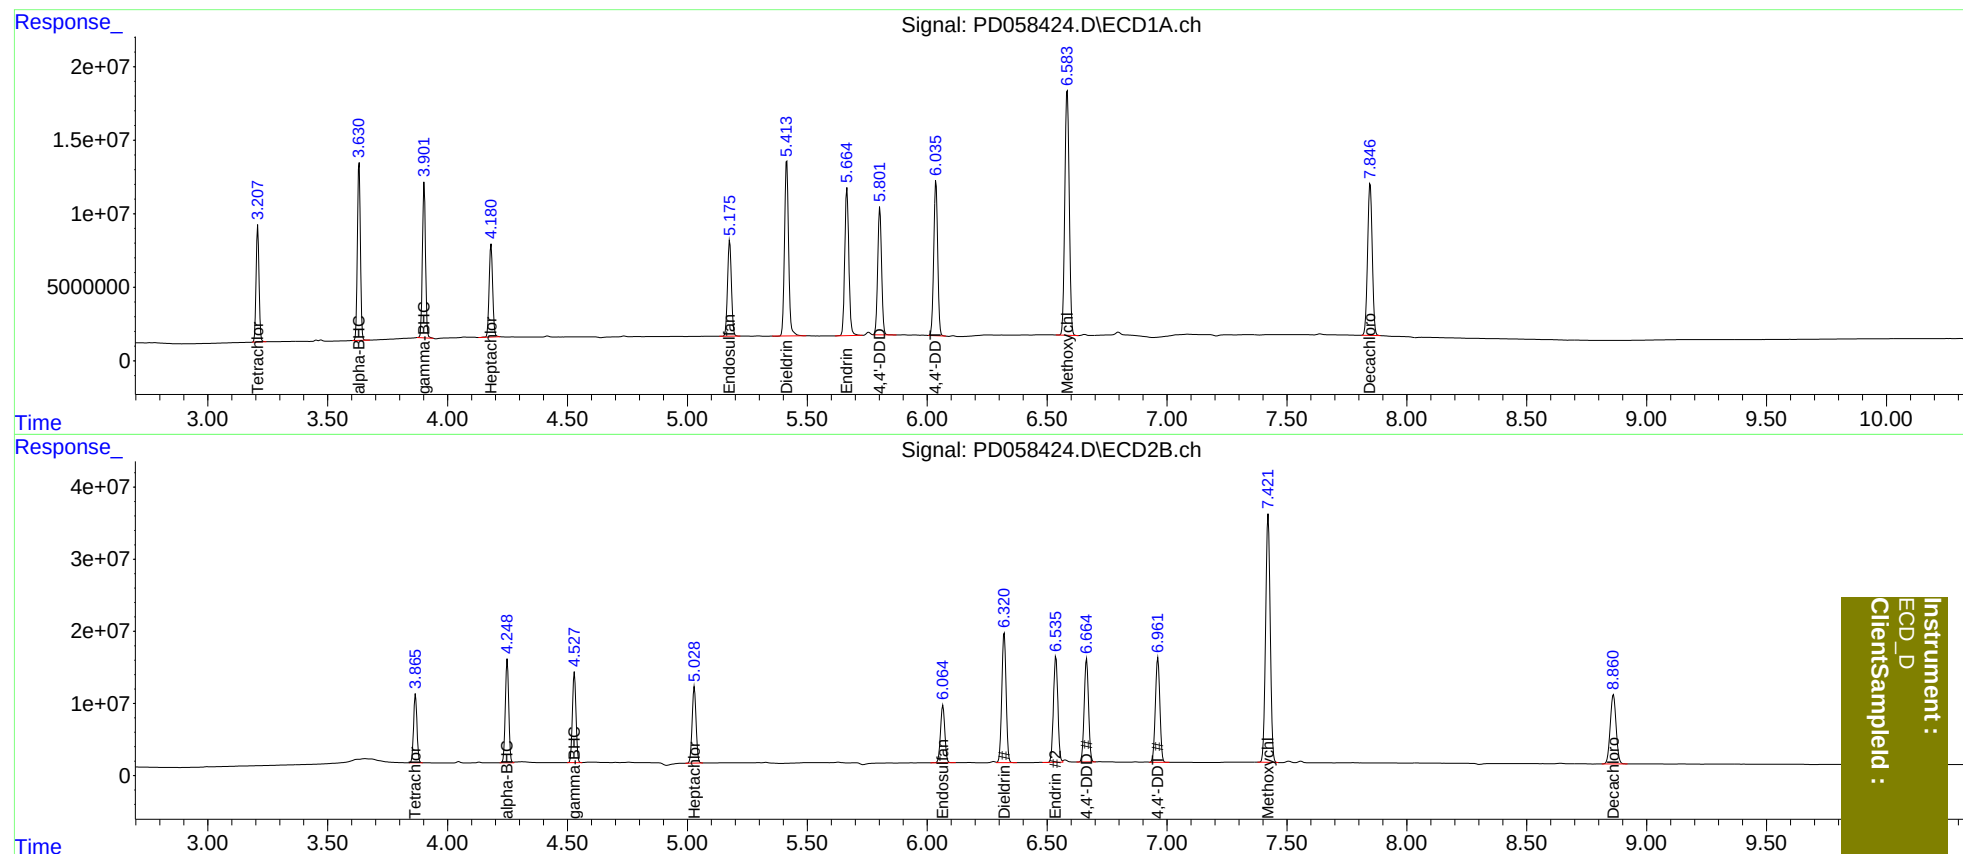


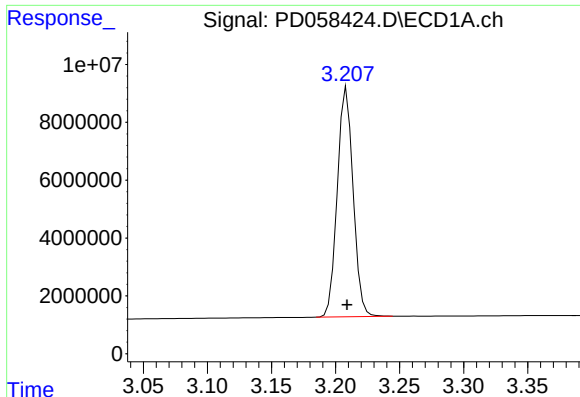

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.000 min
Response: 68058217
Conc: 40.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

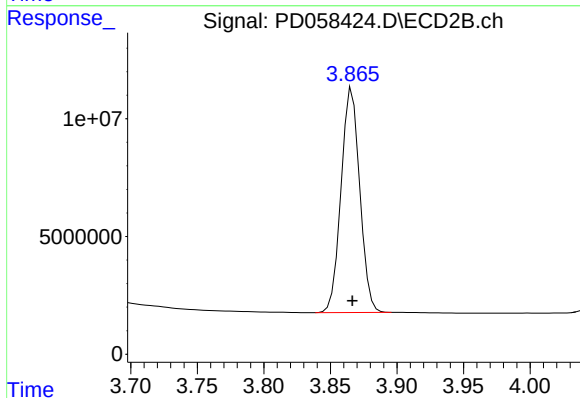


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 93168402
Conc: 39.84 ng/ml

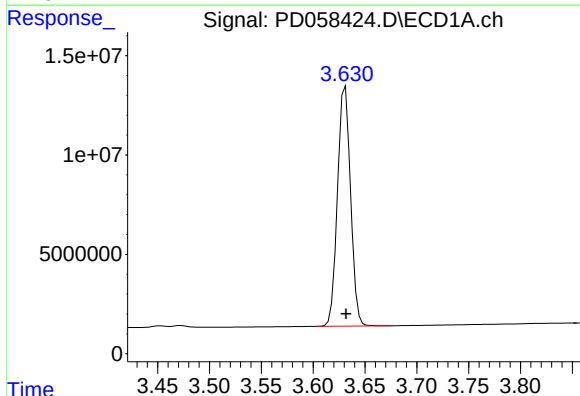


#2 alpha-BHC

R.T.: 3.631 min
Delta R.T.: 0.000 min
Response: 105747292
Conc: 41.80 ng/ml

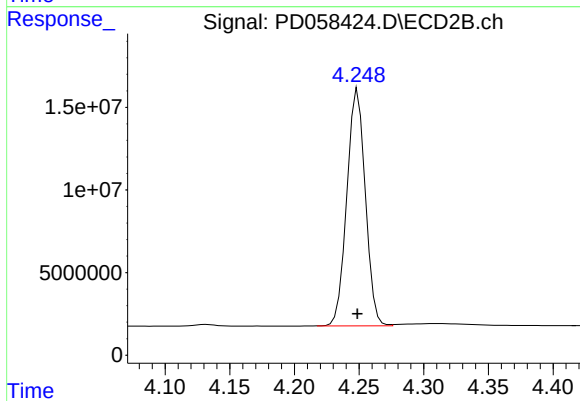

#2 alpha-BHC


R.T.: 4.249 min
Delta R.T.: 0.000 min
Response: 142206121
Conc: 41.01 ng/ml

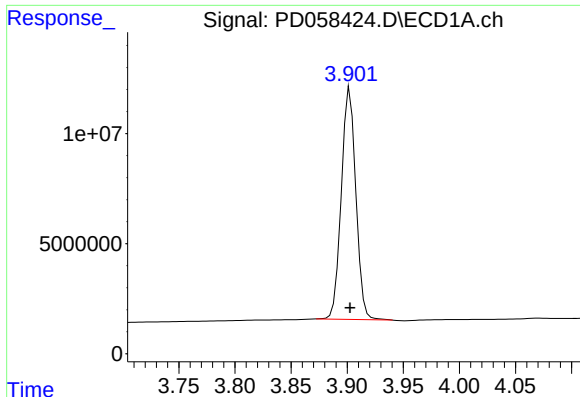

#3 gamma-BHC (Lindane)


R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 94777127
Conc: 40.92 ng/ml

Instrument :
ECD_D
ClientSampleId :

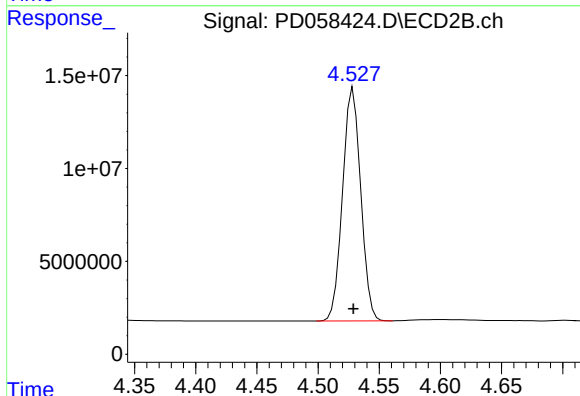


#3 gamma-BHC (Lindane)

R.T.: 4.529 min
Delta R.T.: 0.000 min
Response: 129761826
Conc: 40.80 ng/ml

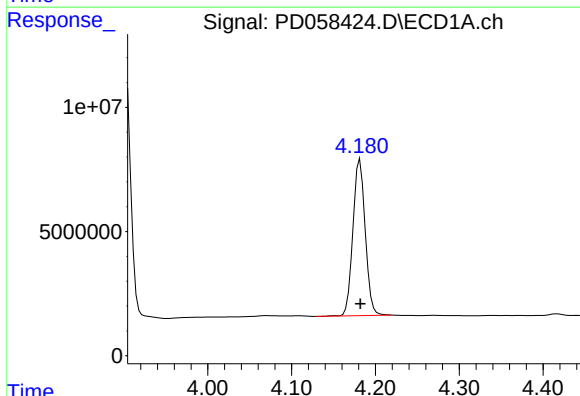


#4 Heptachlor

R.T.: 4.182 min
Delta R.T.: 0.000 min
Response: 64440116
Conc: 40.55 ng/ml

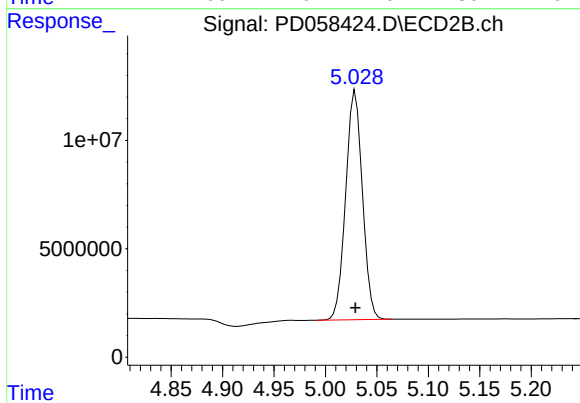

#4 Heptachlor


R.T.: 5.029 min
Delta R.T.: 0.000 min
Response: 119841256
Conc: 40.54 ng/ml

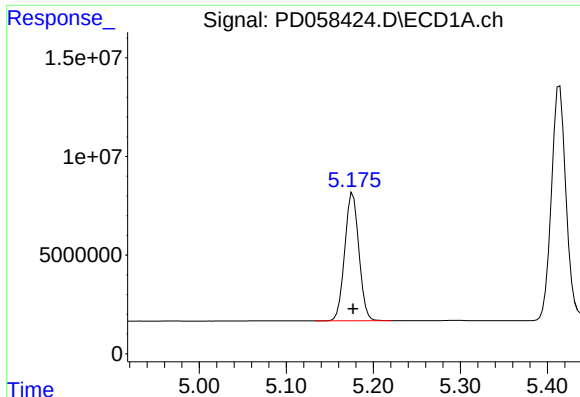

#9 Endosulfan I


R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 73106906
Conc: 40.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

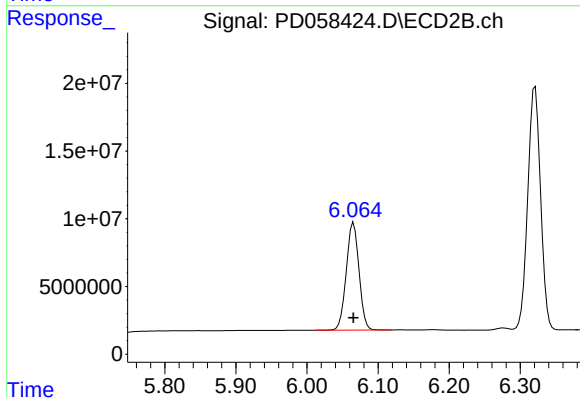


#9 Endosulfan I

R.T.: 6.066 min
Delta R.T.: 0.000 min
Response: 98779359
Conc: 39.88 ng/ml

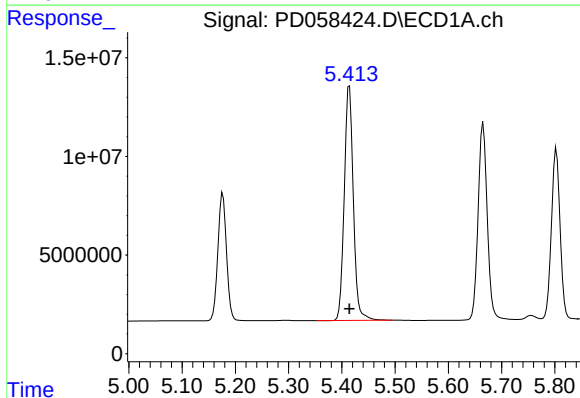


#13 Dieldrin

R.T.: 5.414 min
Delta R.T.: 0.000 min
Response: 141323010
Conc: 81.08 ng/ml

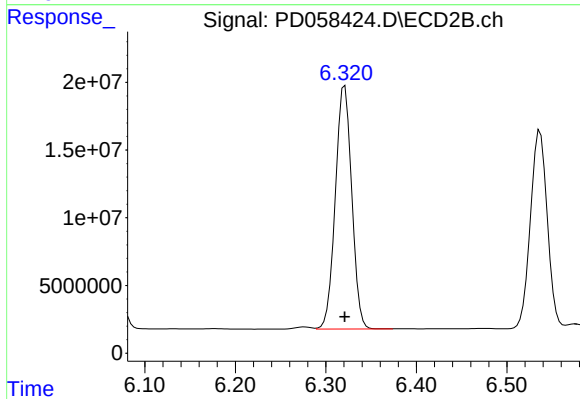

#13 Dieldrin


R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 225855408
Conc: 81.02 ng/ml

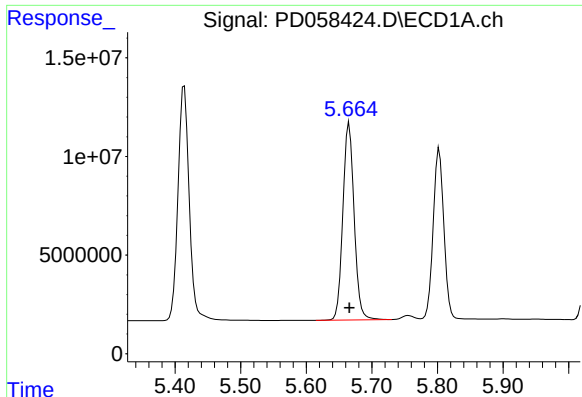

#14 Endrin


R.T.: 5.665 min
Delta R.T.: 0.000 min
Response: 119349595
Conc: 80.80 ng/ml

Instrument :
ECD_D
ClientSampleId :

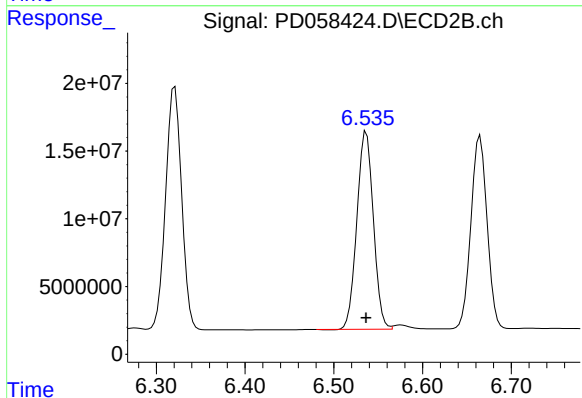


#14 Endrin

R.T.: 6.537 min
Delta R.T.: 0.000 min
Response: 188511758
Conc: 80.66 ng/ml

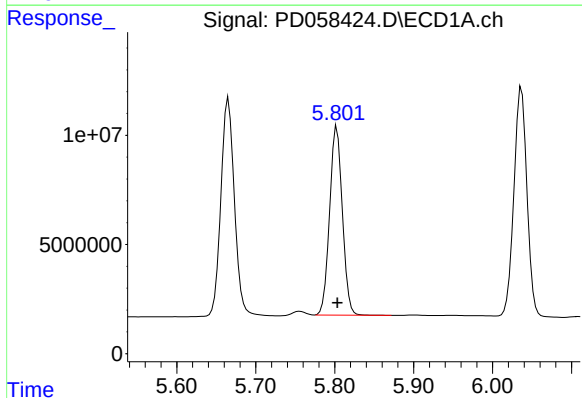


#16 4,4'-DDD

R.T.: 5.803 min
Delta R.T.: 0.000 min
Response: 97123216
Conc: 80.05 ng/ml

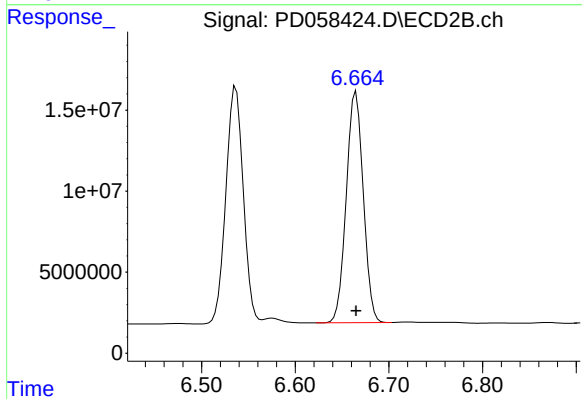

#16 4,4'-DDD


R.T.: 6.665 min
Delta R.T.: 0.000 min
Response: 180004120
Conc: 80.88 ng/ml

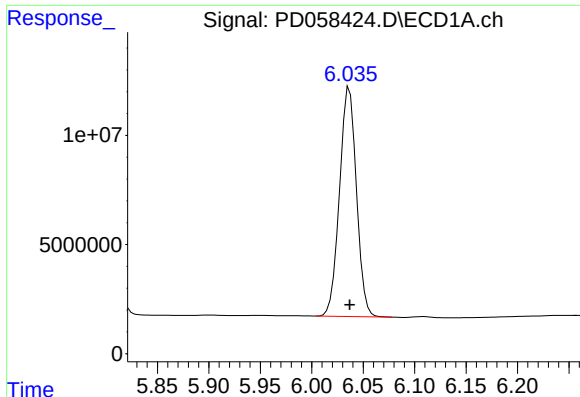

#17 4,4'-DDT


R.T.: 6.037 min
Delta R.T.: 0.000 min
Response: 120100615
Conc: 84.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

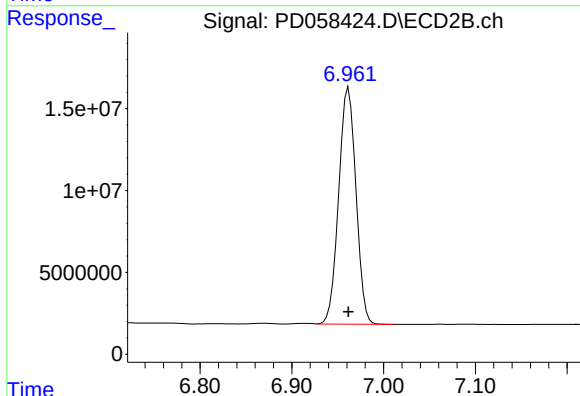


#17 4,4'-DDT

R.T.: 6.962 min
Delta R.T.: 0.000 min
Response: 189127040
Conc: 82.17 ng/ml

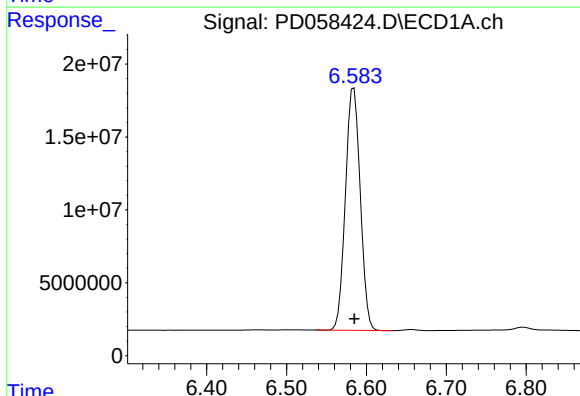


#20 Methoxychlor

R.T.: 6.584 min
Delta R.T.: 0.000 min
Response: 215061151
Conc: 390.08 ng/ml

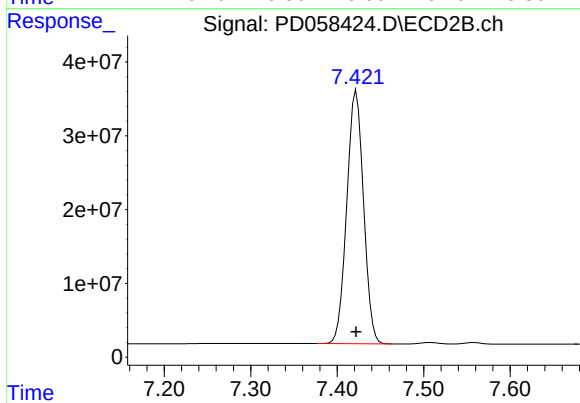

#20 Methoxychlor

R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 460544292
Conc: 385.11 ng/ml

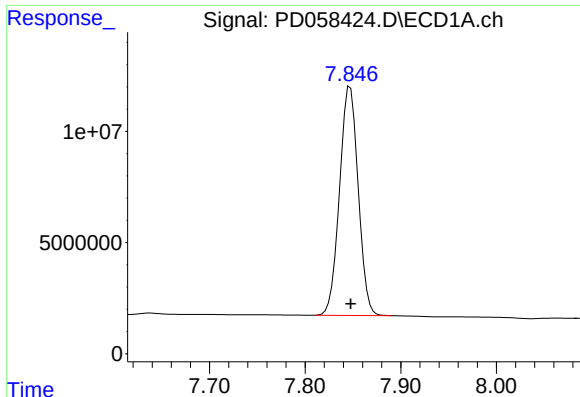

#27 Decachlorobiphenyl


R.T.: 7.847 min

Delta R.T.: 0.000 min

Response: 139940371

Conc: 79.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

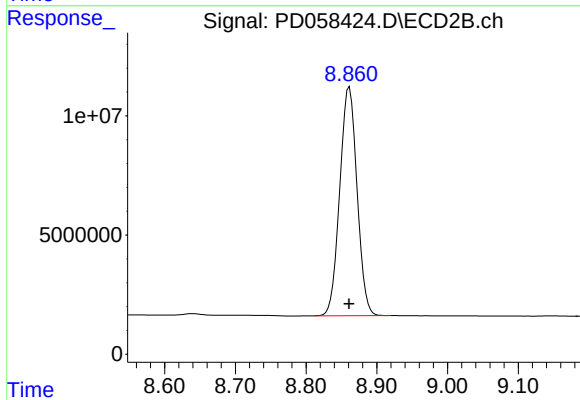

#27 Decachlorobiphenyl

R.T.: 8.861 min

Delta R.T.: 0.000 min

Response: 163095181

Conc: 76.41 ng/ml