

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070220\
 Data File : PD058426.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2020 12:57
 Operator : AJ\MA
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 13:10:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 02 12:31:35 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.866	128.5E6	173.4E6	75.749	74.147
27)	SA Decachlor...	7.847	8.861	263.5E6	295.0E6	149.258	138.232
Target Compounds							
2)	A alpha-BHC	3.631	4.249	204.6E6	270.4E6	80.874	78.000
3)	MA gamma-BHC...	3.902	4.529	181.4E6	245.7E6	78.330	77.262
4)	MA Heptachlor	4.181	5.029	122.2E6	226.0E6	76.925	76.466
9)	A Endosulfan I	5.176	6.066	140.2E6	186.2E6	77.797	75.165
13)	MA Dieldrin	5.414	6.321	270.9E6	424.1E6	155.446	152.156
14)	MA Endrin	5.665	6.536	223.7E6	349.0E6	151.422	149.315
16)	A 4,4'-DDD	5.803	6.665	184.8E6	339.9E6	152.345	152.719
17)	MA 4,4'-DDT	6.036	6.961	233.9E6	358.0E6	164.413	155.558
20)	A Methoxychlor	6.585	7.421	387.1E6	818.4E6	702.078	684.382


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070220\
Data File : PD058426.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2020 12:57
Operator : AJ\MA
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 13:10:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 02 12:31:35 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

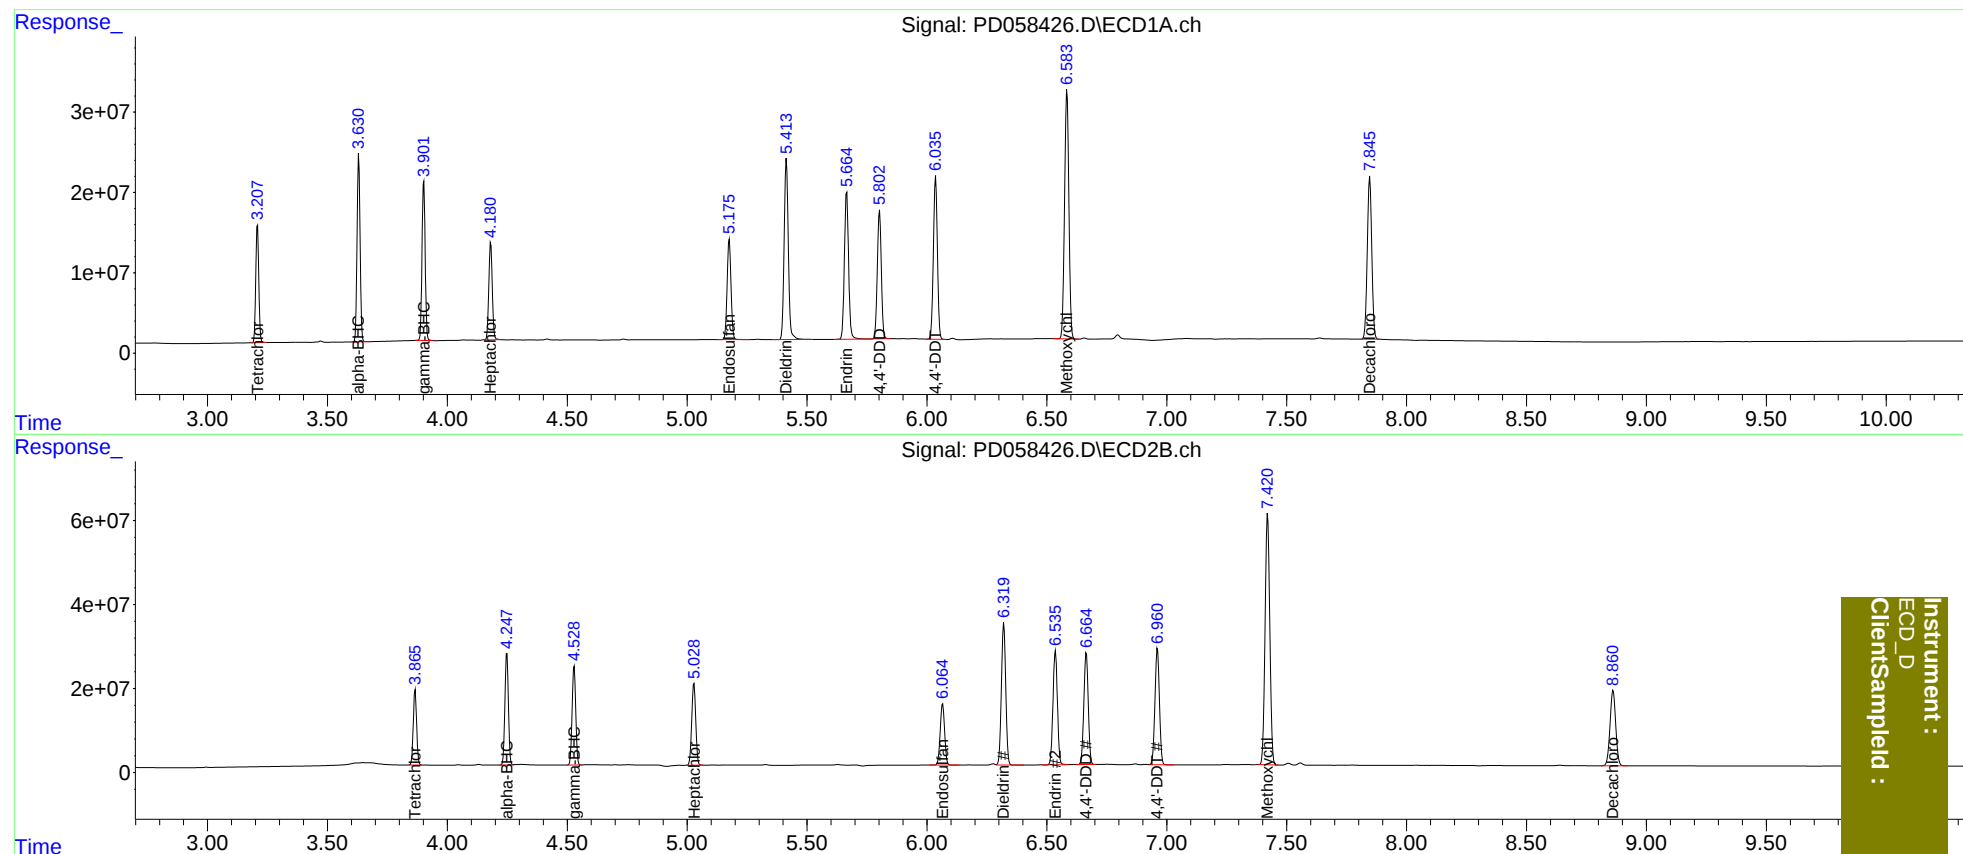


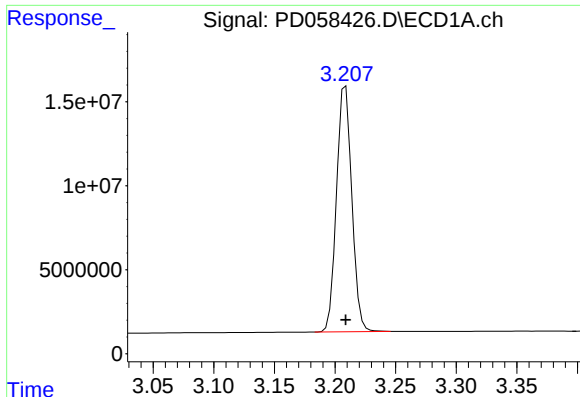

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.000 min
Response: 128540932
Conc: 75.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

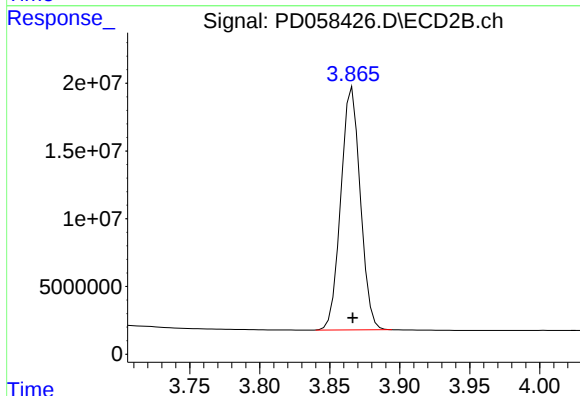


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 173384786
Conc: 74.15 ng/ml

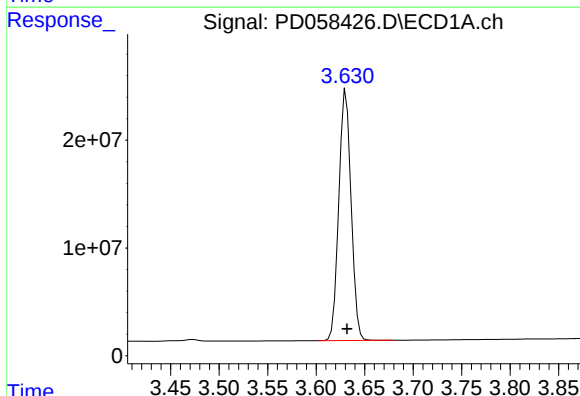


#2 alpha-BHC

R.T.: 3.631 min
Delta R.T.: 0.000 min
Response: 204593755
Conc: 80.87 ng/ml

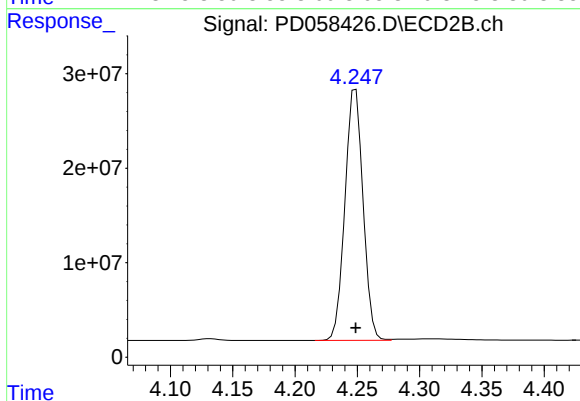

#2 alpha-BHC


R.T.: 4.249 min
Delta R.T.: 0.000 min
Response: 270444172
Conc: 78.00 ng/ml

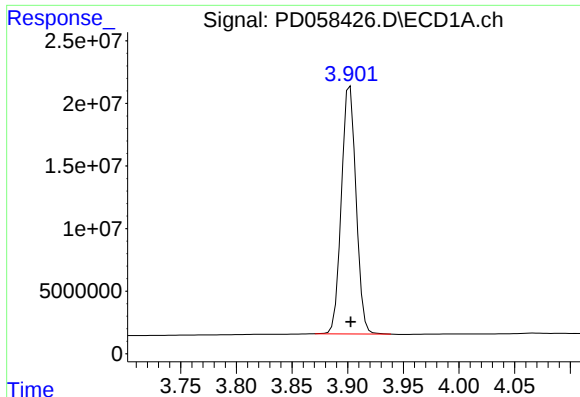

#3 gamma-BHC (Lindane)


R.T.: 3.902 min
Delta R.T.: 0.000 min
Response: 181409816
Conc: 78.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

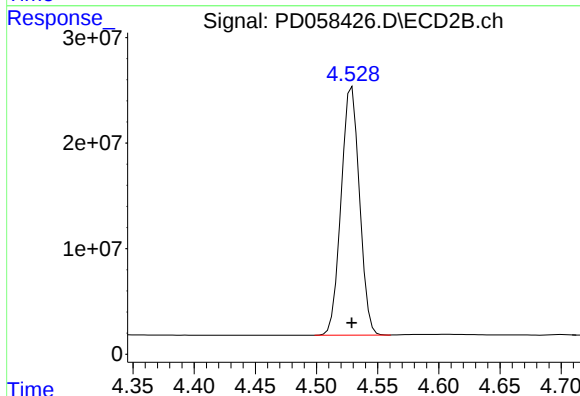


#3 gamma-BHC (Lindane)

R.T.: 4.529 min
Delta R.T.: 0.000 min
Response: 245707820
Conc: 77.26 ng/ml

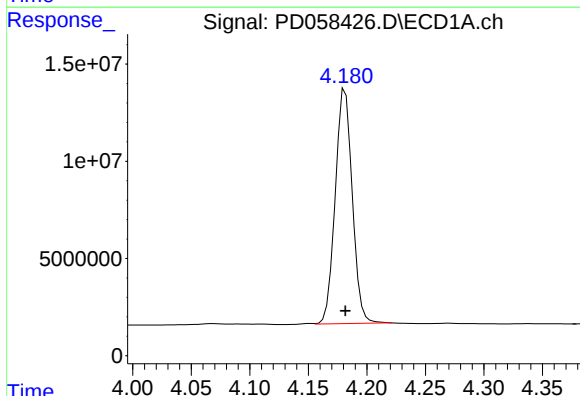


#4 Heptachlor

R.T.: 4.181 min
Delta R.T.: 0.000 min
Response: 122232193
Conc: 76.92 ng/ml

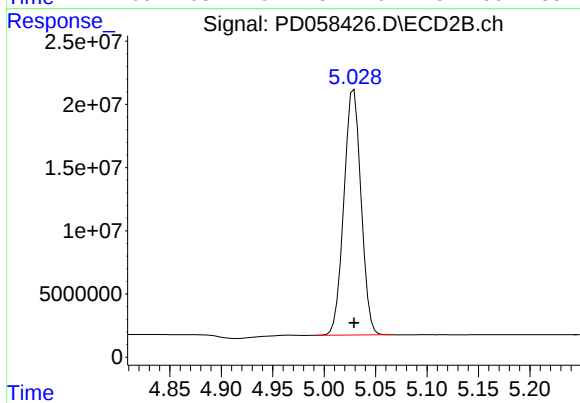

#4 Heptachlor


R.T.: 5.029 min
Delta R.T.: 0.000 min
Response: 226040650
Conc: 76.47 ng/ml

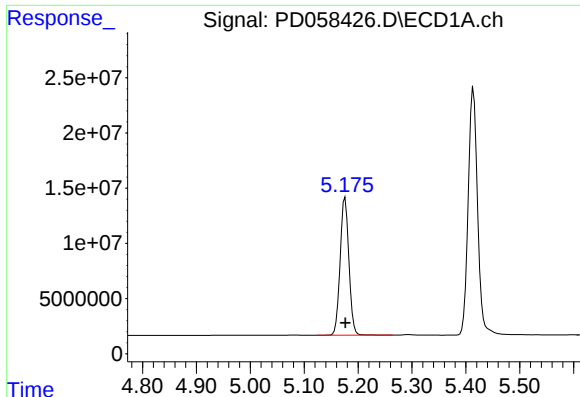

#9 Endosulfan I


R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 140198892
Conc: 77.80 ng/ml

Instrument :
ECD_D
ClientSampleId :

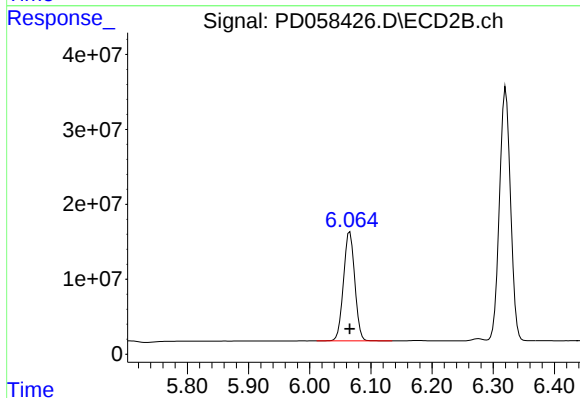


#9 Endosulfan I

R.T.: 6.066 min
Delta R.T.: 0.000 min
Response: 186192353
Conc: 75.16 ng/ml

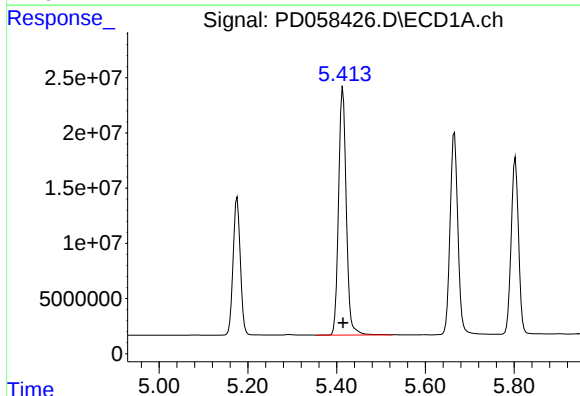


#13 Dieldrin

R.T.: 5.414 min
Delta R.T.: 0.000 min
Response: 270938203
Conc: 155.45 ng/ml

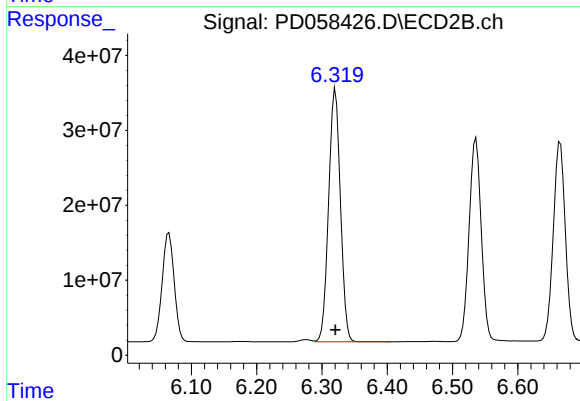

#13 Dieldrin


R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 424139119
Conc: 152.16 ng/ml

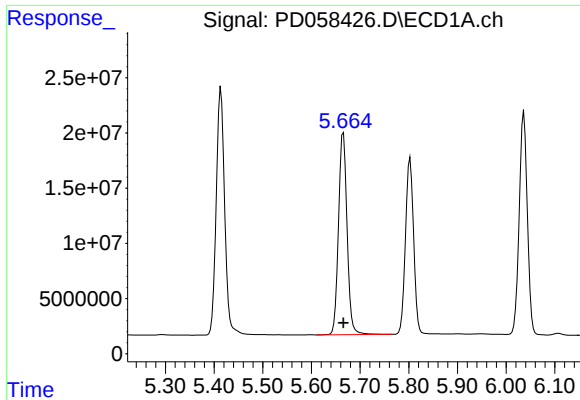

#14 Endrin


R.T.: 5.665 min
Delta R.T.: 0.000 min
Response: 223652869
Conc: 151.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

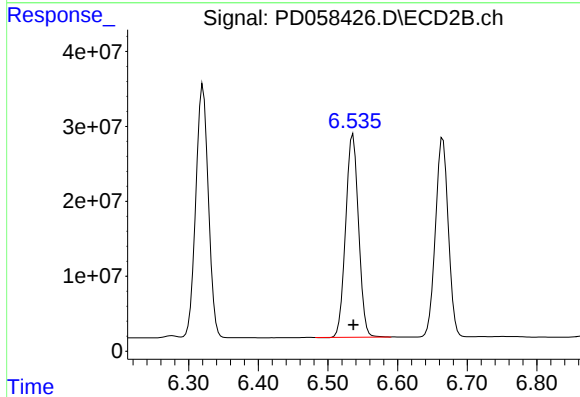


#14 Endrin

R.T.: 6.536 min
Delta R.T.: 0.000 min
Response: 348984240
Conc: 149.31 ng/ml

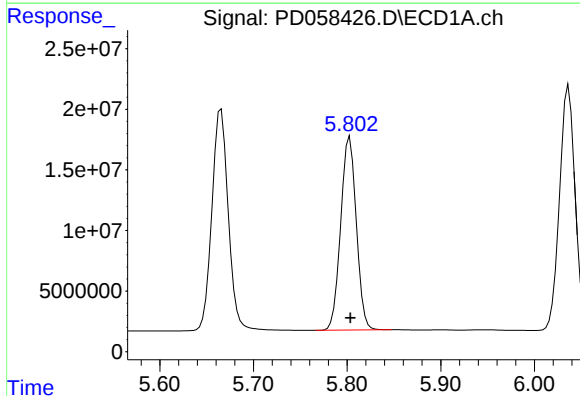


#16 4,4'-DDD

R.T.: 5.803 min
Delta R.T.: 0.000 min
Response: 184826728
Conc: 152.35 ng/ml

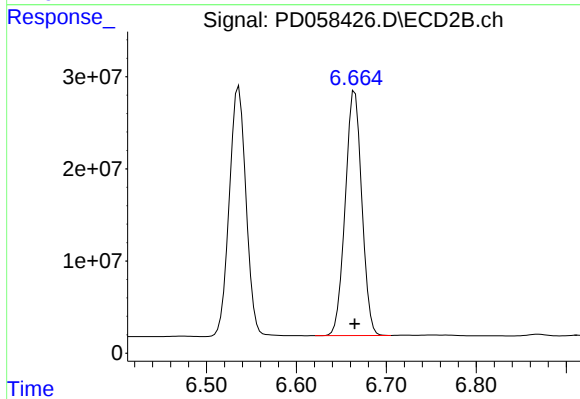

#16 4,4'-DDD


R.T.: 6.665 min
Delta R.T.: 0.000 min
Response: 339887687
Conc: 152.72 ng/ml

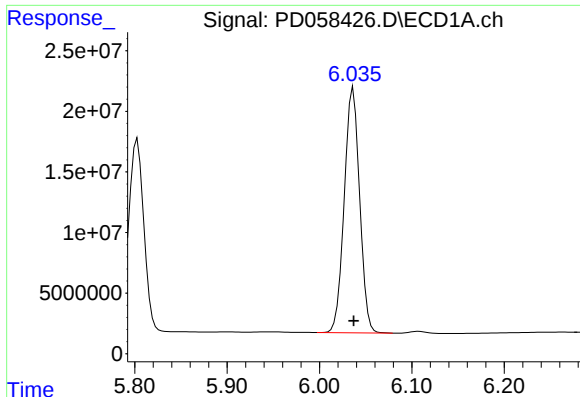

#17 4,4'-DDT


R.T.: 6.036 min
Delta R.T.: 0.000 min
Response: 233905736
Conc: 164.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

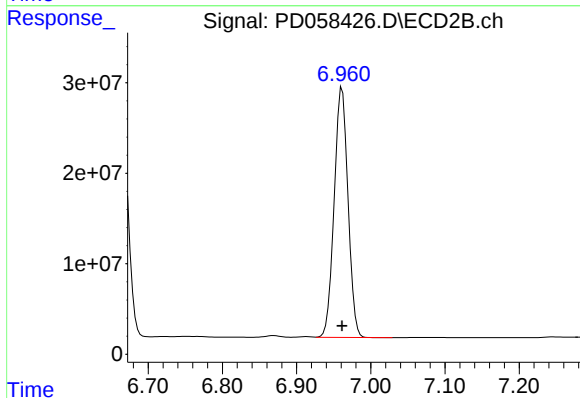


#17 4,4'-DDT

R.T.: 6.961 min
Delta R.T.: 0.000 min
Response: 358049993
Conc: 155.56 ng/ml

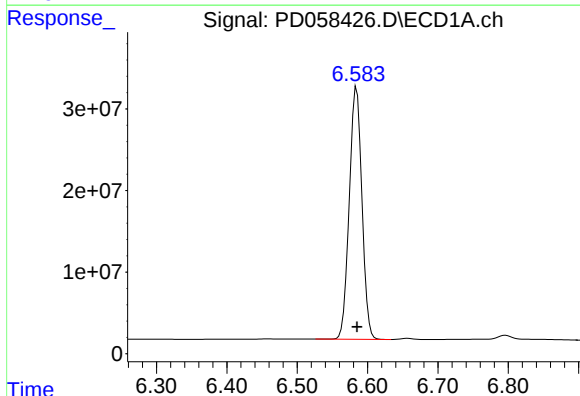


#20 Methoxychlor

R.T.: 6.585 min
Delta R.T.: 0.000 min
Response: 387069600
Conc: 702.08 ng/ml

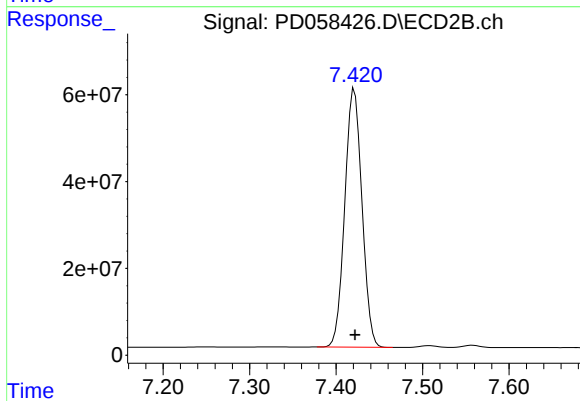

#20 Methoxychlor


R.T.: 7.421 min
Delta R.T.: 0.000 min
Response: 818427688
Conc: 684.38 ng/ml

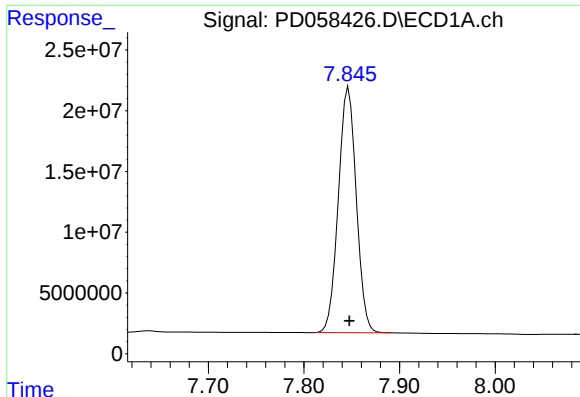

#27 Decachlorobiphenyl

R.T.: 7.847 min
Delta R.T.: -0.001 min
Response: 263510373
Conc: 149.26 ng/ml

Instrument :
ECD_D
ClientSampleId :

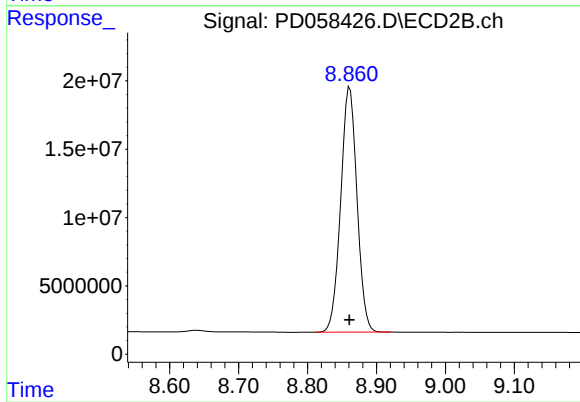

#27 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.000 min
Response: 295040069
Conc: 138.23 ng/ml