

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070318\
 Data File : PD048258.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jul 2018 13:34
 Operator : UA/AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 04 02:23:24 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD062818CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 29 16:27:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

3) MA	gamma-BHC...	4.122	4.633f	1196274	17949630	0.638	0.619
6) B	beta-BHC	4.307f	0.000	1656819	0	2.216	N.D. #
8) B	Heptachlo...	0.000	5.859	0	400.6E6	N.D.	15.605
9) A	Endosulfan I	0.000	6.270f	0	15407734	N.D.	0.655
14) MA	Endrin	0.000	6.763f	0	135.3E6	N.D.	6.852
16) A	4,4'-DDD	0.000	6.763f	0	135.3E6	N.D.	7.210
19) B	Endosulfa...	0.000	7.187f	0	16457143	N.D.	0.817
20) A	Methoxychlor	0.000	7.570	0	6860099	N.D.	0.810
24)	Toxaphene-3	0.000	7.187	0	16457143	N.D.	32.192
25)	Toxaphene-4	0.000	7.187	0	16457143	N.D.	54.188


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070318\
Data File : PD048258.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jul 2018 13:34
Operator : UA/AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 04 02:23:24 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD062818CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 29 16:27:50 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

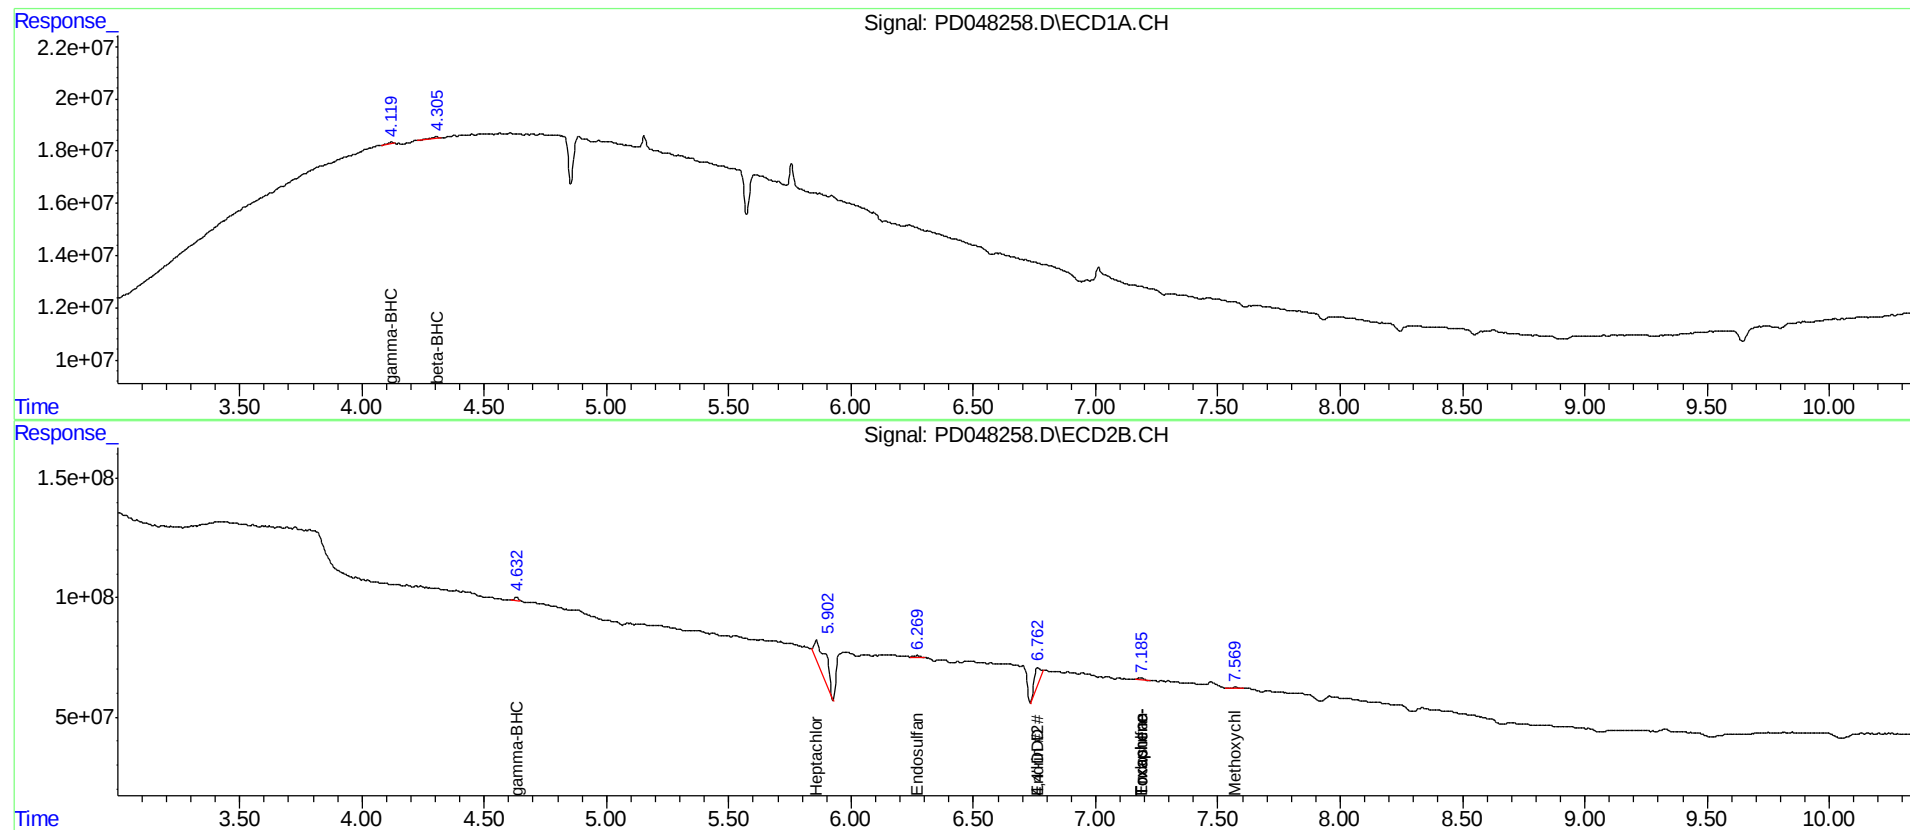


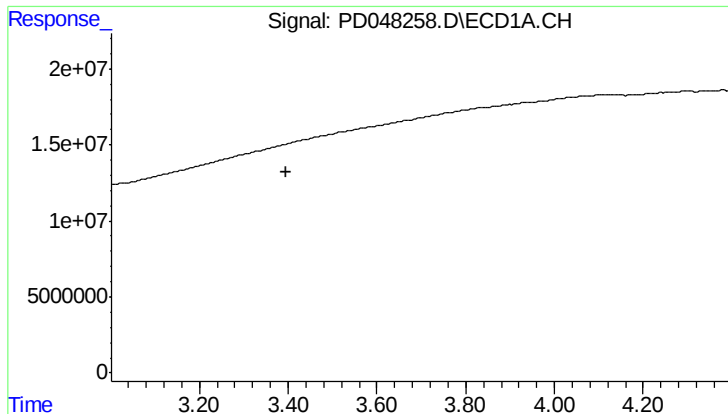

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

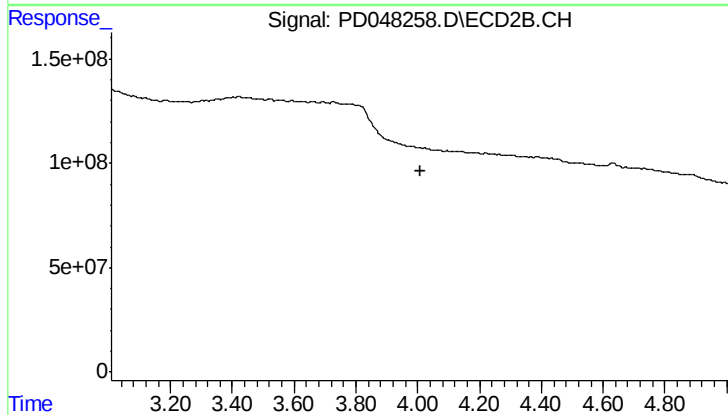


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.007 min
Response: 0
Conc: N.D.

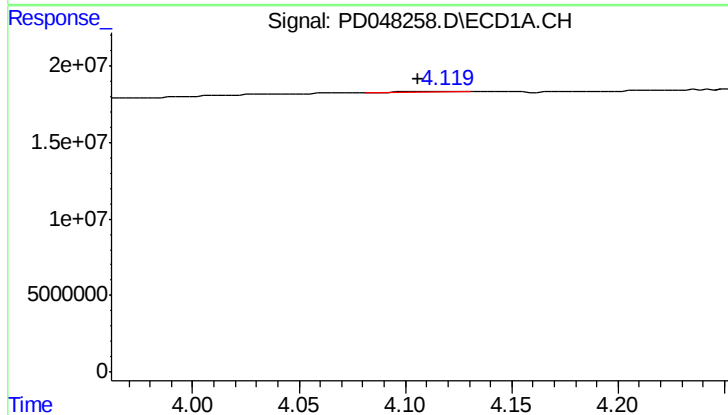


#3 gamma-BHC (Lindane)

R.T.: 4.122 min
Delta R.T.: 0.016 min
Response: 1196274
Conc: 0.64 ng/ml

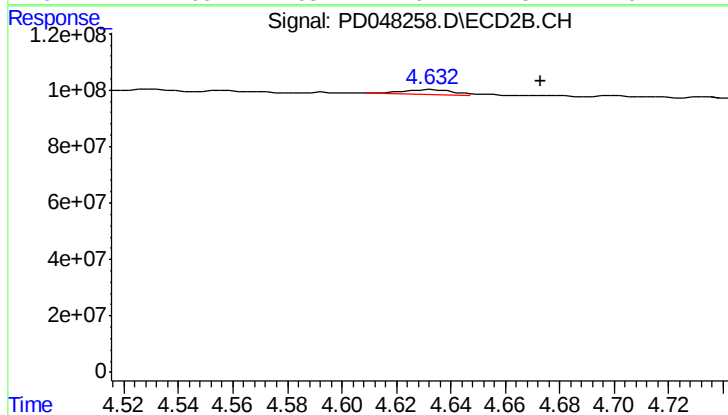

#3 gamma-BHC (Lindane)


R.T.: 4.633 min
Delta R.T.: -0.040 min
Response: 17949630
Conc: 0.62 ng/ml

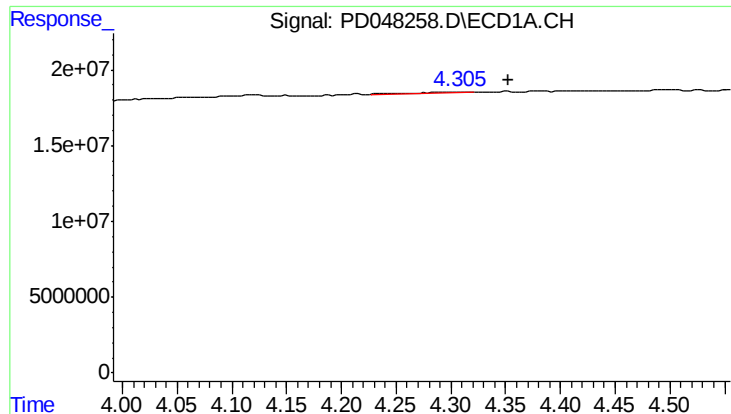

#6 beta-BHC


R.T.: 4.307 min
Delta R.T.: -0.045 min
Response: 1656819
Conc: 2.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

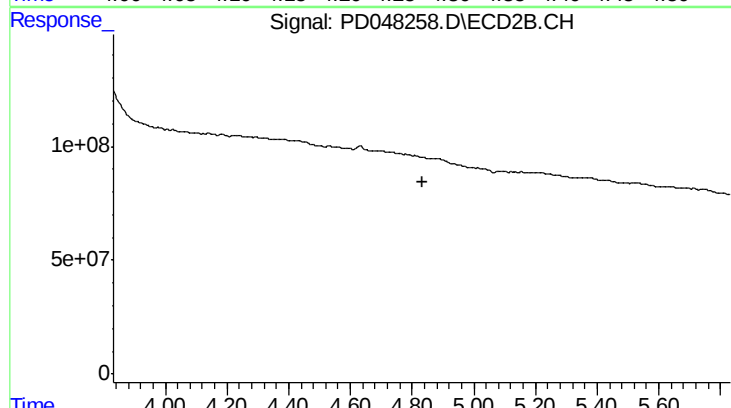


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.832 min
Response: 0
Conc: N.D.

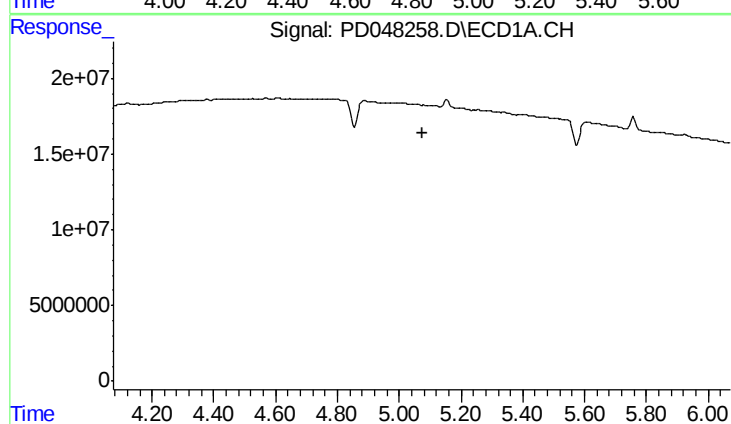


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.075 min
Response: 0
Conc: N.D.

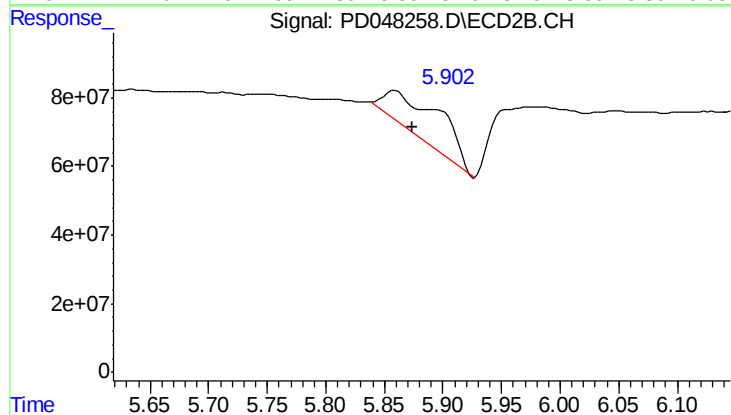

#8 Heptachlor epoxide


R.T.: 5.859 min
Delta R.T.: -0.015 min
Response: 400584595
Conc: 15.61 ng/ml

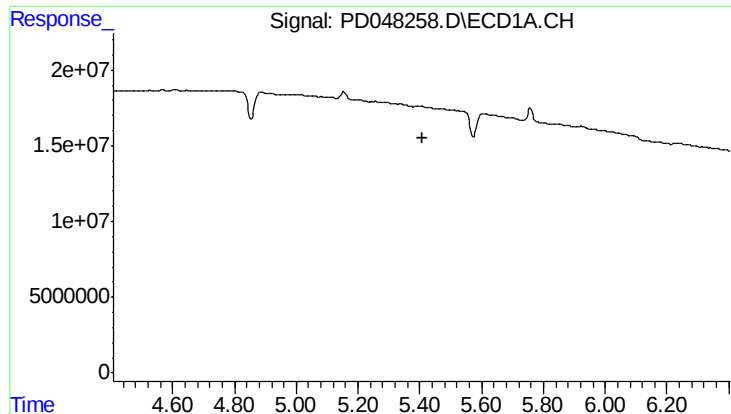

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.408 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

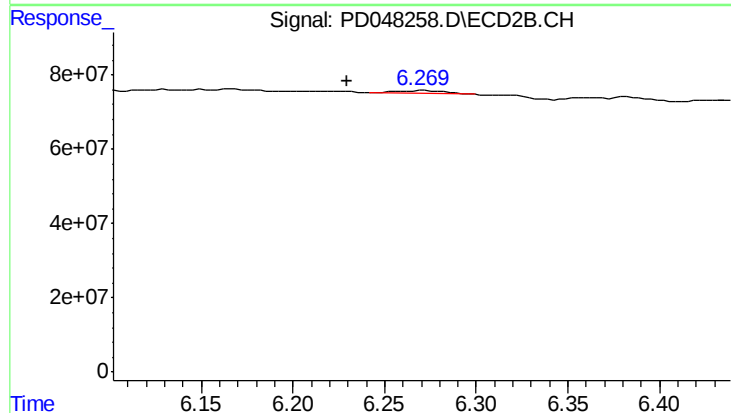


#9 Endosulfan I

R.T.: 6.270 min
Delta R.T.: 0.041 min
Response: 15407734
Conc: 0.65 ng/ml

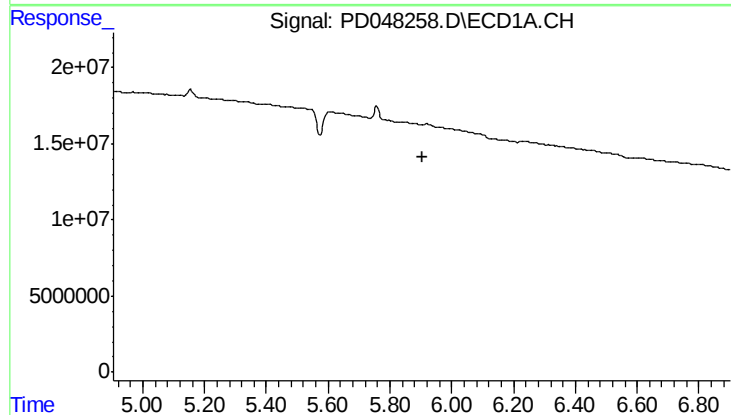


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.904 min
Response: 0
Conc: N.D.

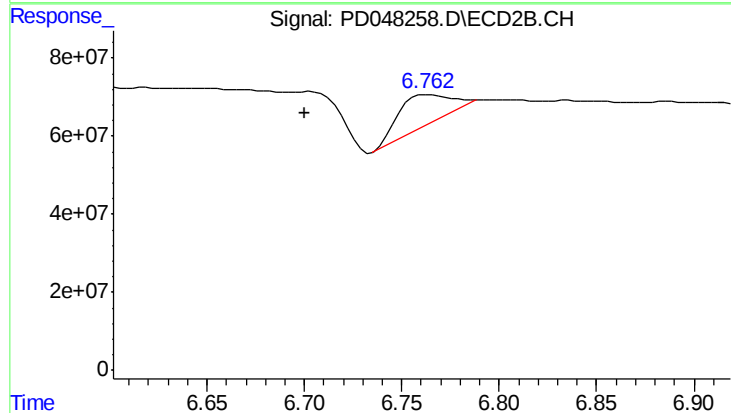

#14 Endrin


R.T.: 6.763 min
Delta R.T.: 0.063 min
Response: 135316884
Conc: 6.85 ng/ml

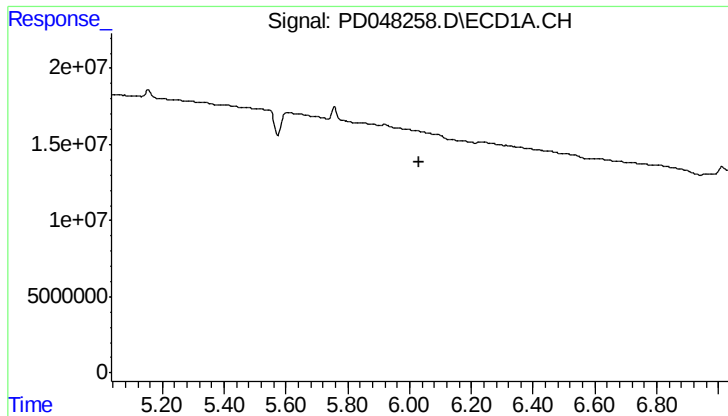

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

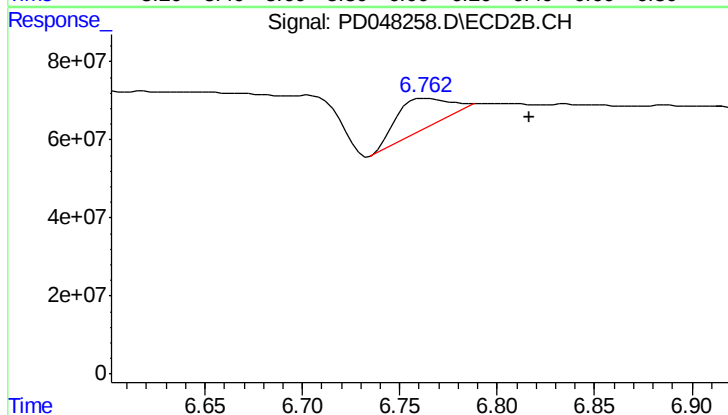


#16 4,4'-DDD

R.T.: 6.763 min
Delta R.T.: -0.053 min
Response: 135316884
Conc: 7.21 ng/ml

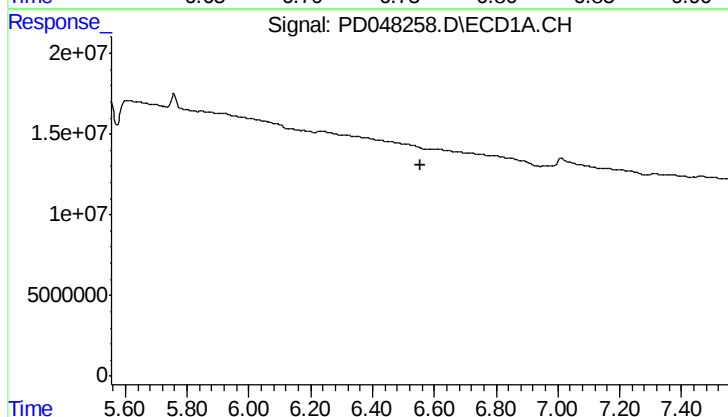


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.554 min
Response: 0
Conc: N.D.

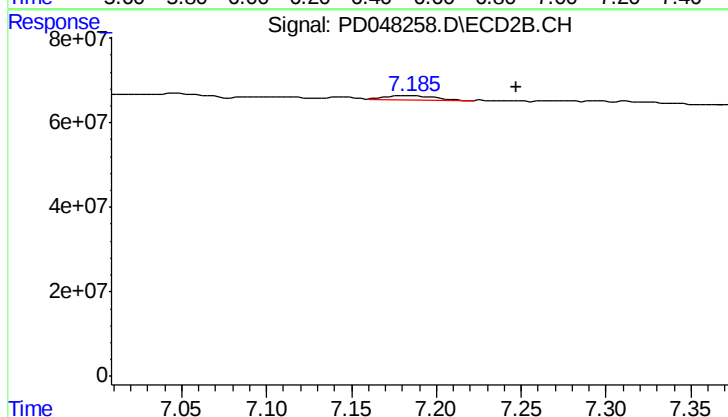

#19 Endosulfan Sulfate


R.T.: 7.187 min
Delta R.T.: -0.060 min
Response: 16457143
Conc: 0.82 ng/ml

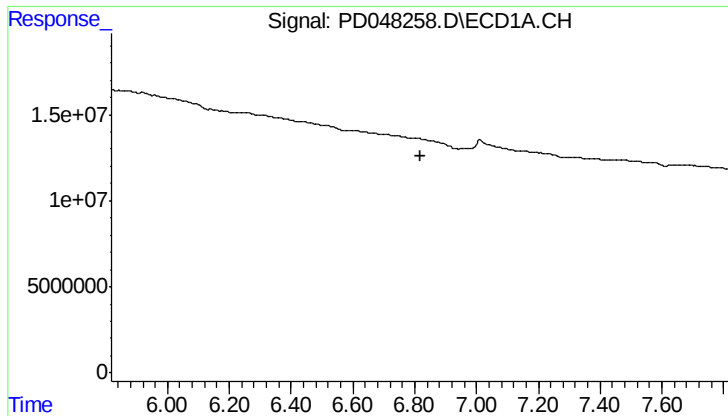

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

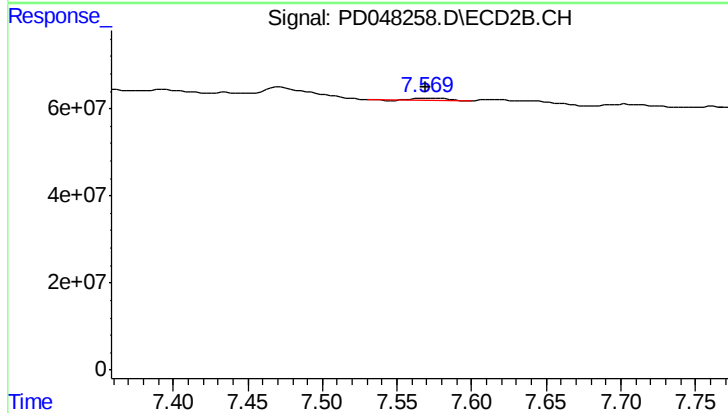


#20 Methoxychlor

R.T.: 7.570 min
Delta R.T.: 0.000 min
Response: 6860099
Conc: 0.81 ng/ml

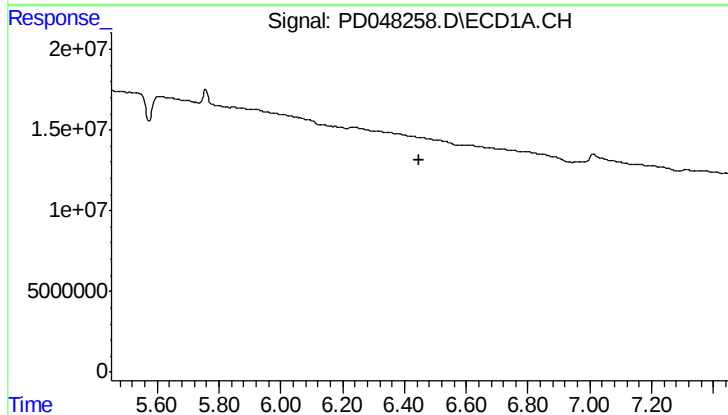


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T.: 6.450 min
Response: 0
Conc: N.D.

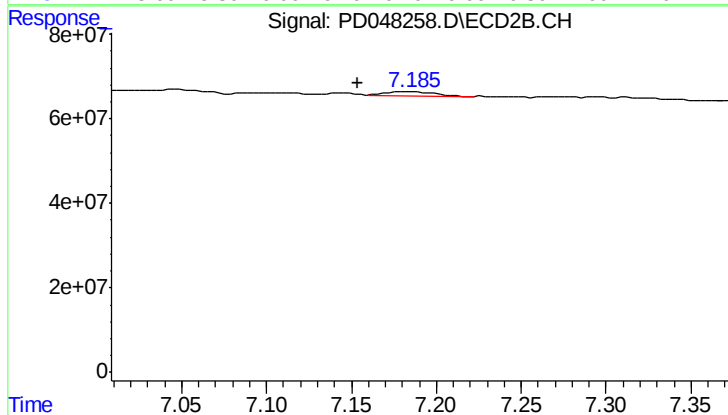

#24 Toxaphene-3


R.T.: 7.187 min
Delta R.T.: 0.033 min
Response: 16457143
Conc: 32.19 ng/ml

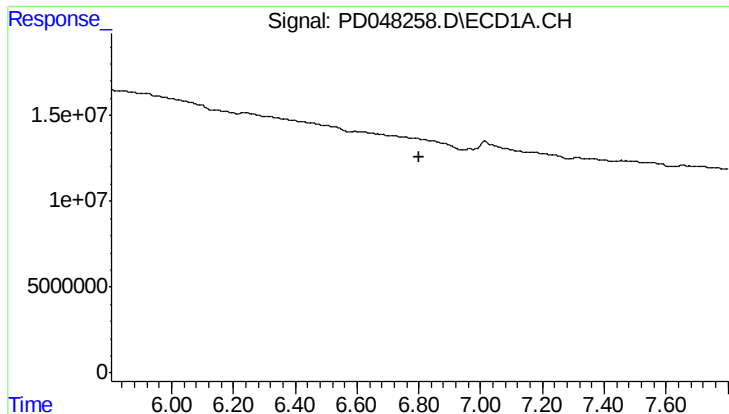

#25 Toxaphene-4


R.T.: 0.000 min
Exp R.T.: 6.802 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

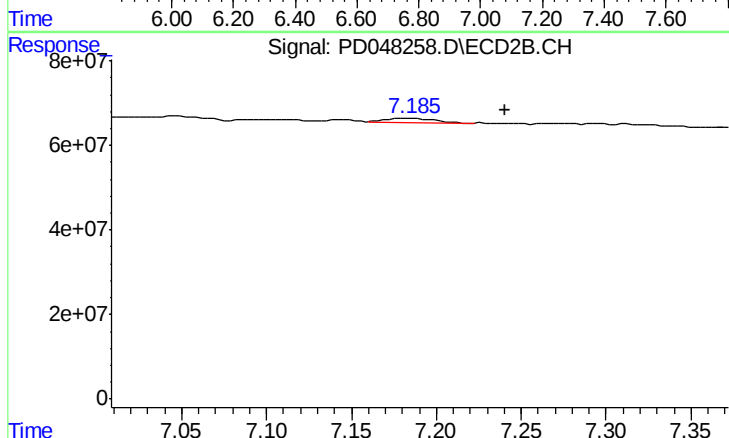


#25 Toxaphene-4

R.T.: 7.187 min
Delta R.T.: -0.054 min
Response: 16457143
Conc: 54.19 ng/ml

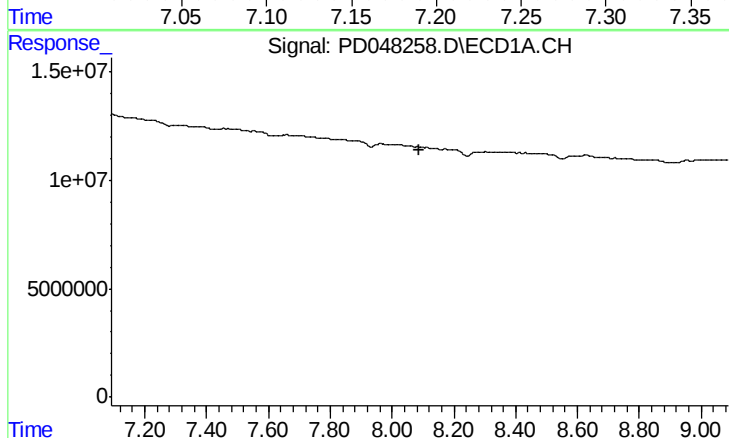

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.089 min
Response: 0
Conc: N.D.

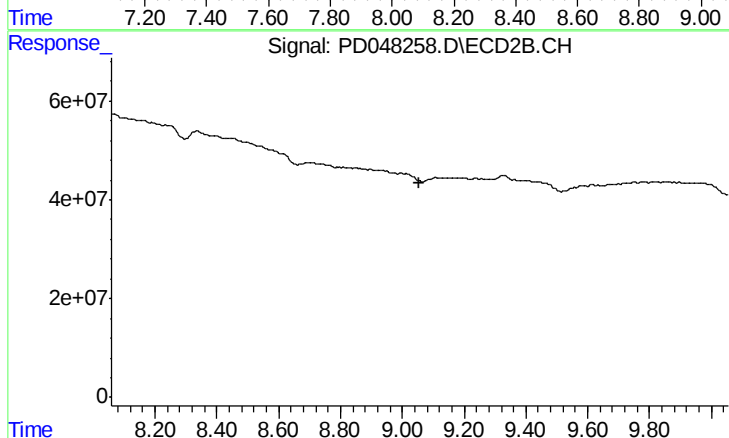

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.056 min
Response: 0
Conc: N.D.