

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070423\
 Data File : PD076310.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jul 2023 13:45
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 04 14:37:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070423.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 04 14:37:22 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.765	164.0E6	92504778	74.596	74.750
28)	SA Decachlor...	9.083	7.908	169.2E6	61204994	74.788	74.196
Target Compounds							
23)	Chlordane-1	4.709	3.763	88654575	33155490	745.759	748.017
24)	Chlordane-2	5.241	4.339	92116078	34452690	741.593	734.500
25)	Chlordane-3	5.952	4.970	391.5E6	106.9E6	743.614	743.102
26)	Chlordane-4	6.034	5.033	469.2E6	108.5E6	742.844	759.677
27)	Chlordane-5	6.886	5.929	74707395	36656542	737.701	746.670



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070423\
Data File : PD076310.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jul 2023 13:45
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 04 14:37:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070423.M
Quant Title : GC Extractables
QLast Update : Tue Jul 04 14:37:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

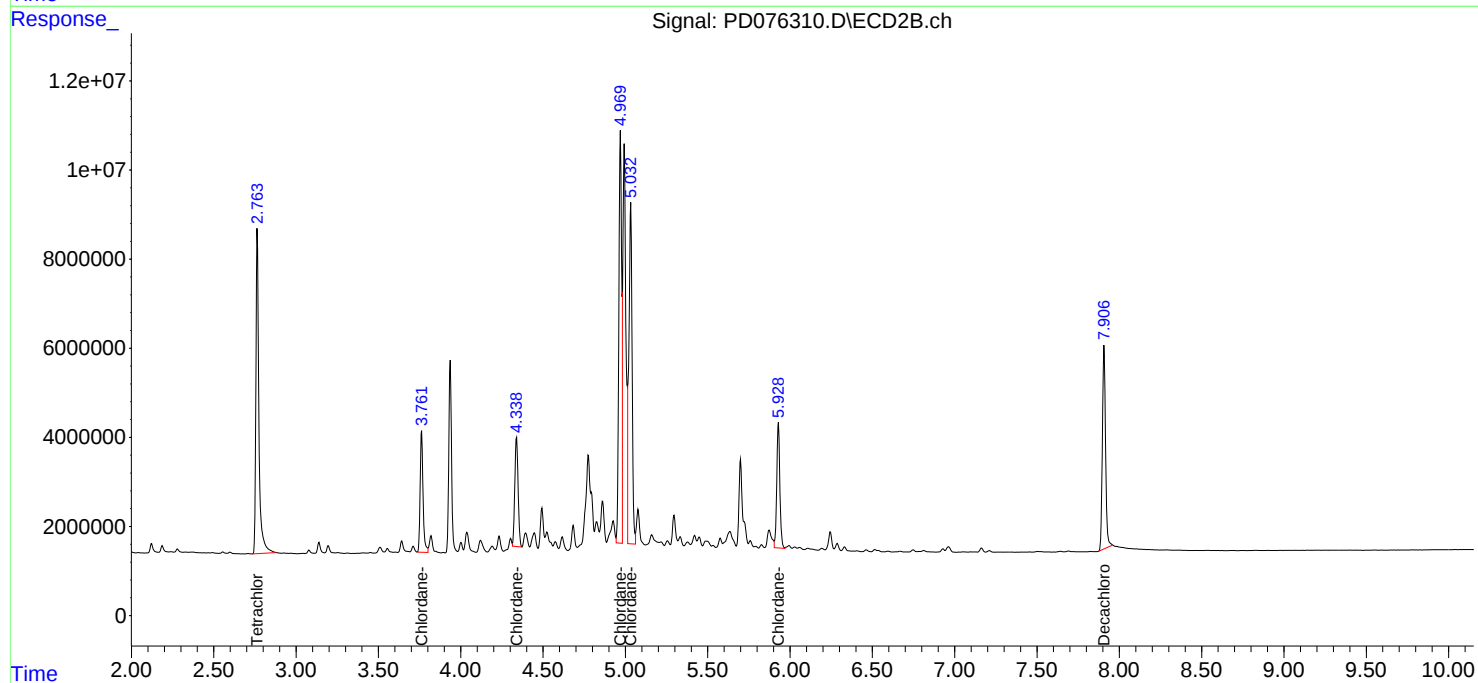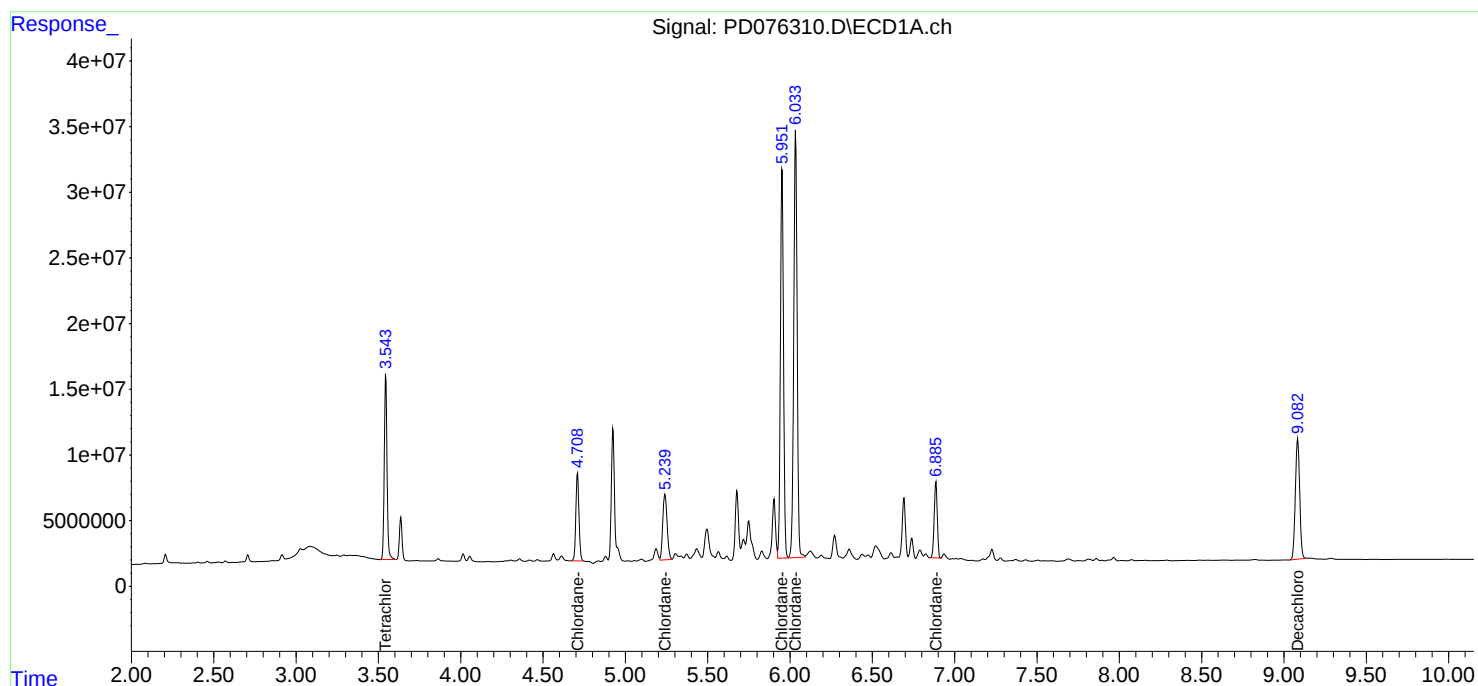


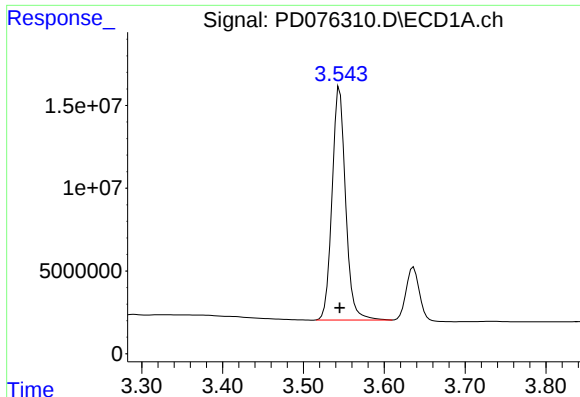

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 164002169
Conc: 74.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

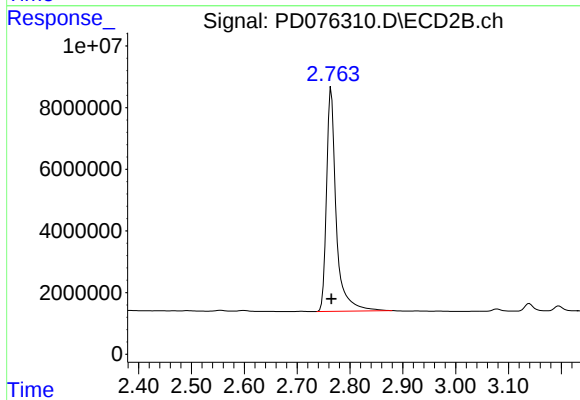


#1 Tetrachloro-m-xylene

R.T.: 2.765 min
Delta R.T.: 0.000 min
Response: 92504778
Conc: 74.75 ng/ml

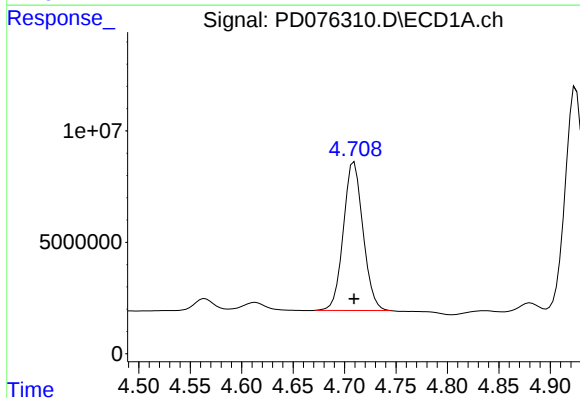


#23 Chlordane-1

R.T.: 4.709 min
Delta R.T.: 0.000 min
Response: 88654575
Conc: 745.76 ng/ml

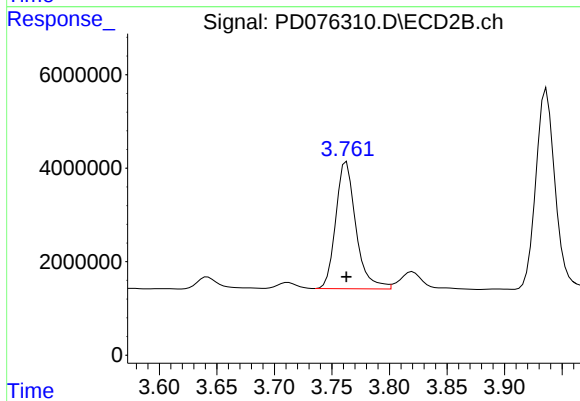

#23 Chlordane-1


R.T.: 3.763 min
Delta R.T.: 0.000 min
Response: 33155490
Conc: 748.02 ng/ml

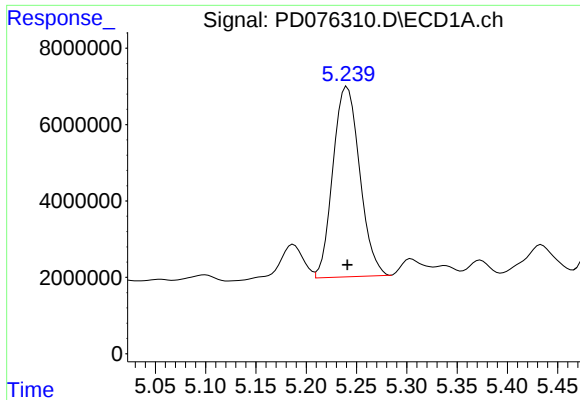

#24 Chlordane-2


R.T.: 5.241 min
Delta R.T.: 0.000 min
Response: 92116078
Conc: 741.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

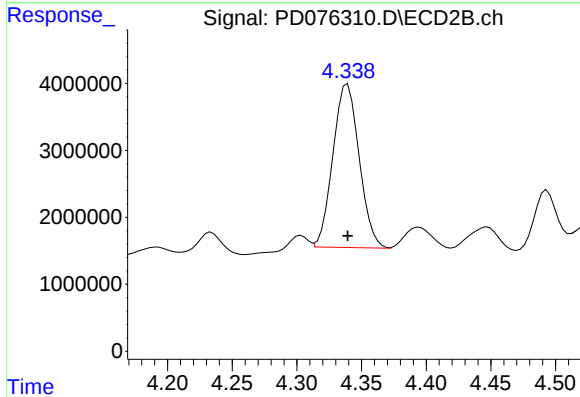


#24 Chlordane-2

R.T.: 4.339 min
Delta R.T.: 0.000 min
Response: 34452690
Conc: 734.50 ng/ml

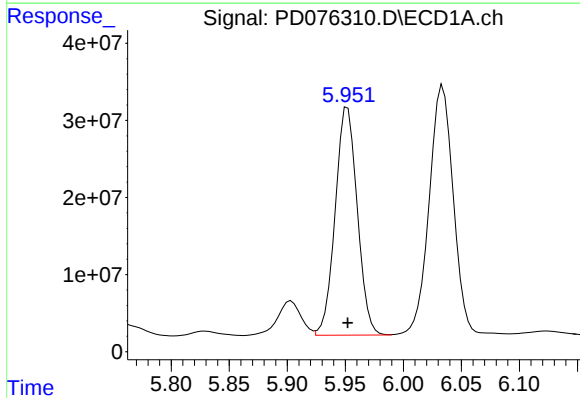


#25 Chlordane-3

R.T.: 5.952 min
Delta R.T.: 0.000 min
Response: 391543765
Conc: 743.61 ng/ml

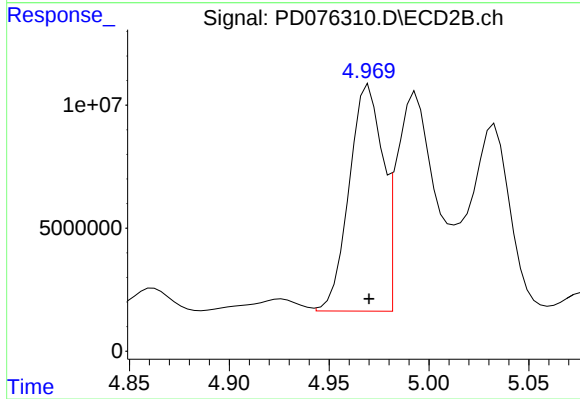

#25 Chlordane-3


R.T.: 4.970 min
Delta R.T.: 0.000 min
Response: 106859023
Conc: 743.10 ng/ml

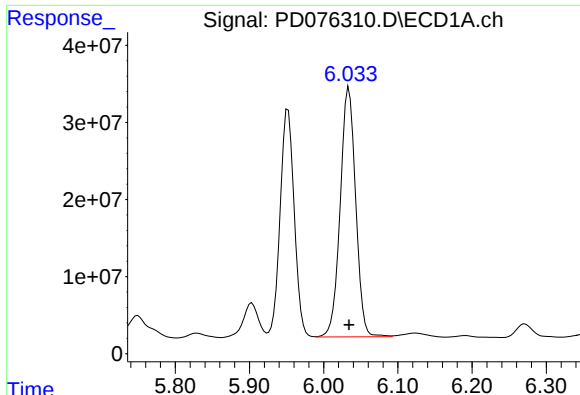

#26 Chlordane-4


R.T.: 6.034 min
Delta R.T.: 0.000 min
Response: 469233643
Conc: 742.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

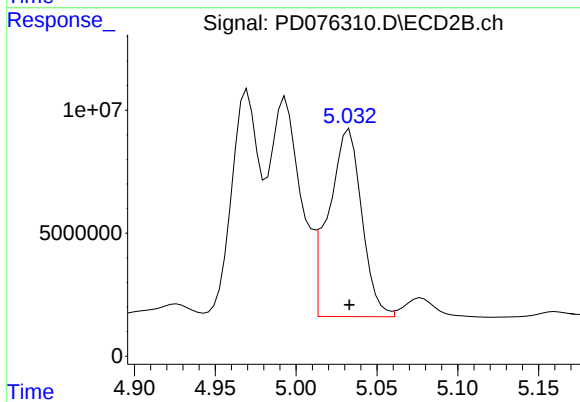


#26 Chlordane-4

R.T.: 5.033 min
Delta R.T.: 0.000 min
Response: 108513042
Conc: 759.68 ng/ml

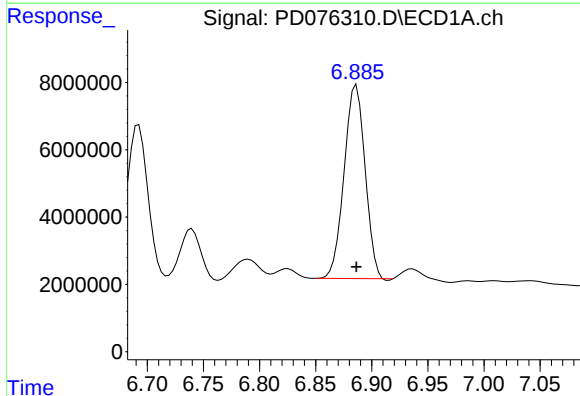


#27 Chlordane-5

R.T.: 6.886 min
Delta R.T.: 0.000 min
Response: 74707395
Conc: 737.70 ng/ml

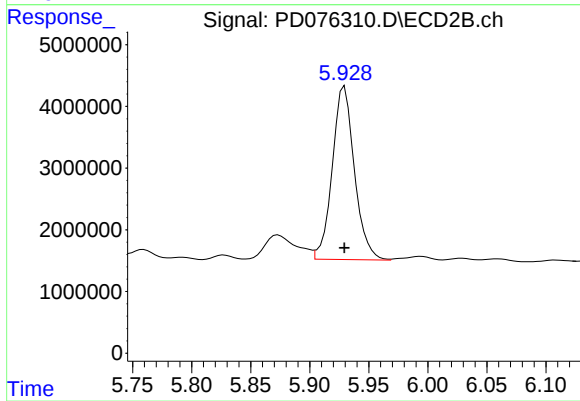

#27 Chlordane-5

R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 36656542
Conc: 746.67 ng/ml

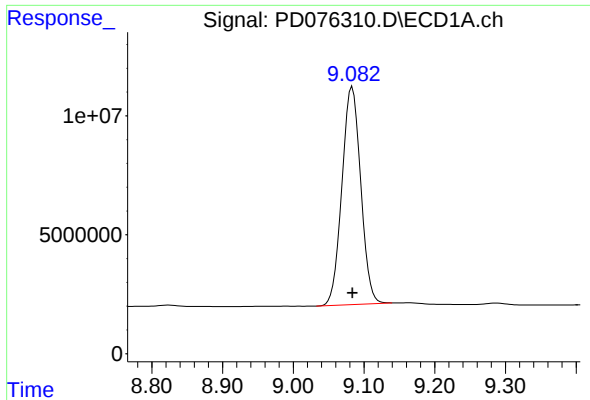

#28 Decachlorobiphenyl


R.T.: 9.083 min

Delta R.T.: 0.000 min

Response: 169249694

Conc: 74.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

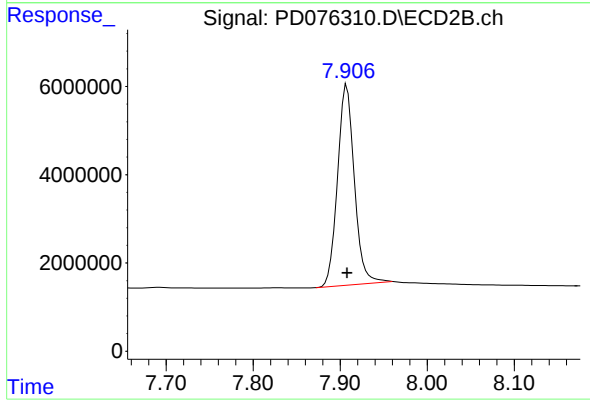

#28 Decachlorobiphenyl

R.T.: 7.908 min

Delta R.T.: 0.000 min

Response: 61204994

Conc: 74.20 ng/ml