

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070423\
 Data File : PD076311.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jul 2023 13:58
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 04 14:33:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070423.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 04 14:30:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.765	109.1E6	60982063	50.000	50.000
28)	SA Decachlor...	9.083	7.907	115.1E6	41862679	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.710	3.763	58140300	22004734	500.000	500.000
24)	Chlordane-2	5.240	4.339	63058161	23780338	500.000	500.000
25)	Chlordane-3	5.952	4.969	256.9E6	70545287	500.000	500.000
26)	Chlordane-4	6.035	5.033	310.4E6	69436383	500.000	500.000
27)	Chlordane-5	6.886	5.929	50377454	24181129	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070423\
Data File : PD076311.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jul 2023 13:58
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 04 14:33:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070423.M
Quant Title : GC Extractables
QLast Update : Tue Jul 04 14:30:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

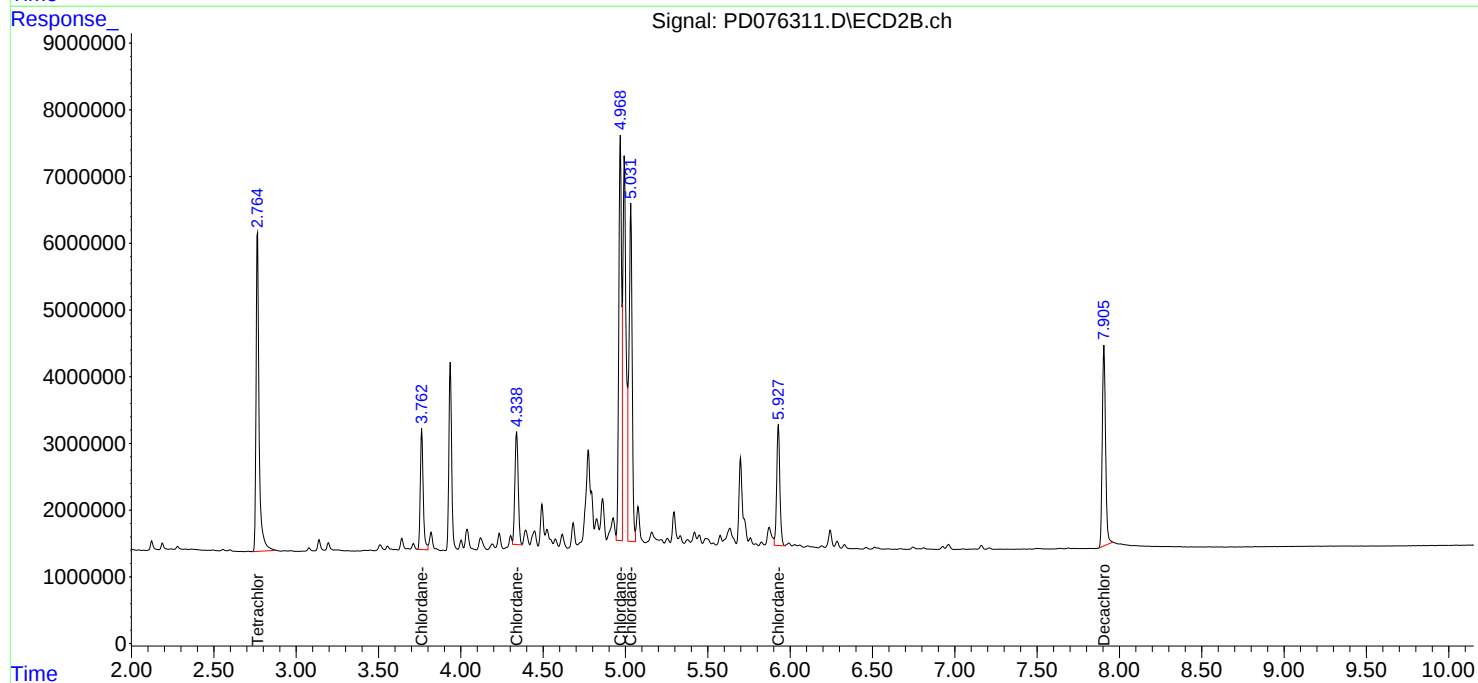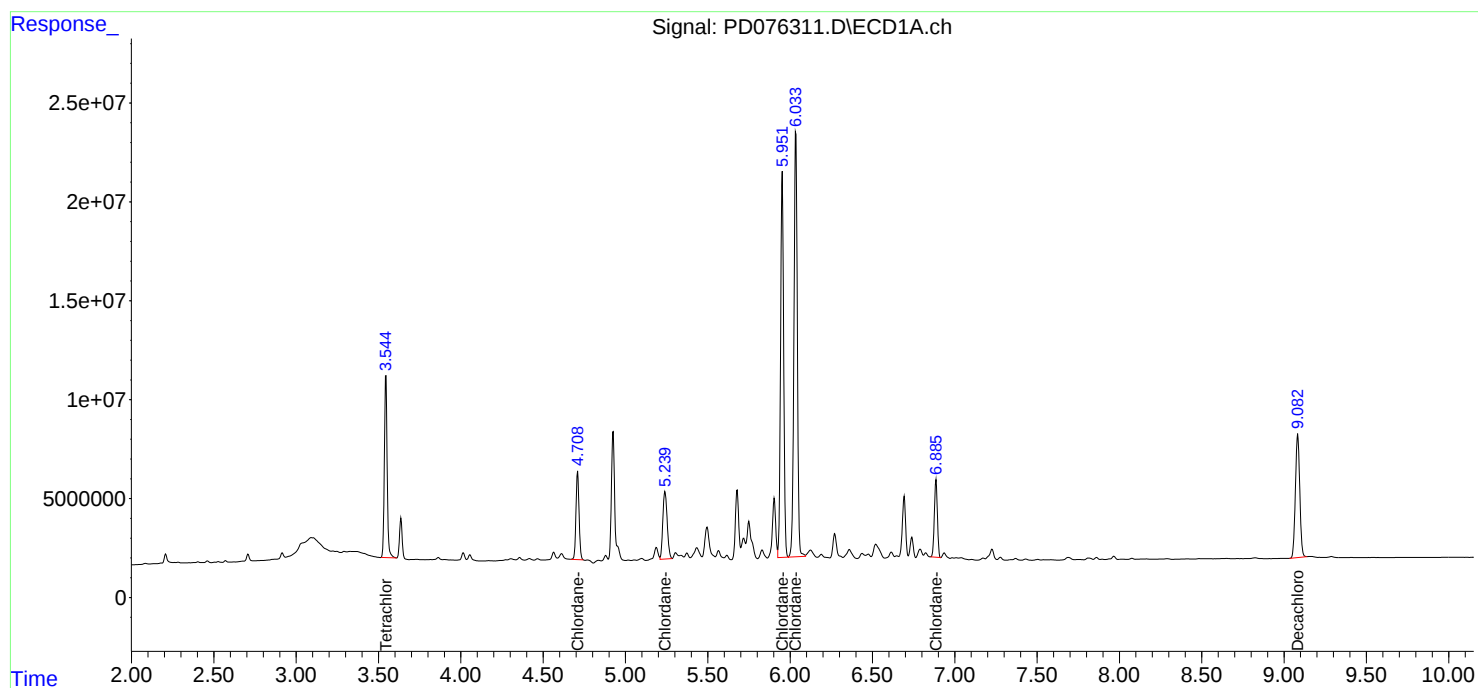


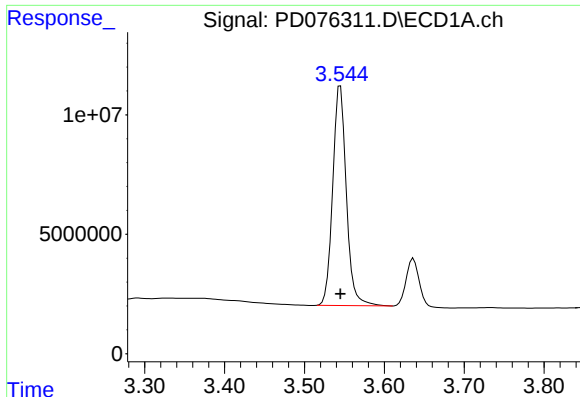

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 109109547
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

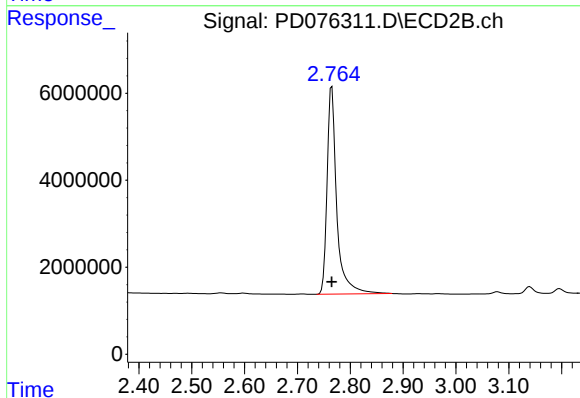


#1 Tetrachloro-m-xylene

R.T.: 2.765 min
Delta R.T.: 0.000 min
Response: 60982063
Conc: 50.00 ng/ml

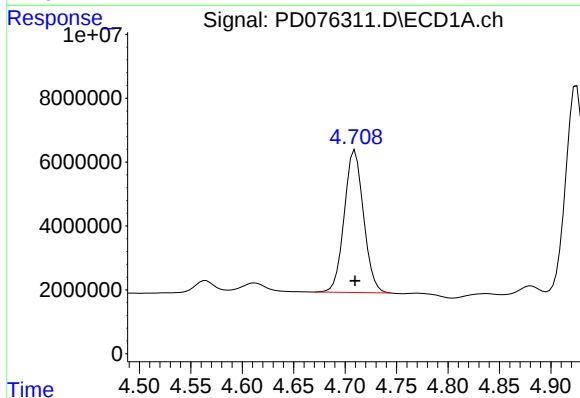


#23 Chlordane-1

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 58140300
Conc: 500.00 ng/ml

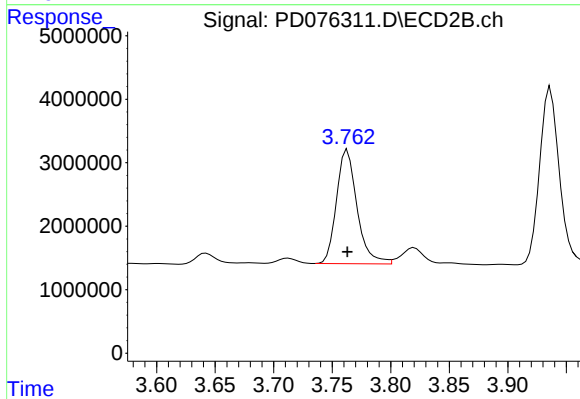

#23 Chlordane-1


R.T.: 3.763 min
Delta R.T.: 0.000 min
Response: 22004734
Conc: 500.00 ng/ml

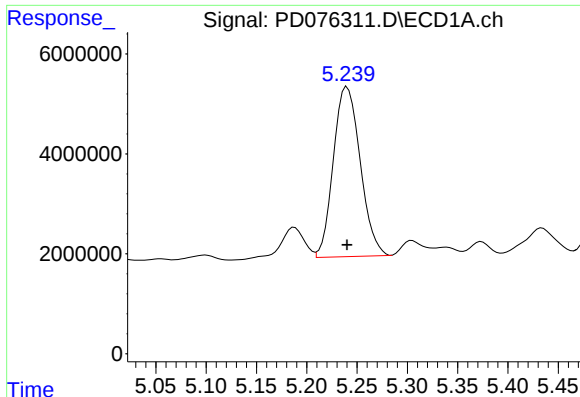

#24 Chlordane-2


R.T.: 5.240 min
Delta R.T.: 0.000 min
Response: 63058161
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

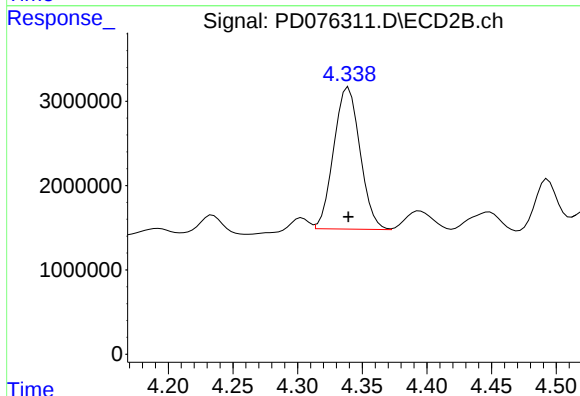


#24 Chlordane-2

R.T.: 4.339 min
Delta R.T.: 0.000 min
Response: 23780338
Conc: 500.00 ng/ml

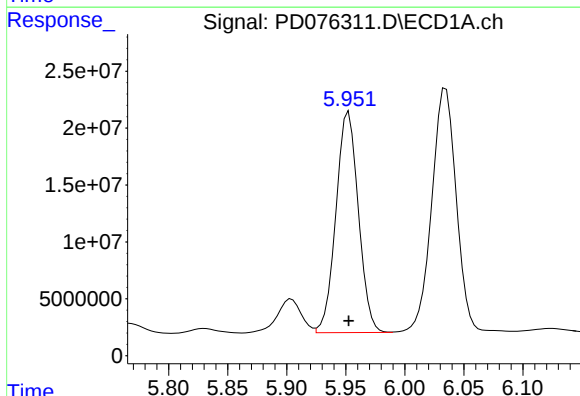


#25 Chlordane-3

R.T.: 5.952 min
Delta R.T.: 0.000 min
Response: 256891788
Conc: 500.00 ng/ml

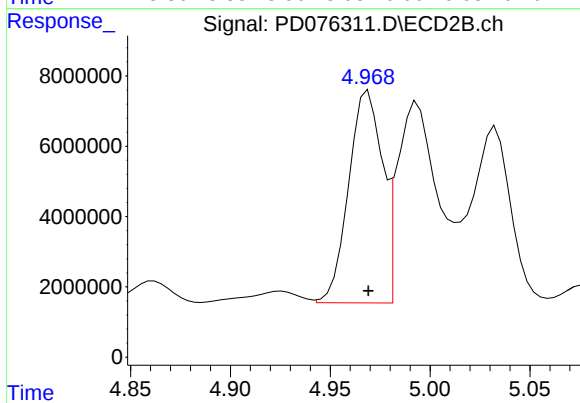

#25 Chlordane-3


R.T.: 4.969 min
Delta R.T.: 0.000 min
Response: 70545287
Conc: 500.00 ng/ml

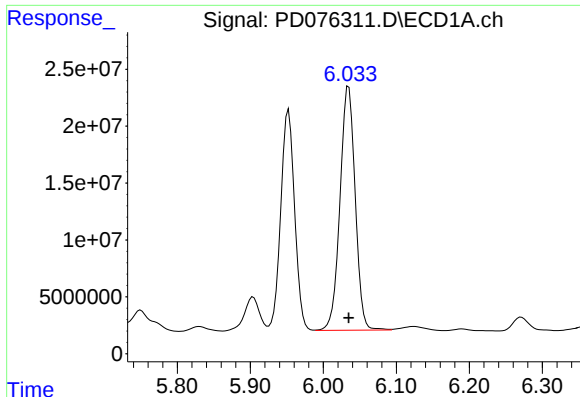

#26 Chlordane-4


R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 310375935
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

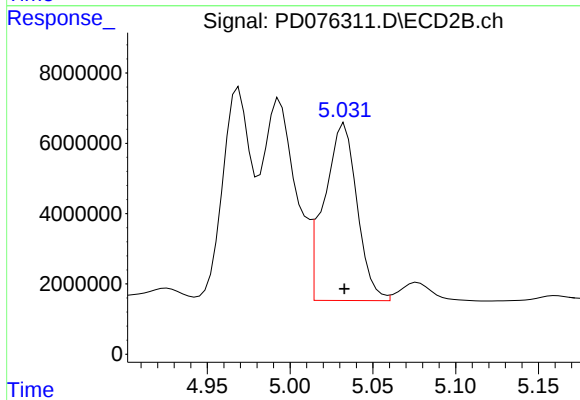


#26 Chlordane-4

R.T.: 5.033 min
Delta R.T.: 0.000 min
Response: 69436383
Conc: 500.00 ng/ml

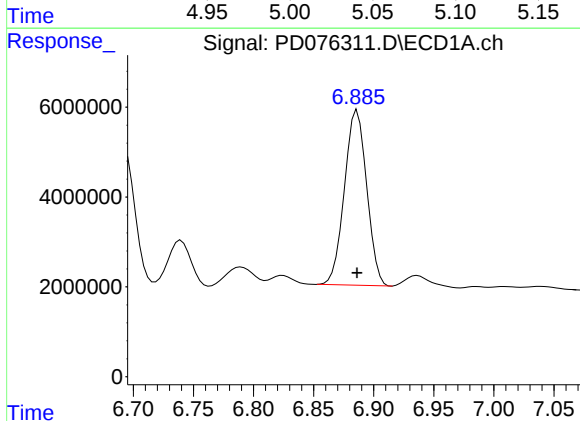


#27 Chlordane-5

R.T.: 6.886 min
Delta R.T.: 0.000 min
Response: 50377454
Conc: 500.00 ng/ml

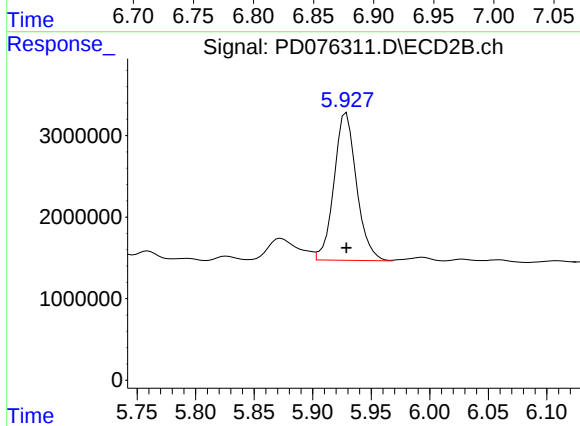

#27 Chlordane-5


R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 24181129
Conc: 500.00 ng/ml

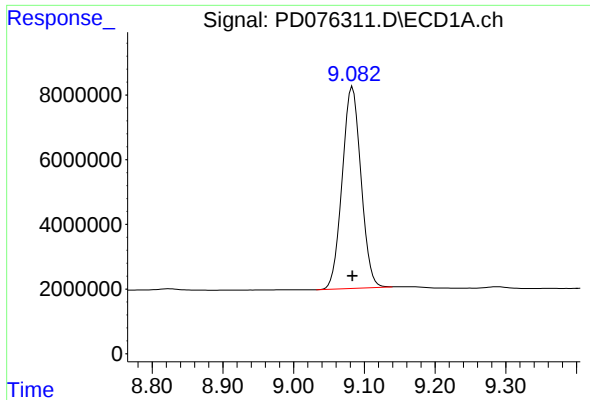

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 115145277
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

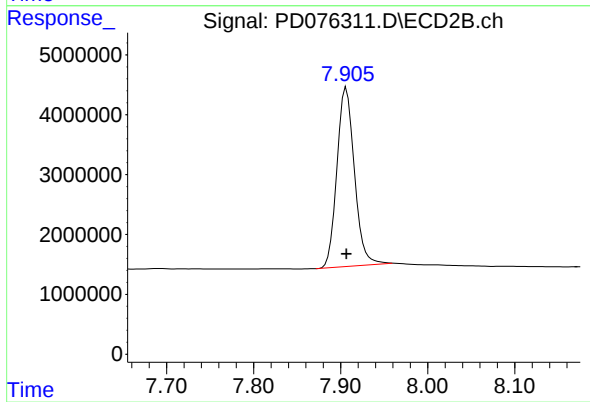

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 41862679
Conc: 50.00 ng/ml