

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070423\
 Data File : PD076312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jul 2023 14:12
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 04 14:38:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070423.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 04 14:38:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.765	53897353	30028601	24.635	24.445
28)	SA Decachlor...	9.083	7.907	60731573	21703021	26.352	25.970
Target Compounds							
23)	Chlordane-1	4.710	3.763	28472155	11137945	242.047	250.960
24)	Chlordane-2	5.240	4.339	32434464	12808519	258.247	266.909
25)	Chlordane-3	5.953	4.970	122.1E6	34285237	236.098	241.214
26)	Chlordane-4	6.035	5.033	149.6E6	34512708	240.052	243.659
27)	Chlordane-5	6.887	5.929	23839248	11793637	238.889	242.599



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070423\
Data File : PD076312.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jul 2023 14:12
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 04 14:38:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070423.M
Quant Title : GC Extractables
QLast Update : Tue Jul 04 14:38:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

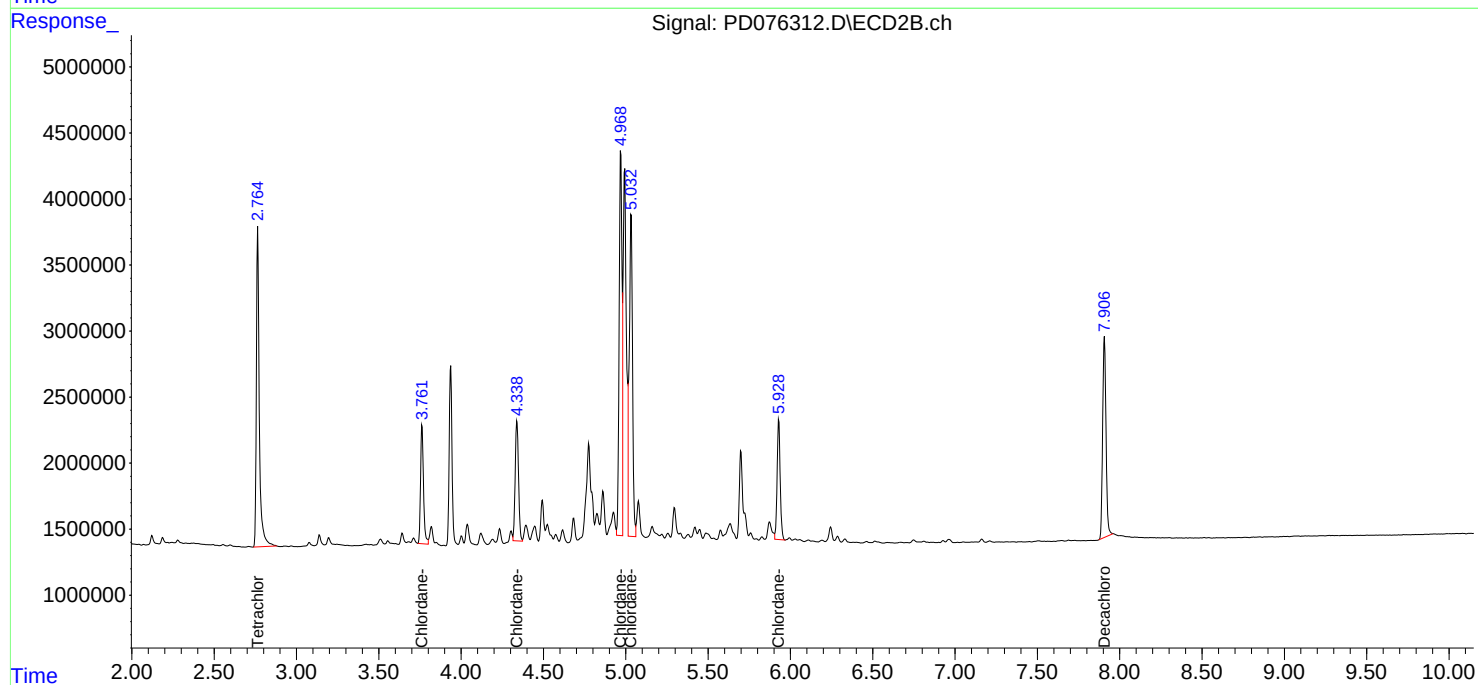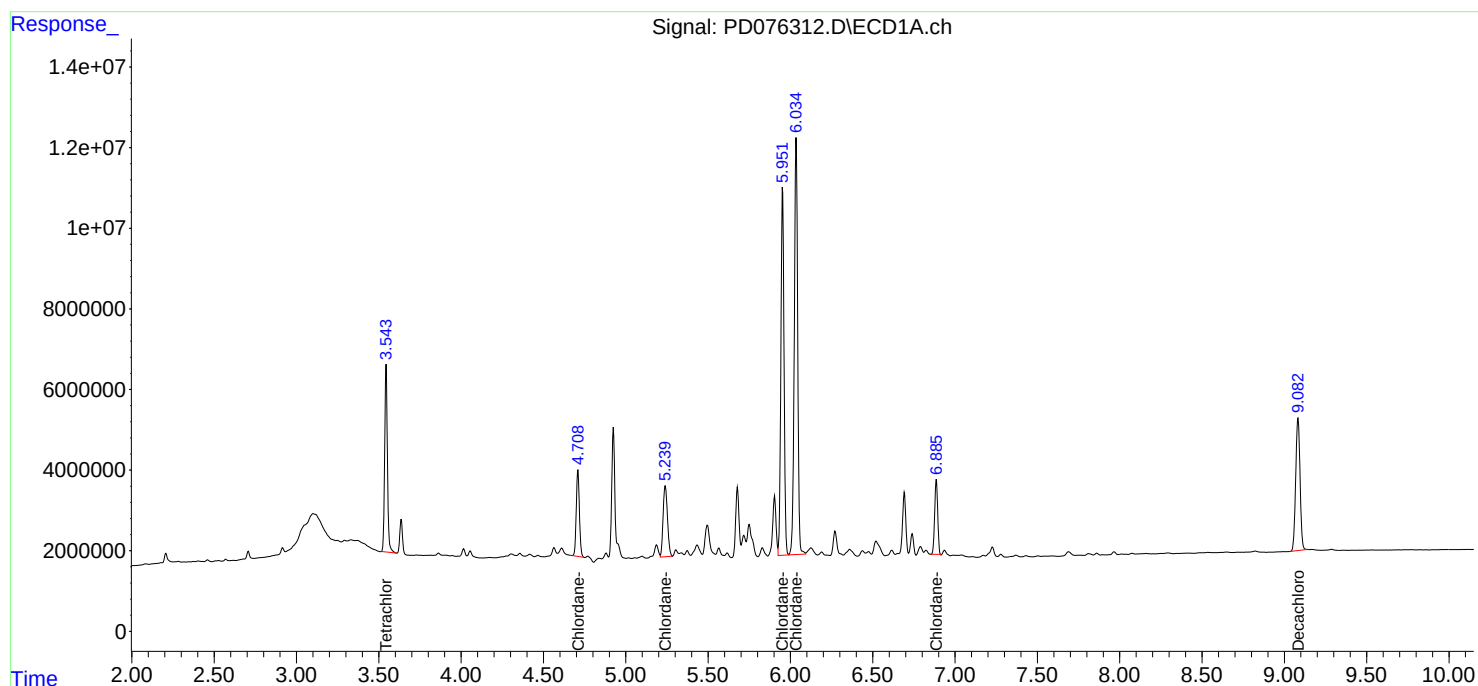


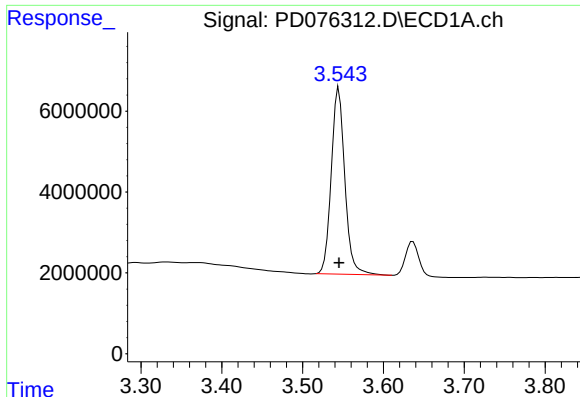

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 53897353
Conc: 24.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

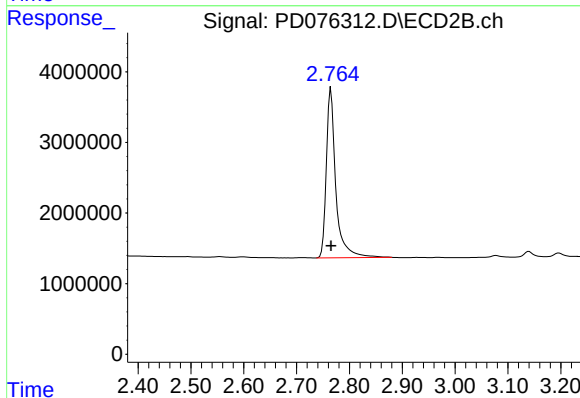


#1 Tetrachloro-m-xylene

R.T.: 2.765 min
Delta R.T.: 0.000 min
Response: 30028601
Conc: 24.44 ng/ml

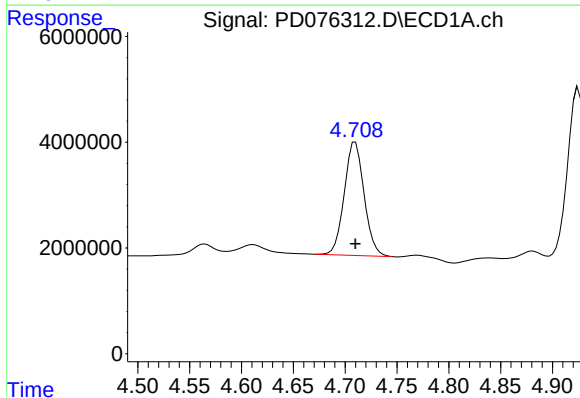


#23 Chlordane-1

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 28472155
Conc: 242.05 ng/ml

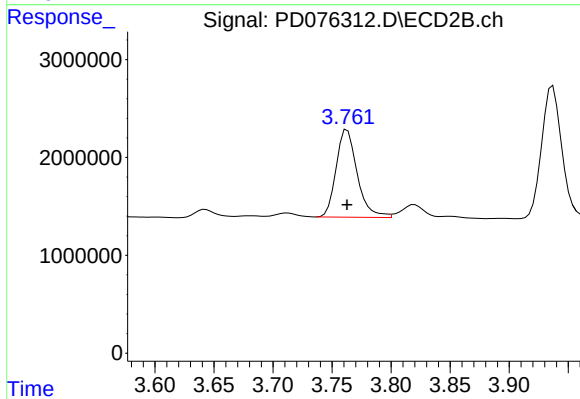

#23 Chlordane-1


R.T.: 3.763 min
Delta R.T.: 0.000 min
Response: 11137945
Conc: 250.96 ng/ml

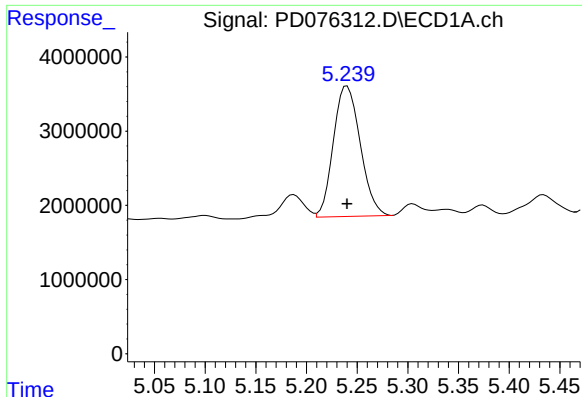

#24 Chlordane-2


R.T.: 5.240 min
Delta R.T.: 0.000 min
Response: 32434464
Conc: 258.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

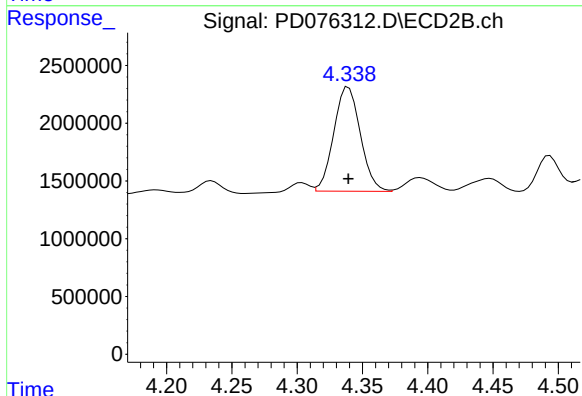


#24 Chlordane-2

R.T.: 4.339 min
Delta R.T.: 0.000 min
Response: 12808519
Conc: 266.91 ng/ml

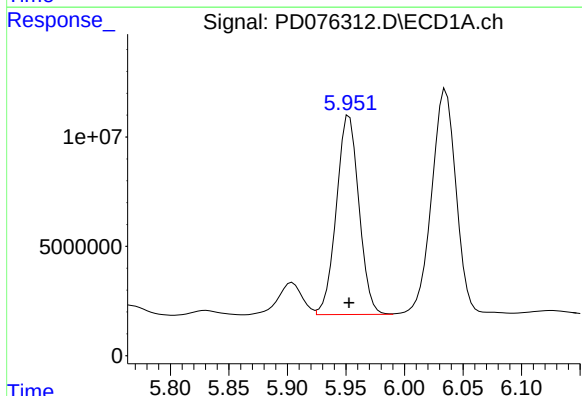


#25 Chlordane-3

R.T.: 5.953 min
Delta R.T.: 0.000 min
Response: 122052947
Conc: 236.10 ng/ml

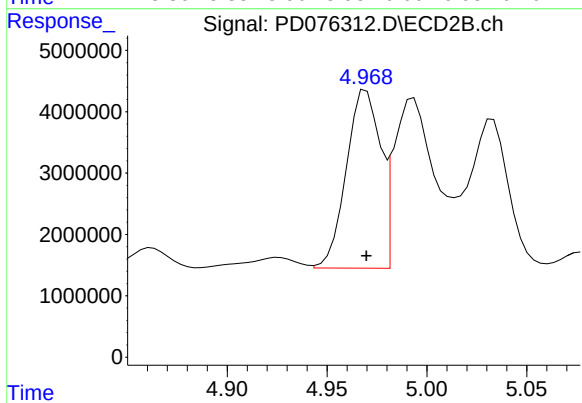

#25 Chlordane-3


R.T.: 4.970 min
Delta R.T.: 0.000 min
Response: 34285237
Conc: 241.21 ng/ml

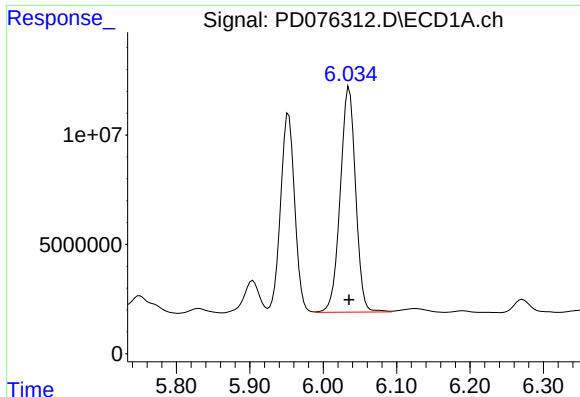

#26 Chlordane-4


R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 149649459
Conc: 240.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

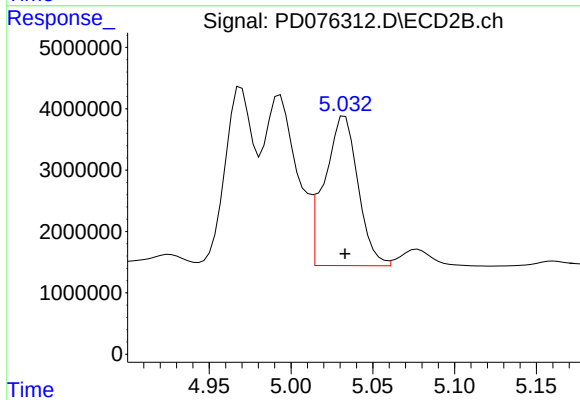


#26 Chlordane-4

R.T.: 5.033 min
Delta R.T.: 0.000 min
Response: 34512708
Conc: 243.66 ng/ml

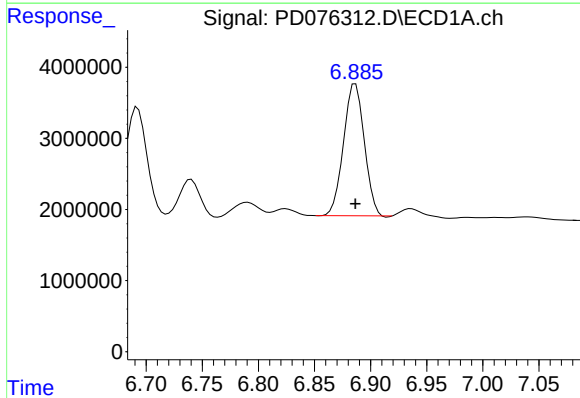


#27 Chlordane-5

R.T.: 6.887 min
Delta R.T.: 0.000 min
Response: 23839248
Conc: 238.89 ng/ml

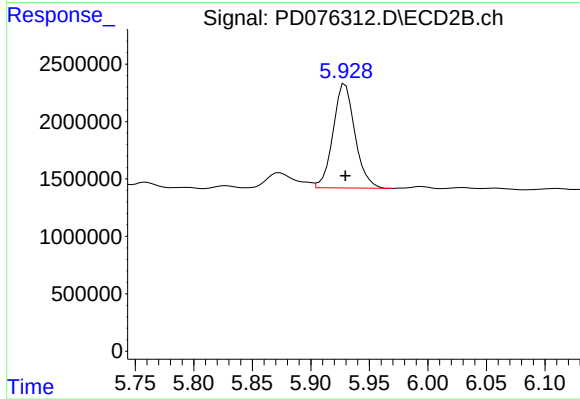

#27 Chlordane-5


R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 11793637
Conc: 242.60 ng/ml

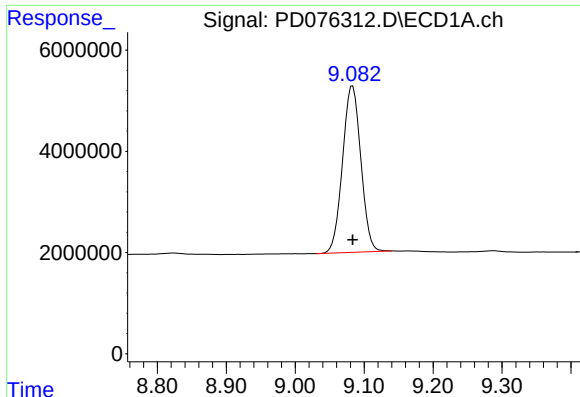

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 60731573
Conc: 26.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

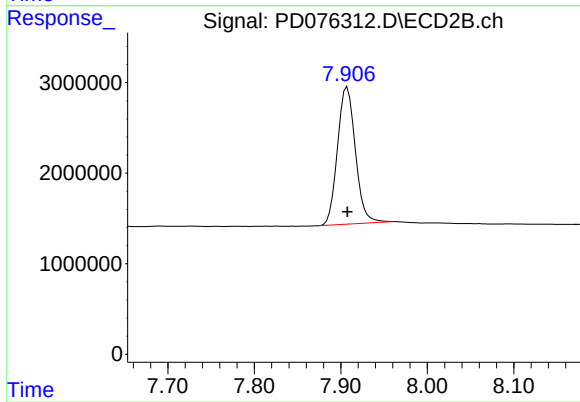

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 21703021
Conc: 25.97 ng/ml