

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070423\
 Data File : PD076320.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jul 2023 16:01
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD070423

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 05 05:18:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070423.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 05 05:16:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.765	111.8E6	62833340	51.170	52.213
28)	SA Decachlor...	9.083	7.907	121.3E6	43487982	51.291	51.080
Target Compounds							
23)	Chlordane-1	4.709	3.763	60344667	22484216	520.335	508.101
24)	Chlordane-2	5.240	4.339	65131064	25139306	508.600	517.354
25)	Chlordane-3	5.952	4.969	264.8E6	72277154	523.142	515.048
26)	Chlordane-4	6.035	5.033	320.0E6	70900943	520.518	503.491
27)	Chlordane-5	6.886	5.929	51203672	24903649	524.325	535.163



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070423\
Data File : PD076320.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jul 2023 16:01
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD070423

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 05 05:18:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070423.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 05:16:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

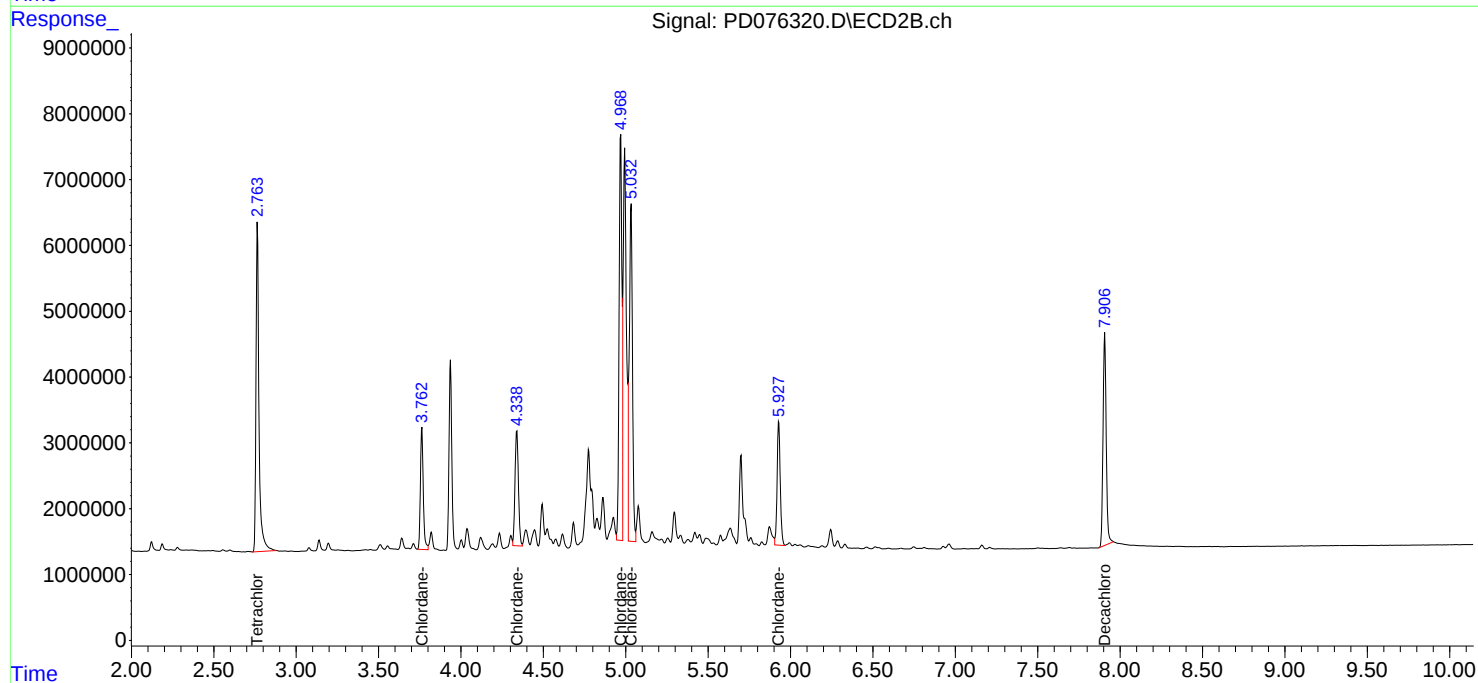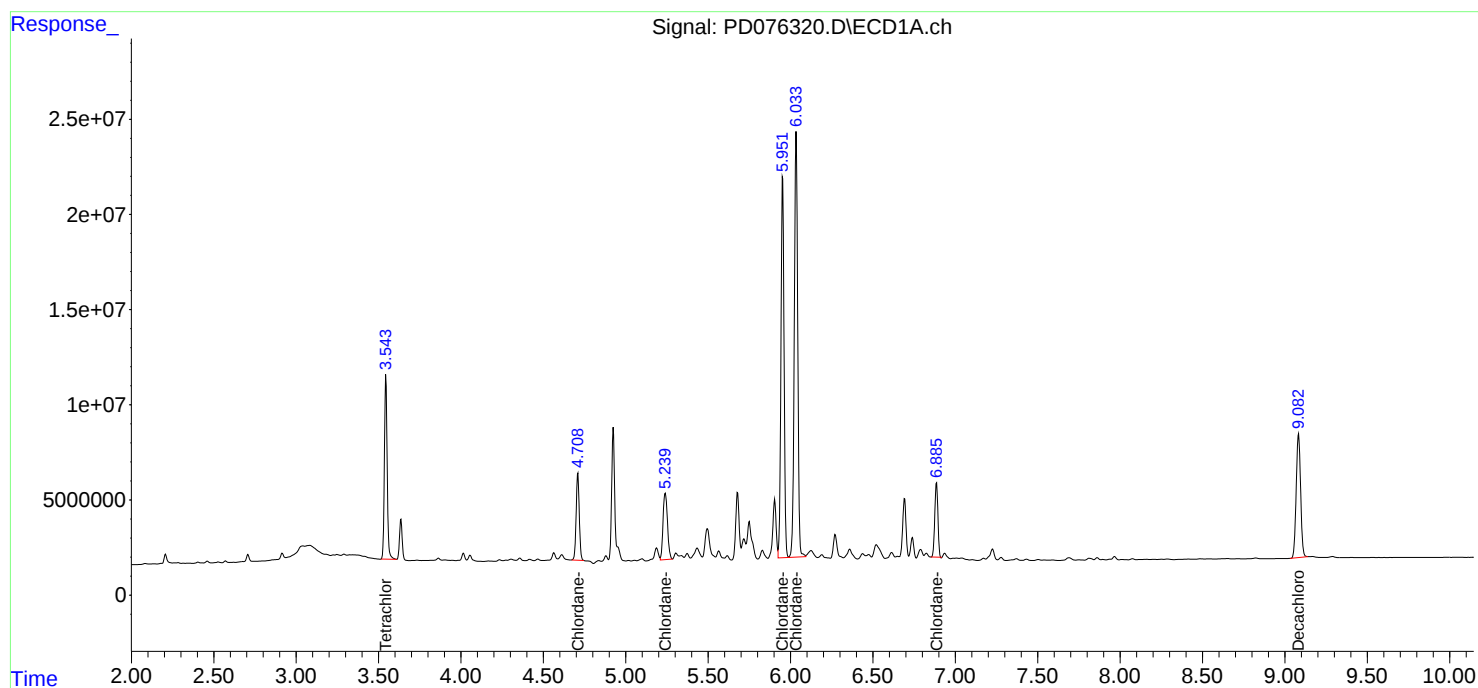


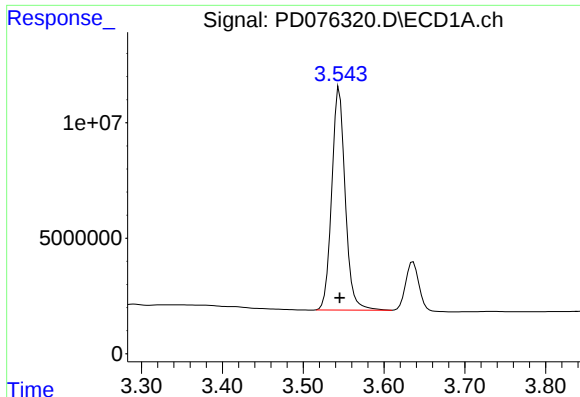

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 111760809
Conc: 51.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD070423

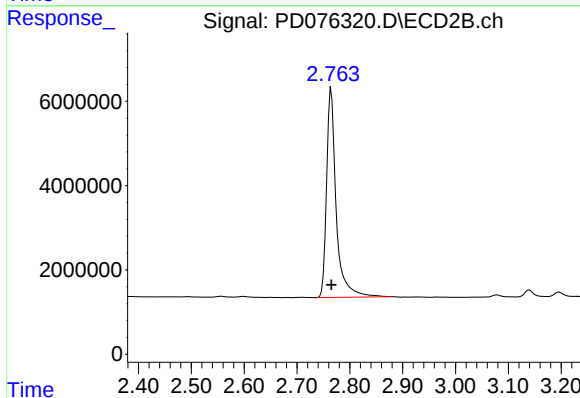


#1 Tetrachloro-m-xylene

R.T.: 2.765 min
Delta R.T.: 0.000 min
Response: 62833340
Conc: 52.21 ng/ml

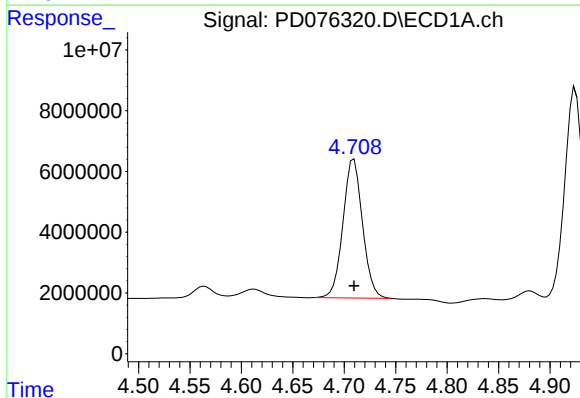


#23 Chlordane-1

R.T.: 4.709 min
Delta R.T.: 0.000 min
Response: 60344667
Conc: 520.34 ng/ml

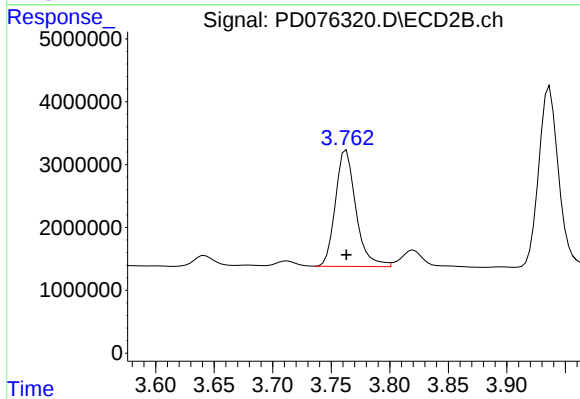

#23 Chlordane-1


R.T.: 3.763 min
Delta R.T.: 0.000 min
Response: 22484216
Conc: 508.10 ng/ml

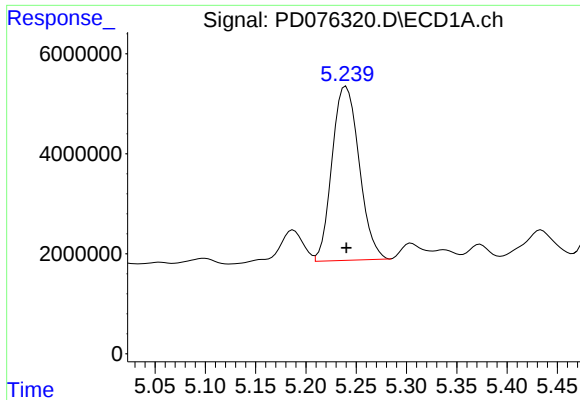

#24 Chlordane-2


R.T.: 5.240 min
Delta R.T.: 0.000 min
Response: 65131064
Conc: 508.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD070423

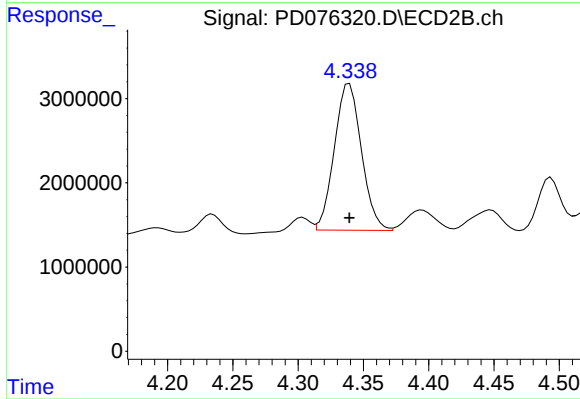


#24 Chlordane-2

R.T.: 4.339 min
Delta R.T.: 0.000 min
Response: 25139306
Conc: 517.35 ng/ml

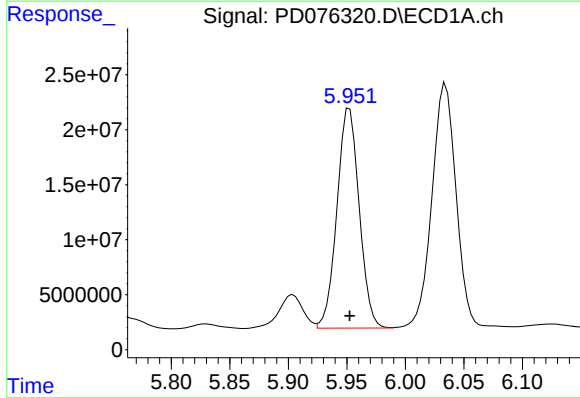


#25 Chlordane-3

R.T.: 5.952 min
Delta R.T.: 0.000 min
Response: 264750515
Conc: 523.14 ng/ml

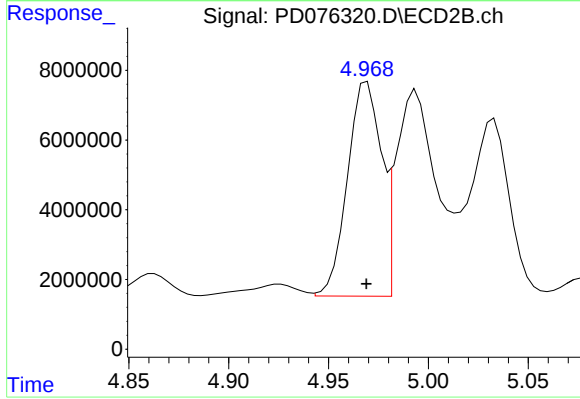

#25 Chlordane-3


R.T.: 4.969 min
Delta R.T.: 0.000 min
Response: 72277154
Conc: 515.05 ng/ml

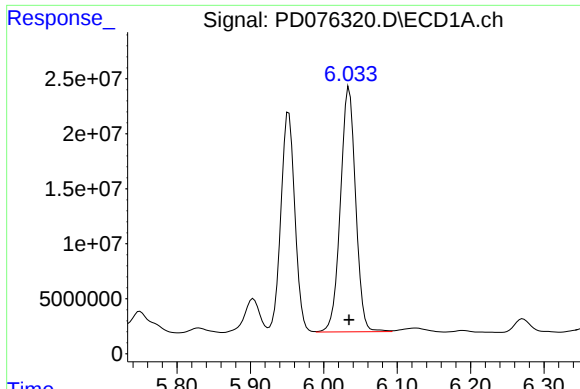

#26 Chlordane-4


R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 320017896
Conc: 520.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD070423

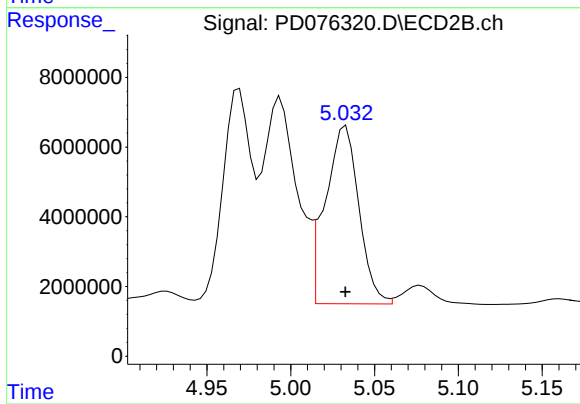


#26 Chlordane-4

R.T.: 5.033 min
Delta R.T.: 0.000 min
Response: 70900943
Conc: 503.49 ng/ml

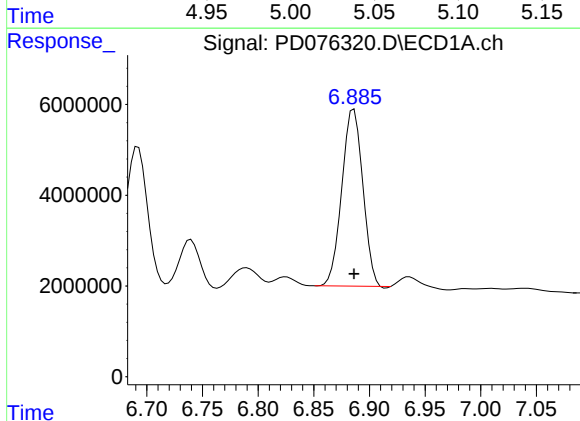


#27 Chlordane-5

R.T.: 6.886 min
Delta R.T.: 0.000 min
Response: 51203672
Conc: 524.32 ng/ml

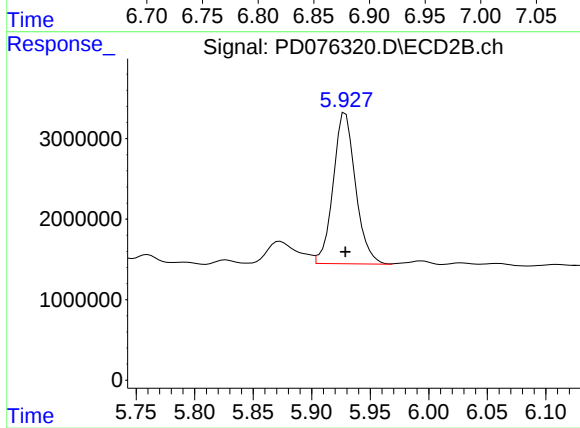

#27 Chlordane-5


R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 24903649
Conc: 535.16 ng/ml

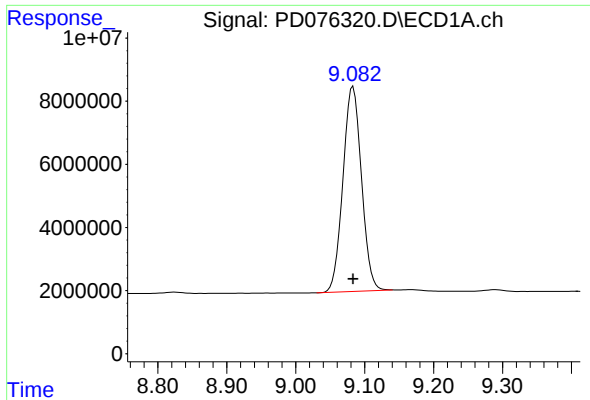

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 121347214
Conc: 51.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD070423

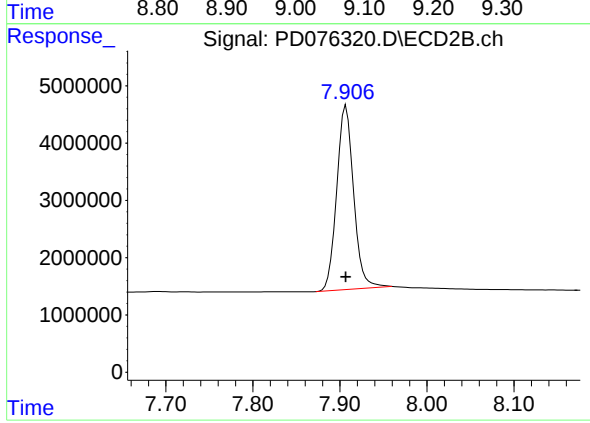

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 43487982
Conc: 51.08 ng/ml