

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070519\
 Data File : PD053875.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jul 2019 14:03
 Operator : SM\AJ
 Sample : K3670-18
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C6BB8

Manual Integrations
 APPROVED

Ankita
 7/8/2019 3:14:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 11:19:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070319CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 05 03:58:18 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.313	3.983	11889443	17082185	15.582	15.146
27) SA Decachlor...	8.007	9.021	24274701	29037757	32.685m	27.792m
Target Compounds						
12) B 4,4'-DDE	5.435	6.307	2330572	6418981	2.572m	4.561 #
14) MA Endrin	5.814	6.667	1229469	5261458	1.478m	4.585 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070519\
Data File : PD053875.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jul 2019 14:03
Operator : SM\AJ
Sample : K3670-18
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 11:19:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070319CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 05 03:58:18 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

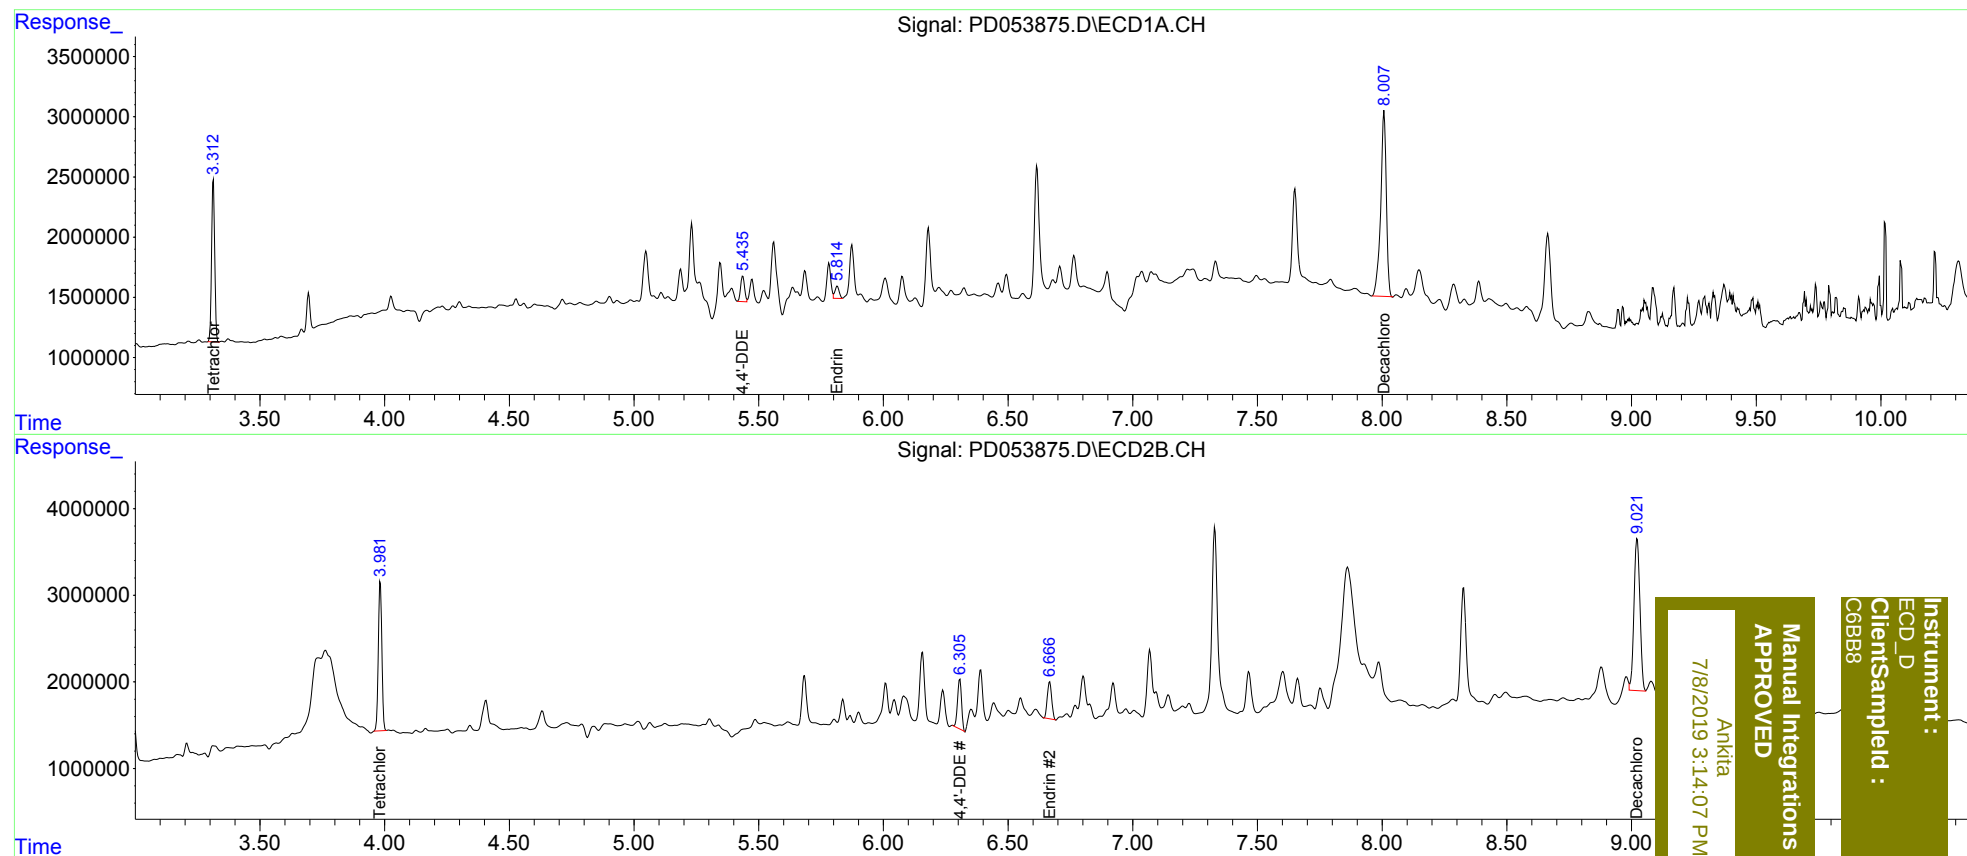

7/8/2019 3:14:07 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSampled :
C6BB8