

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070519\
 Data File : PD053900.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jul 2019 20:45
 Operator : SM\AJ
 Sample : K3671-03
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C5BC5

Manual Integrations
 APPROVED

Ankita
 7/8/2019 3:15:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 10:33:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070319CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 05 03:58:18 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.983	13630195	19697241	17.864	17.465
2)	SA Decachlor...	8.008	9.023	24014348	30568108	32.334	29.257
Target Compounds							
10)	B trans-Chl...	5.213	6.077	1308989	7203073	1.368m	4.772m#
11)	B cis-Chlor...	5.266	6.156	2979180	17891733	3.190	12.150 #
12)	B 4,4'-DDE	5.435	6.305	1011966	1881687	1.117m	1.337m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070519\
Data File : PD053900.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jul 2019 20:45
Operator : SM\AJ
Sample : K3671-03
Misc :
ALS Vial : 49 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 10:33:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070319CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 05 03:58:18 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

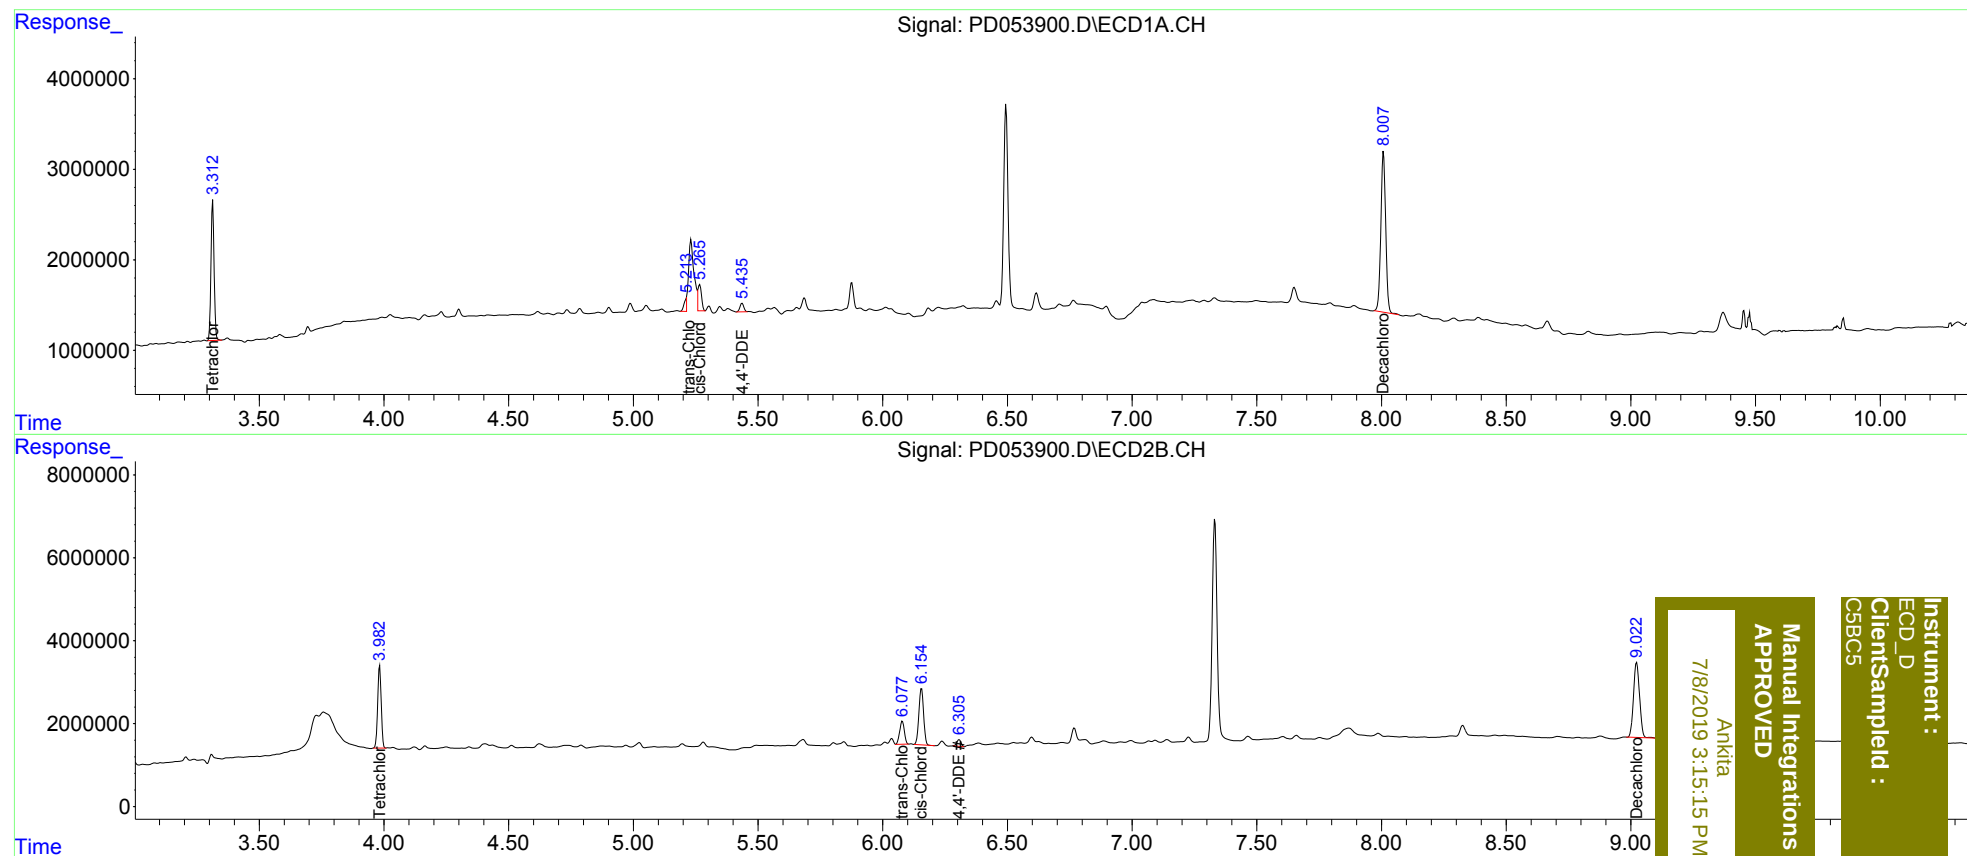

7/8/2019 3:15:15 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSampled :
C5BC5