

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070522\
 Data File : PD070697.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2022 13:35
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 05 14:55:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070522.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 05 14:55:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	4.123	259.3E6	2189.9E6	98.631	92.651
28)	SA Decachlor...	8.264	9.311	213.7E6	688.5E6	93.549	90.362
Target Compounds							
23)	Chlordane-1	4.362	5.142	80266921	915.7E6	963.929	909.938
24)	Chlordane-2	4.865	5.620	87498166	759.9E6	917.000	895.551
25)	Chlordane-3	5.437	6.278	282.0E6	2800.5E6	991.931	940.810
26)	Chlordane-4	5.496	6.352	227.2E6	3200.1E6	981.752	934.504
27)	Chlordane-5	6.336	7.174	95285935	514.4E6	960.622	913.873



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070522\
Data File : PD070697.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2022 13:35
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 05 14:55:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070522.M
Quant Title : GC Extractables
QLast Update : Tue Jul 05 14:55:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

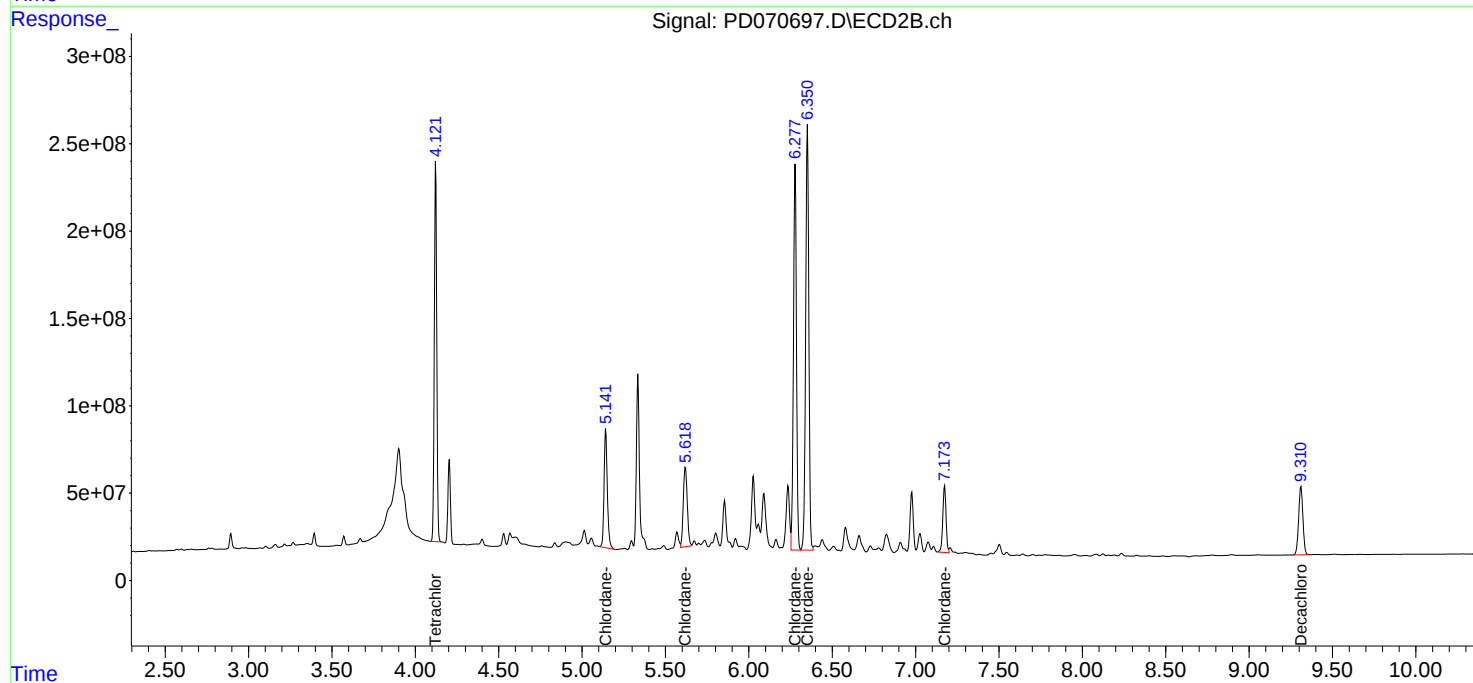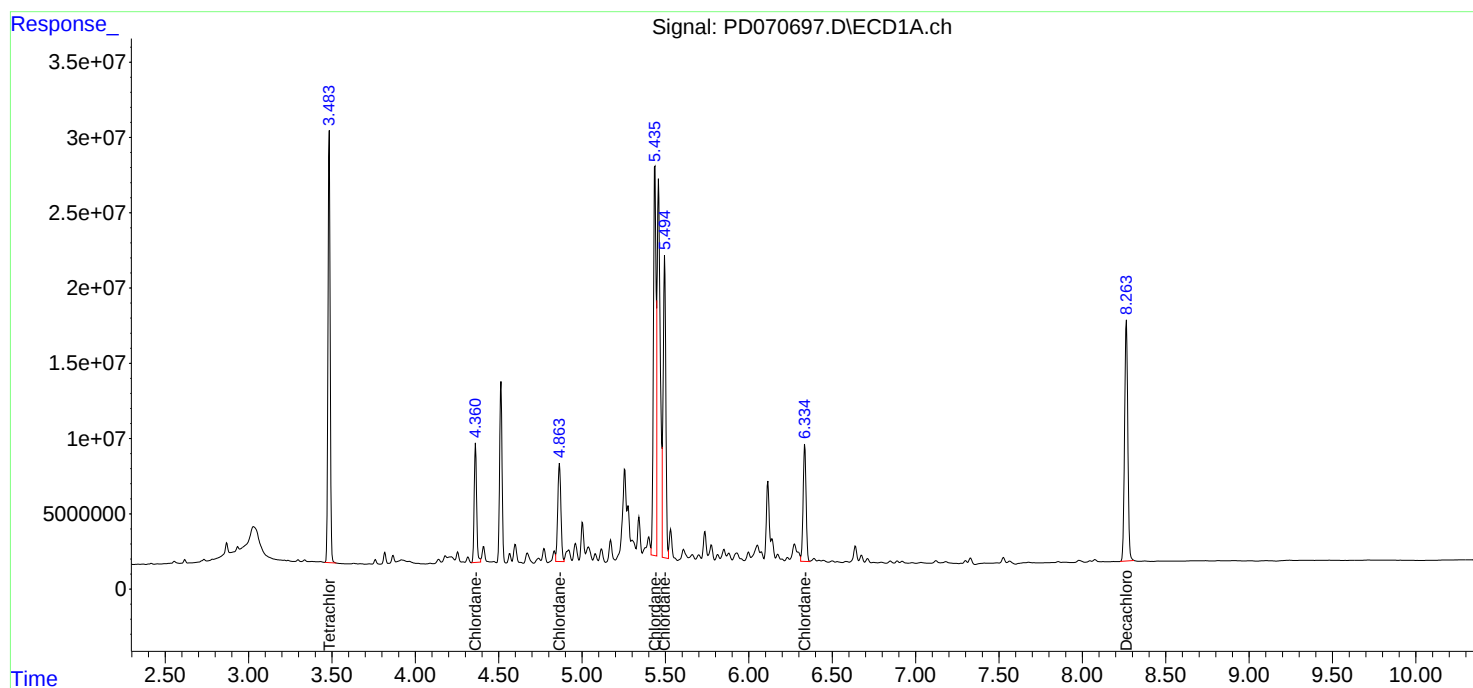


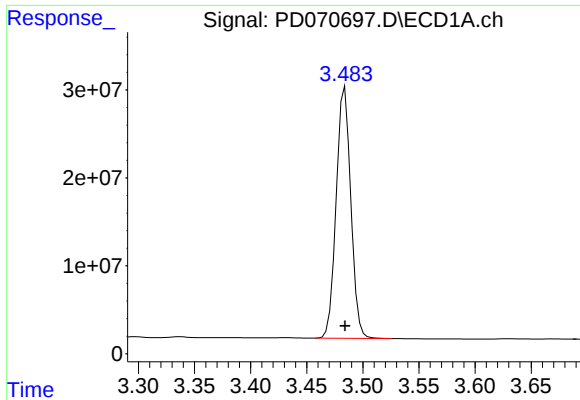

#1 Tetrachloro-m-xylene


R.T.: 3.484 min
Delta R.T.: 0.000 min
Response: 259290660
Conc: 98.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

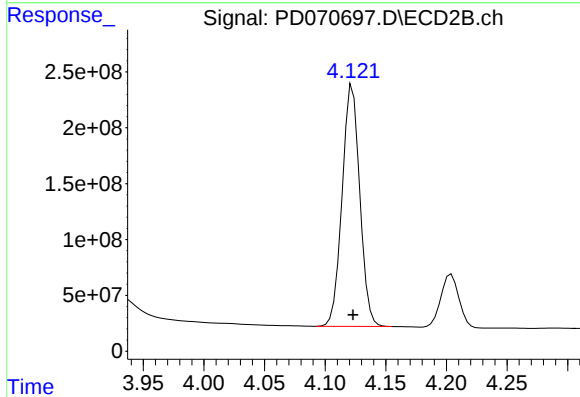


#1 Tetrachloro-m-xylene

R.T.: 4.123 min
Delta R.T.: 0.000 min
Response: 2189913292
Conc: 92.65 ng/ml

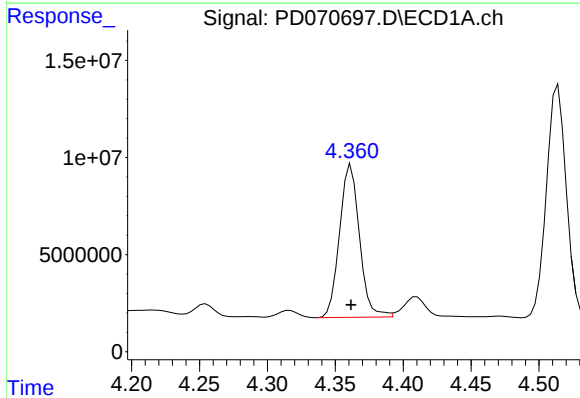


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 80266921
Conc: 963.93 ng/ml

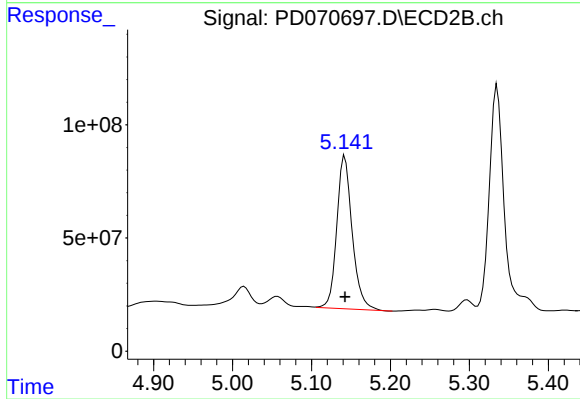

#23 Chlordane-1


R.T.: 5.142 min
Delta R.T.: 0.000 min
Response: 915709263
Conc: 909.94 ng/ml

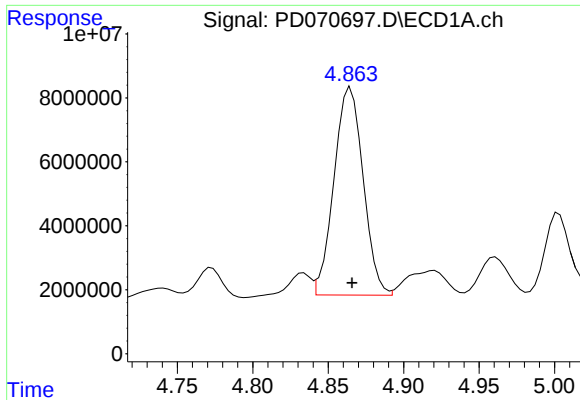

#24 Chlordane-2


R.T.: 4.865 min
Delta R.T.: 0.000 min
Response: 87498166
Conc: 917.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

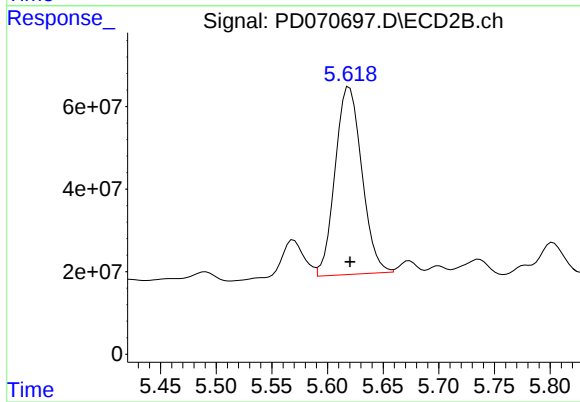


#24 Chlordane-2

R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 759865503
Conc: 895.55 ng/ml

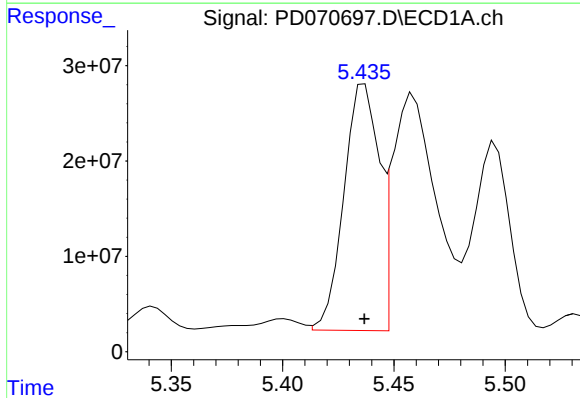


#25 Chlordane-3

R.T.: 5.437 min
Delta R.T.: 0.000 min
Response: 282045210
Conc: 991.93 ng/ml

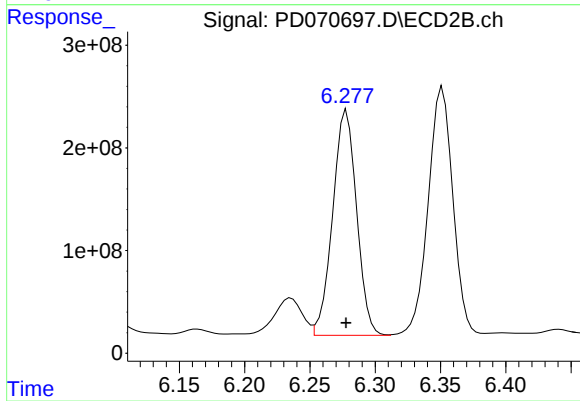

#25 Chlordane-3


R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 2800454570
Conc: 940.81 ng/ml

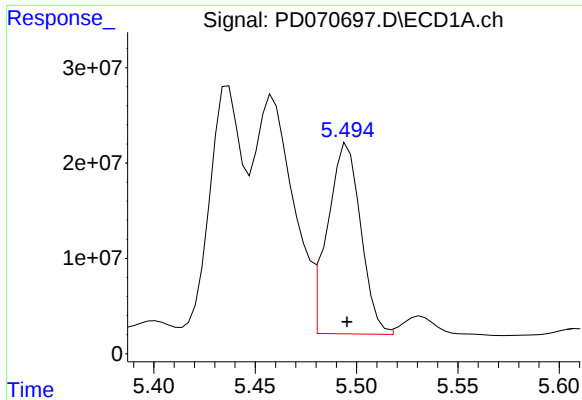

#26 Chlordane-4


R.T.: 5.496 min
Delta R.T.: 0.000 min
Response: 227169801
Conc: 981.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

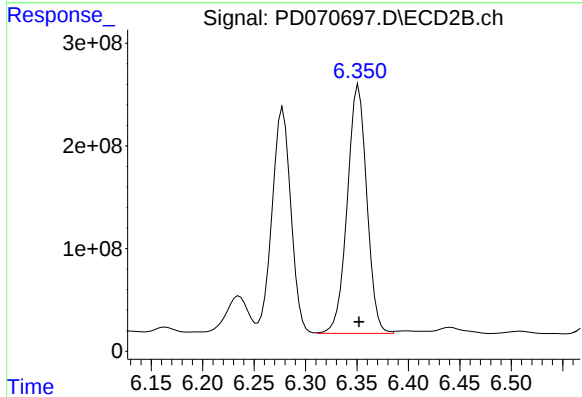


#26 Chlordane-4

R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 3200099997
Conc: 934.50 ng/ml

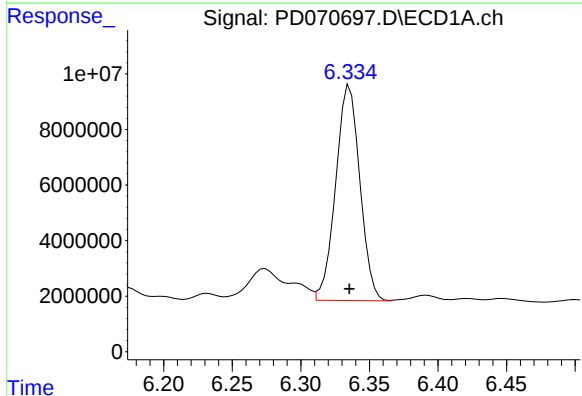


#27 Chlordane-5

R.T.: 6.336 min
Delta R.T.: 0.000 min
Response: 95285935
Conc: 960.62 ng/ml

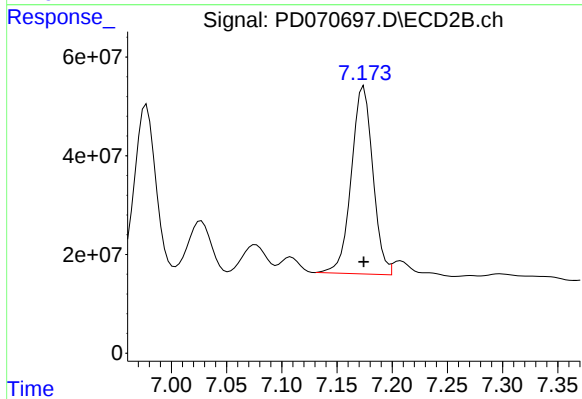

#27 Chlordane-5


R.T.: 7.174 min
Delta R.T.: 0.000 min
Response: 514385300
Conc: 913.87 ng/ml

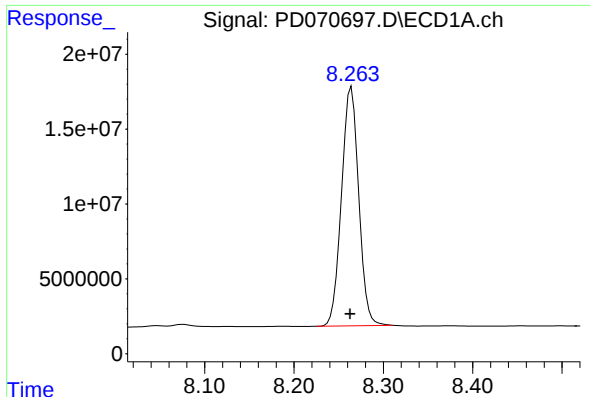

#28 Decachlorobiphenyl

R.T.: 8.264 min
Delta R.T.: 0.001 min
Response: 213687715
Conc: 93.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

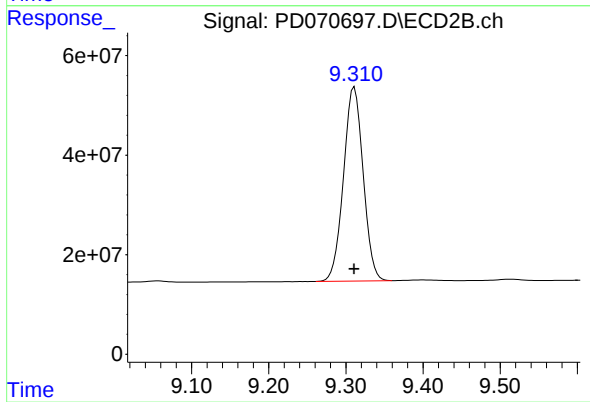

#28 Decachlorobiphenyl

R.T.: 9.311 min
Delta R.T.: 0.000 min
Response: 688513012
Conc: 90.36 ng/ml