

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070522\
 Data File : PD070698.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2022 13:50
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 05 14:56:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070522.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 05 14:55:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	4.123	190.1E6	1657.5E6	72.299	70.124
28)	SA Decachlor...	8.263	9.311	159.9E6	527.8E6	69.981	69.272
Target Compounds							
23)	Chlordane-1	4.362	5.143	59109604	692.7E6	709.850	688.301
24)	Chlordane-2	4.866	5.620	65831164	575.3E6	689.925	678.067
25)	Chlordane-3	5.438	6.278	204.8E6	2091.7E6	720.153	702.693
26)	Chlordane-4	5.496	6.351	166.6E6	2397.9E6	719.989	700.248
27)	Chlordane-5	6.336	7.174	70402931	390.0E6	709.765	692.831



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070522\
Data File : PD070698.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2022 13:50
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 05 14:56:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070522.M
Quant Title : GC Extractables
QLast Update : Tue Jul 05 14:55:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

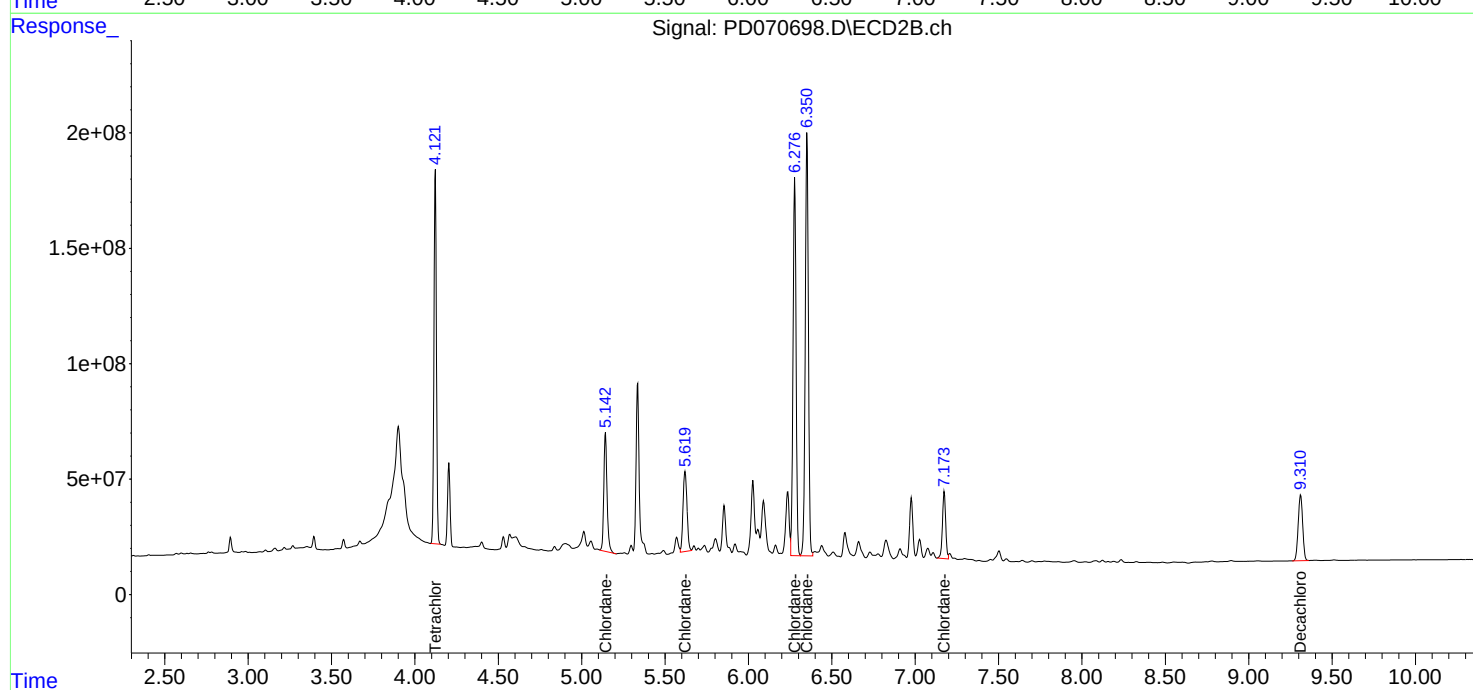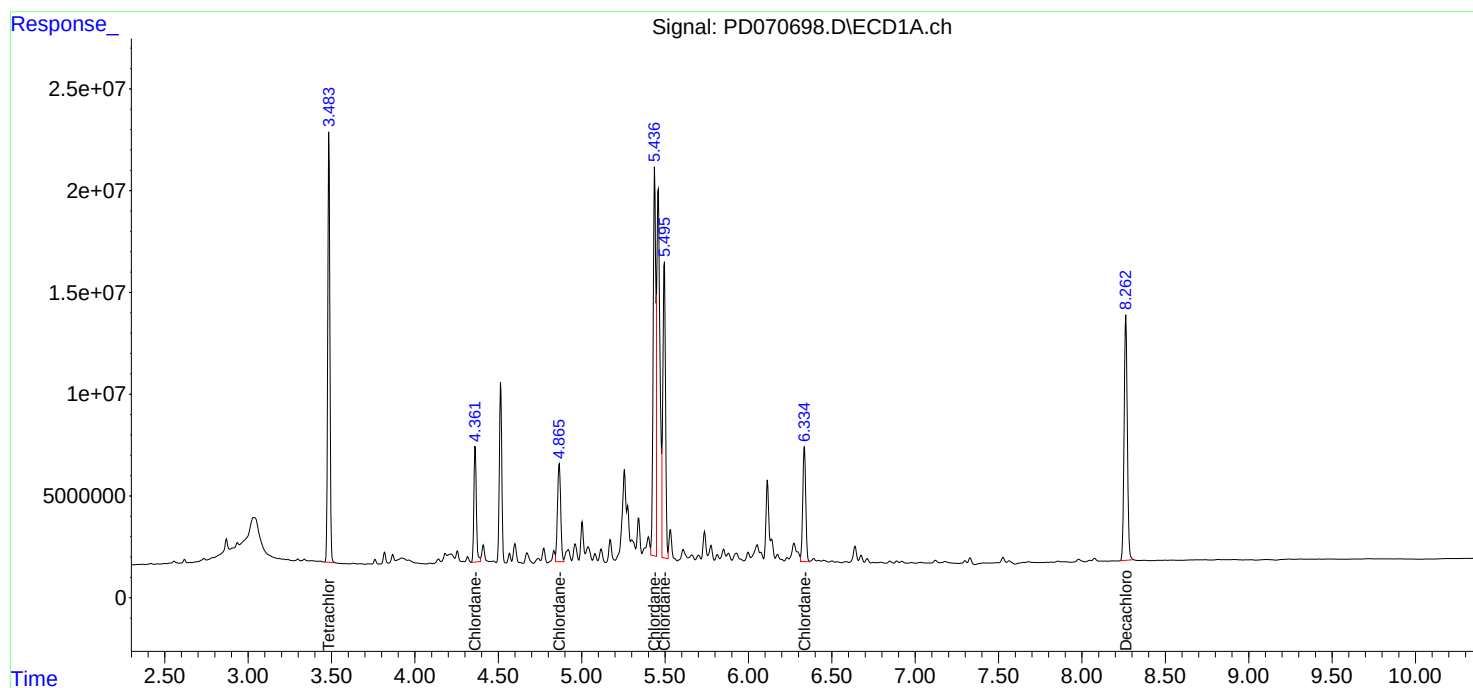


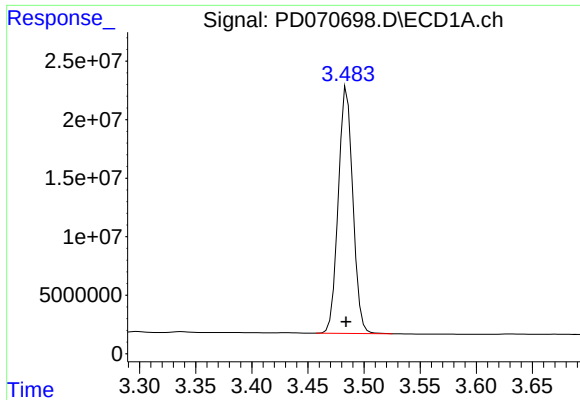

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 190065786
Conc: 72.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

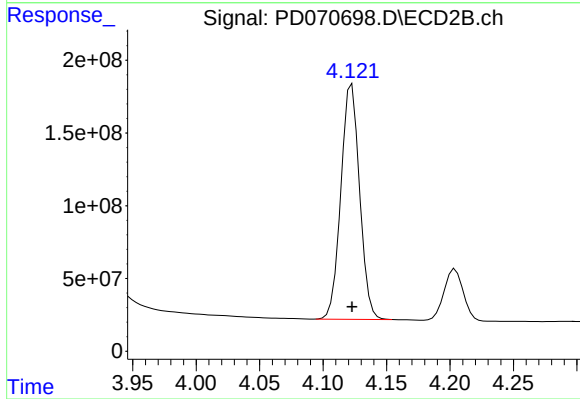


#1 Tetrachloro-m-xylene

R.T.: 4.123 min
Delta R.T.: 0.000 min
Response: 1657462171
Conc: 70.12 ng/ml

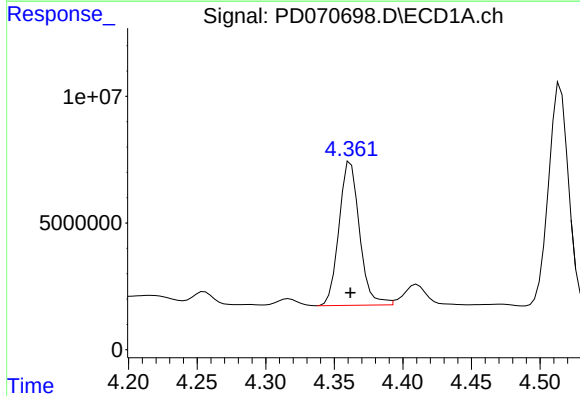


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 59109604
Conc: 709.85 ng/ml

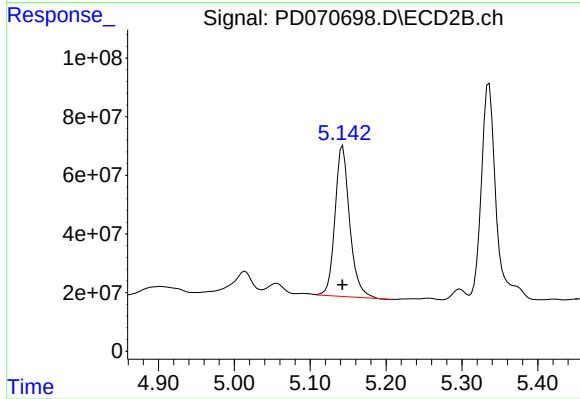

#23 Chlordane-1


R.T.: 5.143 min
Delta R.T.: 0.000 min
Response: 692666366
Conc: 688.30 ng/ml

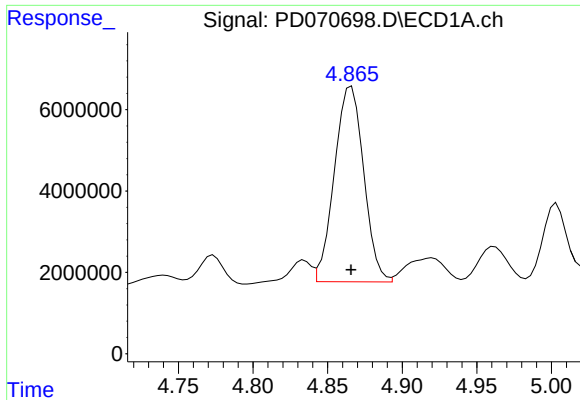

#24 Chlordane-2


R.T.: 4.866 min
Delta R.T.: 0.000 min
Response: 65831164
Conc: 689.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

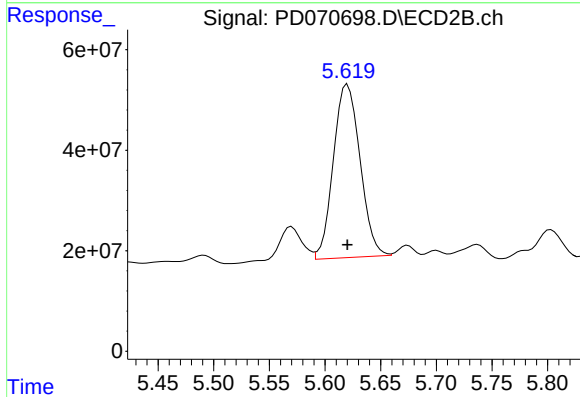


#24 Chlordane-2

R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 575332551
Conc: 678.07 ng/ml

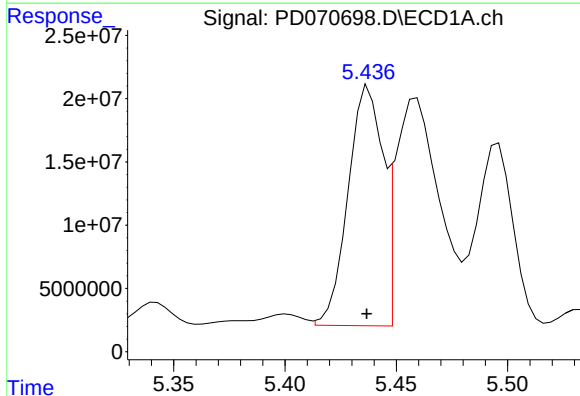


#25 Chlordane-3

R.T.: 5.438 min
Delta R.T.: 0.001 min
Response: 204767937
Conc: 720.15 ng/ml

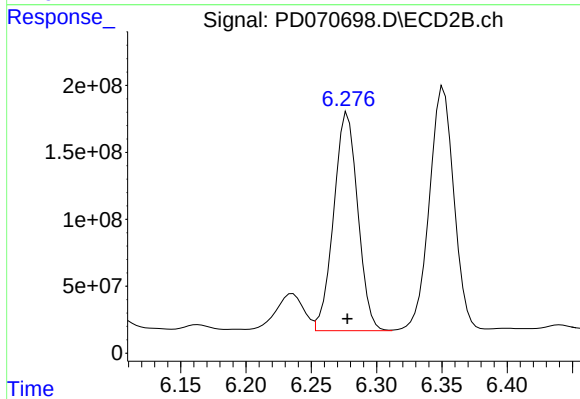

#25 Chlordane-3


R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 2091667003
Conc: 702.69 ng/ml

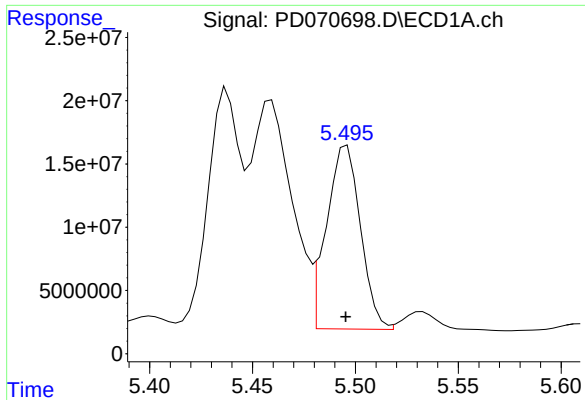

#26 Chlordane-4


R.T.: 5.496 min
Delta R.T.: 0.000 min
Response: 166599942
Conc: 719.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

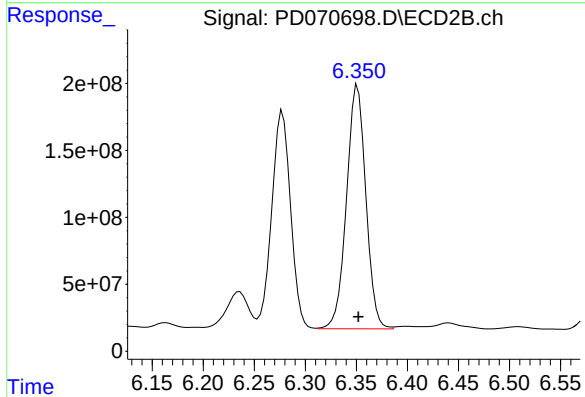


#26 Chlordane-4

R.T.: 6.351 min
Delta R.T.: 0.000 min
Response: 2397917379
Conc: 700.25 ng/ml

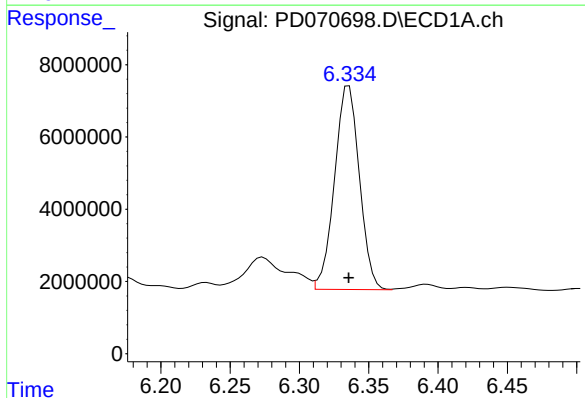


#27 Chlordane-5

R.T.: 6.336 min
Delta R.T.: 0.000 min
Response: 70402931
Conc: 709.76 ng/ml

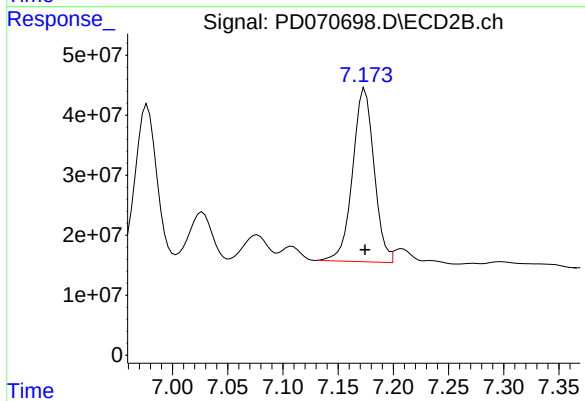

#27 Chlordane-5


R.T.: 7.174 min
Delta R.T.: 0.000 min
Response: 389968585
Conc: 692.83 ng/ml

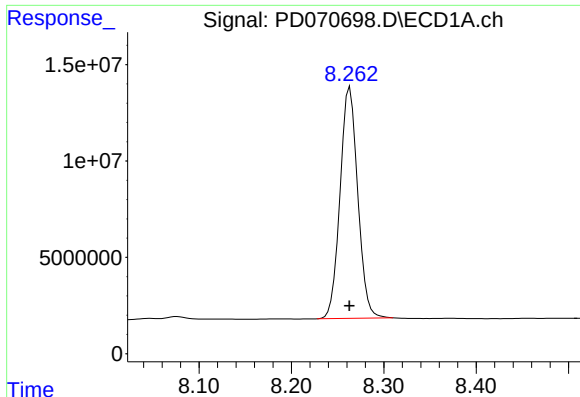

#28 Decachlorobiphenyl

R.T.: 8.263 min
Delta R.T.: 0.000 min
Response: 159853867
Conc: 69.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

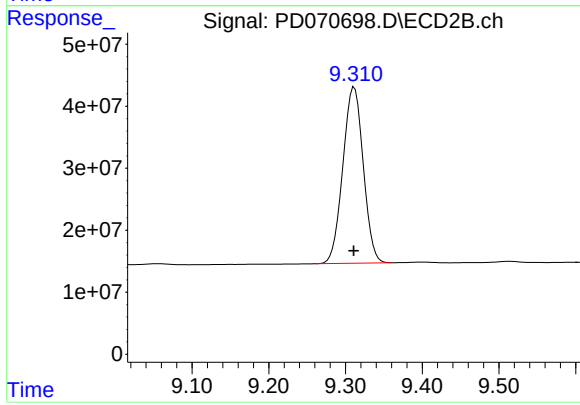

#28 Decachlorobiphenyl

R.T.: 9.311 min
Delta R.T.: 0.000 min
Response: 527816123
Conc: 69.27 ng/ml