

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070522\
 Data File : PD070699.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2022 14:04
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 05 14:56:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070522.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 05 14:55:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	4.123	131.4E6	1181.8E6	50.000	50.000
28)	SA Decachlor...	8.263	9.311	114.2E6	381.0E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.362	5.143	41635277	503.2E6	500.000	500.000
24)	Chlordane-2	4.866	5.620	47708940	424.2E6	500.000	500.000
25)	Chlordane-3	5.437	6.278	142.2E6	1488.3E6	500.000	500.000
26)	Chlordane-4	5.495	6.352	115.7E6	1712.2E6	500.000	500.000
27)	Chlordane-5	6.336	7.174	49595947	281.4E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070522\
Data File : PD070699.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2022 14:04
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 05 14:56:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070522.M
Quant Title : GC Extractables
QLast Update : Tue Jul 05 14:55:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

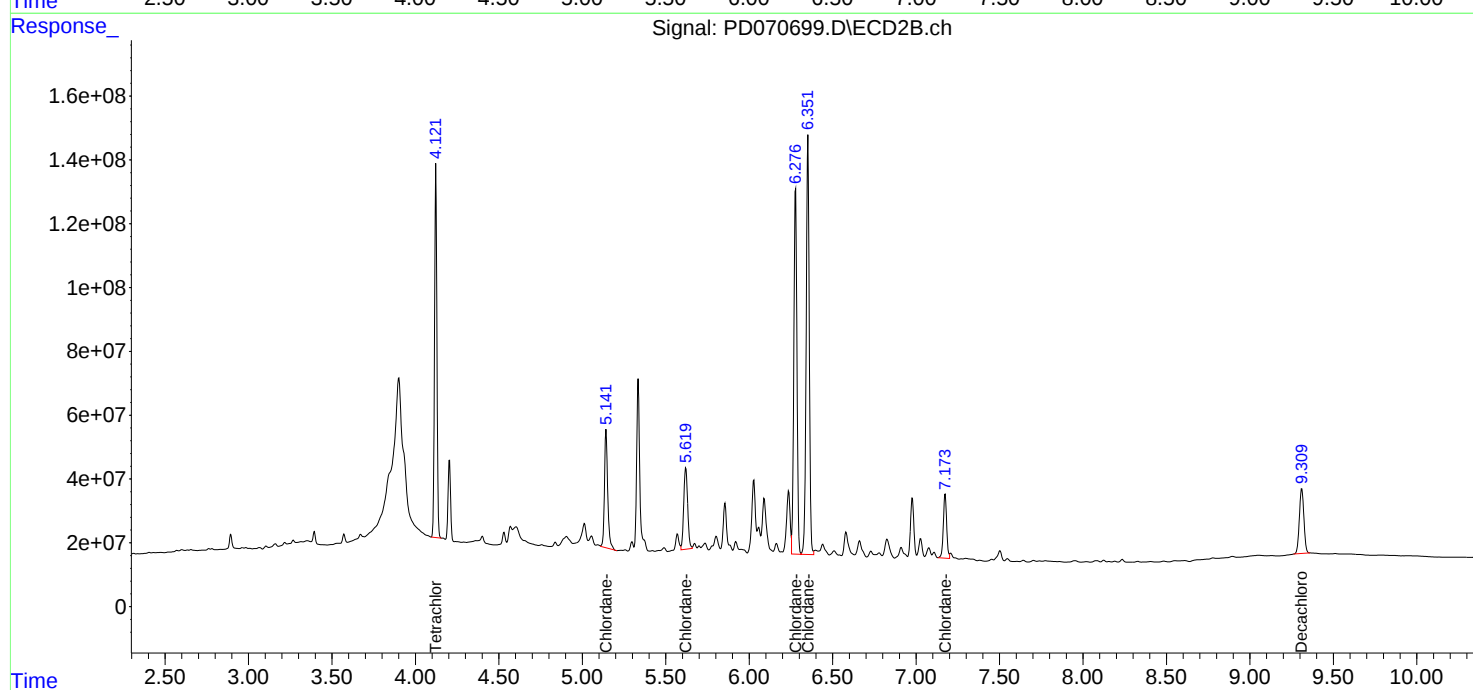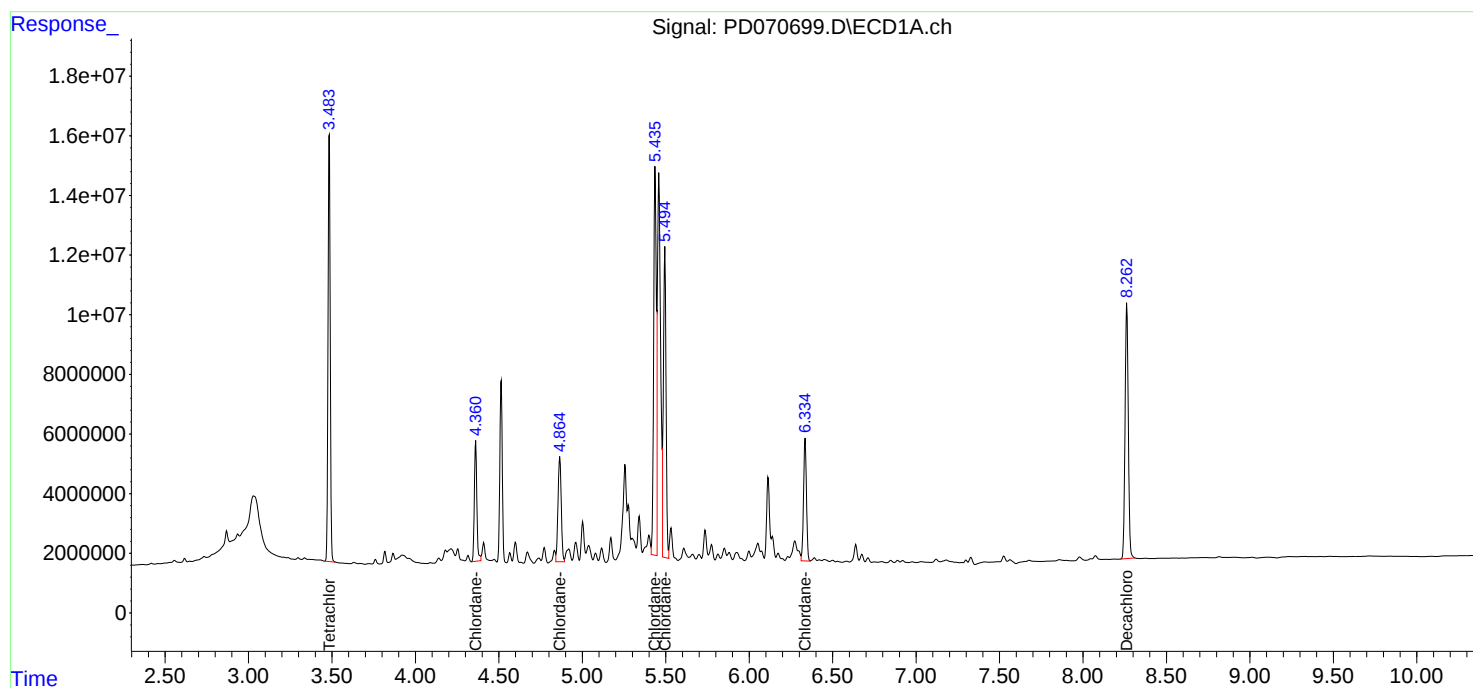


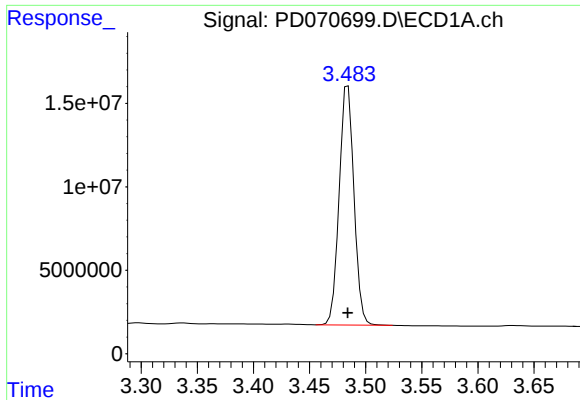

#1 Tetrachloro-m-xylene


R.T.: 3.484 min
Delta R.T.: 0.000 min
Response: 131444682
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

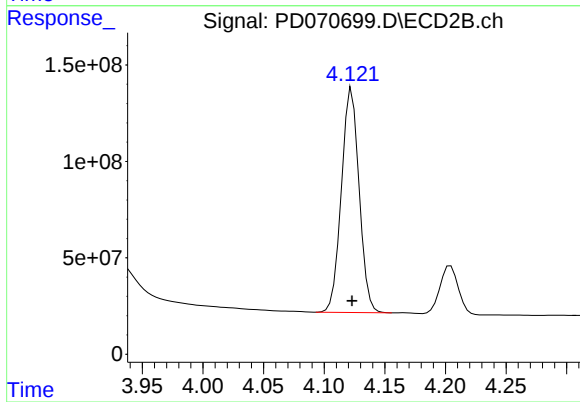


#1 Tetrachloro-m-xylene

R.T.: 4.123 min
Delta R.T.: 0.000 min
Response: 1181807759
Conc: 50.00 ng/ml

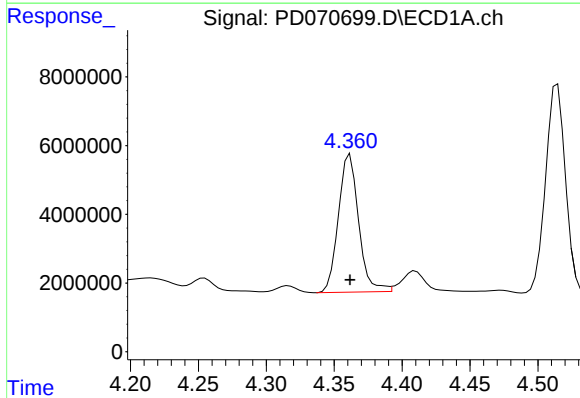


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 41635277
Conc: 500.00 ng/ml

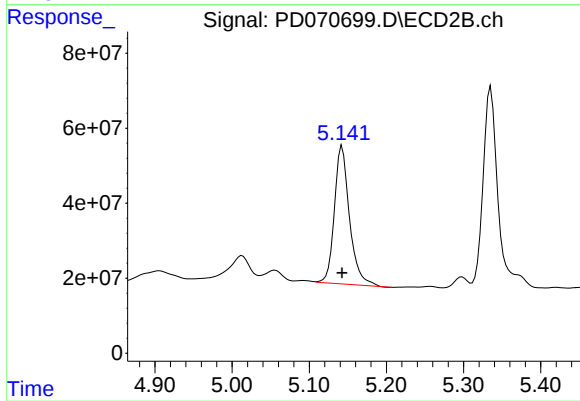

#23 Chlordane-1


R.T.: 5.143 min
Delta R.T.: 0.000 min
Response: 503171435
Conc: 500.00 ng/ml

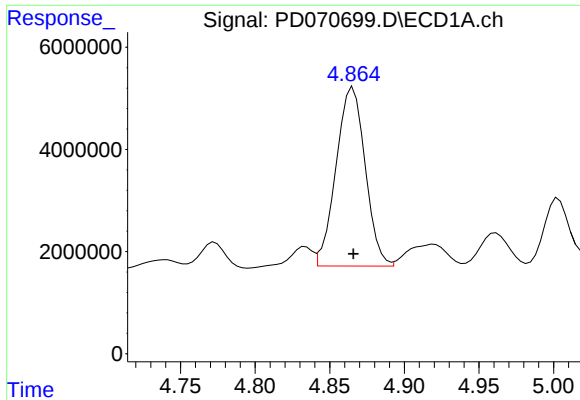

#24 Chlordane-2


R.T.: 4.866 min
Delta R.T.: 0.000 min
Response: 47708940
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

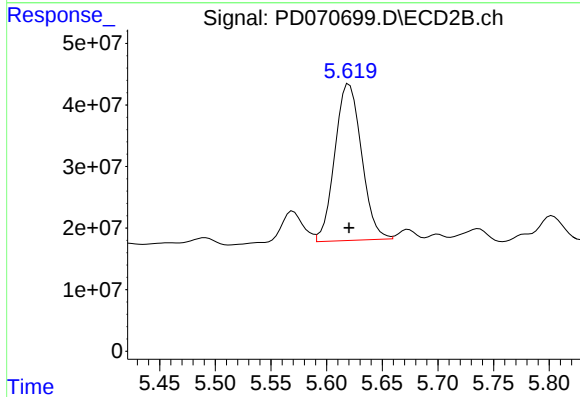


#24 Chlordane-2

R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 424244792
Conc: 500.00 ng/ml

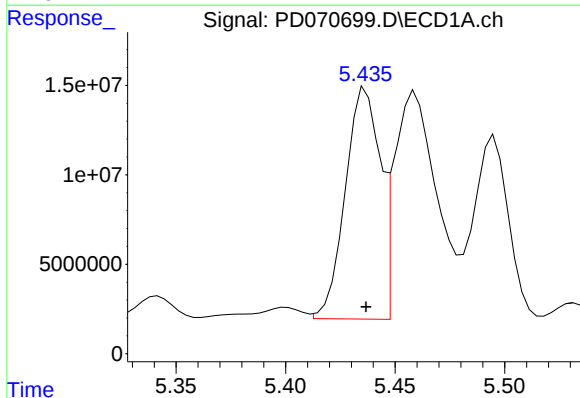


#25 Chlordane-3

R.T.: 5.437 min
Delta R.T.: 0.000 min
Response: 142169794
Conc: 500.00 ng/ml

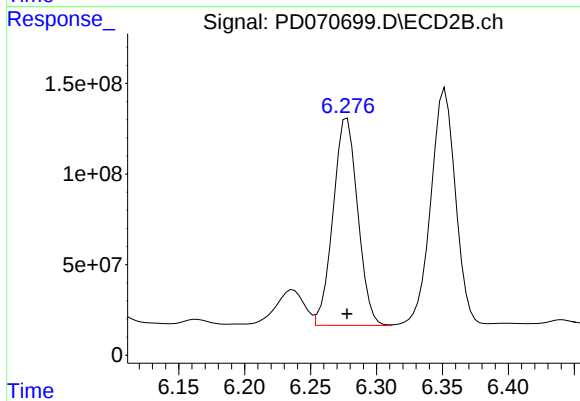

#25 Chlordane-3


R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 1488321464
Conc: 500.00 ng/ml

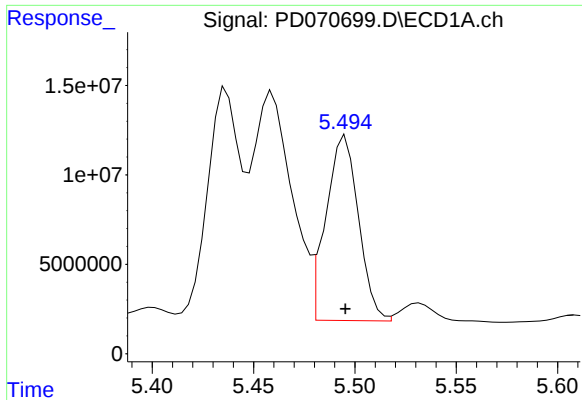

#26 Chlordane-4


R.T.: 5.495 min
Delta R.T.: 0.000 min
Response: 115696181
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

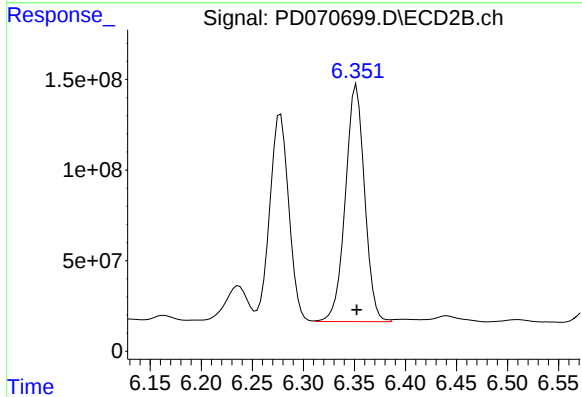


#26 Chlordane-4

R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 1712192545
Conc: 500.00 ng/ml

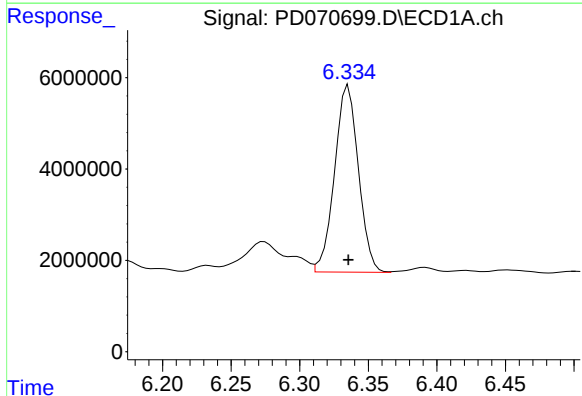


#27 Chlordane-5

R.T.: 6.336 min
Delta R.T.: 0.000 min
Response: 49595947
Conc: 500.00 ng/ml

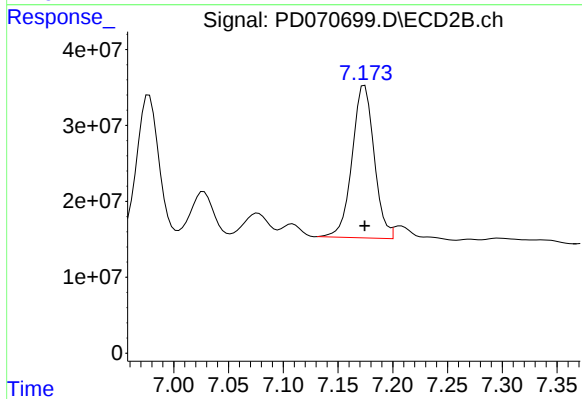

#27 Chlordane-5


R.T.: 7.174 min
Delta R.T.: 0.000 min
Response: 281431382
Conc: 500.00 ng/ml

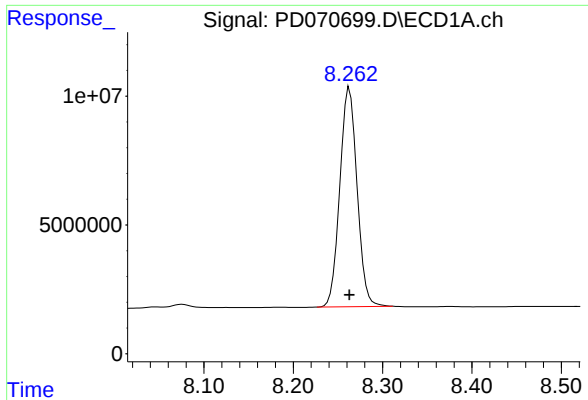

#28 Decachlorobiphenyl

R.T.: 8.263 min
Delta R.T.: 0.000 min
Response: 114211850
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

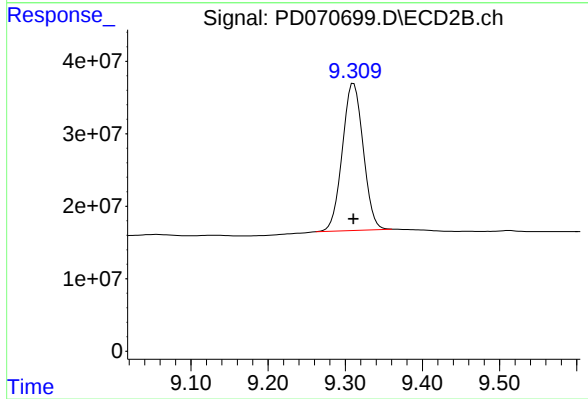

#28 Decachlorobiphenyl

R.T.: 9.311 min
Delta R.T.: 0.000 min
Response: 380974040
Conc: 50.00 ng/ml