

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070522\
 Data File : PD070700.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2022 14:19
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 05 14:56:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070522.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 05 14:55:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	4.123	61934951	588.6E6	23.559	24.904
28)	SA Decachlor...	8.264	9.311	56404961	192.4E6	24.693	25.253
Target Compounds							
23)	Chlordane-1	4.362	5.143	20680082	260.7E6	248.348	259.024
24)	Chlordane-2	4.865	5.619	24124890	217.2E6	252.834	256.029
25)	Chlordane-3	5.437	6.278	66420762	730.9E6	233.597	245.536
26)	Chlordane-4	5.495	6.352	55363163	848.6E6	239.261	247.805
27)	Chlordane-5	6.336	7.175	24101856	140.2E6	242.982	249.015



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070522\
Data File : PD070700.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2022 14:19
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 05 14:56:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070522.M
Quant Title : GC Extractables
QLast Update : Tue Jul 05 14:55:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

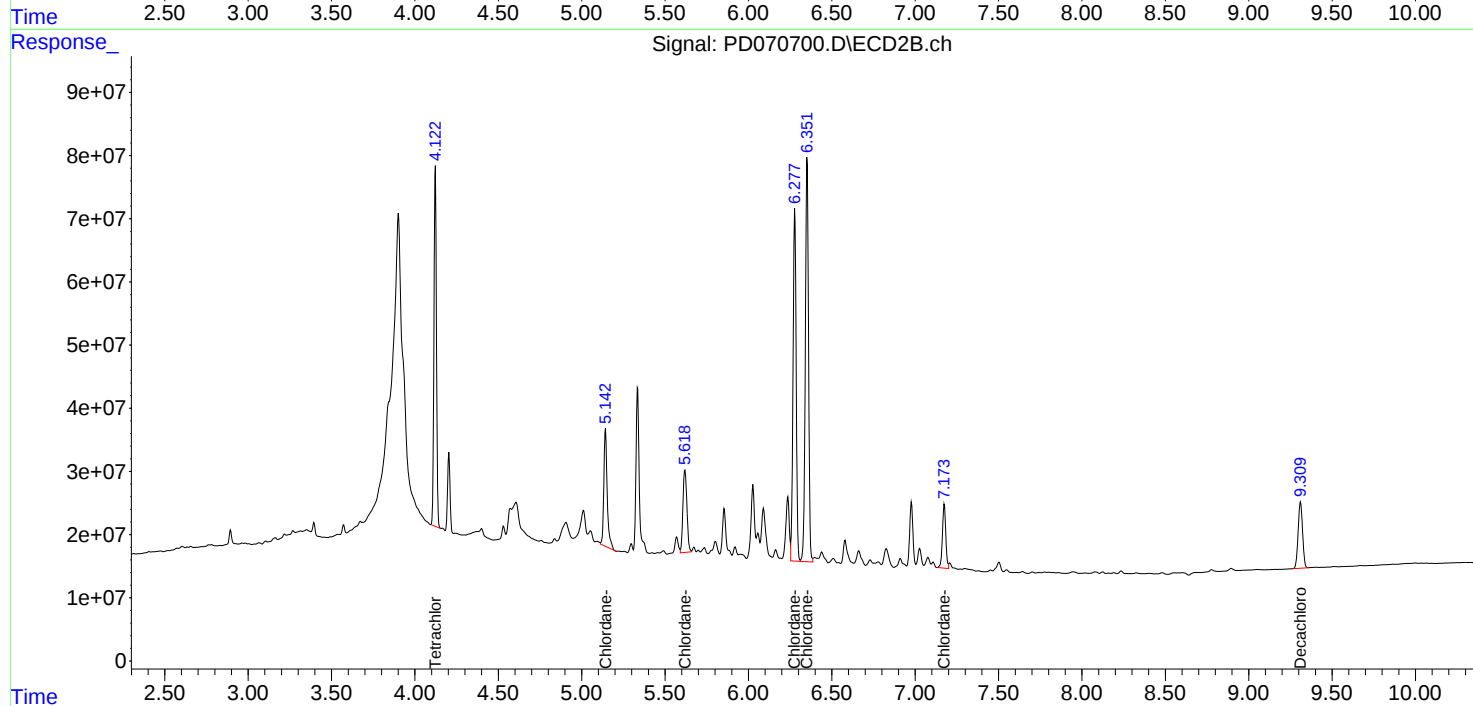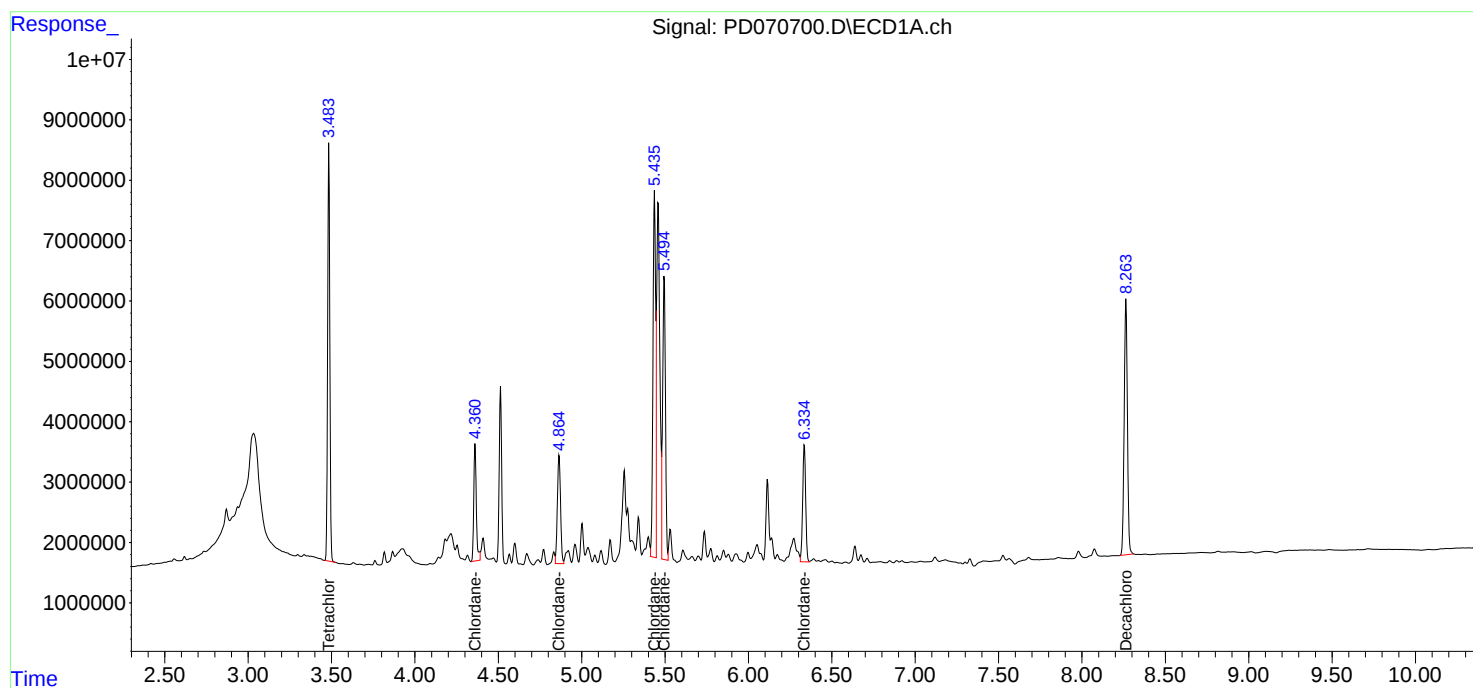


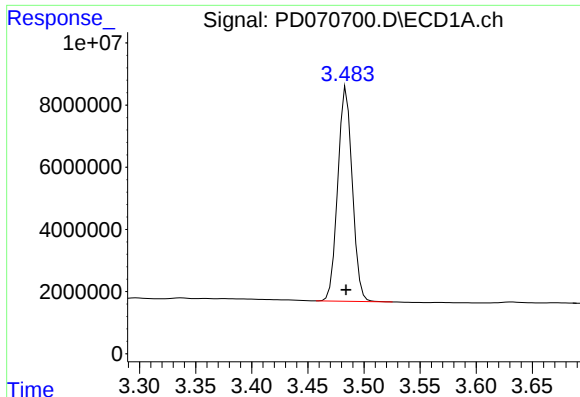

#1 Tetrachloro-m-xylene


R.T.: 3.484 min
Delta R.T.: 0.000 min
Response: 61934951
Conc: 23.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

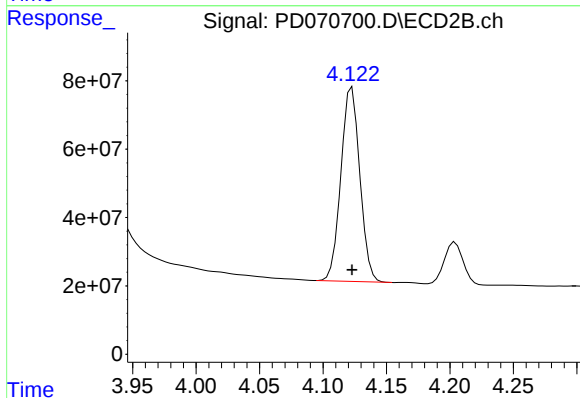


#1 Tetrachloro-m-xylene

R.T.: 4.123 min
Delta R.T.: 0.000 min
Response: 588624615
Conc: 24.90 ng/ml

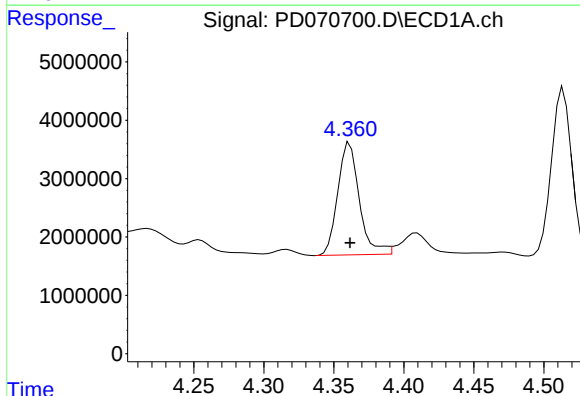


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 20680082
Conc: 248.35 ng/ml

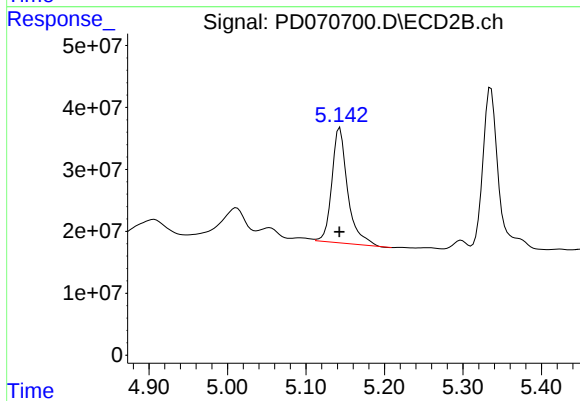

#23 Chlordane-1


R.T.: 5.143 min
Delta R.T.: 0.000 min
Response: 260667146
Conc: 259.02 ng/ml

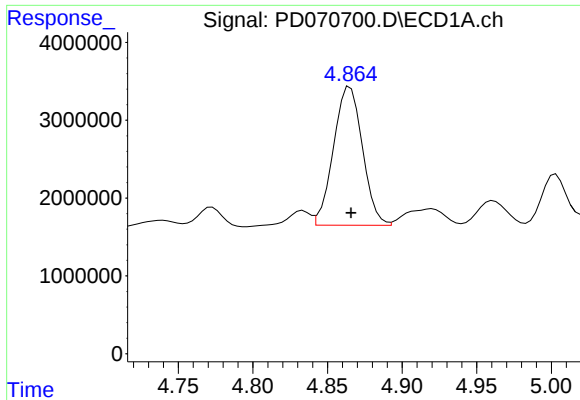

#24 Chlordane-2


R.T.: 4.865 min
Delta R.T.: 0.000 min
Response: 24124890
Conc: 252.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

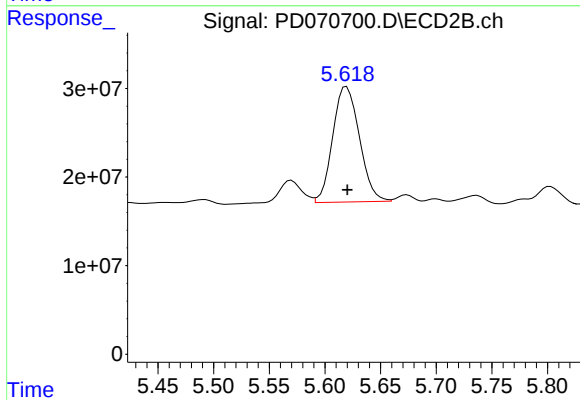


#24 Chlordane-2

R.T.: 5.619 min
Delta R.T.: 0.000 min
Response: 217237758
Conc: 256.03 ng/ml

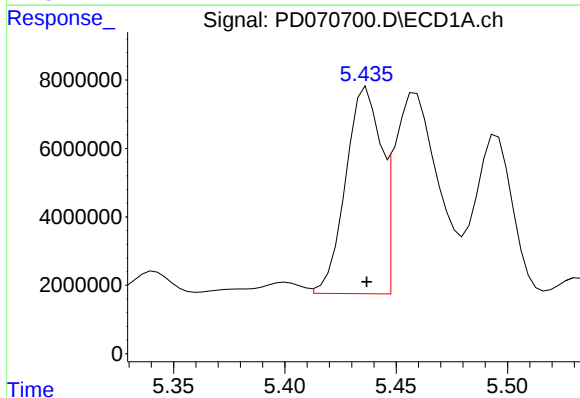


#25 Chlordane-3

R.T.: 5.437 min
Delta R.T.: 0.000 min
Response: 66420762
Conc: 233.60 ng/ml

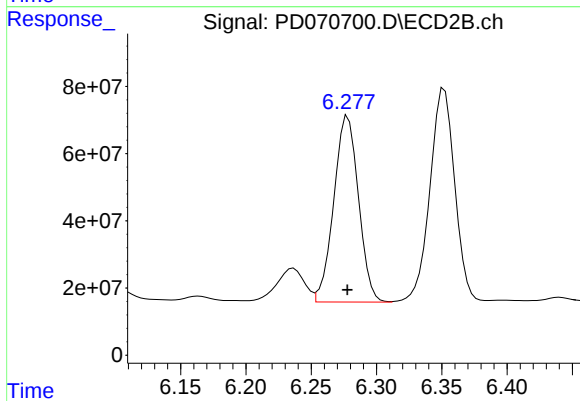

#25 Chlordane-3


R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 730873950
Conc: 245.54 ng/ml

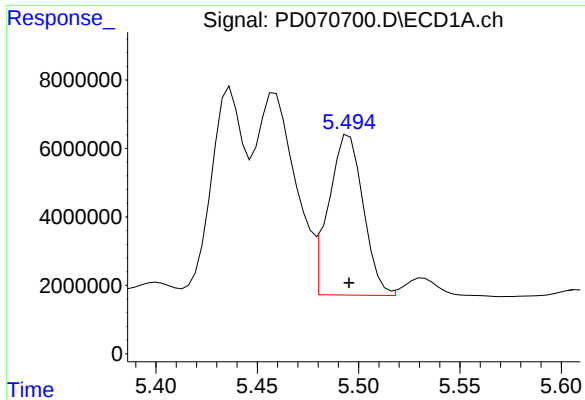

#26 Chlordane-4


R.T.: 5.495 min
Delta R.T.: 0.000 min
Response: 55363163
Conc: 239.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

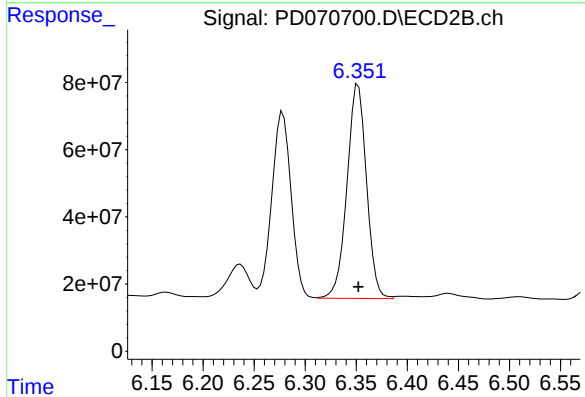


#26 Chlordane-4

R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 848578941
Conc: 247.80 ng/ml

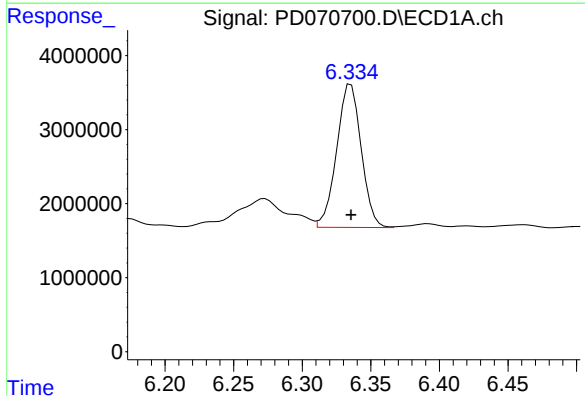


#27 Chlordane-5

R.T.: 6.336 min
Delta R.T.: 0.000 min
Response: 24101856
Conc: 242.98 ng/ml

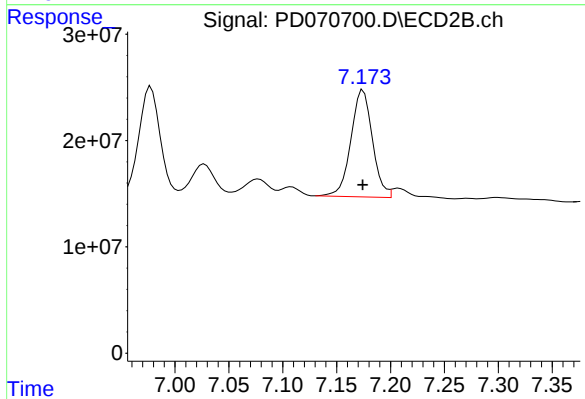

#27 Chlordane-5


R.T.: 7.175 min
Delta R.T.: 0.000 min
Response: 140161541
Conc: 249.02 ng/ml

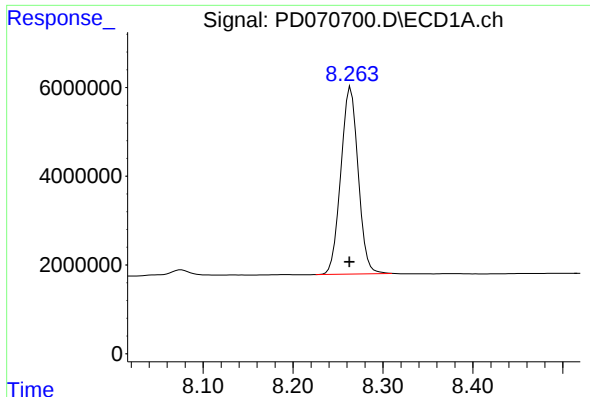

#28 Decachlorobiphenyl

R.T.: 8.264 min
Delta R.T.: 0.001 min
Response: 56404961
Conc: 24.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

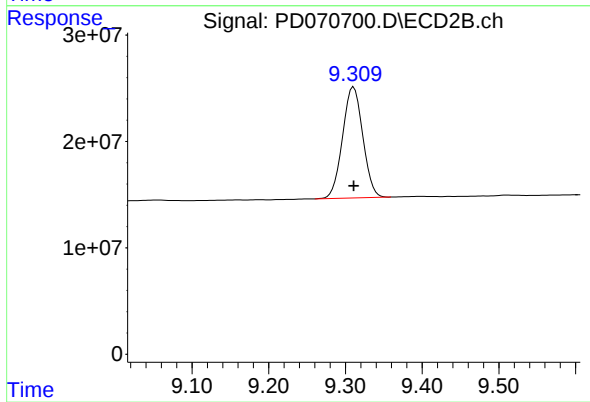

#28 Decachlorobiphenyl

R.T.: 9.311 min
Delta R.T.: 0.000 min
Response: 192417673
Conc: 25.25 ng/ml