

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070522\
 Data File : PD070708.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2022 16:14
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD070522CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 05 16:44:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070522.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 05 15:26:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	4.124	129.6E6	1134.4E6	53.090	43.866
28)	SA Decachlor...	8.264	9.313	115.3E6	391.9E6	46.490	47.634
Target Compounds							
23)	Chlordane-1	4.362	5.144	42267747	493.7E6	500.559	509.616
24)	Chlordane-2	4.866	5.621	47498873	424.1E6	489.111	491.493
25)	Chlordane-3	5.438	6.279	141.2E6	1494.9E6	505.561	499.282
26)	Chlordane-4	5.496	6.353	115.6E6	1724.5E6	500.665	497.390
27)	Chlordane-5	6.336	7.176	49681127	281.8E6	495.066	513.090



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070522\
Data File : PD070708.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2022 16:14
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD070522CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 05 16:44:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070522.M
Quant Title : GC Extractables
QLast Update : Tue Jul 05 15:26:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

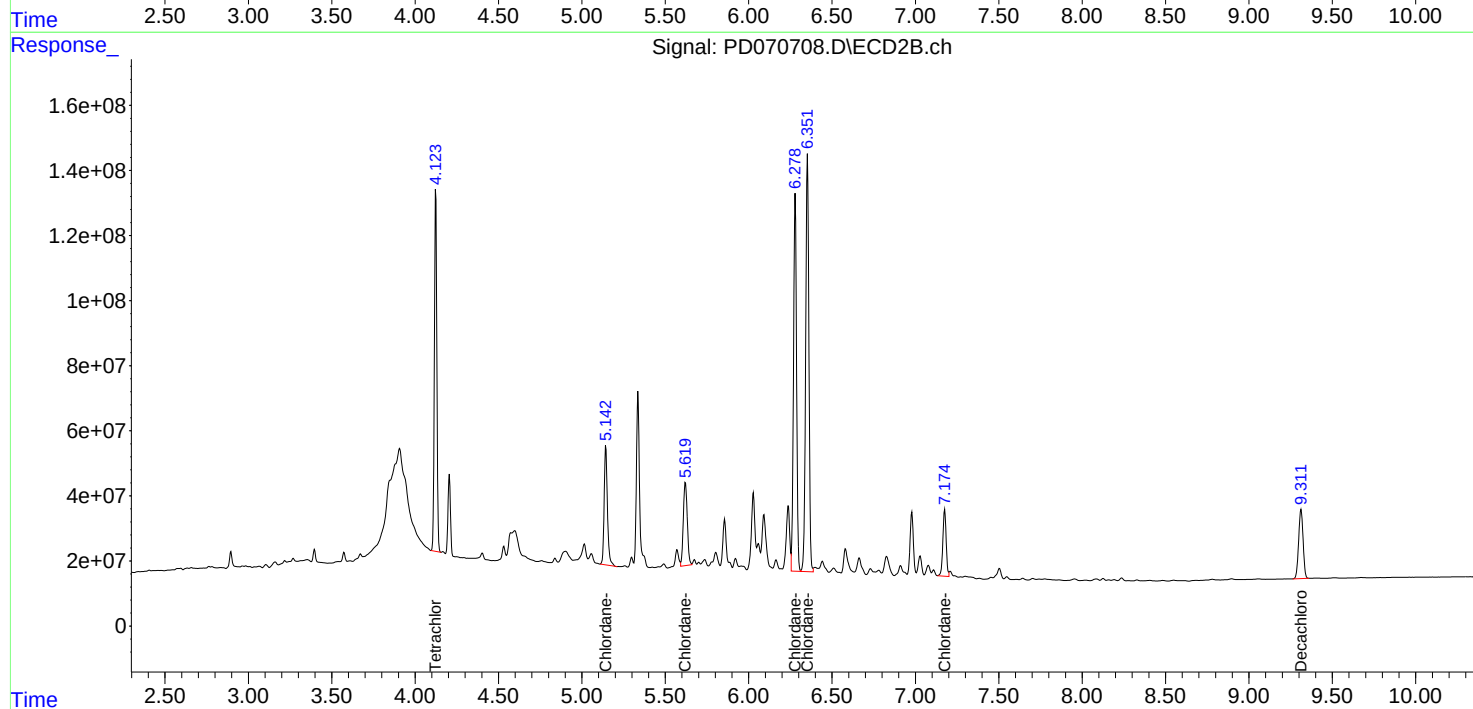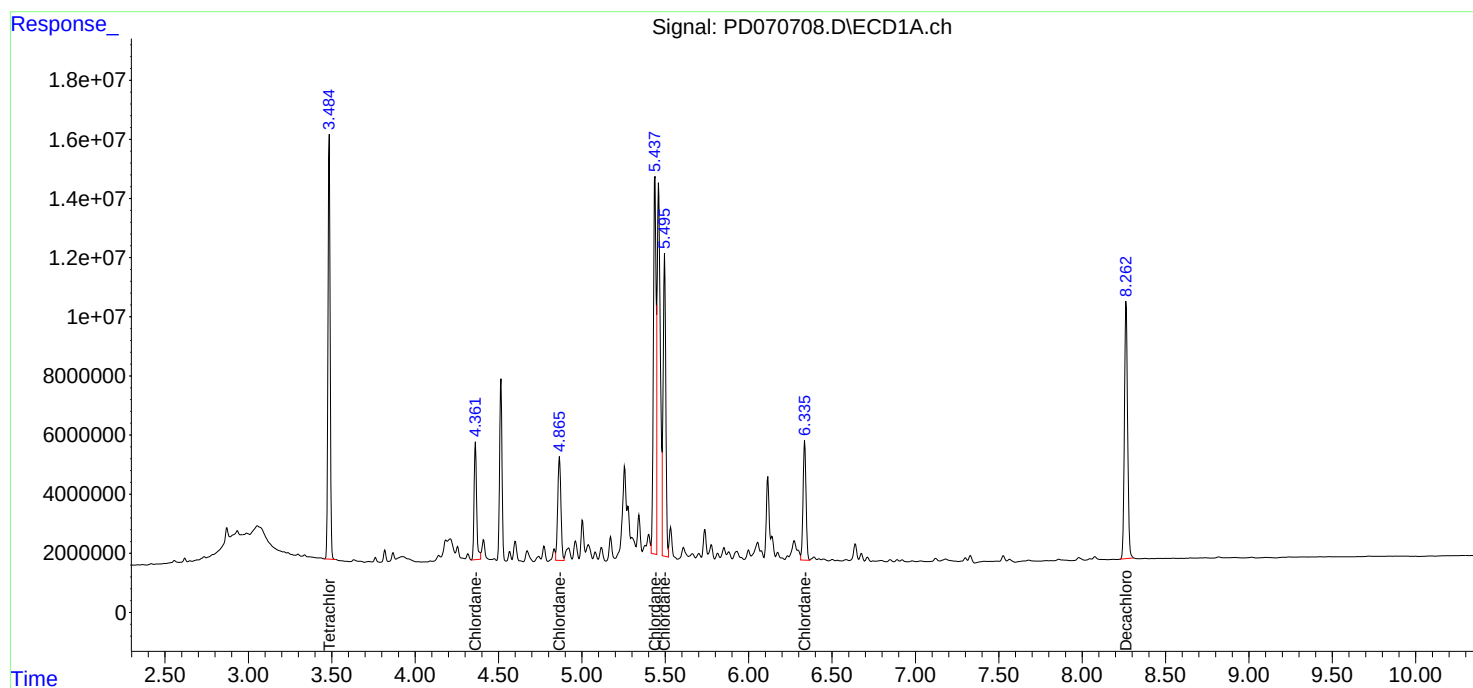


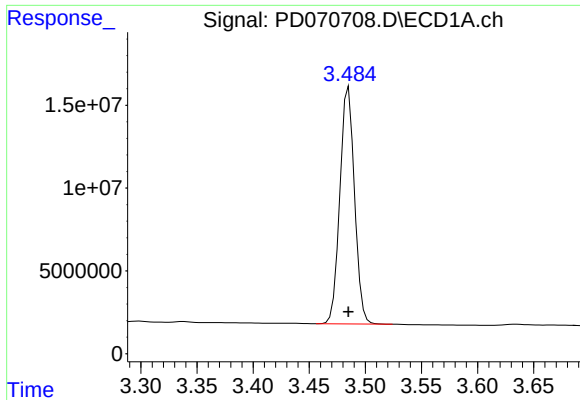

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 129609505
Conc: 53.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD070522CHLOR

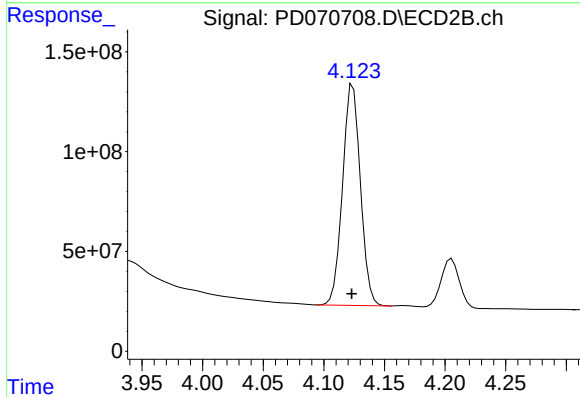


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: 0.001 min
Response: 1134413584
Conc: 43.87 ng/ml

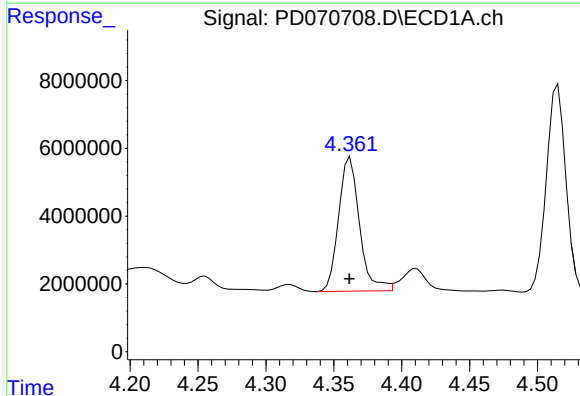


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 42267747
Conc: 500.56 ng/ml

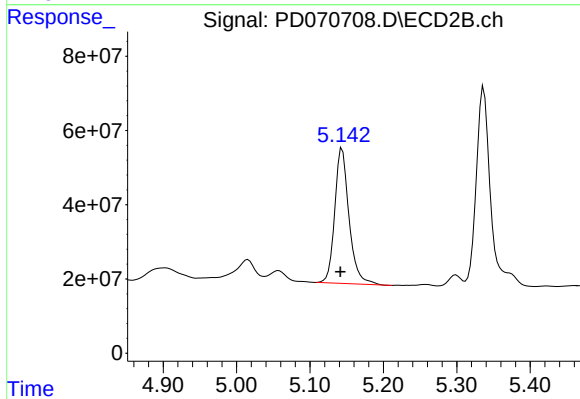

#23 Chlordane-1


R.T.: 5.144 min
Delta R.T.: 0.003 min
Response: 493652443
Conc: 509.62 ng/ml

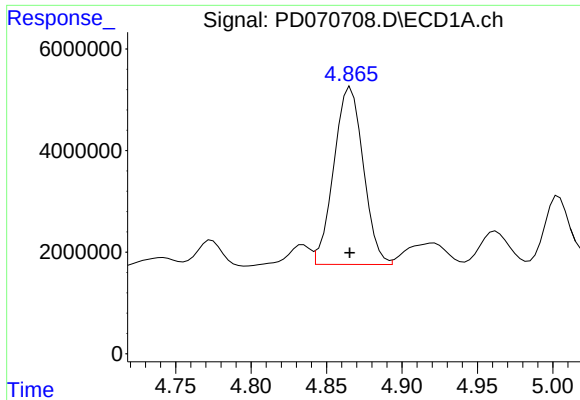

#24 Chlordane-2


R.T.: 4.866 min
Delta R.T.: 0.000 min
Response: 47498873
Conc: 489.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD070522CHLOR

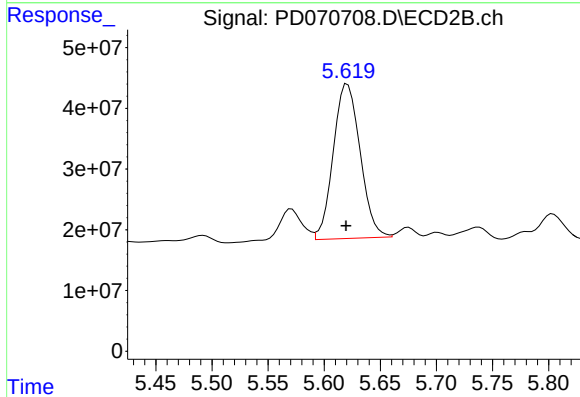


#24 Chlordane-2

R.T.: 5.621 min
Delta R.T.: 0.001 min
Response: 424117966
Conc: 491.49 ng/ml

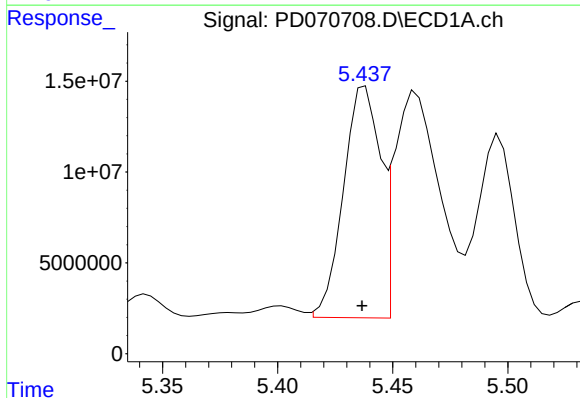


#25 Chlordane-3

R.T.: 5.438 min
Delta R.T.: 0.002 min
Response: 141156975
Conc: 505.56 ng/ml

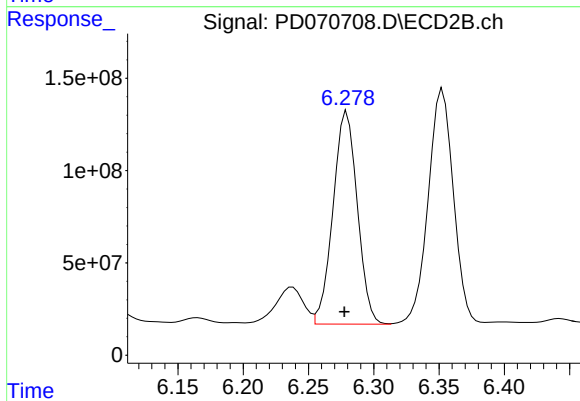

#25 Chlordane-3


R.T.: 6.279 min
Delta R.T.: 0.002 min
Response: 1494855718
Conc: 499.28 ng/ml

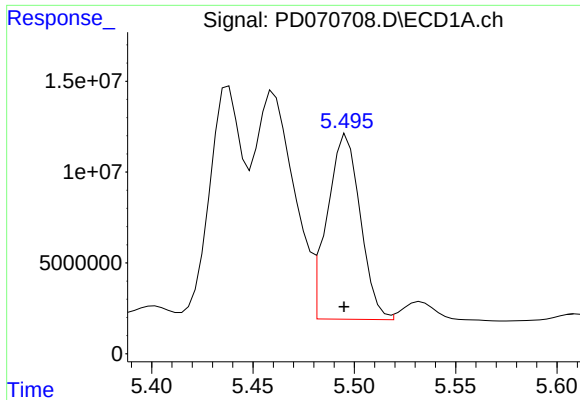

#26 Chlordane-4


R.T.: 5.496 min
Delta R.T.: 0.001 min
Response: 115554867
Conc: 500.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD070522CHLOR

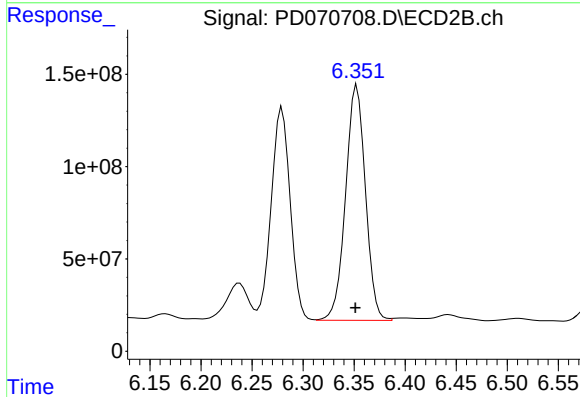


#26 Chlordane-4

R.T.: 6.353 min
Delta R.T.: 0.001 min
Response: 1724513994
Conc: 497.39 ng/ml

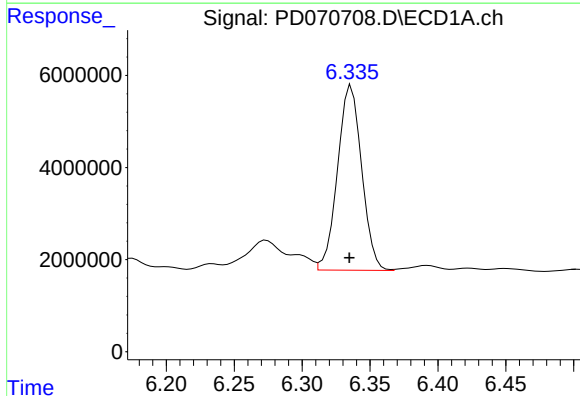


#27 Chlordane-5

R.T.: 6.336 min
Delta R.T.: 0.001 min
Response: 49681127
Conc: 495.07 ng/ml

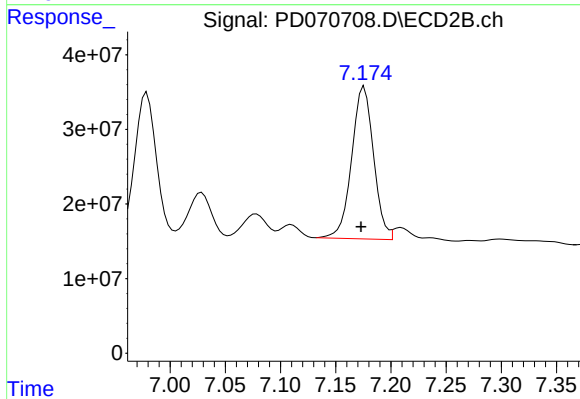

#27 Chlordane-5

R.T.: 7.176 min
Delta R.T.: 0.003 min
Response: 281760432
Conc: 513.09 ng/ml

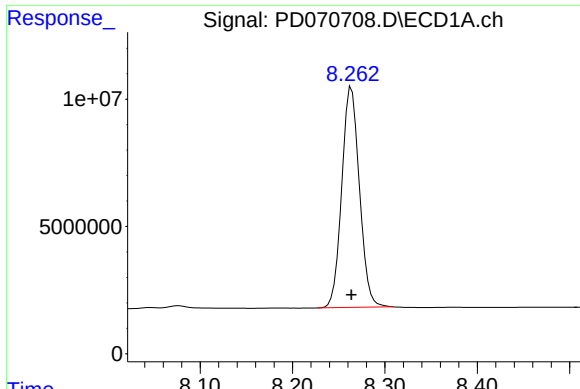

#28 Decachlorobiphenyl


R.T.: 8.264 min

Delta R.T.: 0.000 min

Response: 115274293

Conc: 46.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD070522CHLOR

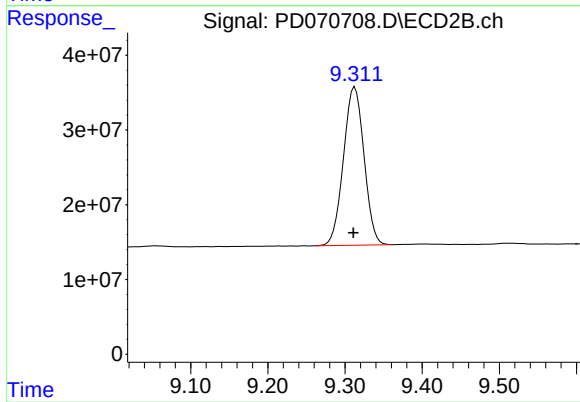

#28 Decachlorobiphenyl

R.T.: 9.313 min

Delta R.T.: 0.002 min

Response: 391882739

Conc: 47.63 ng/ml