

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070523\
 Data File : PD076326.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2023 08:39
 Operator : AR\AJ
 Sample : RESC396
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC012

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 01:18:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 05 14:30:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.766	44268298	21146188	20.416	20.548
2)	SA Decachlor...	9.085	7.908	98797228	37239433	38.949	40.810
Target Compounds							
2)	A alpha-BHC	4.002	3.267	34289554	14882675	9.443	9.698
3)	MA gamma-BHC...	4.335	3.597	32717686	14143460	9.632	9.828
4)	MA Heptachlor	4.926	3.937	34549650	14403503	9.682	9.965
5)	MB Aldrin	5.269	4.217	34464814	14496409	10.025	10.243
6)	B beta-BHC	4.532	3.894	15825036	6765346	10.455	10.089
7)	B delta-BHC	4.780	4.123	32195664	13894847	9.430	9.773
8)	B Heptachlo...	5.696	4.719	31755629	13266879	9.960	10.027
9)	A Endosulfan I	6.083	5.090	28977709	11674755	9.973	10.091
10)	B trans-Chl...	5.953	4.970	30115621	12733316	9.762	10.082
11)	B cis-Chlor...	6.032	5.034	31496355	13003622	9.877	10.024
12)	B 4,4'-DDE	6.205	5.223	54591880	20975290	18.767	19.648
13)	MA Dieldrin	6.359	5.354	61378572	25949569	19.036	19.674
14)	MA Endrin	6.590	5.630	49467544	22486525	19.168	19.844
15)	B Endosulfa...	6.809	5.924	53190063	22393823	19.676	20.148
16)	A 4,4'-DDD	6.723	5.777	43755705	16360667	19.162	20.251
17)	MA 4,4'-DDT	7.039	6.029	42498722	15885338	18.769	19.059
18)	B Endrin al...	6.939	6.103	30837401	13214783	17.135	18.037
19)	B Endosulfa...	7.175	6.326	50341585	20866638	19.887	20.367
20)	A Methoxychlor	7.514	6.604	131.6E6	46168394	98.606	101.193
21)	B Endrin ke...	7.660	6.833	57733566	25119315	20.238	21.319

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070523\
Data File : PD076326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2023 08:39
Operator : AR\AJ
Sample : RESC396
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 01:18:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 14:30:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

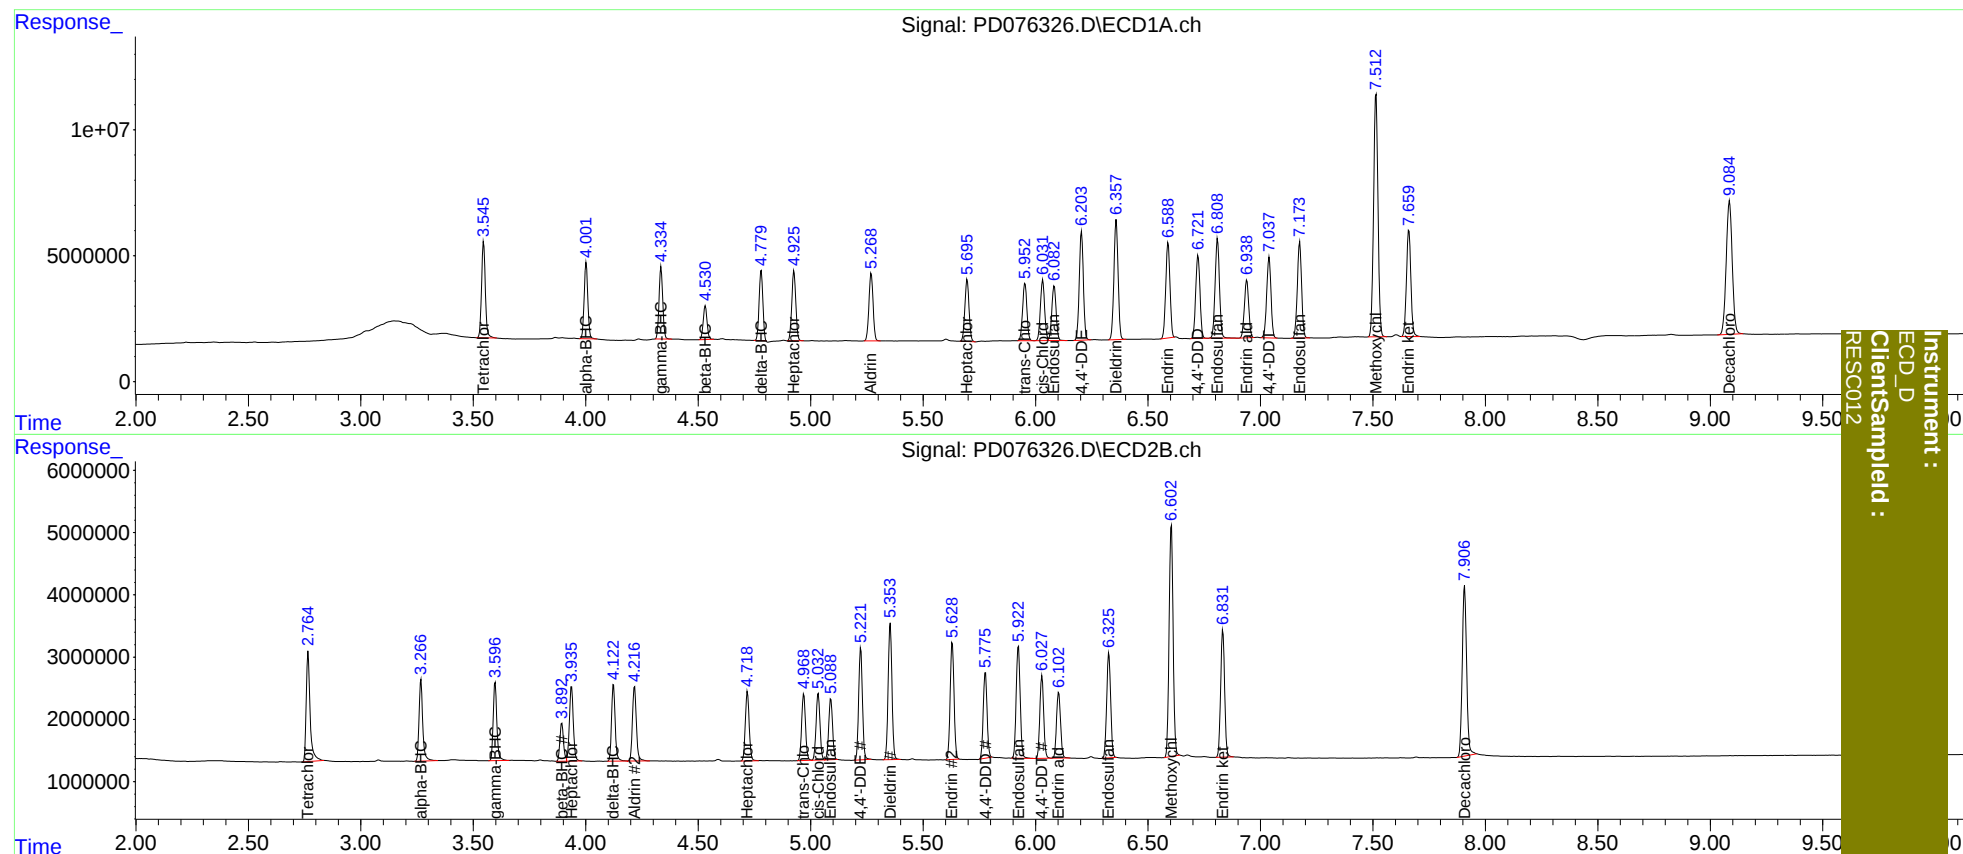

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070523\
Data File : PD076326.D
Acq On : 05 Jul 2023 08:39
Operator : AR\AJ
Sample : RESC396
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC012

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
Title : GC Extractables
Last Update : Wed Jul 05 14:30:19 2023
Integrator: ChemStation

RT#1	RT#2	Resolution
3.546	4.002	100.00%
4.002	4.335	100.00%
4.335	4.532	100.00%
4.532	4.780	100.00%
4.780	4.926	100.00%
4.926	5.269	100.00%
5.269	5.696	100.00%
5.696	5.953	100.00%
5.953	6.032	100.00%
6.032	6.083	96.69%
6.083	6.205	100.00%
6.205	6.359	100.00%
6.359	6.590	100.00%
6.590	6.723	100.00%
6.723	6.809	100.00%
6.809	6.939	100.00%
6.939	7.039	100.00%
7.039	7.175	100.00%
7.175	7.514	100.00%
7.514	7.660	100.00%
7.660	9.085	100.00%

Signal #2


2.766	3.267	100.00%
3.267	3.597	100.00%
3.597	3.894	100.00%
3.894	3.937	92.17%
3.937	4.123	100.00%
4.123	4.217	99.69%
4.217	4.719	100.00%
4.719	4.970	100.00%
4.970	5.034	100.00%
5.034	5.090	99.41%
5.090	5.223	100.00%
5.223	5.354	100.00%
5.354	5.630	100.00%
5.630	5.777	100.00%
5.777	5.924	100.00%
5.924	6.029	100.00%
6.029	6.103	100.00%
6.103	6.326	100.00%
6.326	6.604	100.00%
6.604	6.833	100.00%
6.833	7.908	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070523\
Data File : PD076326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2023 08:39
Operator : AR\AJ
Sample : RESC396
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC012

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 01:18:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 14:30:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

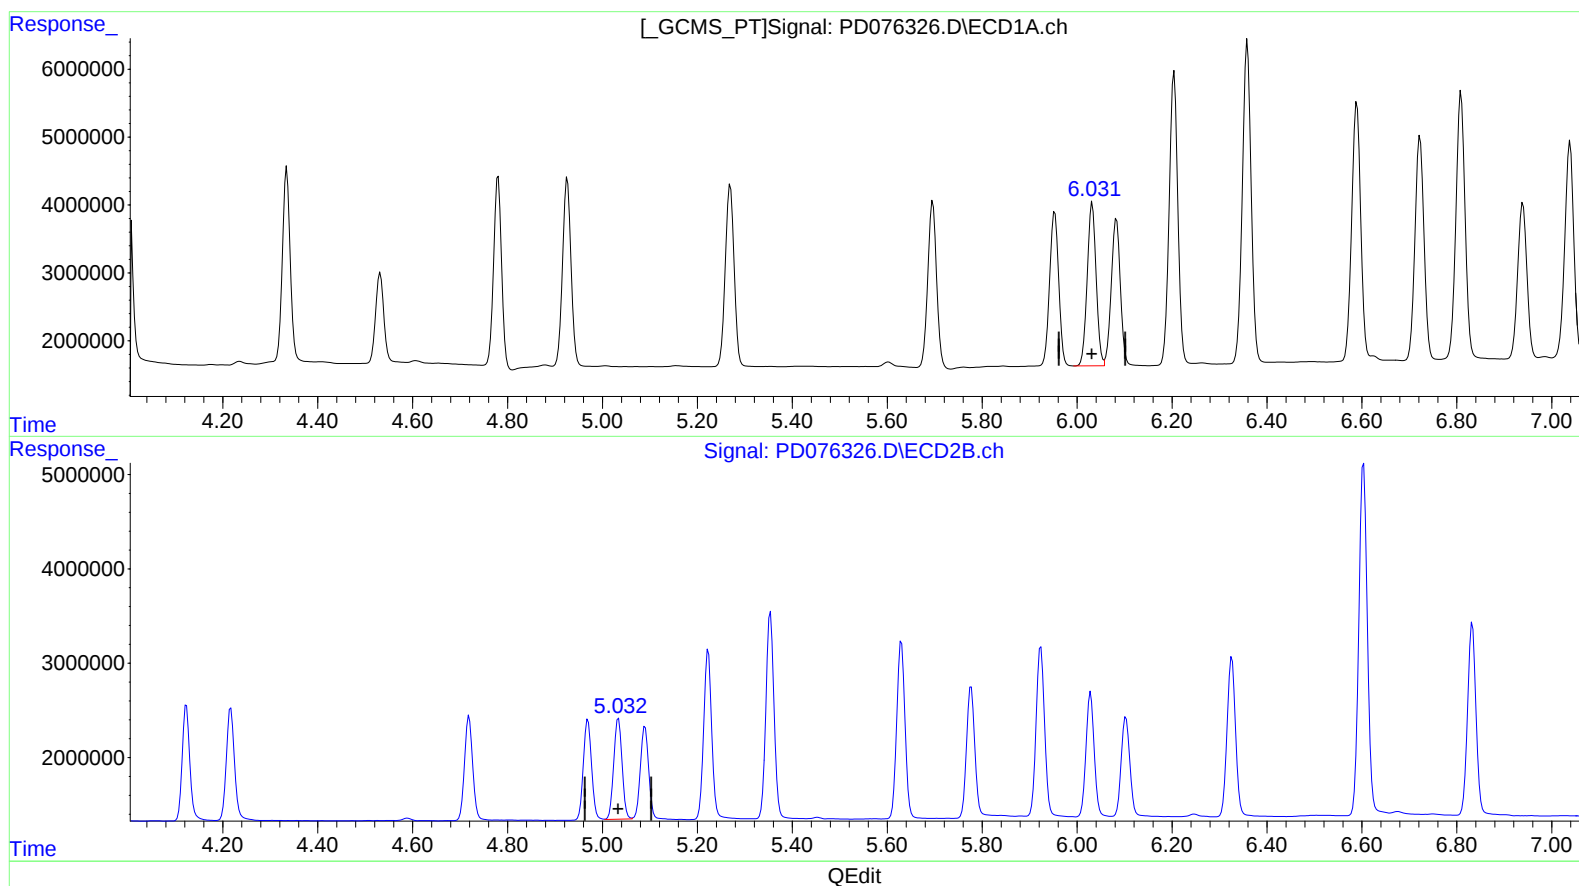

(11) cis-Chlordane (B)

6.032min 9.877 ng/ml

response 31496355

(11) cis-Chlordane #2 (B)

5.034min 10.024 ng/ml


response 13003622

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070523\
Data File : PD076326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2023 08:39
Operator : AR\AJ
Sample : RESC396
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC012

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 01:18:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 14:30:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

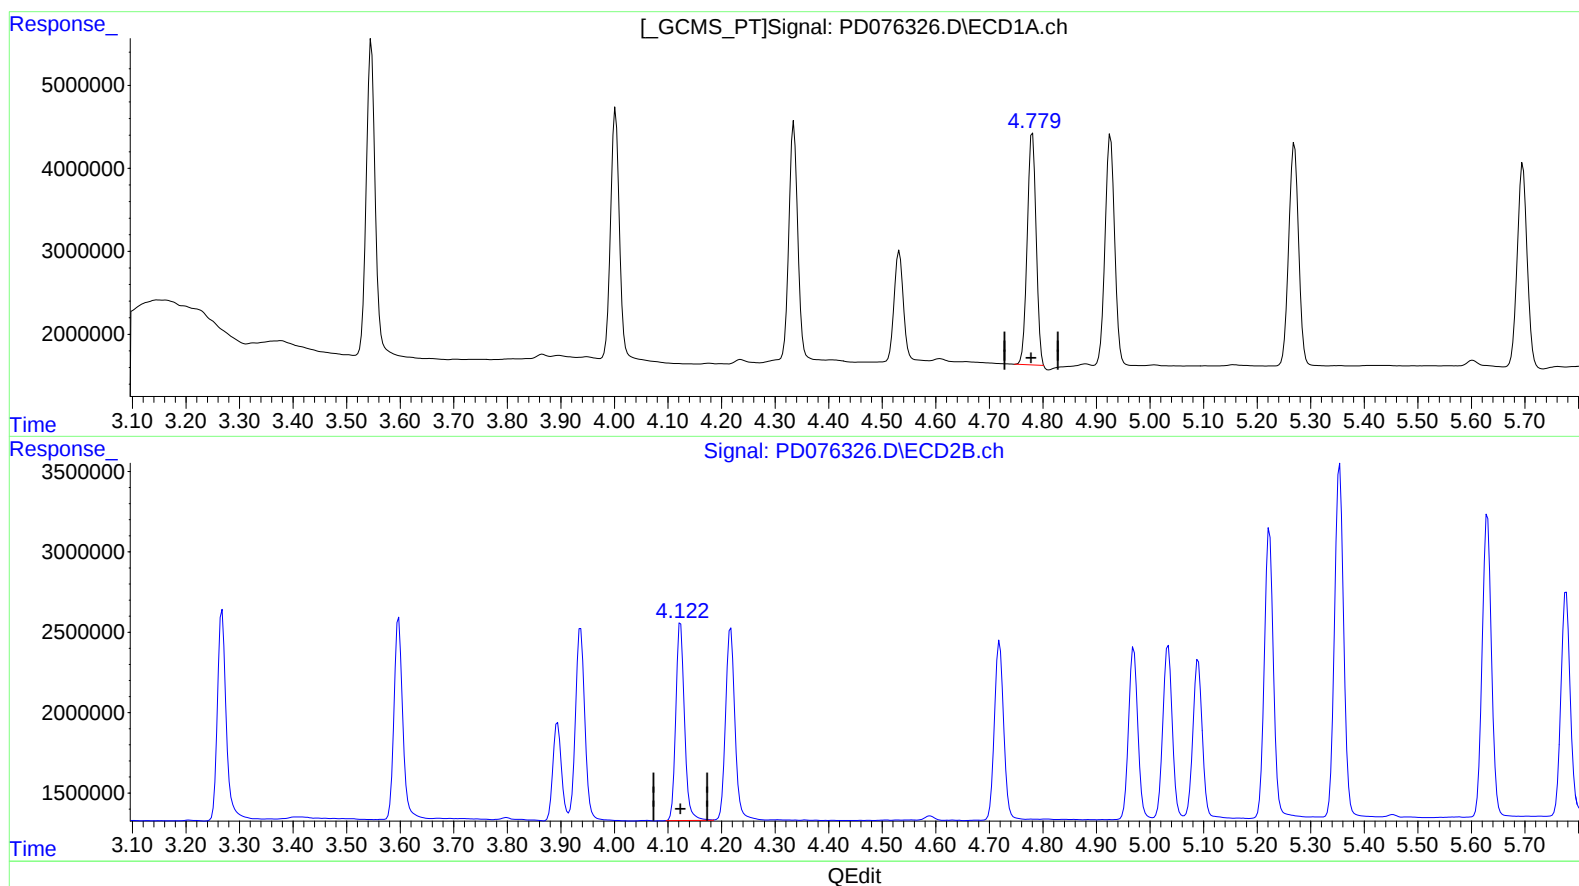

(7) delta-BHC (B)

4.780min 9.430 ng/ml

response 32195664

(7) delta-BHC #2 (B)

4.123min 9.773 ng/ml


response 13894847

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070523\
Data File : PD076326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2023 08:39
Operator : AR\AJ
Sample : RESC396
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC012

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 01:18:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 14:30:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

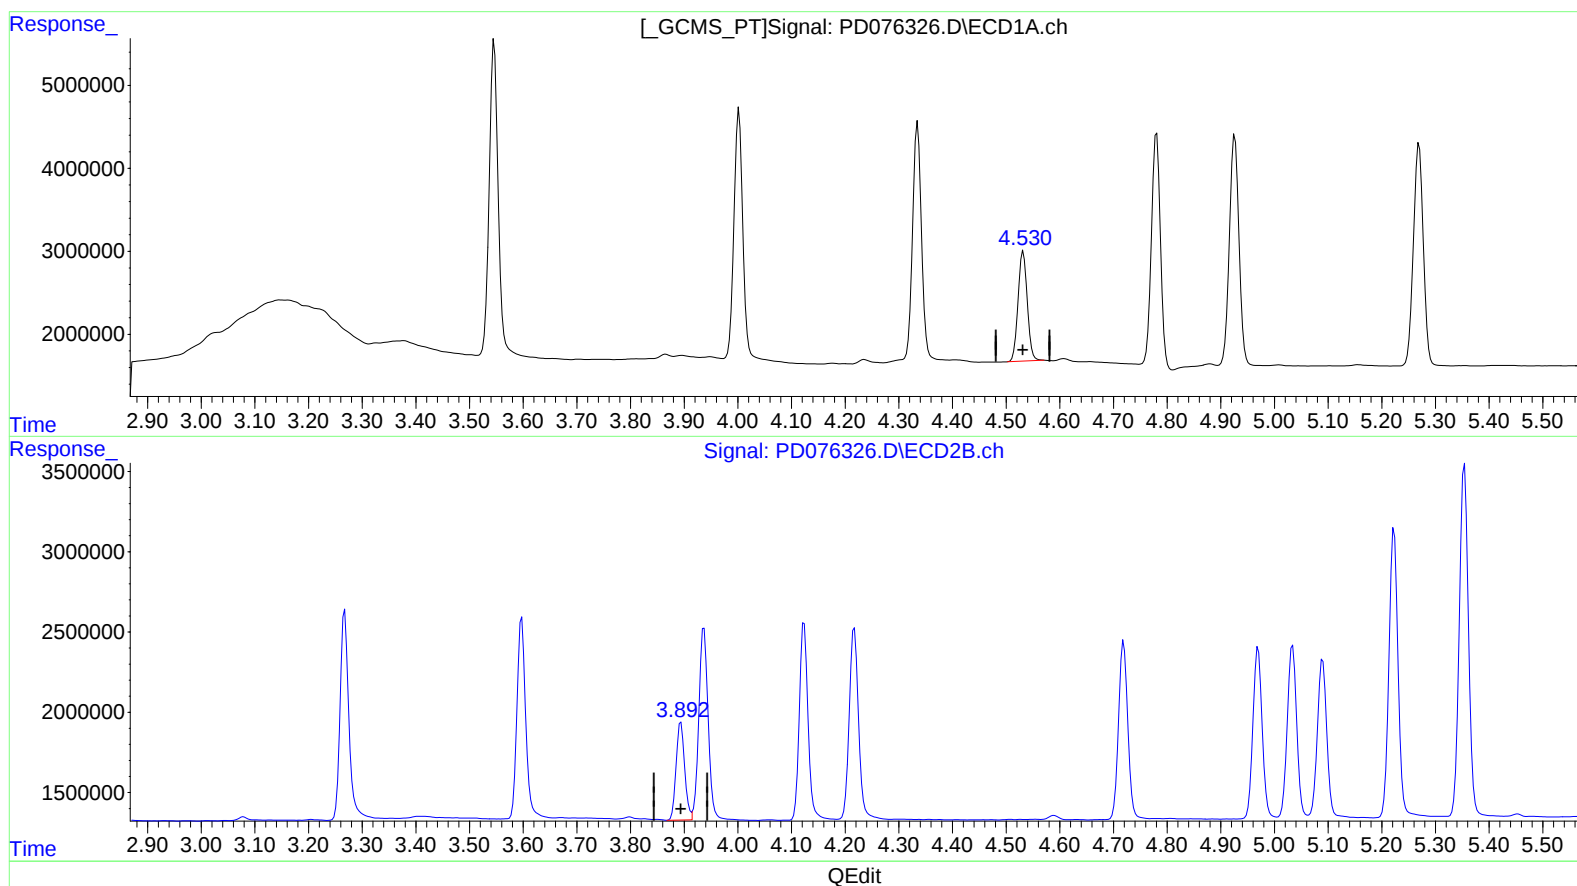

(6) beta-BHC (B)

4.532min 10.455 ng/ml

response 15825036

(6) beta-BHC #2 (B)

3.894min 10.089 ng/ml


response 6765346

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070523\
Data File : PD076326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2023 08:39
Operator : AR\AJ
Sample : RESC396
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC012

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 01:18:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 14:30:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

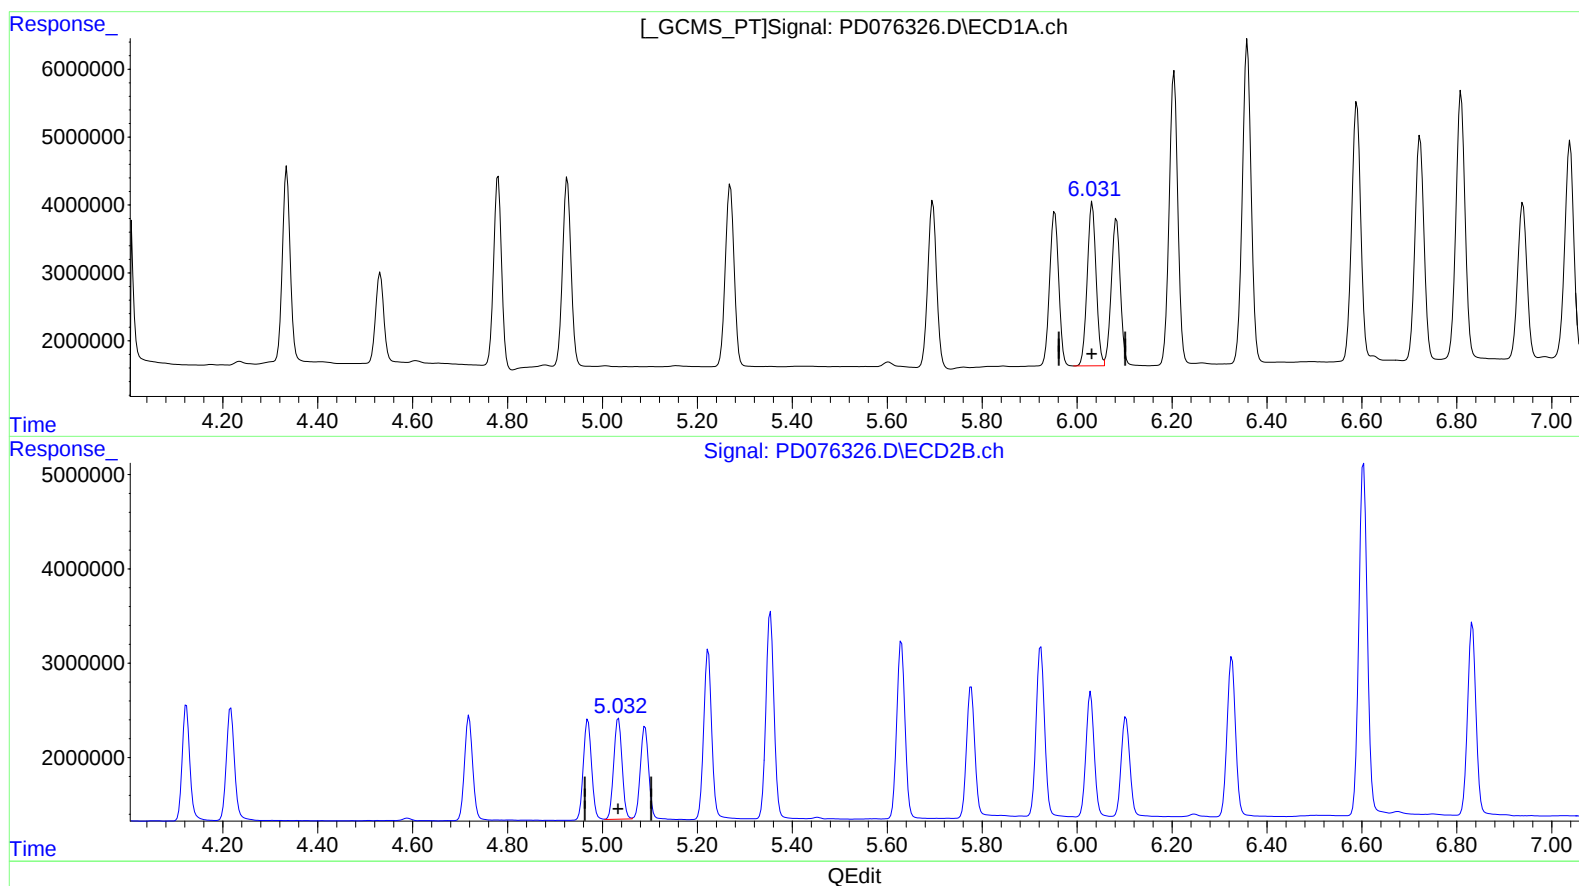

(11) cis-Chlordane (B)

6.032min 9.877 ng/ml

response 31496355

(11) cis-Chlordane #2 (B)

5.034min 10.024 ng/ml

response 13003622