

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070621\
 Data File : PD064088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2021 18:03
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 05:32:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070621CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 07 05:31:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.066	3.515	15195284	89208059	10.685	11.221
27)	SA Decachlor...	9.249	8.265	29390558	110.9E6	21.840	22.295
Target Compounds							
2)	A alpha-BHC	4.468	3.955	20684429	115.8E6	10.347	11.151
3)	MA gamma-BHC...	4.761	4.237	19918638	108.8E6	10.455	11.368
4)	MA Heptachlor	5.274	4.538	19711299	102.3E6	10.364	11.017
9)	A Endosulfan I	6.343	5.566	15182432	84566474	10.233	11.756
13)	MA Dieldrin	6.605	5.809	31105170	155.1E6	20.704	21.554
14)	MA Endrin	6.827	6.067	26163436	133.6E6	20.954	21.878
16)	A 4,4'-DDD	6.951	6.188	27339248	122.9E6	20.536	21.352
17)	MA 4,4'-DDT	7.253	6.430	26122622	129.1E6	20.258	21.582
20)	A Methoxychlor	7.719	6.977	73102642	304.5E6	105.410	109.765


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070621\
Data File : PD064088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2021 18:03
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 05:32:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070621CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 07 05:31:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

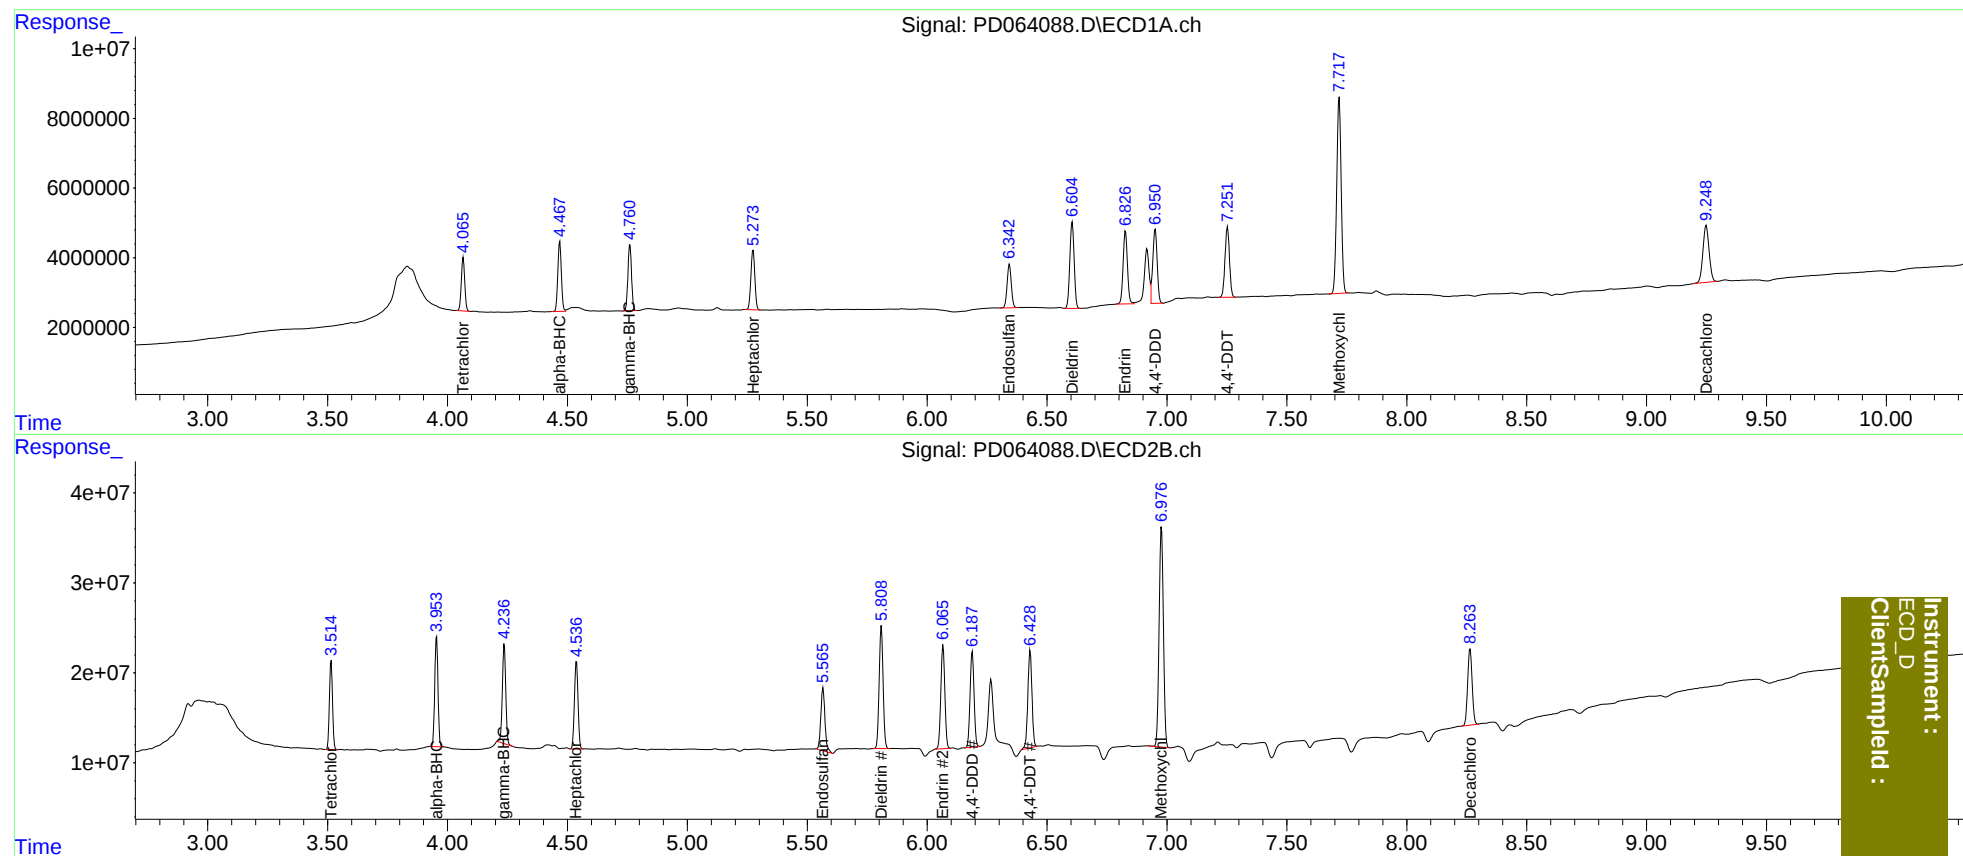


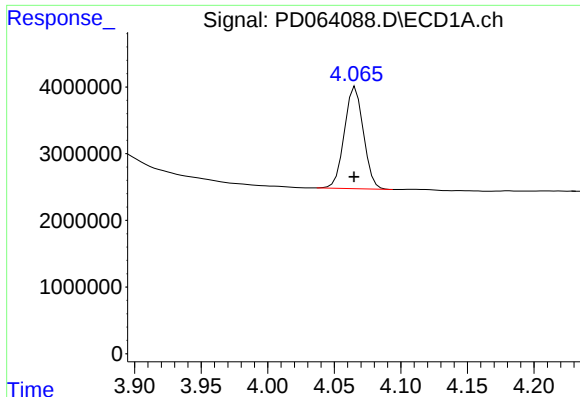

#1 Tetrachloro-m-xylene


R.T.: 4.066 min
Delta R.T.: 0.000 min
Response: 15195284
Conc: 10.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

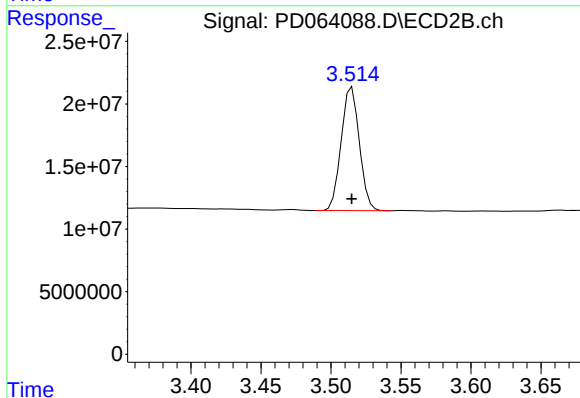


#1 Tetrachloro-m-xylene

R.T.: 3.515 min
Delta R.T.: 0.000 min
Response: 89208059
Conc: 11.22 ng/ml

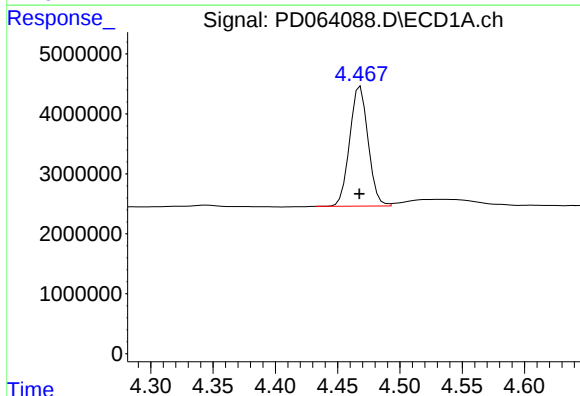


#2 alpha-BHC

R.T.: 4.468 min
Delta R.T.: 0.000 min
Response: 20684429
Conc: 10.35 ng/ml

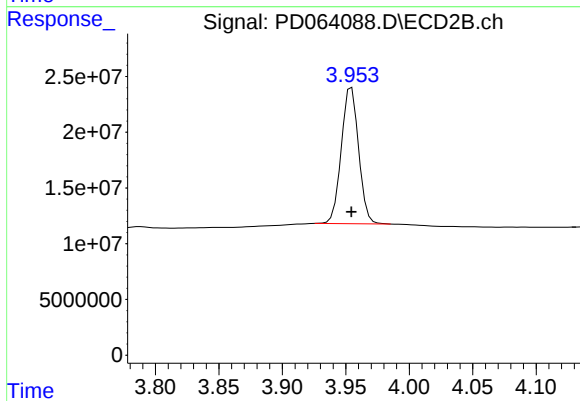

#2 alpha-BHC


R.T.: 3.955 min
Delta R.T.: 0.000 min
Response: 115817726
Conc: 11.15 ng/ml

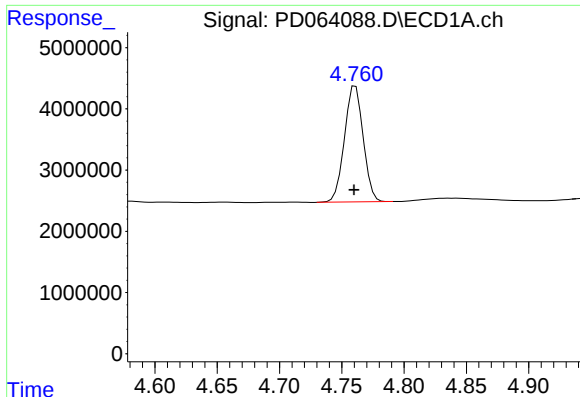

#3 gamma-BHC (Lindane)


R.T.: 4.761 min
Delta R.T.: 0.001 min
Response: 19918638
Conc: 10.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

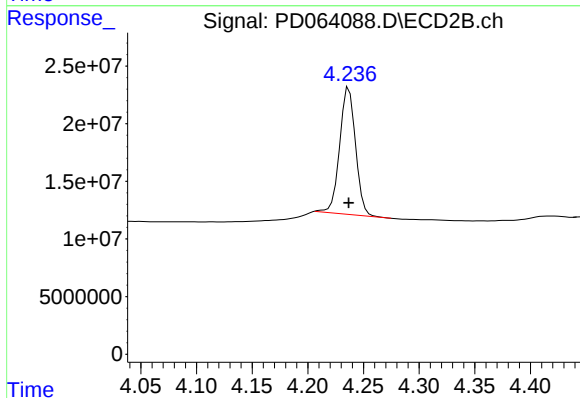


#3 gamma-BHC (Lindane)

R.T.: 4.237 min
Delta R.T.: 0.000 min
Response: 108799862
Conc: 11.37 ng/ml

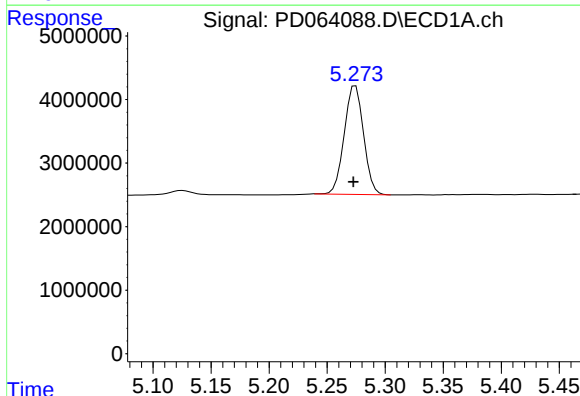


#4 Heptachlor

R.T.: 5.274 min
Delta R.T.: 0.002 min
Response: 19711299
Conc: 10.36 ng/ml

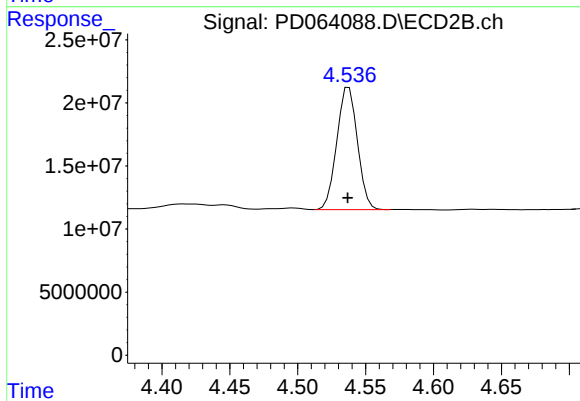

#4 Heptachlor


R.T.: 4.538 min
Delta R.T.: 0.000 min
Response: 102254531
Conc: 11.02 ng/ml

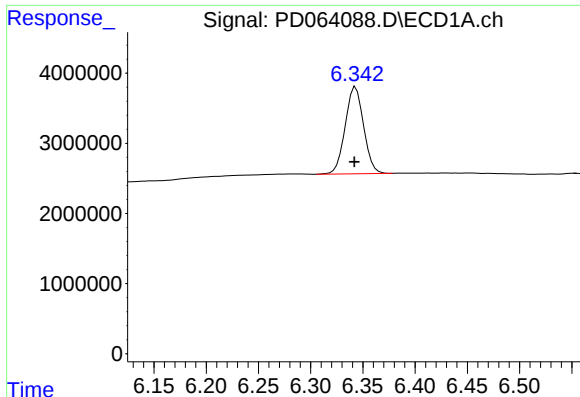

#9 Endosulfan I


R.T.: 6.343 min
Delta R.T.: 0.001 min
Response: 15182432
Conc: 10.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

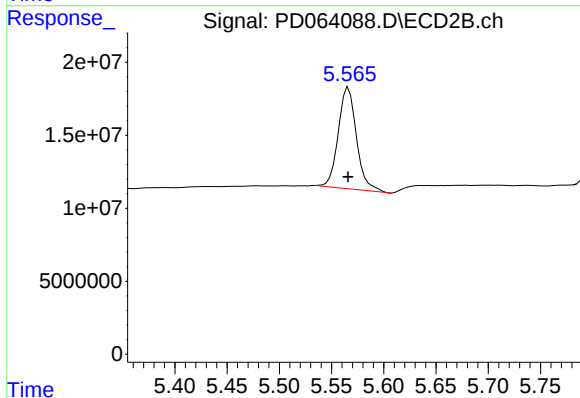


#9 Endosulfan I

R.T.: 5.566 min
Delta R.T.: 0.000 min
Response: 84566474
Conc: 11.76 ng/ml

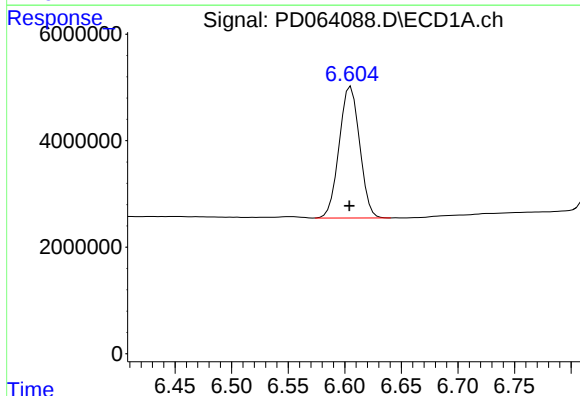


#13 Dieldrin

R.T.: 6.605 min
Delta R.T.: 0.001 min
Response: 31105170
Conc: 20.70 ng/ml

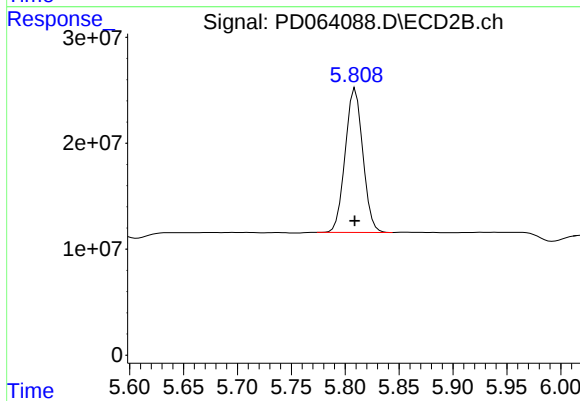

#13 Dieldrin


R.T.: 5.809 min
Delta R.T.: 0.000 min
Response: 155077869
Conc: 21.55 ng/ml

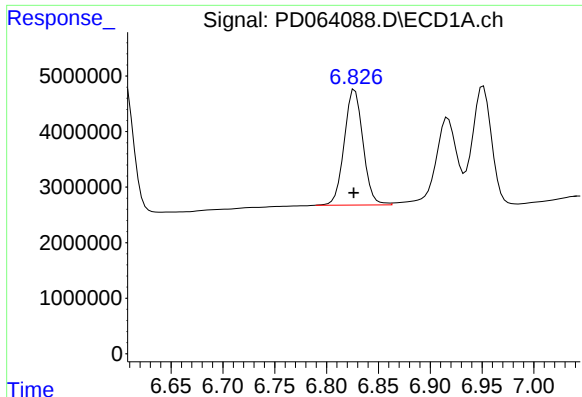

#14 Endrin


R.T.: 6.827 min
Delta R.T.: 0.001 min
Response: 26163436
Conc: 20.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

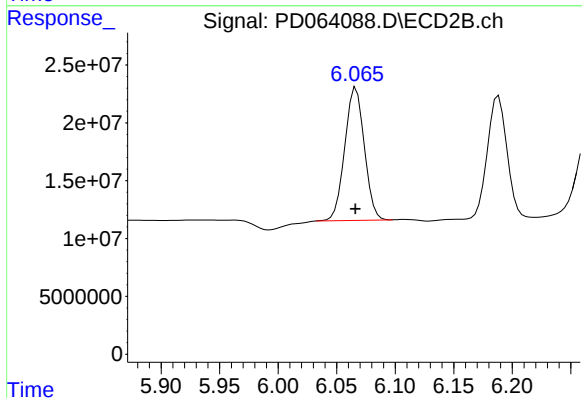


#14 Endrin

R.T.: 6.067 min
Delta R.T.: 0.000 min
Response: 133619145
Conc: 21.88 ng/ml

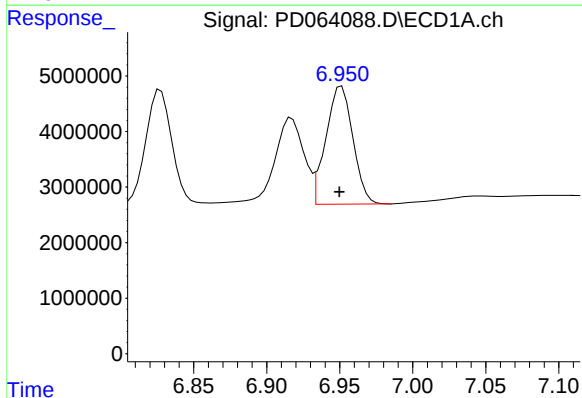


#16 4,4'-DDD

R.T.: 6.951 min
Delta R.T.: 0.002 min
Response: 27339248
Conc: 20.54 ng/ml

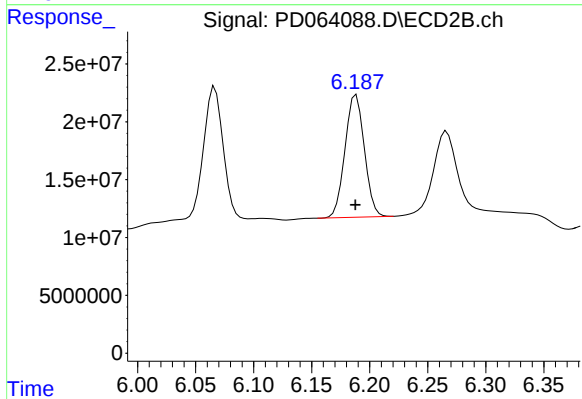

#16 4,4'-DDD


R.T.: 6.188 min
Delta R.T.: 0.000 min
Response: 122907969
Conc: 21.35 ng/ml

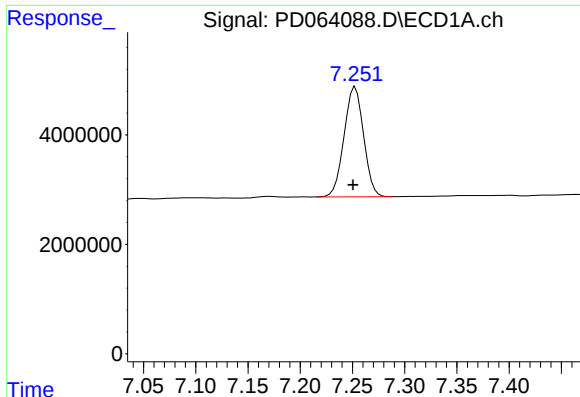

#17 4,4'-DDT


R.T.: 7.253 min
Delta R.T.: 0.002 min
Response: 26122622
Conc: 20.26 ng/ml

Instrument :
ECD_D
ClientSampleId :

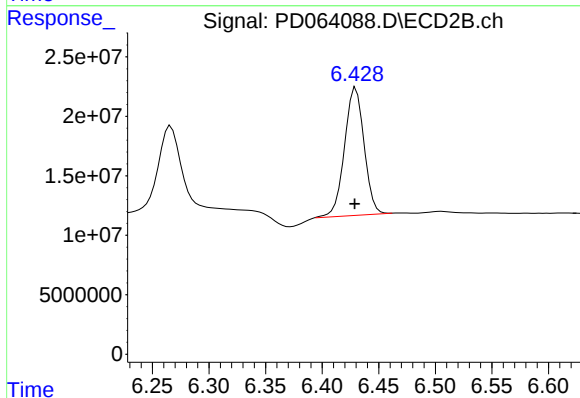


#17 4,4'-DDT

R.T.: 6.430 min
Delta R.T.: 0.001 min
Response: 129119947
Conc: 21.58 ng/ml

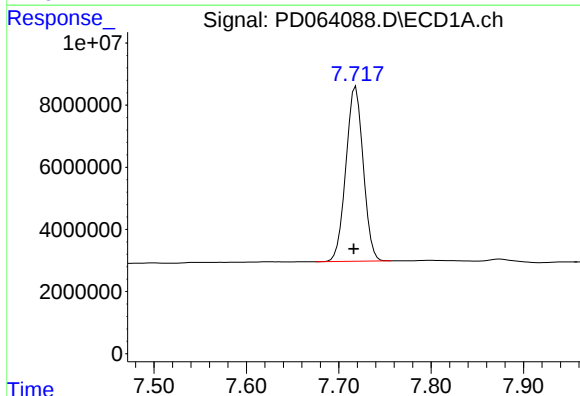


#20 Methoxychlor

R.T.: 7.719 min
Delta R.T.: 0.002 min
Response: 73102642
Conc: 105.41 ng/ml

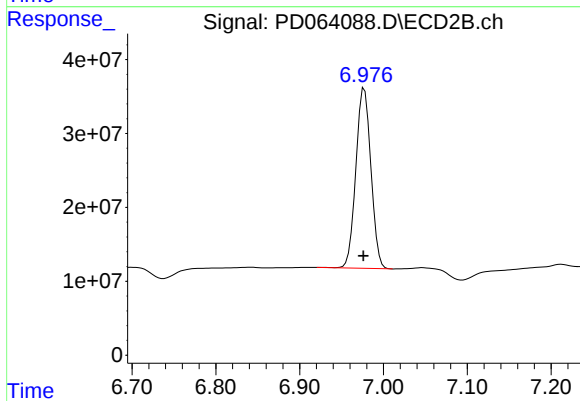

#20 Methoxychlor


R.T.: 6.977 min
Delta R.T.: 0.001 min
Response: 304508478
Conc: 109.76 ng/ml

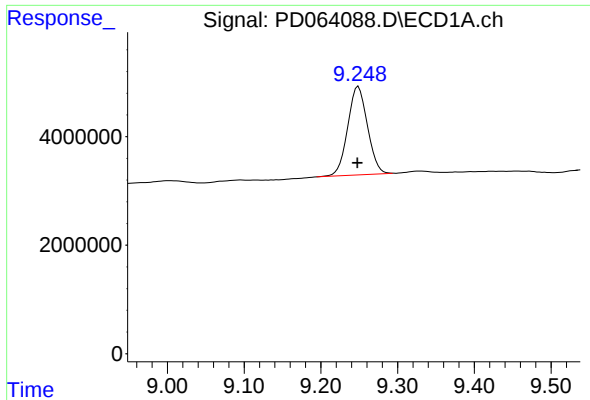

#27 Decachlorobiphenyl

R.T.: 9.249 min
Delta R.T.: 0.001 min
Response: 29390558
Conc: 21.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

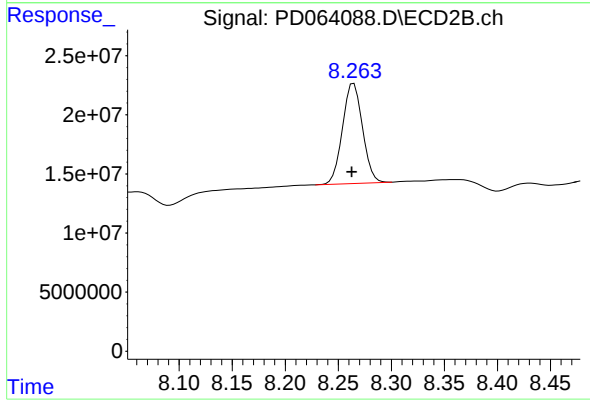

#27 Decachlorobiphenyl

R.T.: 8.265 min
Delta R.T.: 0.002 min
Response: 110888236
Conc: 22.30 ng/ml