

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070621\
 Data File : PD064090.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2021 18:30
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 05:32:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070621CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 07 05:31:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.065	3.515	28442951	159.0E6	20.000	20.000
27)	SA Decachlor...	9.248	8.263	53827918	198.9E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.467	3.954	39980512	207.7E6	20.000	20.000
3)	MA gamma-BHC...	4.760	4.237	38104234	191.4E6	20.000	20.000
4)	MA Heptachlor	5.273	4.537	38039239	185.6E6	20.000	20.000
9)	A Endosulfan I	6.342	5.566	29674615	143.9E6	20.000	20.000
13)	MA Dieldrin	6.604	5.809	60094690	287.8E6	40.000	40.000
14)	MA Endrin	6.826	6.066	49943661	244.3E6	40.000	40.000
16)	A 4,4'-DDD	6.950	6.188	53252490	230.3E6	40.000	40.000
17)	MA 4,4'-DDT	7.251	6.429	51580179	239.3E6	40.000	40.000
20)	A Methoxychlor	7.716	6.976	138.7E6	554.8E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070621\
Data File : PD064090.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2021 18:30
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 05:32:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070621CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 07 05:31:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

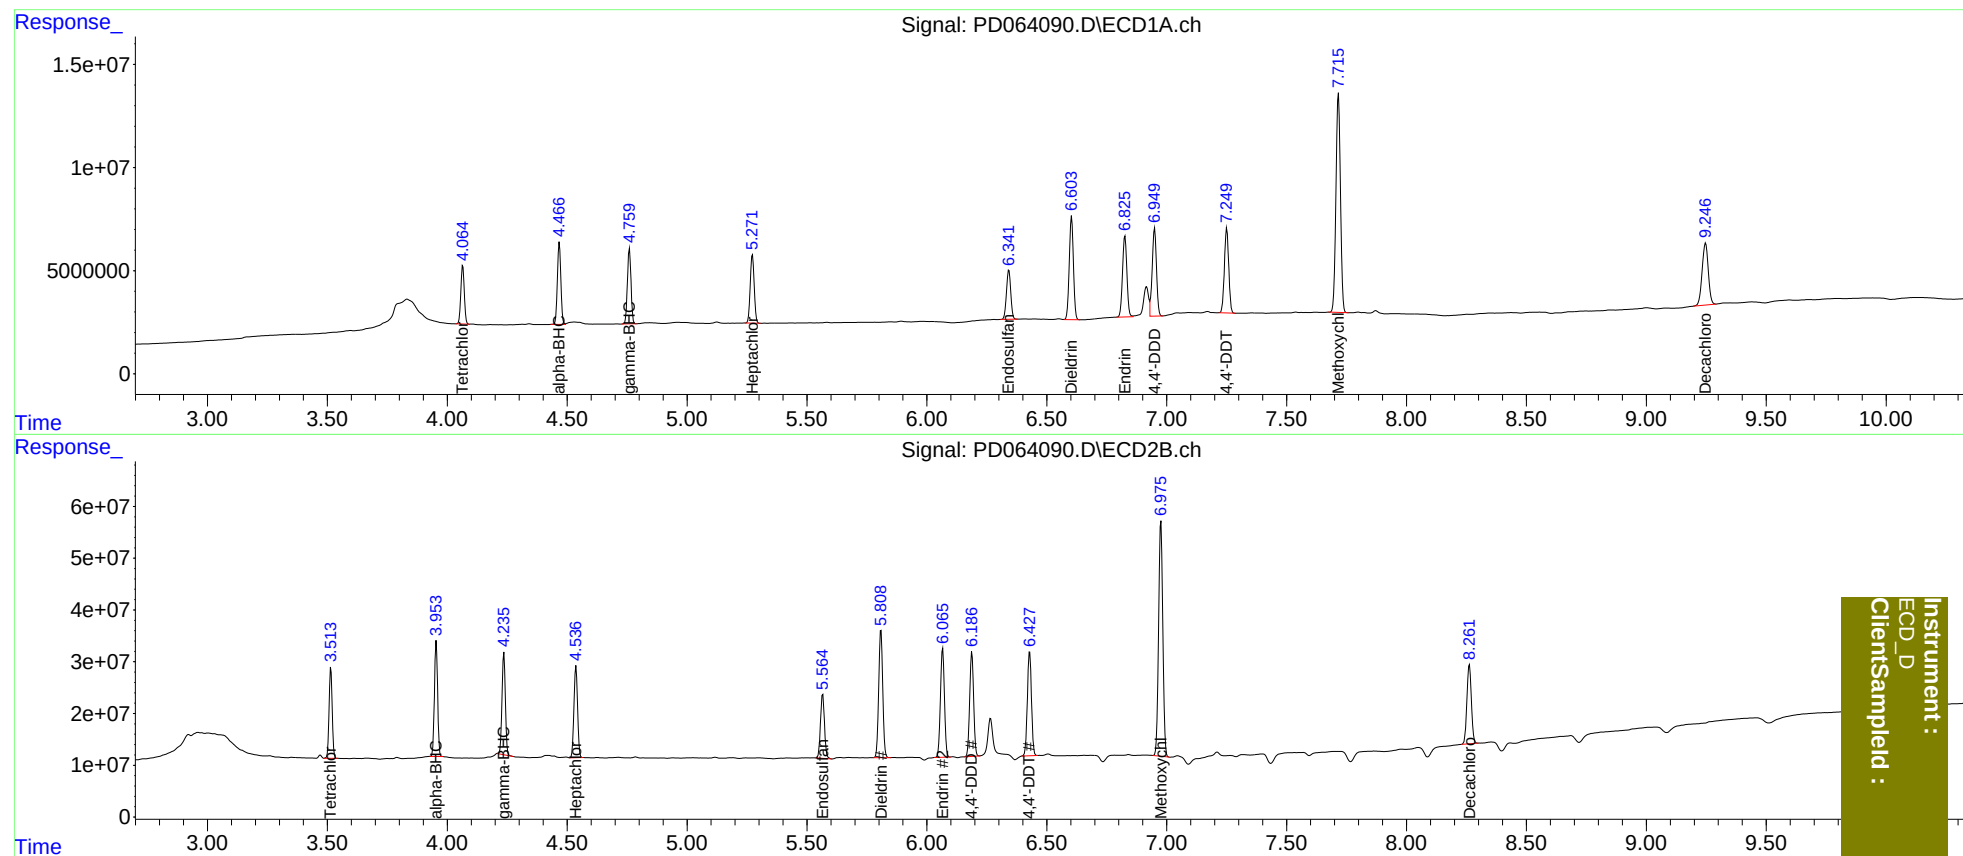


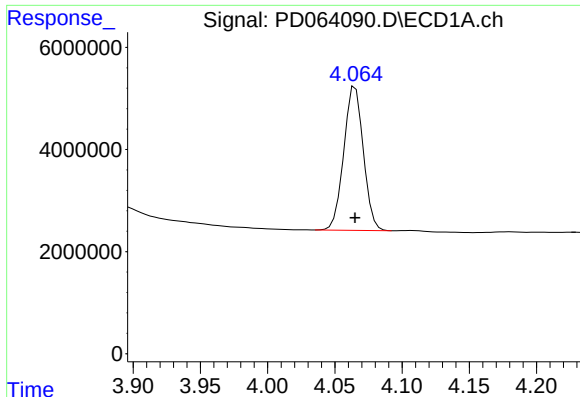

#1 Tetrachloro-m-xylene


R.T.: 4.065 min
Delta R.T.: 0.000 min
Response: 28442951
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

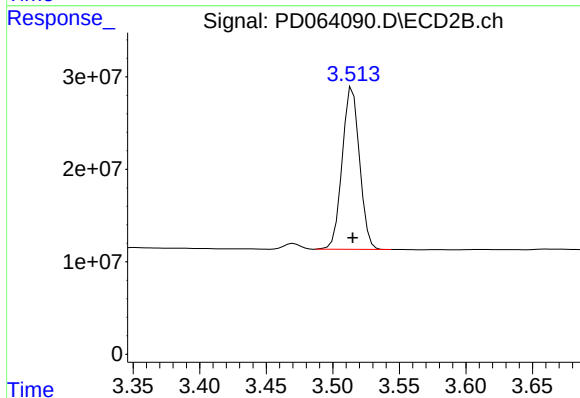


#1 Tetrachloro-m-xylene

R.T.: 3.515 min
Delta R.T.: 0.000 min
Response: 159003435
Conc: 20.00 ng/ml

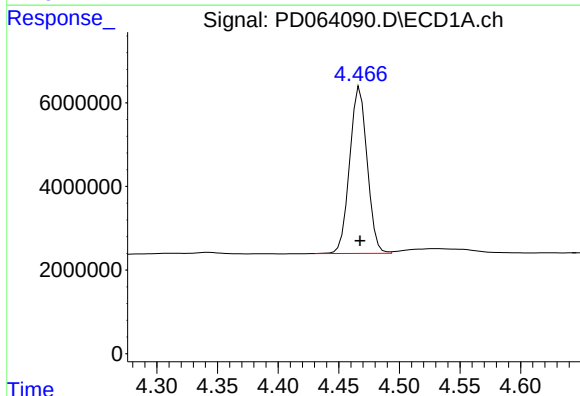


#2 alpha-BHC

R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 39980512
Conc: 20.00 ng/ml

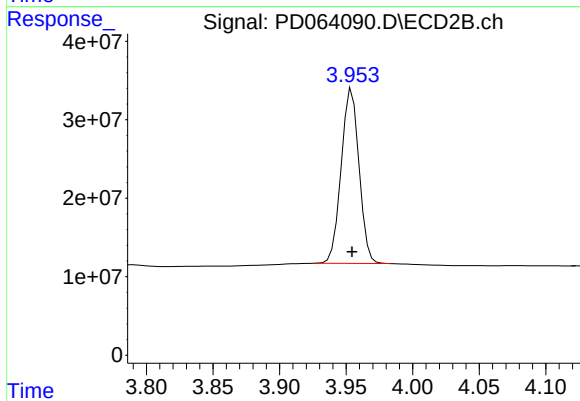

#2 alpha-BHC


R.T.: 3.954 min
Delta R.T.: 0.000 min
Response: 207716990
Conc: 20.00 ng/ml

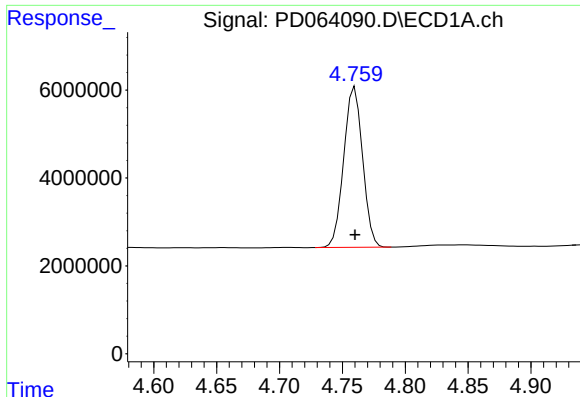

#3 gamma-BHC (Lindane)


R.T.: 4.760 min
Delta R.T.: 0.000 min
Response: 38104234
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

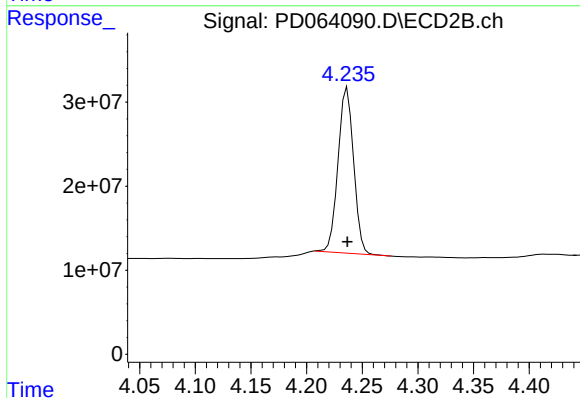


#3 gamma-BHC (Lindane)

R.T.: 4.237 min
Delta R.T.: 0.000 min
Response: 191408522
Conc: 20.00 ng/ml

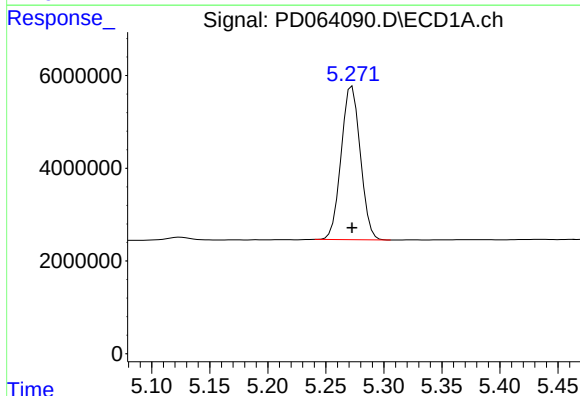


#4 Heptachlor

R.T.: 5.273 min
Delta R.T.: 0.000 min
Response: 38039239
Conc: 20.00 ng/ml

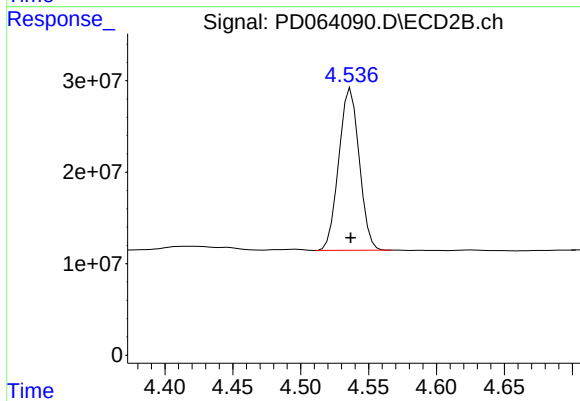

#4 Heptachlor


R.T.: 4.537 min
Delta R.T.: 0.000 min
Response: 185630853
Conc: 20.00 ng/ml

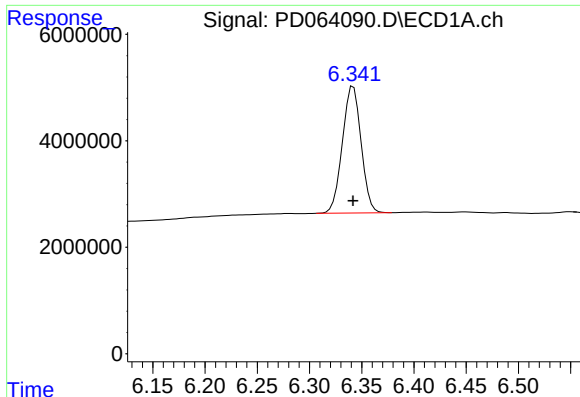

#9 Endosulfan I


R.T.: 6.342 min
Delta R.T.: 0.000 min
Response: 29674615
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

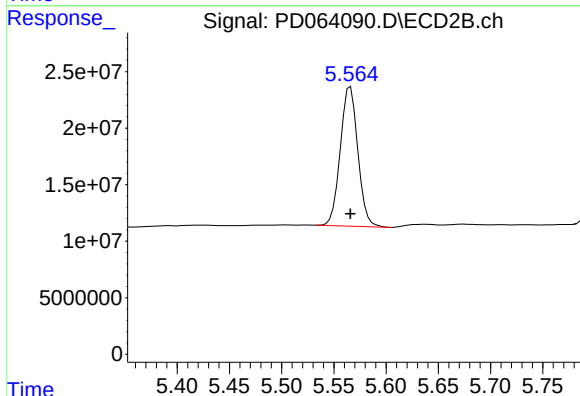


#9 Endosulfan I

R.T.: 5.566 min
Delta R.T.: 0.000 min
Response: 143873312
Conc: 20.00 ng/ml

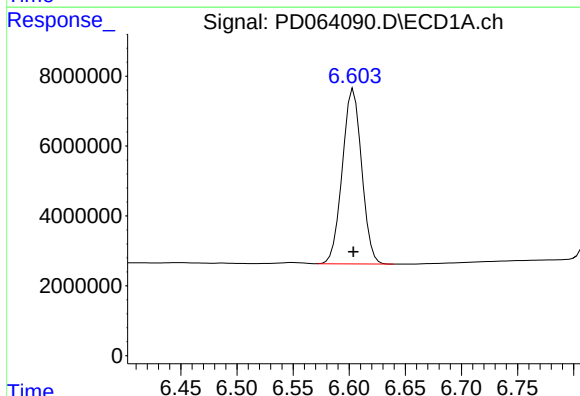


#13 Dieldrin

R.T.: 6.604 min
Delta R.T.: 0.000 min
Response: 60094690
Conc: 40.00 ng/ml

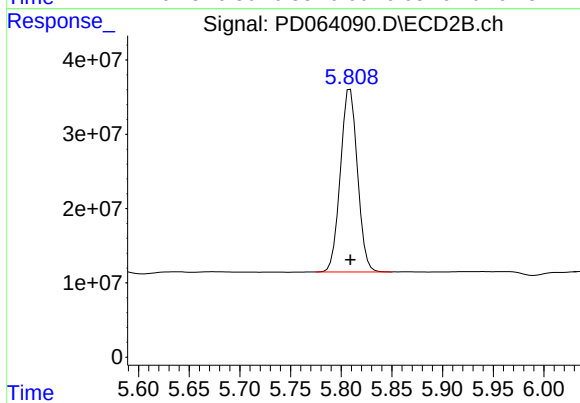

#13 Dieldrin


R.T.: 5.809 min
Delta R.T.: 0.000 min
Response: 287800235
Conc: 40.00 ng/ml

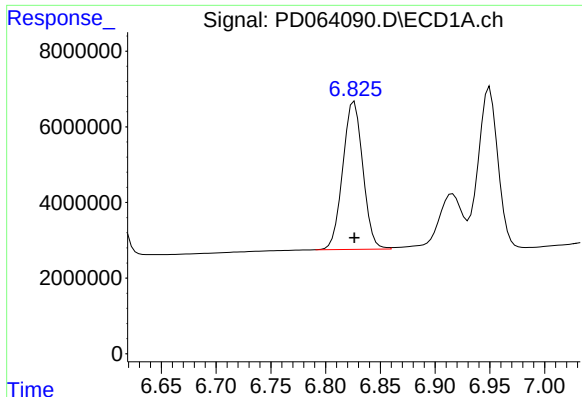

#14 Endrin


R.T.: 6.826 min
Delta R.T.: 0.000 min
Response: 49943661
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

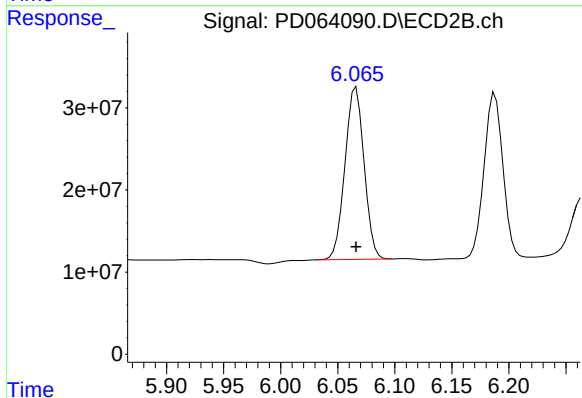


#14 Endrin

R.T.: 6.066 min
Delta R.T.: 0.000 min
Response: 244299752
Conc: 40.00 ng/ml

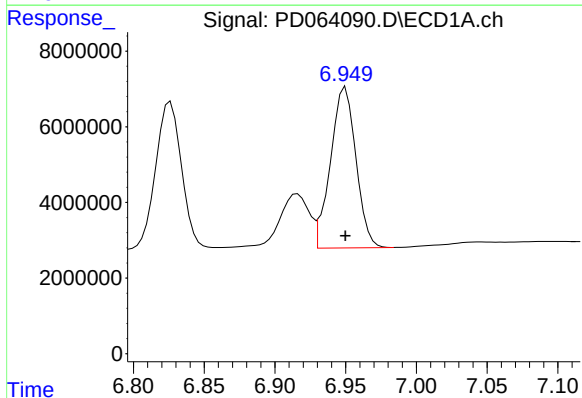


#16 4,4'-DDD

R.T.: 6.950 min
Delta R.T.: 0.000 min
Response: 53252490
Conc: 40.00 ng/ml

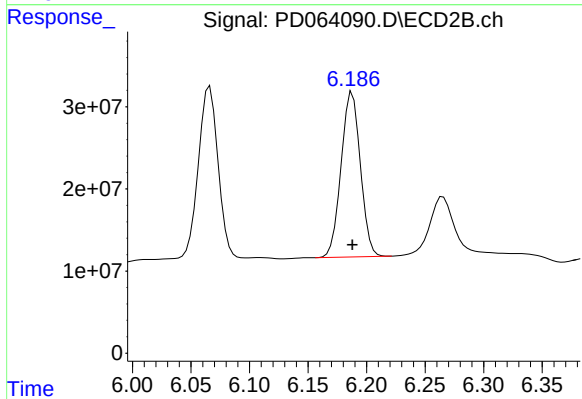

#16 4,4'-DDD


R.T.: 6.188 min
Delta R.T.: 0.000 min
Response: 230250478
Conc: 40.00 ng/ml

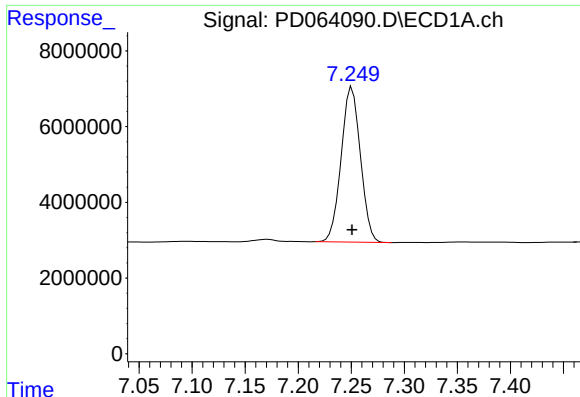

#17 4,4'-DDT


R.T.: 7.251 min
Delta R.T.: 0.000 min
Response: 51580179
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

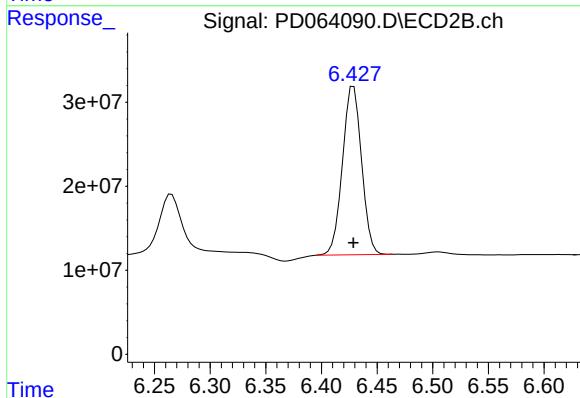


#17 4,4'-DDT

R.T.: 6.429 min
Delta R.T.: 0.000 min
Response: 239308513
Conc: 40.00 ng/ml

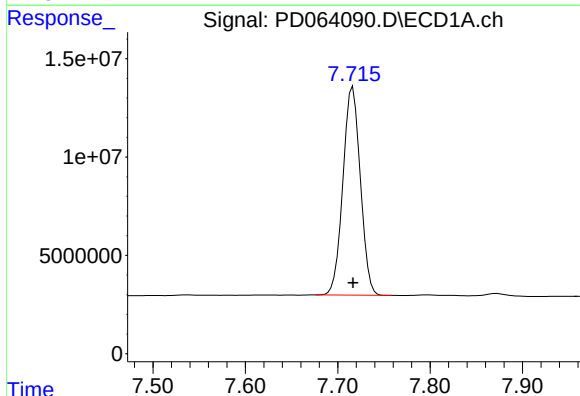


#20 Methoxychlor

R.T.: 7.716 min
Delta R.T.: 0.000 min
Response: 138702000
Conc: 200.00 ng/ml

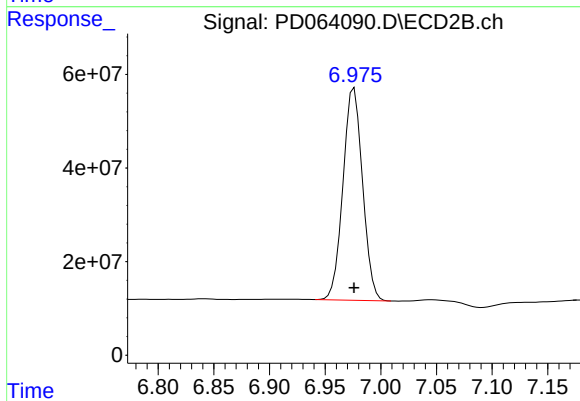

#20 Methoxychlor


R.T.: 6.976 min
Delta R.T.: 0.000 min
Response: 554839129
Conc: 200.00 ng/ml

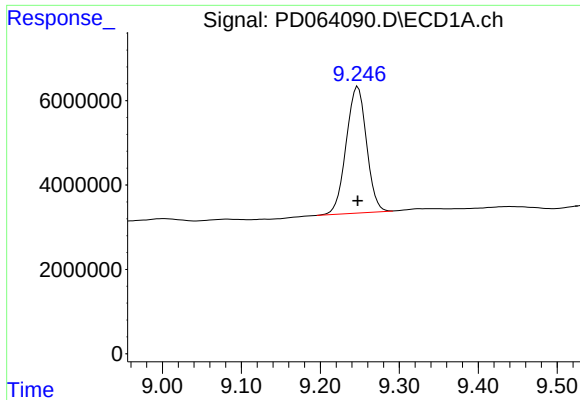

#27 Decachlorobiphenyl

R.T.: 9.248 min
Delta R.T.: 0.000 min
Response: 53827918
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

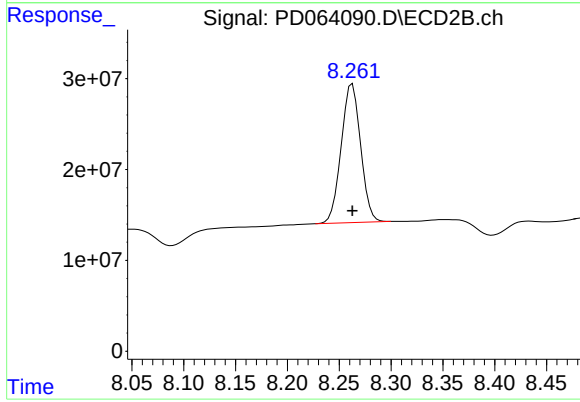

#27 Decachlorobiphenyl

R.T.: 8.263 min
Delta R.T.: 0.000 min
Response: 198946197
Conc: 40.00 ng/ml