

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070621\
 Data File : PD064092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2021 18:58
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 05:32:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070621CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 07 05:31:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.066	3.515	55019715	299.4E6	38.688	37.658
27)	SA Decachlor...	9.248	8.263	101.0E6	379.1E6	75.030	76.229
Target Compounds							
2)	A alpha-BHC	4.469	3.955	79830657	400.4E6	39.935	38.549
3)	MA gamma-BHC...	4.761	4.237	75880026	366.0E6	39.828	38.240
4)	MA Heptachlor	5.274	4.538	74602334	355.2E6	39.224	38.272
9)	A Endosulfan I	6.343	5.566	58468854	275.8E6	39.407	38.344
13)	MA Dieldrin	6.605	5.809	130.1E6	568.6E6	86.602	79.023
14)	MA Endrin	6.827	6.066	101.2E6	475.8E6	81.027	77.898
16)	A 4,4'-DDD	6.952	6.188	105.1E6	456.6E6	78.940	79.327
17)	MA 4,4'-DDT	7.252	6.429	102.1E6	476.9E6	79.197	79.707
20)	A Methoxychlor	7.718	6.976	265.7E6	1050.5E6	383.100	378.656


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070621\
Data File : PD064092.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2021 18:58
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 05:32:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070621CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 07 05:31:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

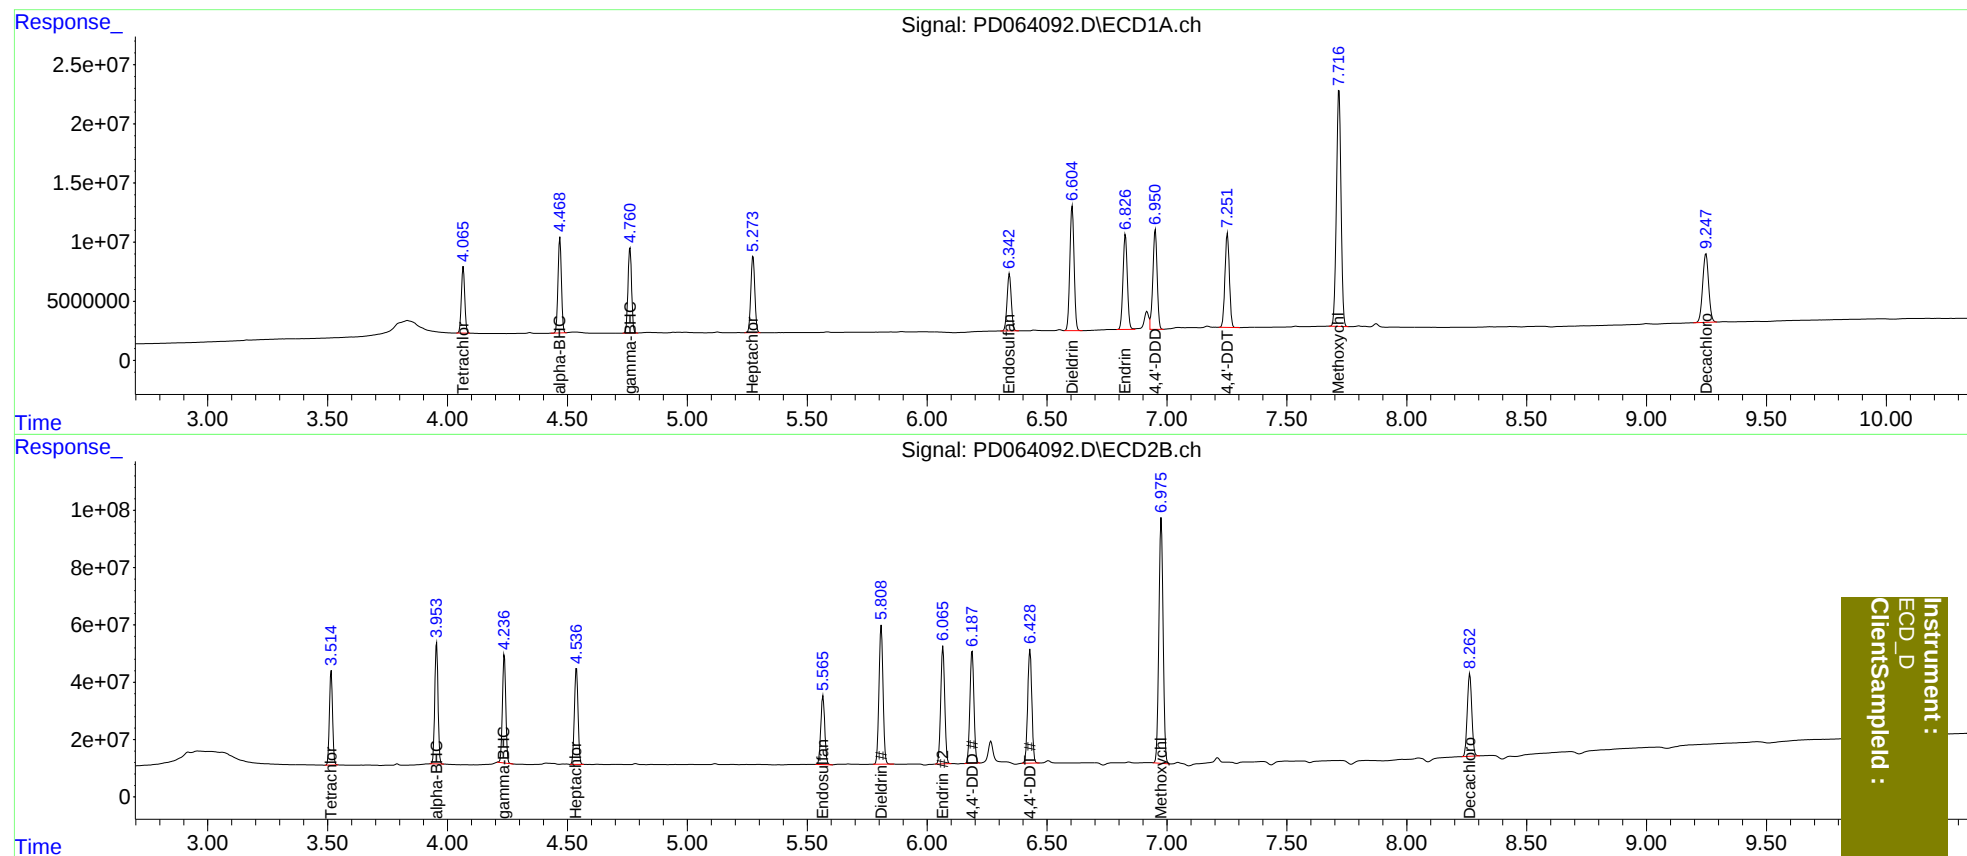


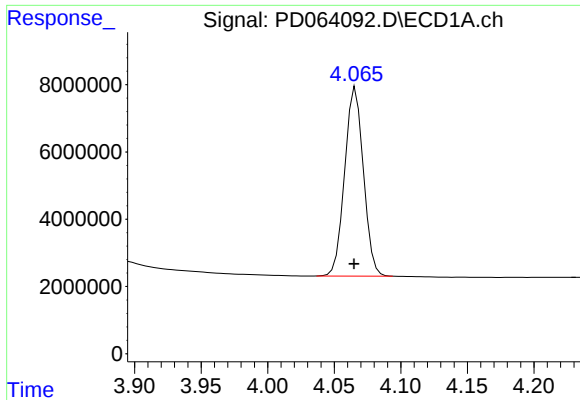

#1 Tetrachloro-m-xylene


R.T.: 4.066 min
Delta R.T.: 0.001 min
Response: 55019715
Conc: 38.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

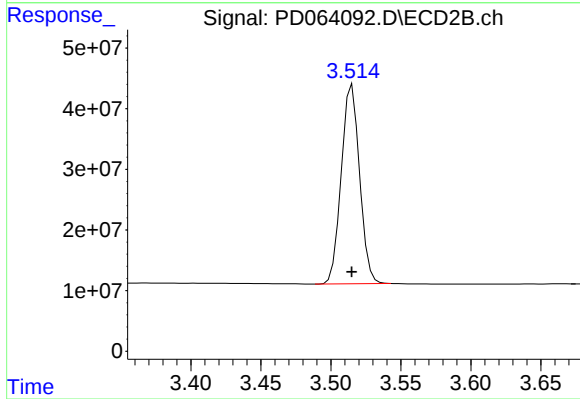


#1 Tetrachloro-m-xylene

R.T.: 3.515 min
Delta R.T.: 0.000 min
Response: 299388981
Conc: 37.66 ng/ml

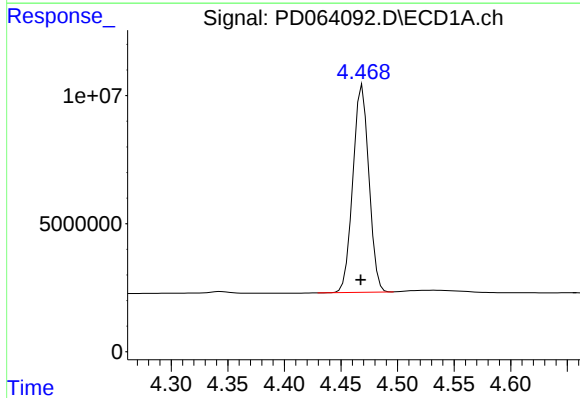


#2 alpha-BHC

R.T.: 4.469 min
Delta R.T.: 0.001 min
Response: 79830657
Conc: 39.93 ng/ml

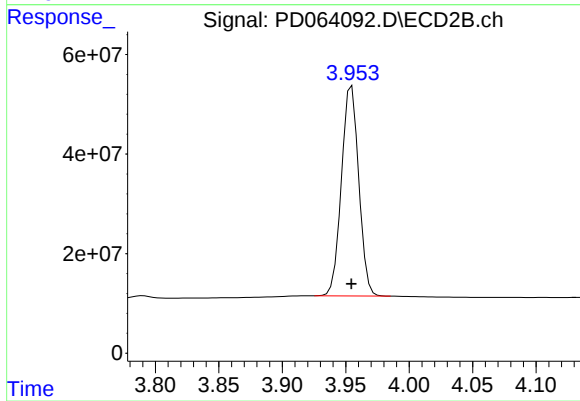

#2 alpha-BHC


R.T.: 3.955 min
Delta R.T.: 0.000 min
Response: 400359792
Conc: 38.55 ng/ml

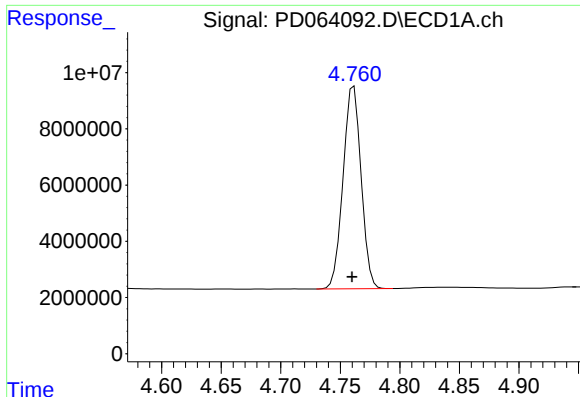

#3 gamma-BHC (Lindane)


R.T.: 4.761 min
Delta R.T.: 0.001 min
Response: 75880026
Conc: 39.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

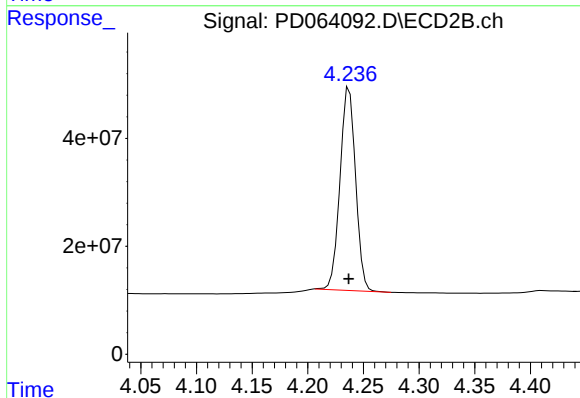


#3 gamma-BHC (Lindane)

R.T.: 4.237 min
Delta R.T.: 0.000 min
Response: 365969050
Conc: 38.24 ng/ml

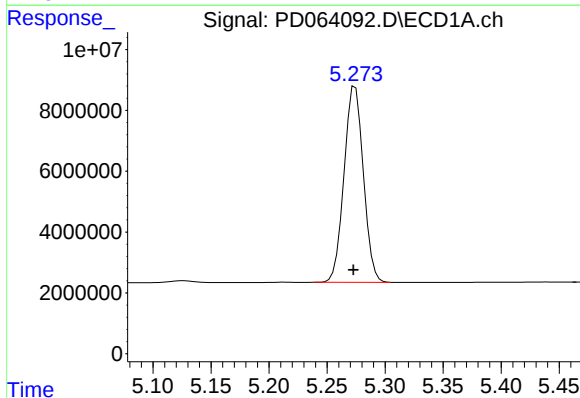


#4 Heptachlor

R.T.: 5.274 min
Delta R.T.: 0.002 min
Response: 74602334
Conc: 39.22 ng/ml

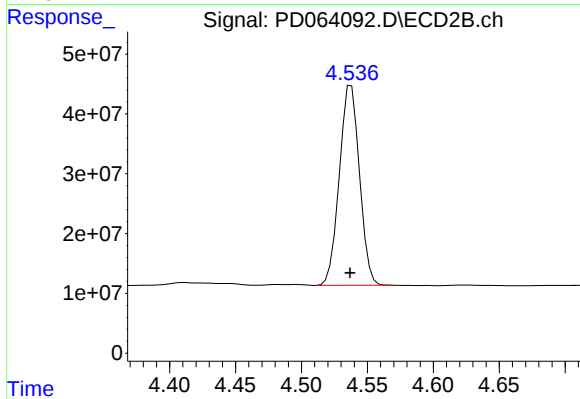

#4 Heptachlor


R.T.: 4.538 min
Delta R.T.: 0.000 min
Response: 355225065
Conc: 38.27 ng/ml

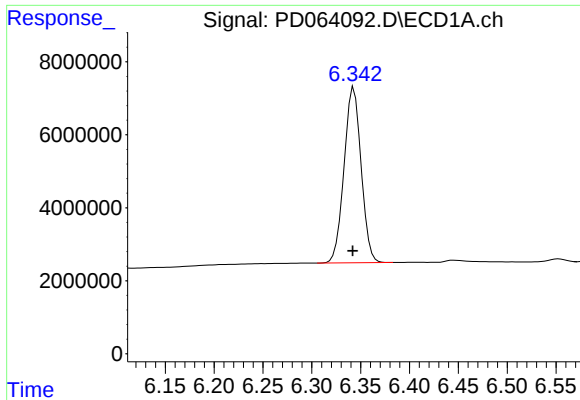

#9 Endosulfan I


R.T.: 6.343 min
Delta R.T.: 0.001 min
Response: 58468854
Conc: 39.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

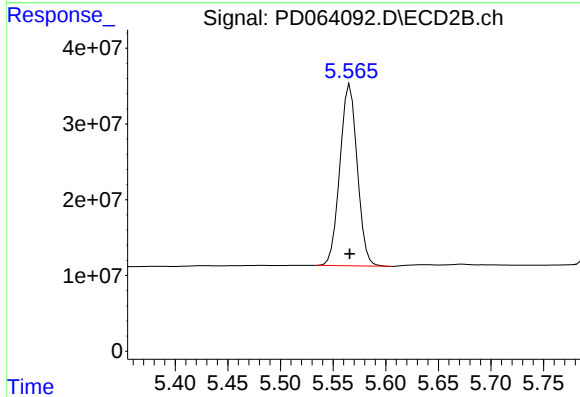


#9 Endosulfan I

R.T.: 5.566 min
Delta R.T.: 0.000 min
Response: 275833210
Conc: 38.34 ng/ml

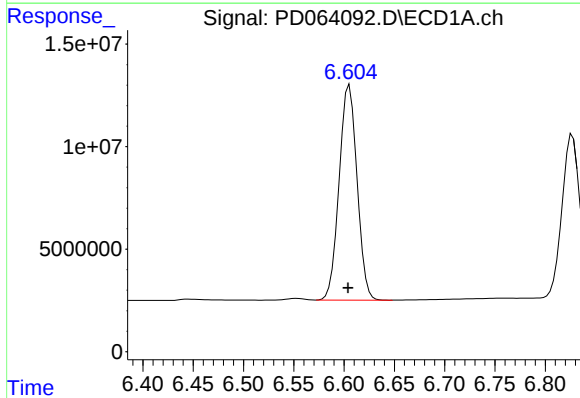


#13 Dieldrin

R.T.: 6.605 min
Delta R.T.: 0.001 min
Response: 130107367
Conc: 86.60 ng/ml

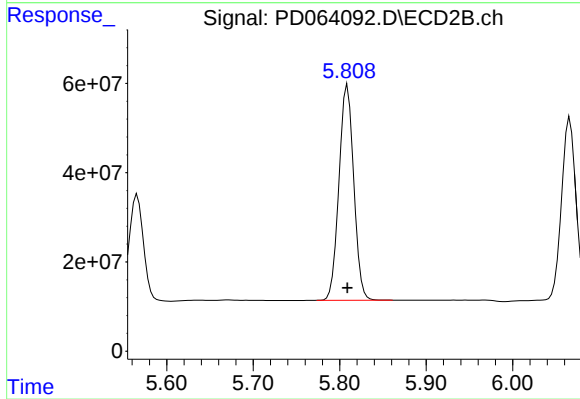

#13 Dieldrin


R.T.: 5.809 min
Delta R.T.: 0.000 min
Response: 568571364
Conc: 79.02 ng/ml

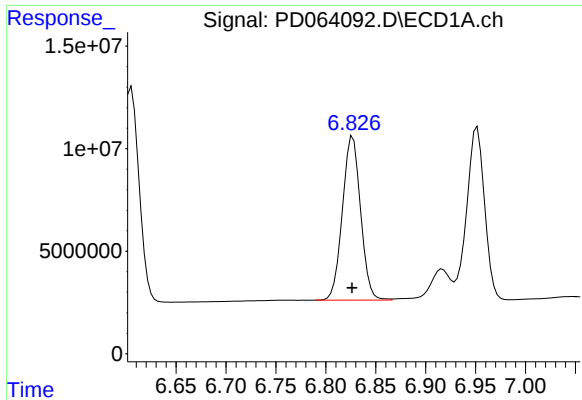

#14 Endrin


R.T.: 6.827 min
Delta R.T.: 0.000 min
Response: 101169121
Conc: 81.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

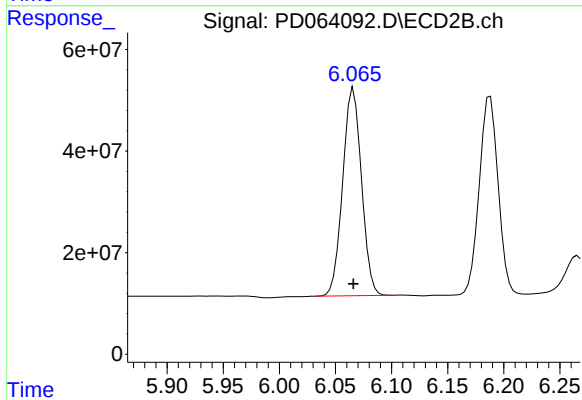


#14 Endrin

R.T.: 6.066 min
Delta R.T.: 0.000 min
Response: 475760215
Conc: 77.90 ng/ml

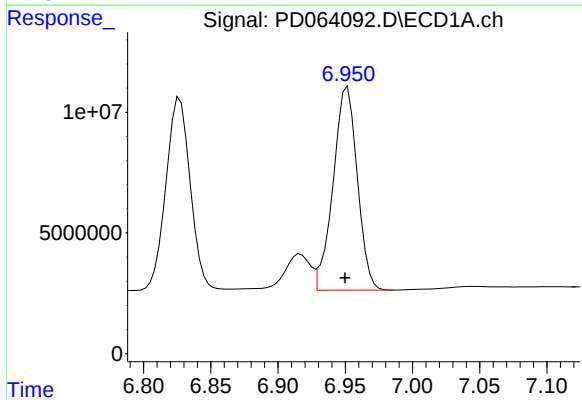


#16 4,4'-DDD

R.T.: 6.952 min
Delta R.T.: 0.002 min
Response: 105094217
Conc: 78.94 ng/ml

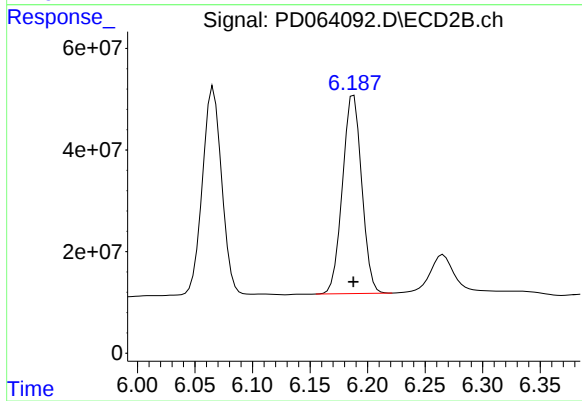

#16 4,4'-DDD


R.T.: 6.188 min
Delta R.T.: 0.000 min
Response: 456625205
Conc: 79.33 ng/ml

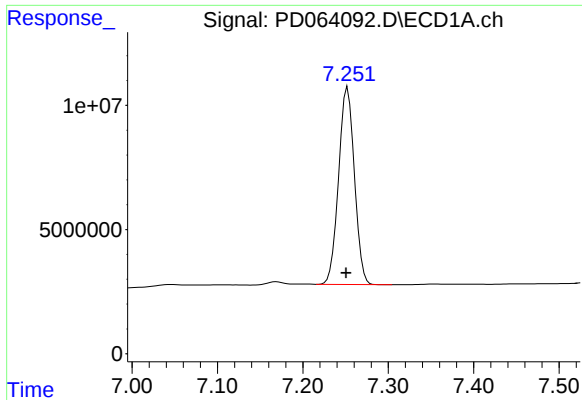

#17 4,4'-DDT


R.T.: 7.252 min
Delta R.T.: 0.002 min
Response: 102124758
Conc: 79.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

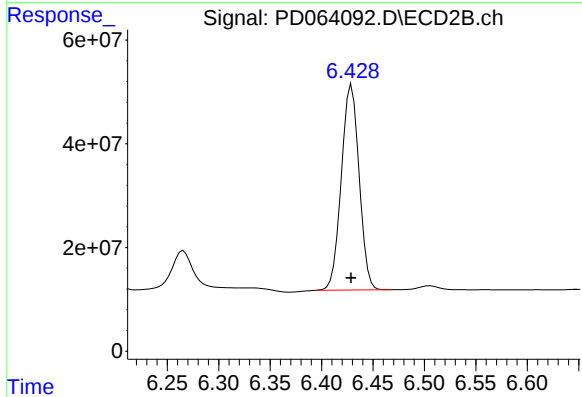


#17 4,4'-DDT

R.T.: 6.429 min
Delta R.T.: 0.000 min
Response: 476864542
Conc: 79.71 ng/ml

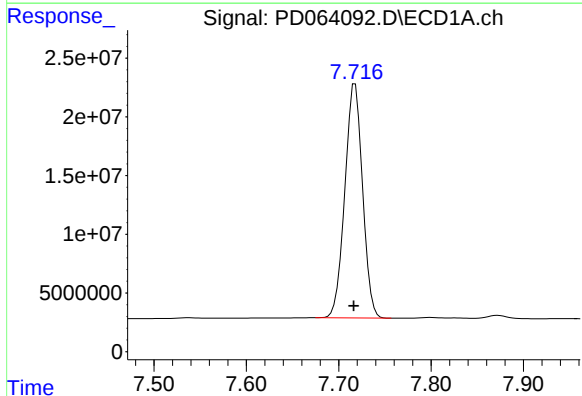


#20 Methoxychlor

R.T.: 7.718 min
Delta R.T.: 0.001 min
Response: 265684002
Conc: 383.10 ng/ml

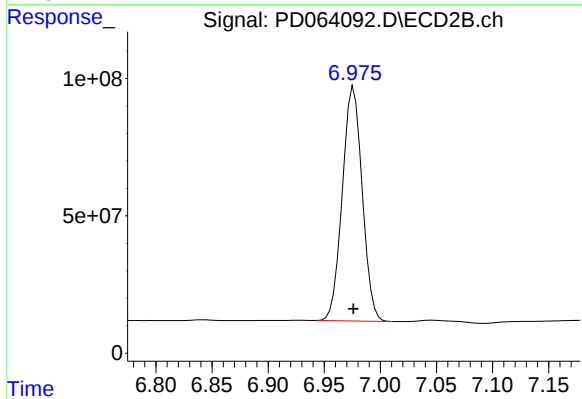

#20 Methoxychlor


R.T.: 6.976 min
Delta R.T.: 0.000 min
Response: 1050466940
Conc: 378.66 ng/ml

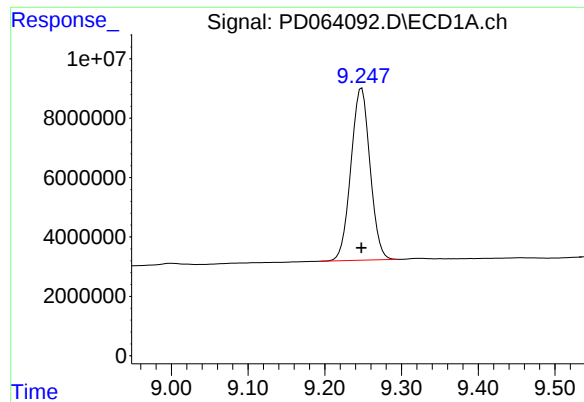

#27 Decachlorobiphenyl

R.T.: 9.248 min
Delta R.T.: 0.000 min
Response: 100967368
Conc: 75.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

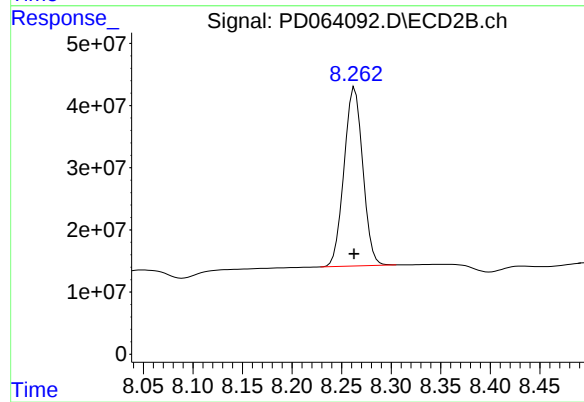

#27 Decachlorobiphenyl

R.T.: 8.263 min
Delta R.T.: 0.000 min
Response: 379137549
Conc: 76.23 ng/ml