

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070621\
 Data File : PD064094.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2021 19:25
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 05:32:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070621CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 07 05:31:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.066	3.516	112.1E6	549.8E6	78.845	69.161
27)	SA Decachlor...	9.247	8.263	198.0E6	697.5E6	147.152	140.231
Target Compounds							
2)	A alpha-BHC	4.469	3.955	168.9E6	757.5E6	84.505	72.933
3)	MA gamma-BHC...	4.761	4.237	160.3E6	683.0E6	84.130	71.369
4)	MA Heptachlor	5.275	4.538	154.9E6	653.8E6	81.456	70.438
9)	A Endosulfan I	6.344	5.566	119.0E6	509.5E6	80.222	70.827
13)	MA Dieldrin	6.605	5.809	272.0E6	1076.1E6	181.075	149.561
14)	MA Endrin	6.827	6.067	207.8E6	893.8E6	166.422	146.349
16)	A 4,4'-DDD	6.951	6.188	217.2E6	870.3E6	163.179	151.188
17)	MA 4,4'-DDT	7.253	6.429	212.9E6	909.5E6	165.091	152.022
20)	A Methoxychlor	7.718	6.976	532.1E6	1961.9E6	767.243	707.194


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070621\
Data File : PD064094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2021 19:25
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 05:32:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070621CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 07 05:31:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

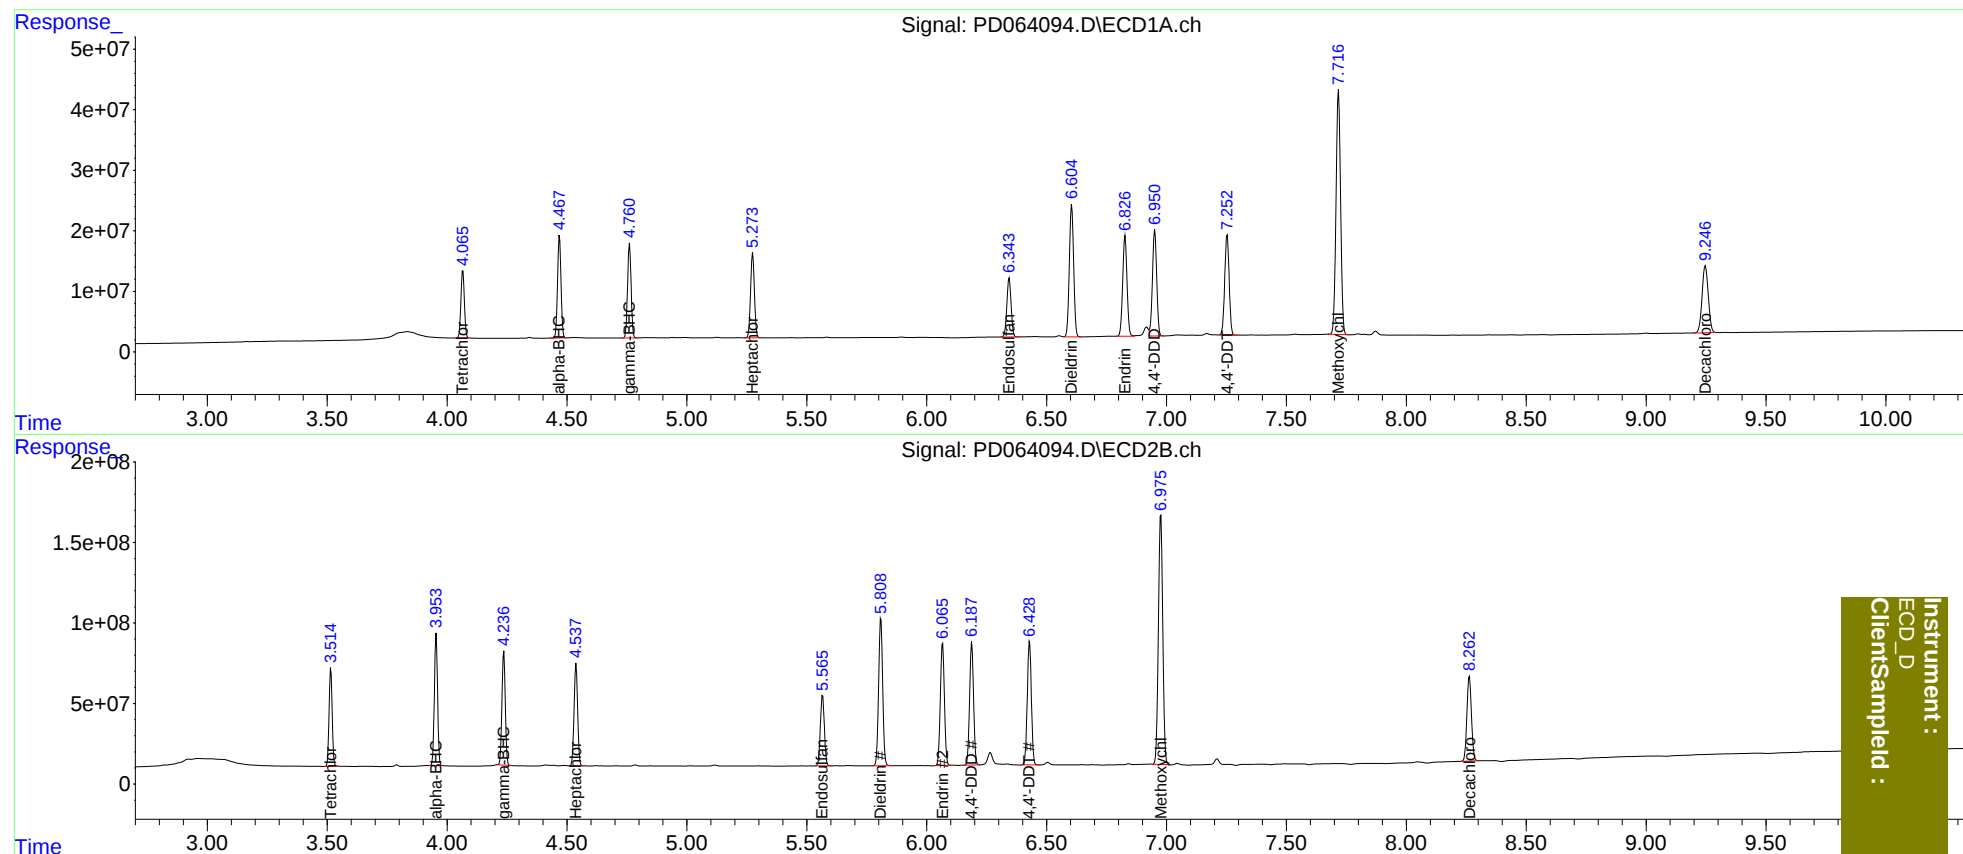


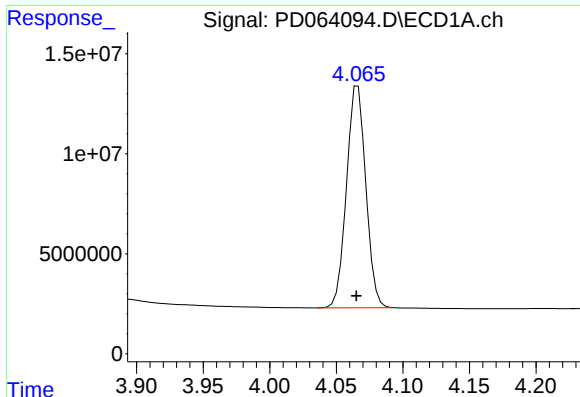

#1 Tetrachloro-m-xylene


R.T.: 4.066 min
Delta R.T.: 0.001 min
Response: 112129200
Conc: 78.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

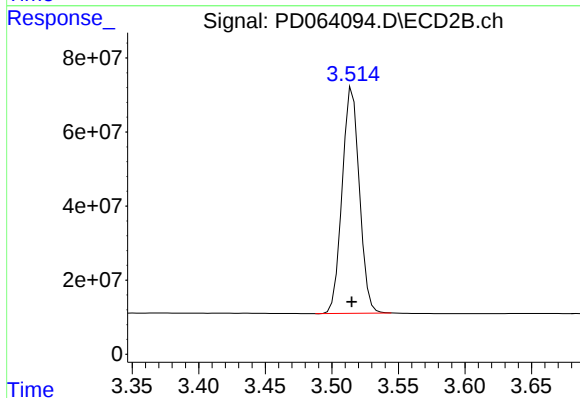


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: 0.000 min
Response: 549842069
Conc: 69.16 ng/ml

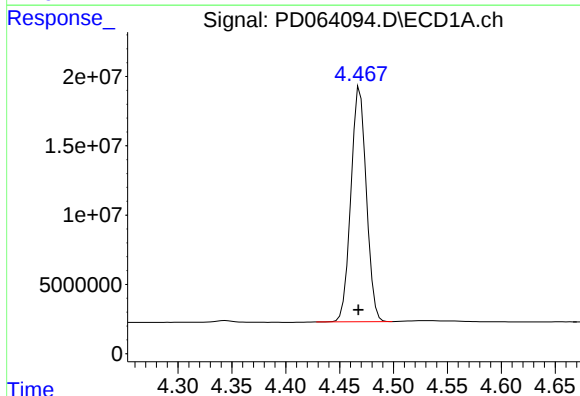


#2 alpha-BHC

R.T.: 4.469 min
Delta R.T.: 0.001 min
Response: 168927979
Conc: 84.51 ng/ml

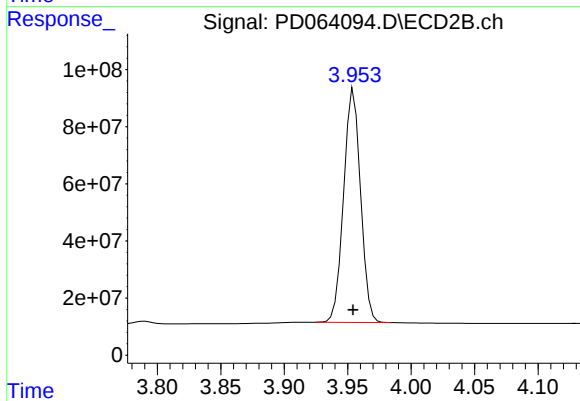

#2 alpha-BHC


R.T.: 3.955 min
Delta R.T.: 0.000 min
Response: 757469921
Conc: 72.93 ng/ml

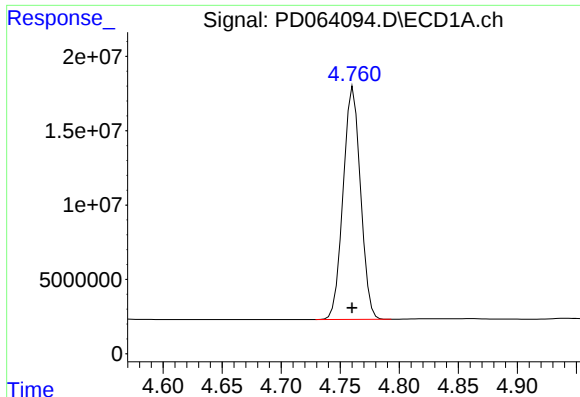

#3 gamma-BHC (Lindane)


R.T.: 4.761 min
Delta R.T.: 0.001 min
Response: 160285641
Conc: 84.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

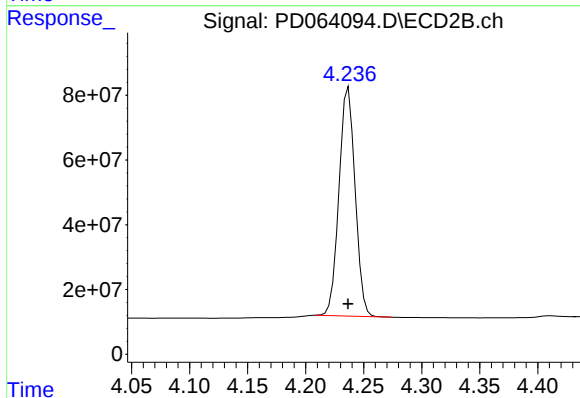


#3 gamma-BHC (Lindane)

R.T.: 4.237 min
Delta R.T.: 0.000 min
Response: 683027326
Conc: 71.37 ng/ml

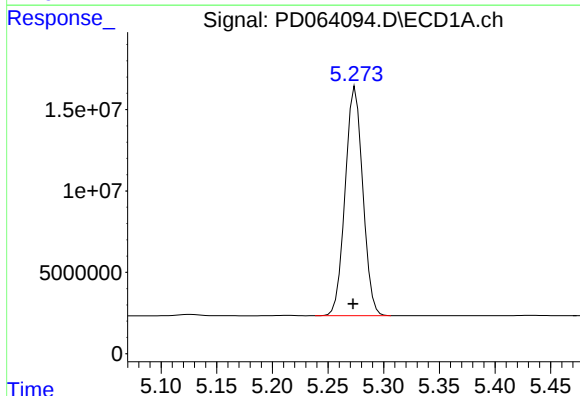


#4 Heptachlor

R.T.: 5.275 min
Delta R.T.: 0.002 min
Response: 154926939
Conc: 81.46 ng/ml

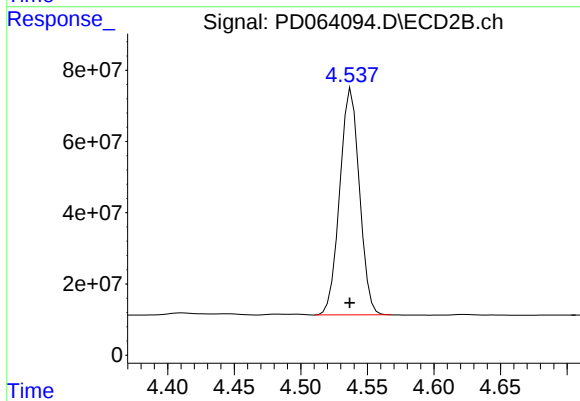

#4 Heptachlor


R.T.: 4.538 min
Delta R.T.: 0.001 min
Response: 653771784
Conc: 70.44 ng/ml

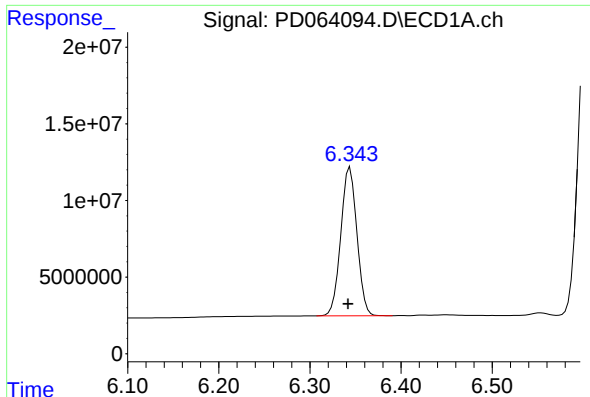

#9 Endosulfan I


R.T.: 6.344 min
Delta R.T.: 0.002 min
Response: 119028294
Conc: 80.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

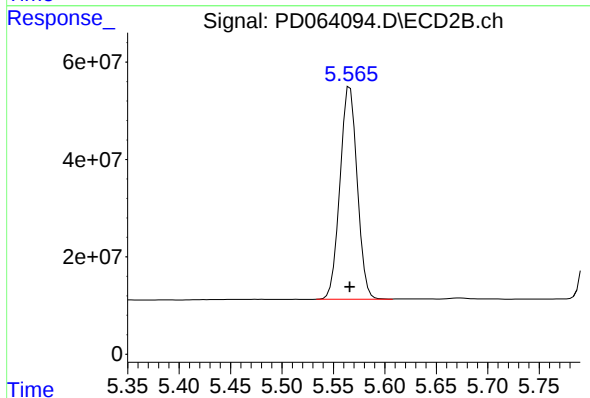


#9 Endosulfan I

R.T.: 5.566 min
Delta R.T.: 0.000 min
Response: 509502402
Conc: 70.83 ng/ml

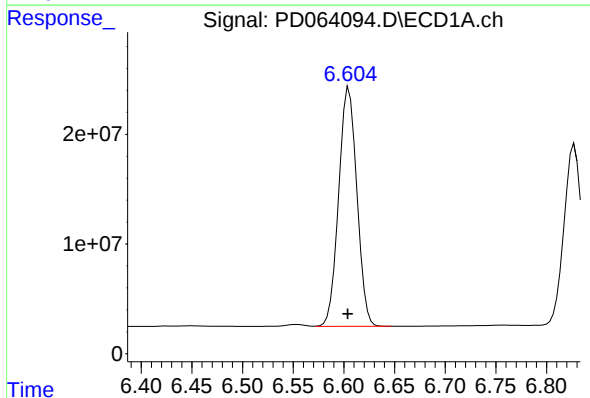


#13 Dieldrin

R.T.: 6.605 min
Delta R.T.: 0.001 min
Response: 272040781
Conc: 181.07 ng/ml

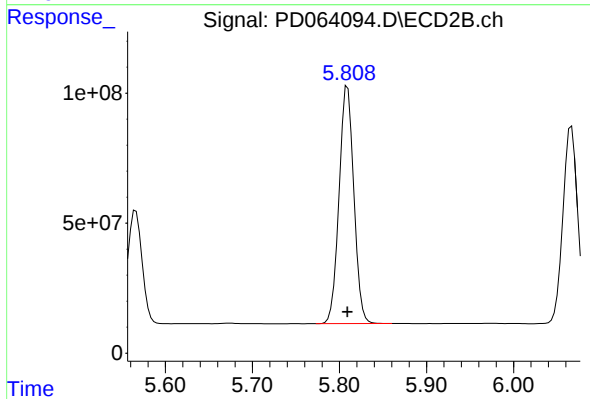

#13 Dieldrin


R.T.: 5.809 min
Delta R.T.: 0.000 min
Response: 1076095199
Conc: 149.56 ng/ml

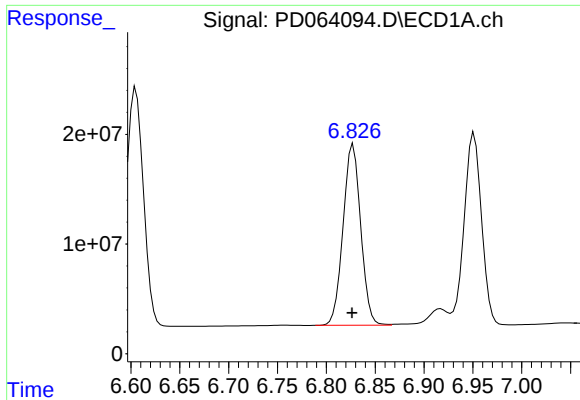

#14 Endrin


R.T.: 6.827 min
Delta R.T.: 0.001 min
Response: 207793060
Conc: 166.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

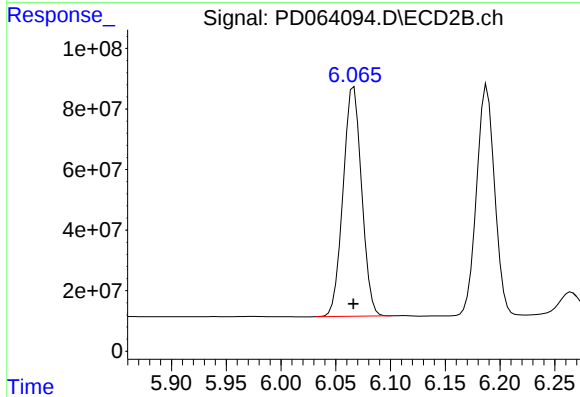


#14 Endrin

R.T.: 6.067 min
Delta R.T.: 0.000 min
Response: 893826037
Conc: 146.35 ng/ml

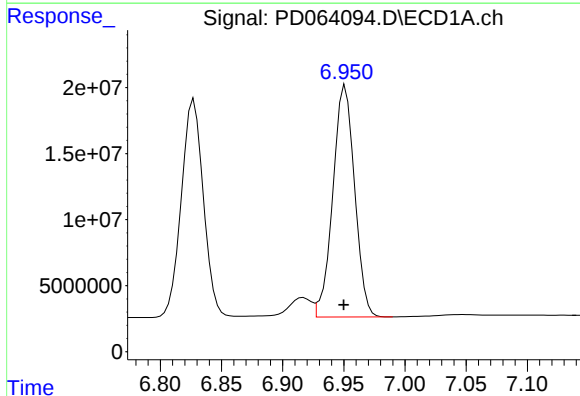


#16 4,4'-DDD

R.T.: 6.951 min
Delta R.T.: 0.001 min
Response: 217241575
Conc: 163.18 ng/ml

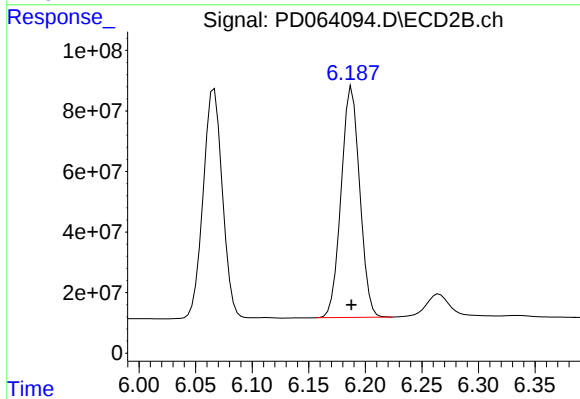

#16 4,4'-DDD


R.T.: 6.188 min
Delta R.T.: 0.000 min
Response: 870276281
Conc: 151.19 ng/ml

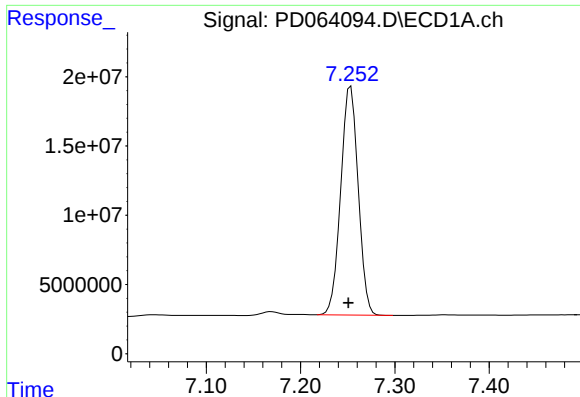

#17 4,4'-DDT


R.T.: 7.253 min
Delta R.T.: 0.002 min
Response: 212885717
Conc: 165.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

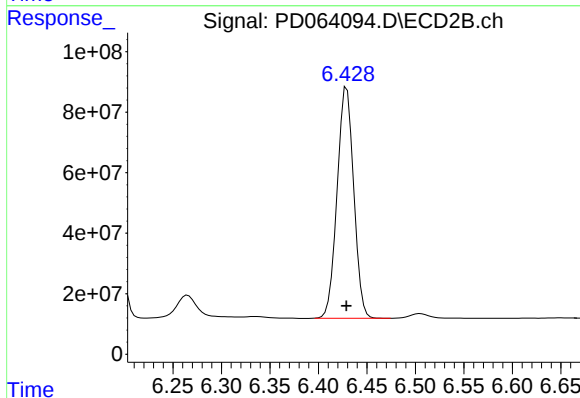


#17 4,4'-DDT

R.T.: 6.429 min
Delta R.T.: 0.000 min
Response: 909501276
Conc: 152.02 ng/ml

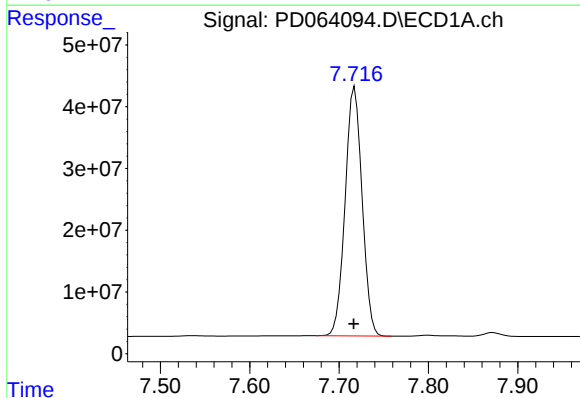


#20 Methoxychlor

R.T.: 7.718 min
Delta R.T.: 0.001 min
Response: 532090951
Conc: 767.24 ng/ml

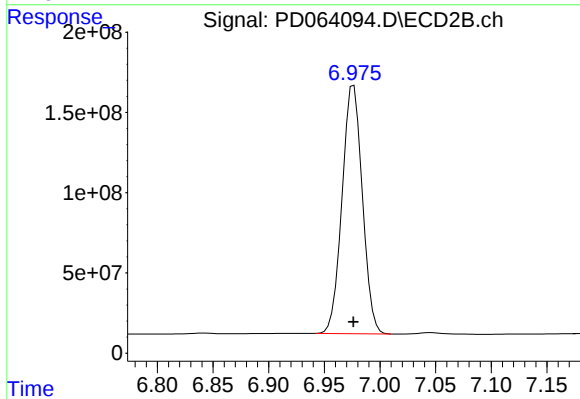

#20 Methoxychlor

R.T.: 6.976 min
Delta R.T.: 0.000 min
Response: 1961894772
Conc: 707.19 ng/ml

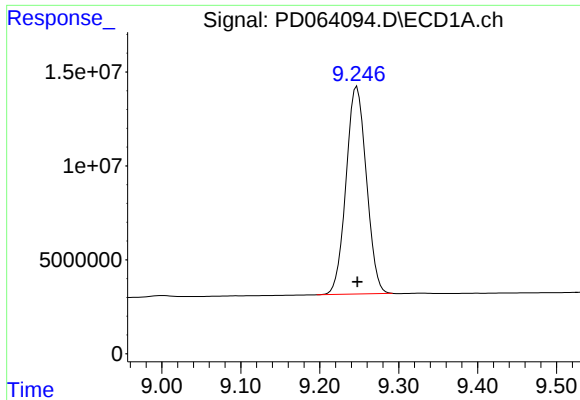

#27 Decachlorobiphenyl


R.T.: 9.247 min

Delta R.T.: 0.000 min

Response: 198021694

Conc: 147.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

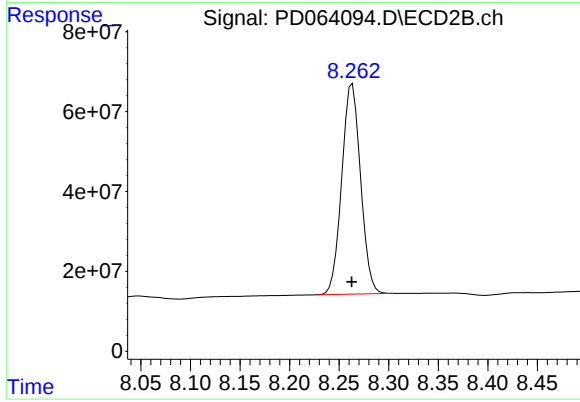

#27 Decachlorobiphenyl

R.T.: 8.263 min

Delta R.T.: 0.000 min

Response: 697461502

Conc: 140.23 ng/ml