

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070623\
 Data File : PD076353.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2023 20:00
 Operator : AR\AJ
 Sample : 03507-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CP-2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/06/2023
 Supervised By : Ankita Jodhani 07/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 05 22:33:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070423.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 05 05:21:22 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.766	40772394	19369016	12.444m	12.193
28) SA Decachlor...	9.083	7.907	41153154	16808713	11.574	13.356
Target Compounds						
17) MA 4,4'-DDT	7.036	6.027	9143768	5079438	2.601m	4.197 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070623\
Data File : PD076353.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2023 20:00
Operator : AR\AJ
Sample : 03507-04
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
CP-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/06/2023
Supervised By : Ankita Jodhani 07/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 05 22:33:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070423.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 05:21:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

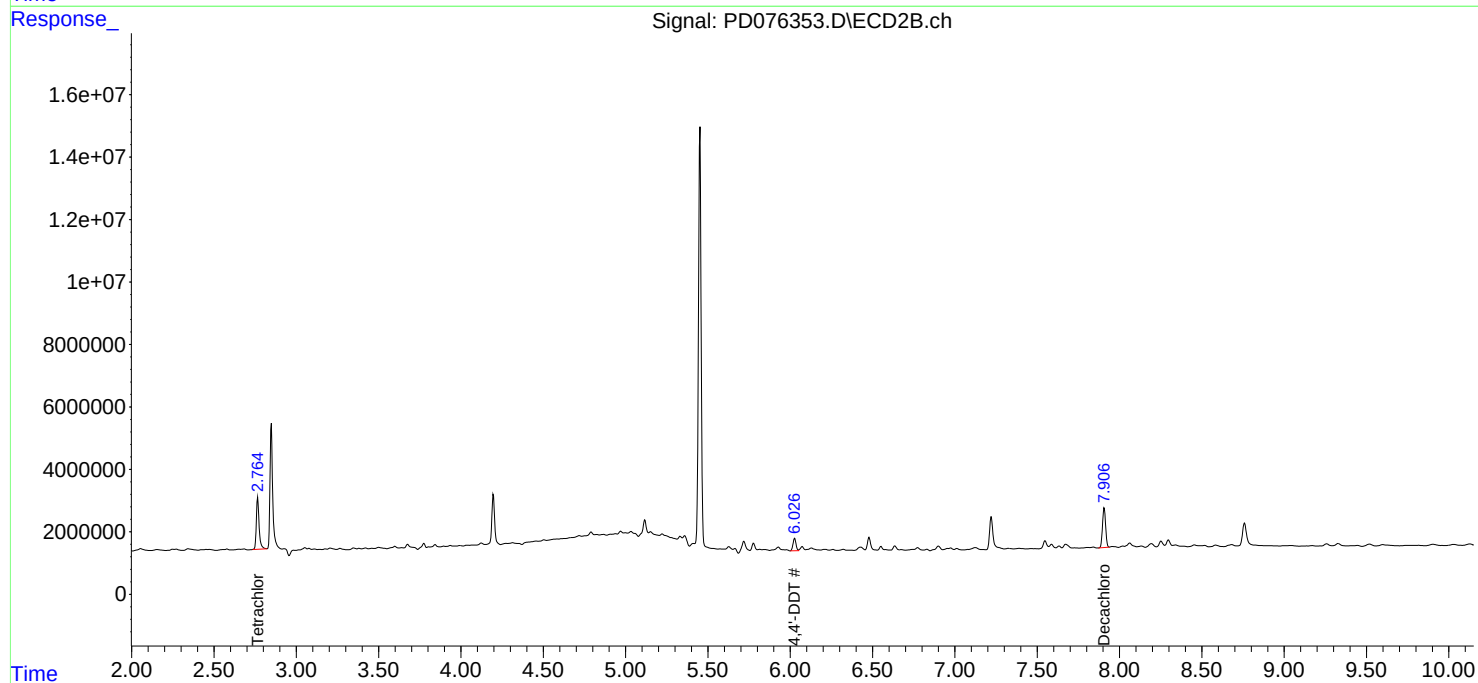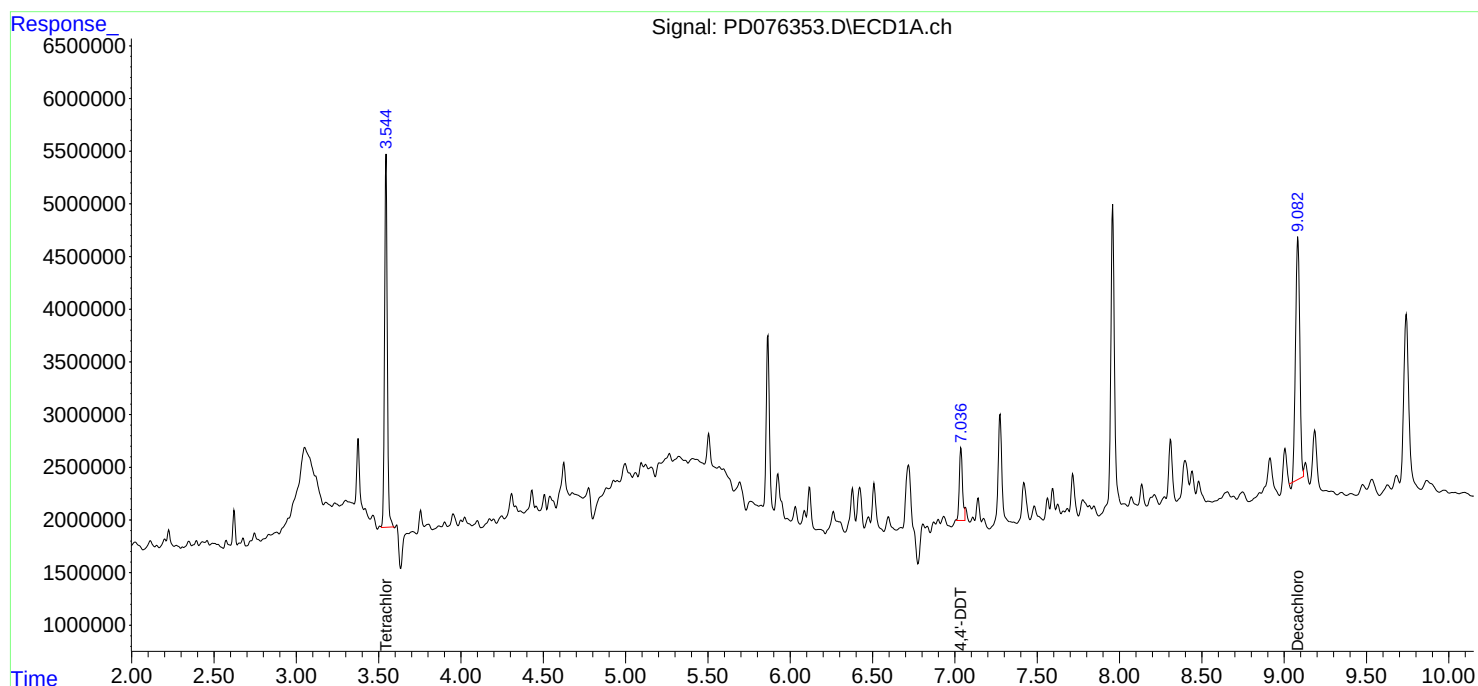

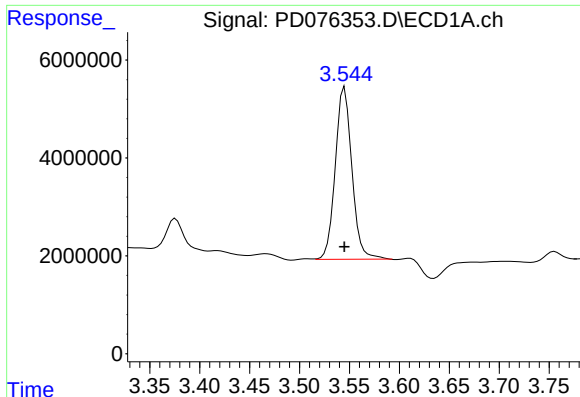


#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: -0.001 min
Response: 40772394
Conc: 12.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
CP-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/06/2023
Supervised By :Ankita Jodhani 07/06/2023

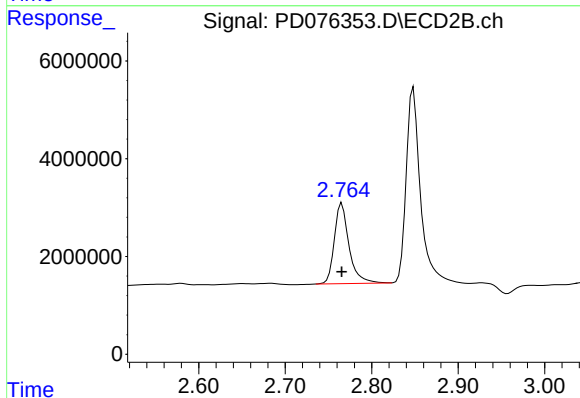


#1 Tetrachloro-m-xylene

R.T.: 2.766 min
Delta R.T.: 0.000 min
Response: 19369016
Conc: 12.19 ng/ml

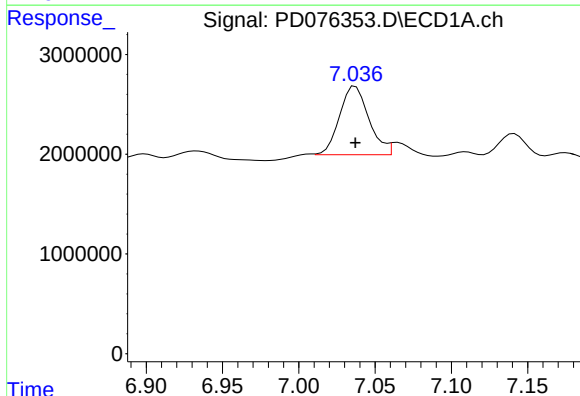


#17 4,4'-DDT

R.T.: 7.036 min
Delta R.T.: -0.001 min
Response: 9143768
Conc: 2.60 ng/ml m

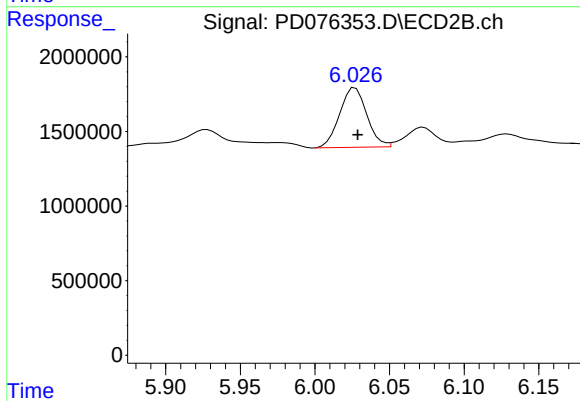

#17 4,4'-DDT

R.T.: 6.027 min
Delta R.T.: -0.002 min
Response: 5079438
Conc: 4.20 ng/ml

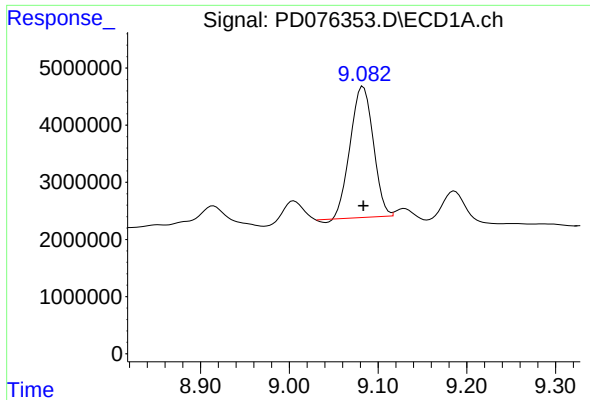


#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 41153154
Conc: 11.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
CP-2

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/06/2023
Supervised By :Ankita Jodhani 07/06/2023

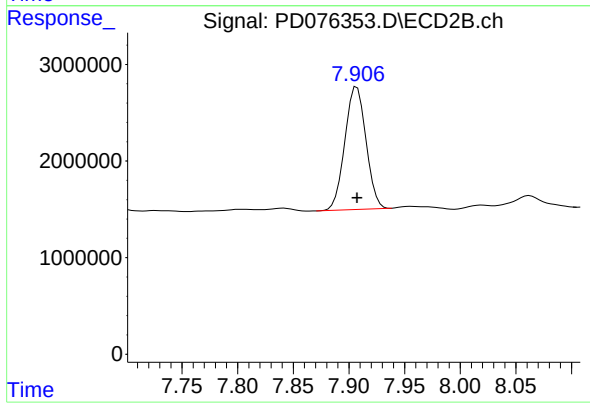

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 16808713
Conc: 13.36 ng/ml