

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070623\
 Data File : PD076357.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2023 20:54
 Operator : AR\AJ
 Sample : 03513-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 500-1-AB

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/06/2023
 Supervised By : Ankita Jodhani 07/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 05 22:36:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070423.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 05 05:21:22 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.765	27514996	13176540	8.398m	8.295m
28) SA Decachlor...	9.083	7.906	40774621	15020871	11.468	11.935

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070623\
Data File : PD076357.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2023 20:54
Operator : AR\AJ
Sample : 03513-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
500-1-AB


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/06/2023
Supervised By : Ankita Jodhani 07/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 05 22:36:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070423.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 05:21:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

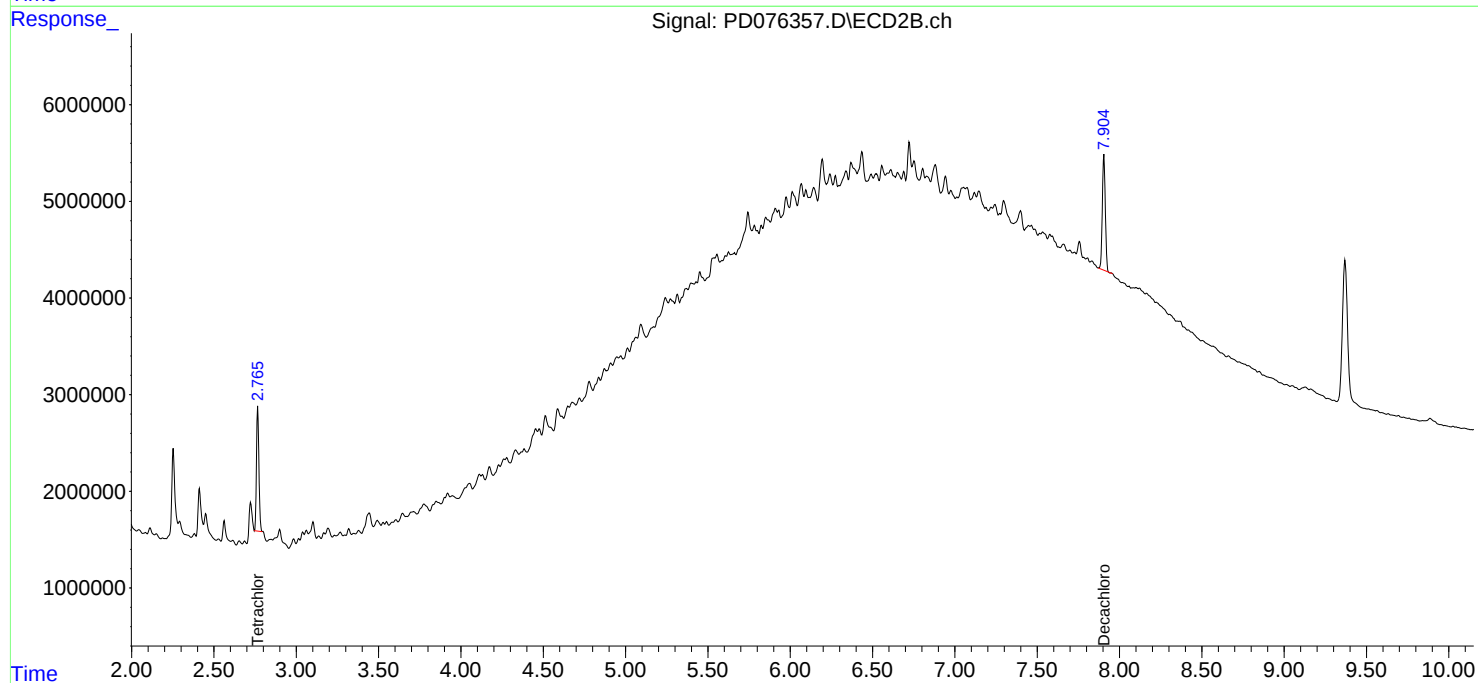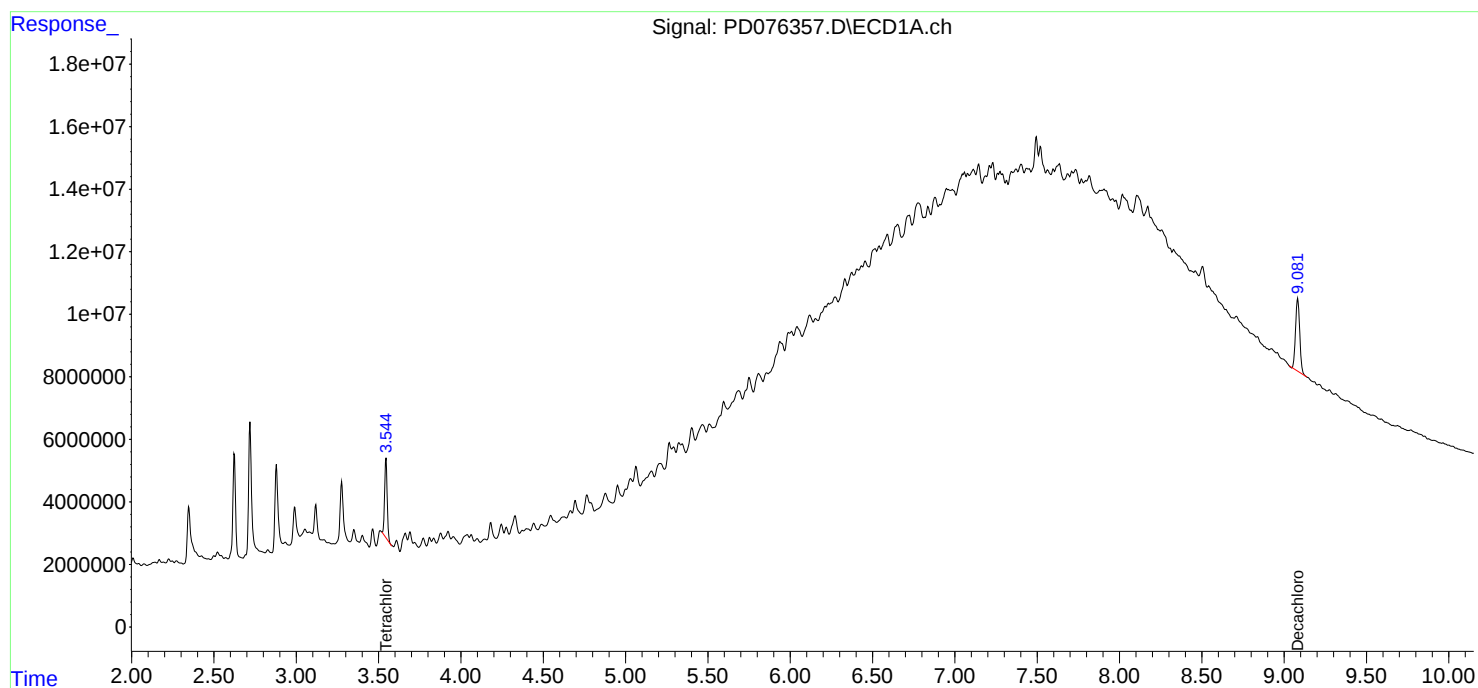

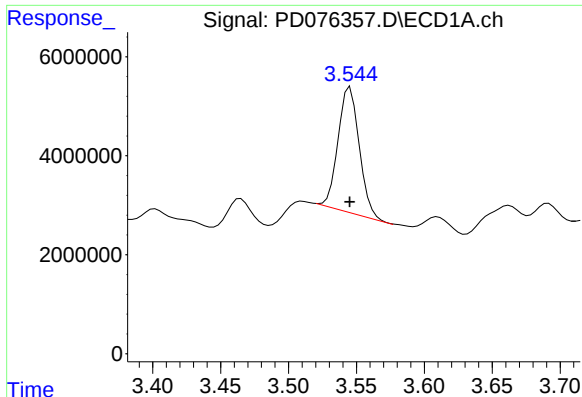


#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: -0.001 min
Response: 27514996
Conc: 8.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
500-1-AB


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/06/2023
Supervised By :Ankita Jodhani 07/06/2023

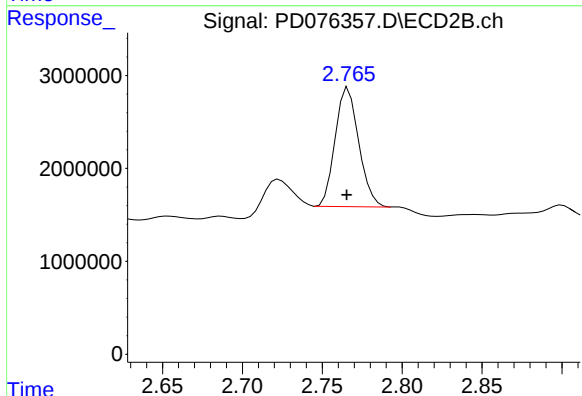


#1 Tetrachloro-m-xylene

R.T.: 2.765 min
Delta R.T.: 0.000 min
Response: 13176540
Conc: 8.29 ng/ml m

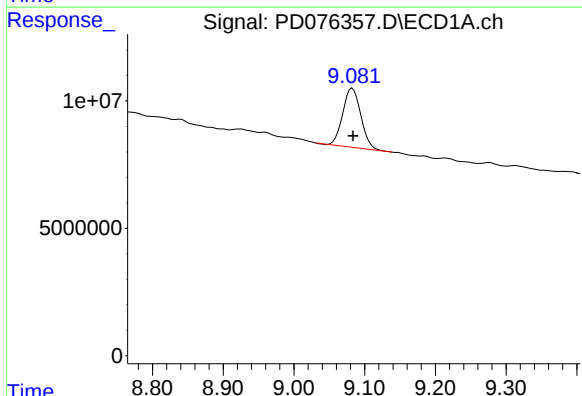

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 40774621
Conc: 11.47 ng/ml

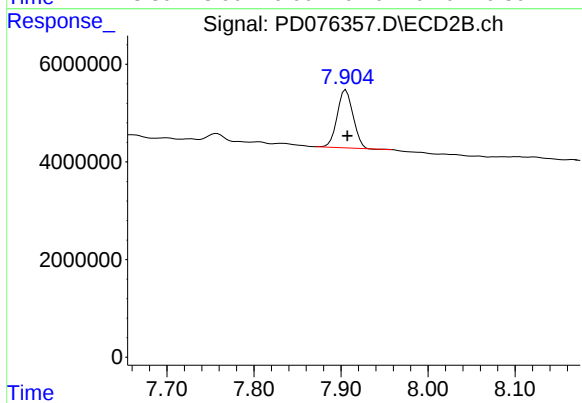

#28 Decachlorobiphenyl

R.T.: 7.906 min
Delta R.T.: -0.002 min
Response: 15020871
Conc: 11.94 ng/ml