

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070720\
 Data File : PD058462.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2020 09:48
 Operator : AJ\MA
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 12:47:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 07 12:46:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.210	3.867	43226574	58323300	23.708	23.605
28)	SA Decachlor...	7.846	8.861	41900827	51110047	23.203	23.442
Target Compounds							
9)	A Endosulfan I	5.177	6.065	21308495	28521458	10.753	10.818
10)	B gamma-Chl...	5.069	5.946	23821744	32170807	10.700	11.055
12)	B 4,4'-DDE	5.296	6.178	47579856	59940579	22.046	21.809
13)	MA Dieldrin	5.414	6.320	39304810	62985561	22.041	22.048
19)	B Endosulfa...	6.317	7.092	33728520	49756077	21.196	21.700
20)	A Methoxychlor	6.585	7.421	61943975	132.2E6	105.144	109.956
21)	B Endrin ke...	6.798	7.558	37361579	58357438	20.543	21.441
25)	Chlordane-3	5.069	5.946	23821744	32170807	116.378	86.493 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070720\
Data File : PD058462.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2020 09:48
Operator : AJ\MA
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 12:47:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Tue Jul 07 12:46:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

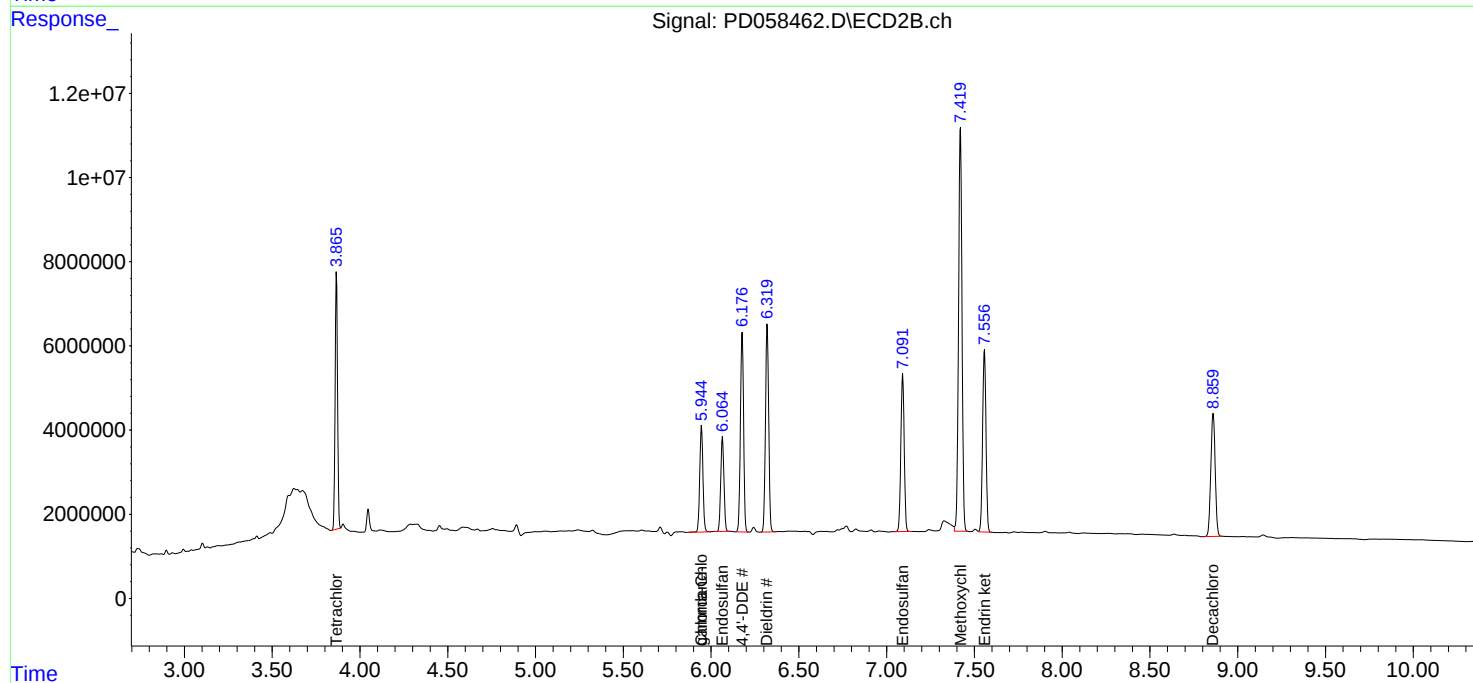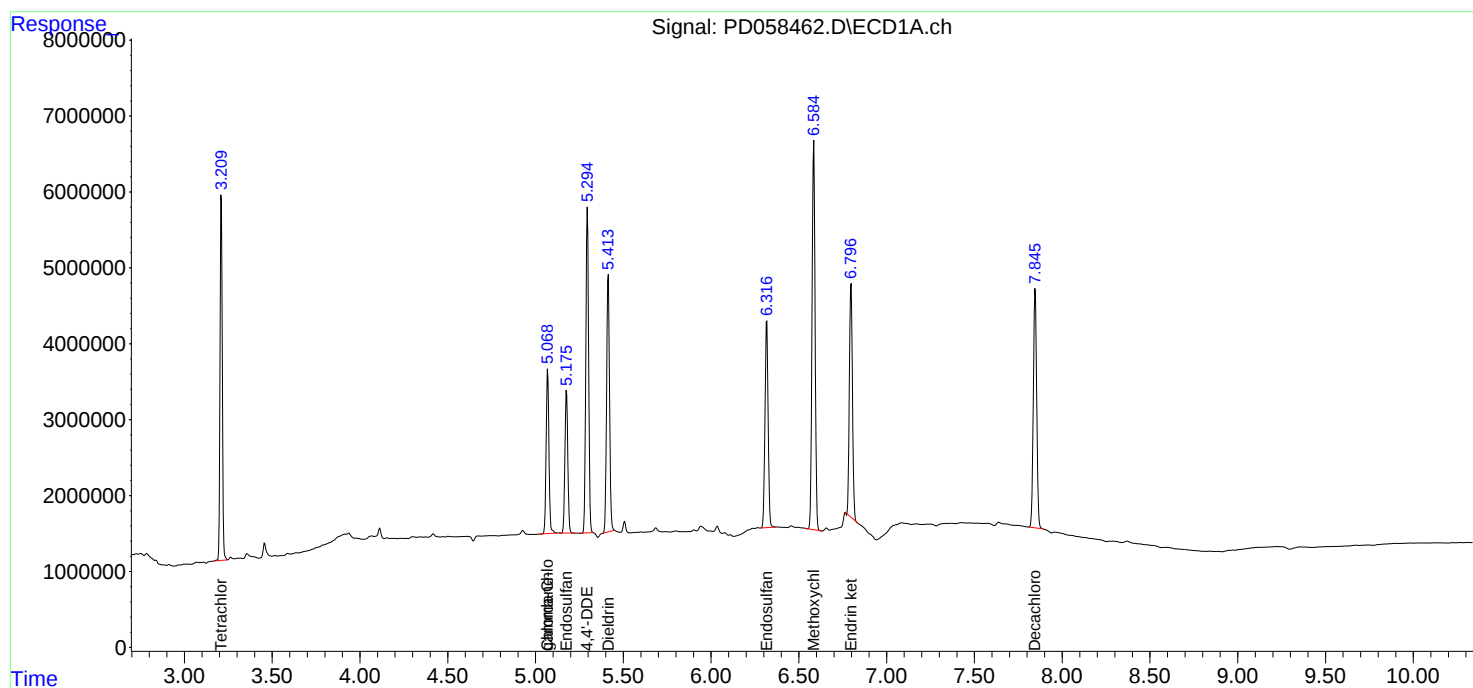


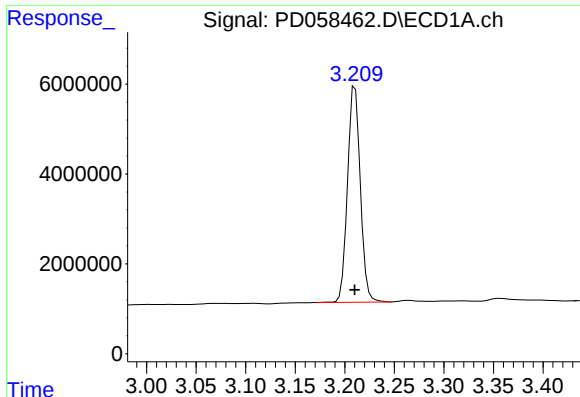

#1 Tetrachloro-m-xylene


R.T.: 3.210 min
Delta R.T.: 0.000 min
Response: 43226574
Conc: 23.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

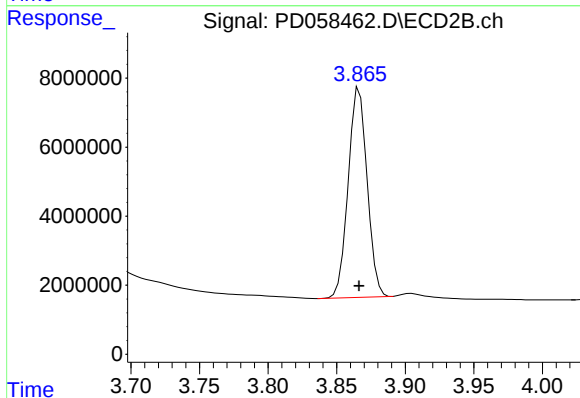


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 58323300
Conc: 23.61 ng/ml

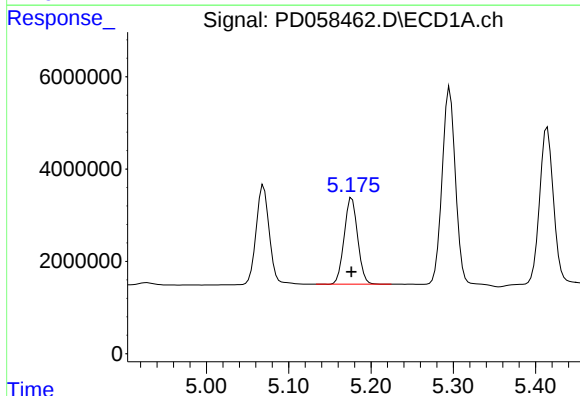


#9 Endosulfan I

R.T.: 5.177 min
Delta R.T.: 0.000 min
Response: 21308495
Conc: 10.75 ng/ml

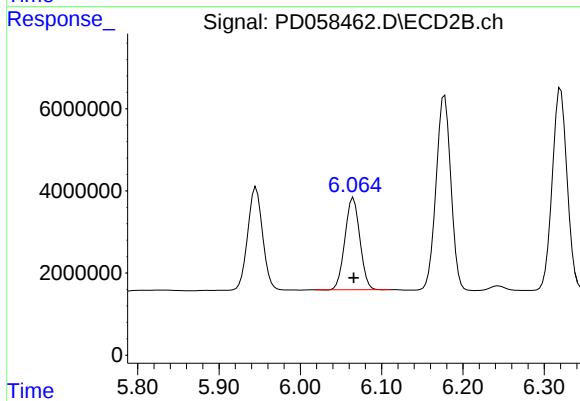

#9 Endosulfan I


R.T.: 6.065 min
Delta R.T.: 0.000 min
Response: 28521458
Conc: 10.82 ng/ml

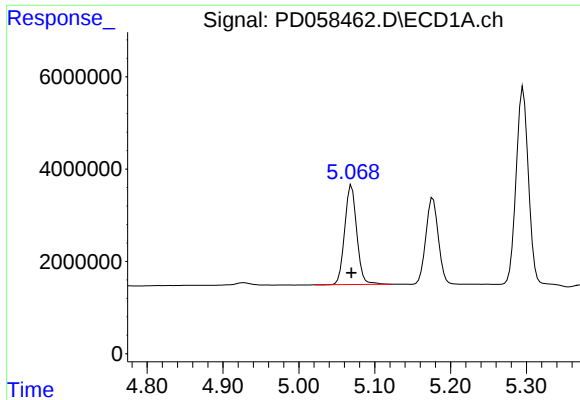

#10 gamma-Chlordane


R.T.: 5.069 min
Delta R.T.: 0.000 min
Response: 23821744
Conc: 10.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

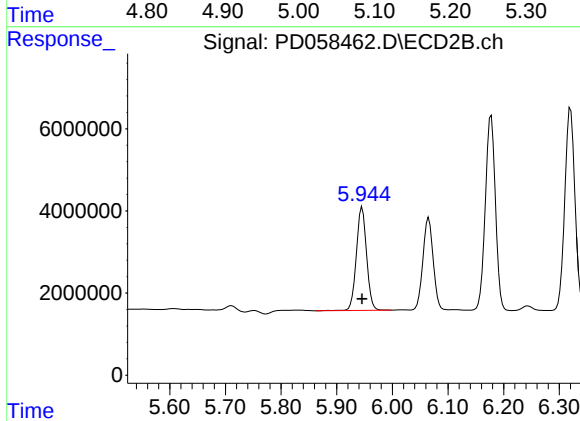


#10 gamma-Chlordane

R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 32170807
Conc: 11.06 ng/ml

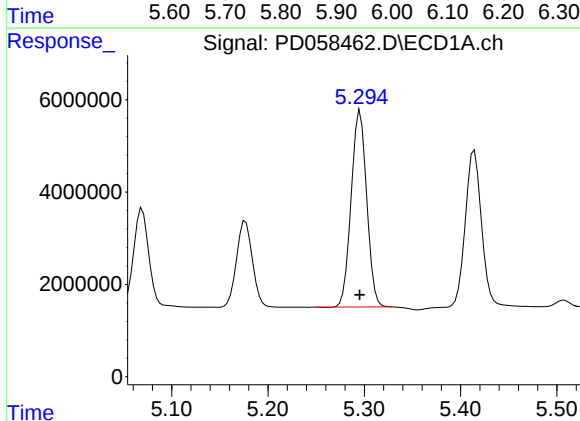


#12 4,4'-DDE

R.T.: 5.296 min
Delta R.T.: 0.000 min
Response: 47579856
Conc: 22.05 ng/ml

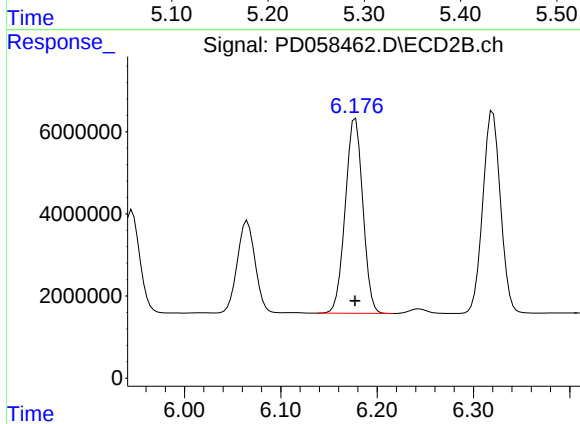

#12 4,4'-DDE


R.T.: 6.178 min
Delta R.T.: 0.000 min
Response: 59940579
Conc: 21.81 ng/ml

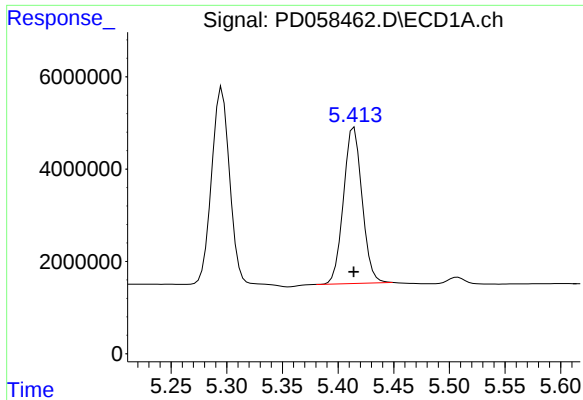

#13 Dieldrin


R.T.: 5.414 min
Delta R.T.: 0.000 min
Response: 39304810
Conc: 22.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

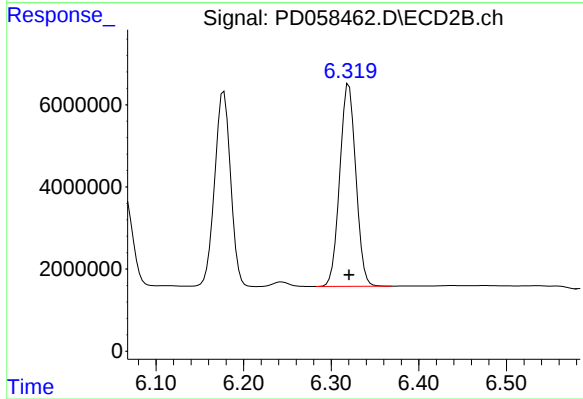


#13 Dieldrin

R.T.: 6.320 min
Delta R.T.: 0.000 min
Response: 62985561
Conc: 22.05 ng/ml

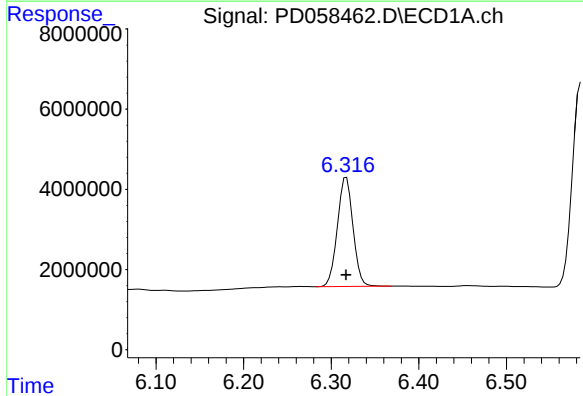


#19 Endosulfan Sulfate

R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 33728520
Conc: 21.20 ng/ml

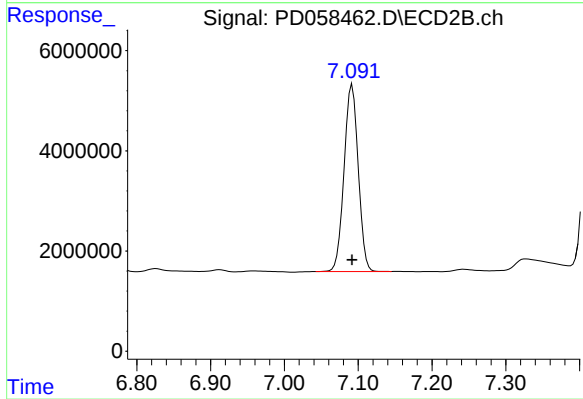

#19 Endosulfan Sulfate


R.T.: 7.092 min
Delta R.T.: 0.000 min
Response: 49756077
Conc: 21.70 ng/ml

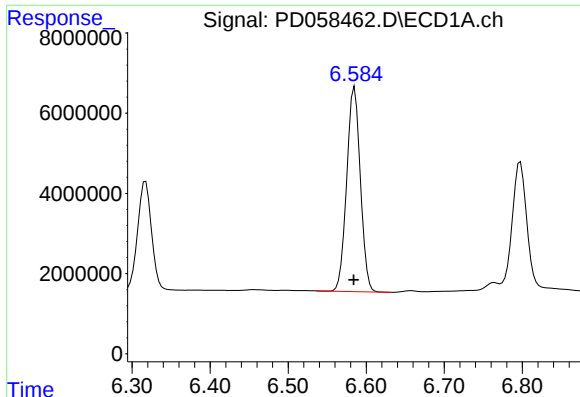

#20 Methoxychlor


R.T.: 6.585 min
Delta R.T.: 0.000 min
Response: 61943975
Conc: 105.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

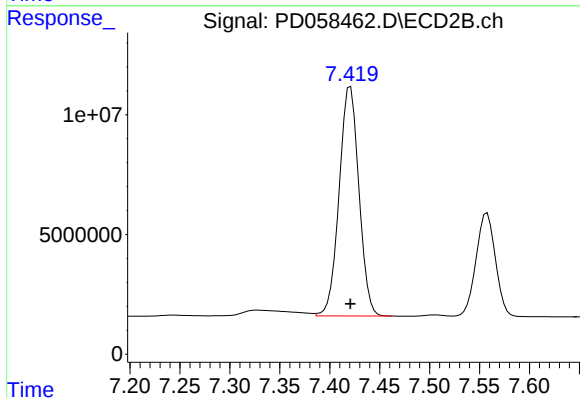


#20 Methoxychlor

R.T.: 7.421 min
Delta R.T.: 0.000 min
Response: 132183291
Conc: 109.96 ng/ml

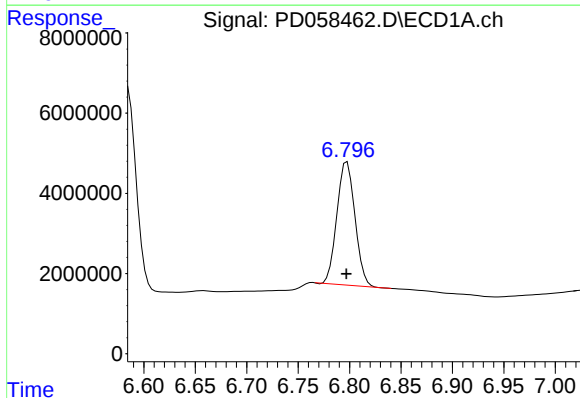


#21 Endrin ketone

R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 37361579
Conc: 20.54 ng/ml

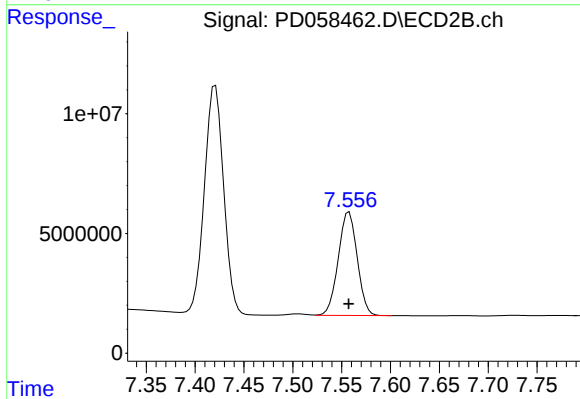

#21 Endrin ketone


R.T.: 7.558 min
Delta R.T.: 0.000 min
Response: 58357438
Conc: 21.44 ng/ml

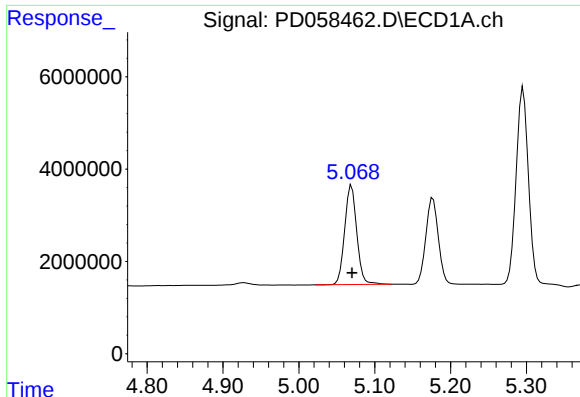

#25 Chlordane-3


R.T.: 5.069 min
Delta R.T.: 0.000 min
Response: 23821744
Conc: 116.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

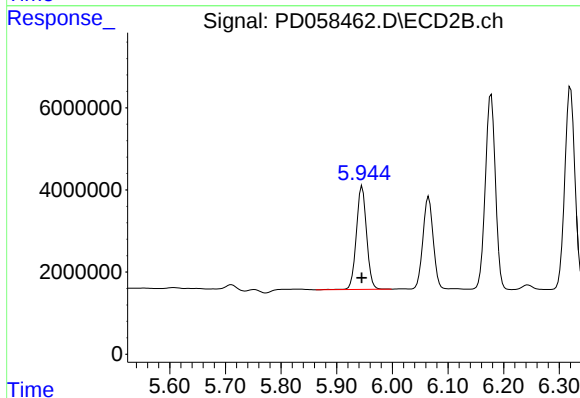


#25 Chlordane-3

R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 32170807
Conc: 86.49 ng/ml

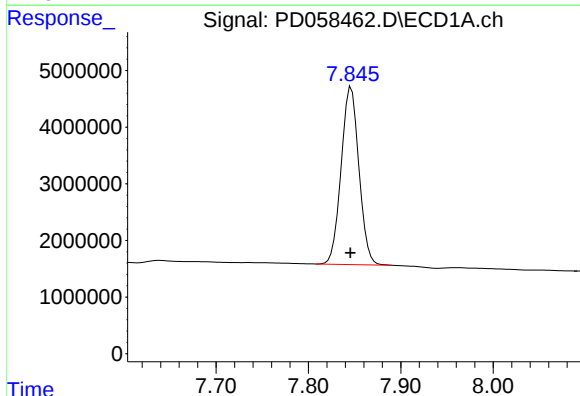

#28 Decachlorobiphenyl

R.T.: 7.846 min
Delta R.T.: 0.001 min
Response: 41900827
Conc: 23.20 ng/ml

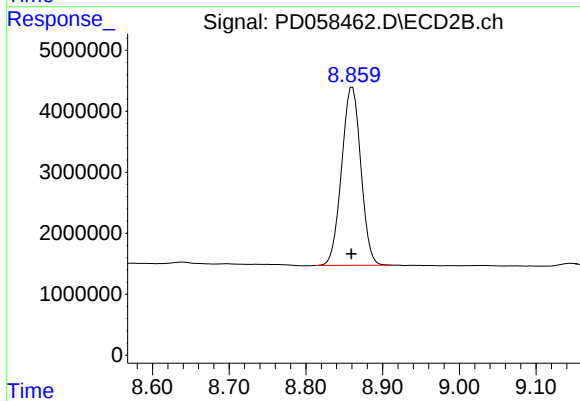

#28 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.001 min
Response: 51110047
Conc: 23.44 ng/ml