

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070720\
 Data File : PD058473.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2020 12:30
 Operator : AJ\MA
 Sample : PTOXICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 13:55:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX070720.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 07 13:52:21 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.210	3.866	180.5E6	240.1E6	98.332	96.386
7) SA Decachlor...	7.845	8.859	165.8E6	193.8E6	94.062	92.005
Target Compounds						
2) Toxaphene-1	5.595	6.412	16346871	24763818	875.079	970.913
3) Toxaphene-2	5.969	6.703	27536964	26554288	940.594	932.976
4) Toxaphene-3	6.211	6.991	26351198	62673955	940.386	1013.140
5) Toxaphene-4	6.346	7.076	9957644	37512120	810.969	1004.800
6) Toxaphene-5	6.629	7.486	10778363	27197752	1034.985	993.118

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070720\
Data File : PD058473.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2020 12:30
Operator : AJ\MA
Sample : PTOXICC1000
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 13:55:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX070720.M
Quant Title : GC Extractables
QLast Update : Tue Jul 07 13:52:21 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

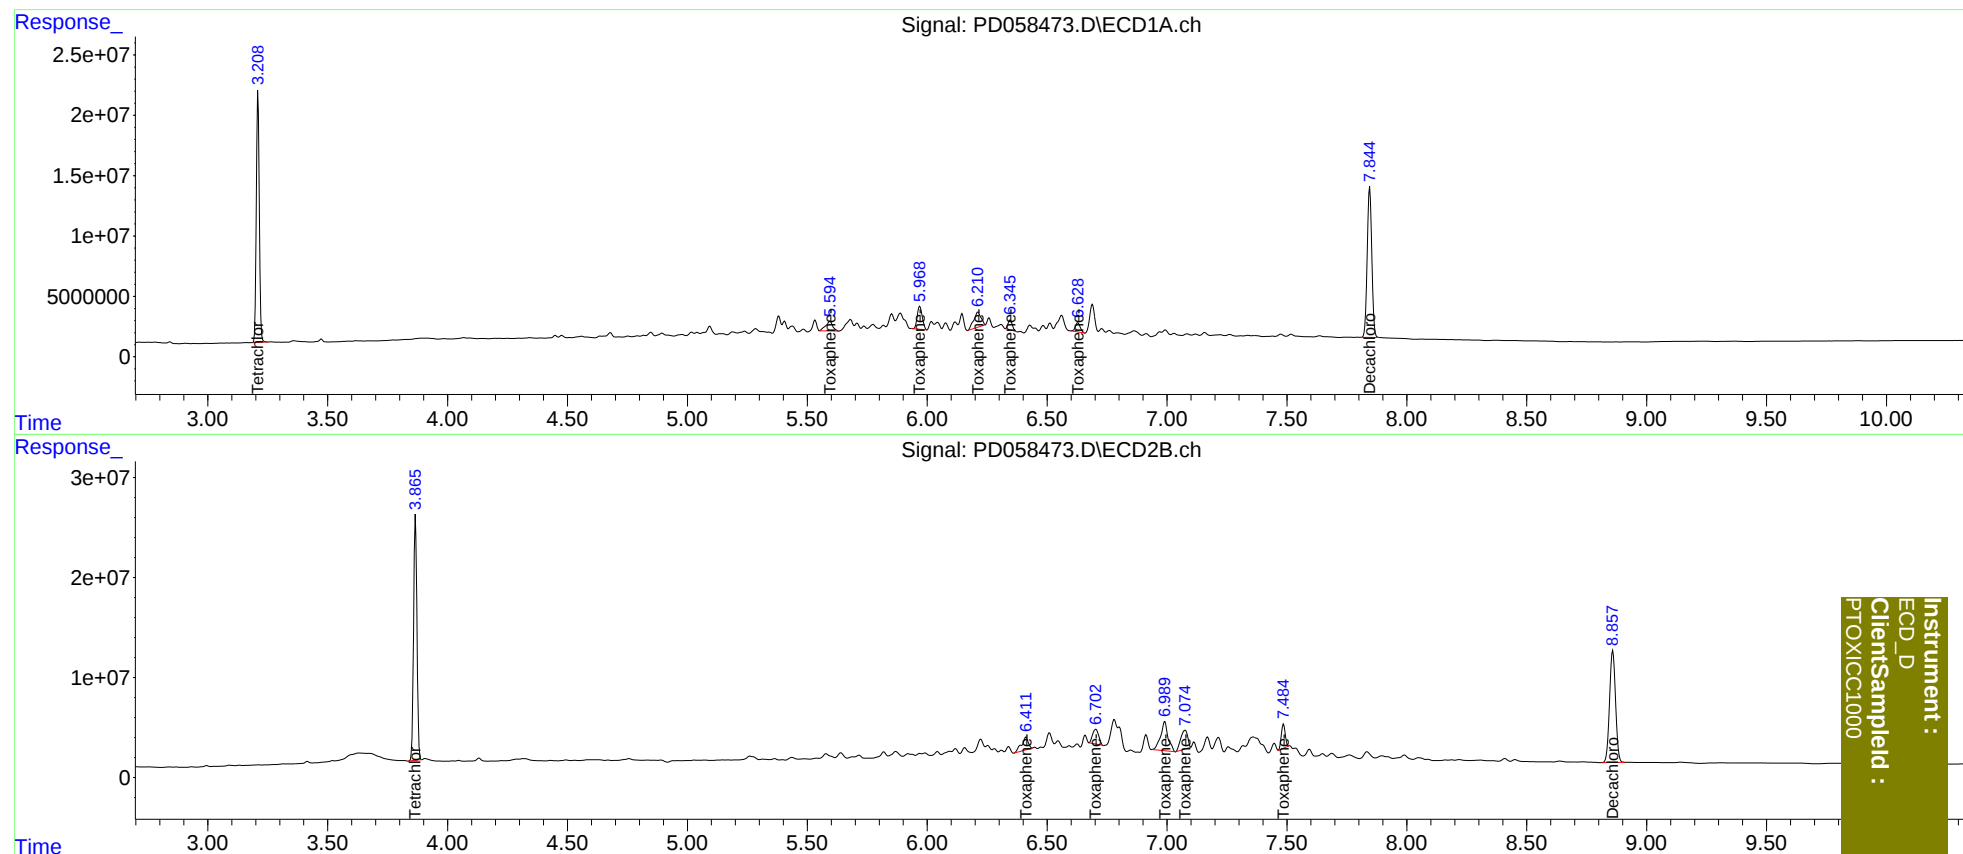

Instrument :
ECD_D
ClientSampled :
PTOXICC1000