

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070720\
 Data File : PD058469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2020 11:31
 Operator : AJ\MA
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 12:10:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 07 12:08:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.210	3.867	151.7E6	186.2E6	74.696	74.280
28)	SA Decachlor...	7.846	8.860	131.1E6	148.0E6	73.745	71.056
Target Compounds							
23)	Chlordane-1	4.038	4.843	44013616	67832733	750.171	752.333
24)	Chlordane-2	4.522	5.307	46670487	69566224	714.608	730.623
25)	Chlordane-3	5.071	5.946	159.4E6	289.6E6	752.865	758.239
26)	Chlordane-4	5.126	6.020	149.8E6	335.3E6	775.030	752.286
27)	Chlordane-5	5.942	6.816	46667832	62884147	735.586	770.993



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070720\
Data File : PD058469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2020 11:31
Operator : AJ\MA
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 12:10:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Tue Jul 07 12:08:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

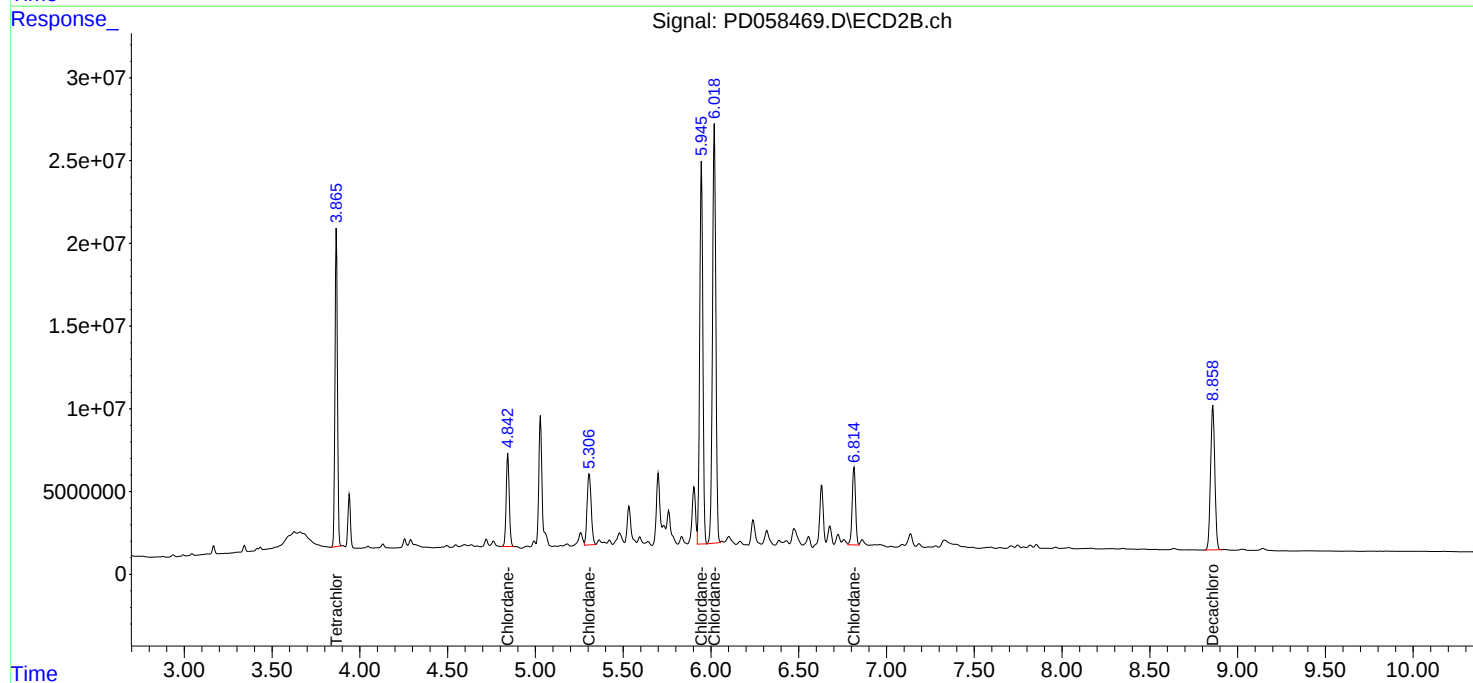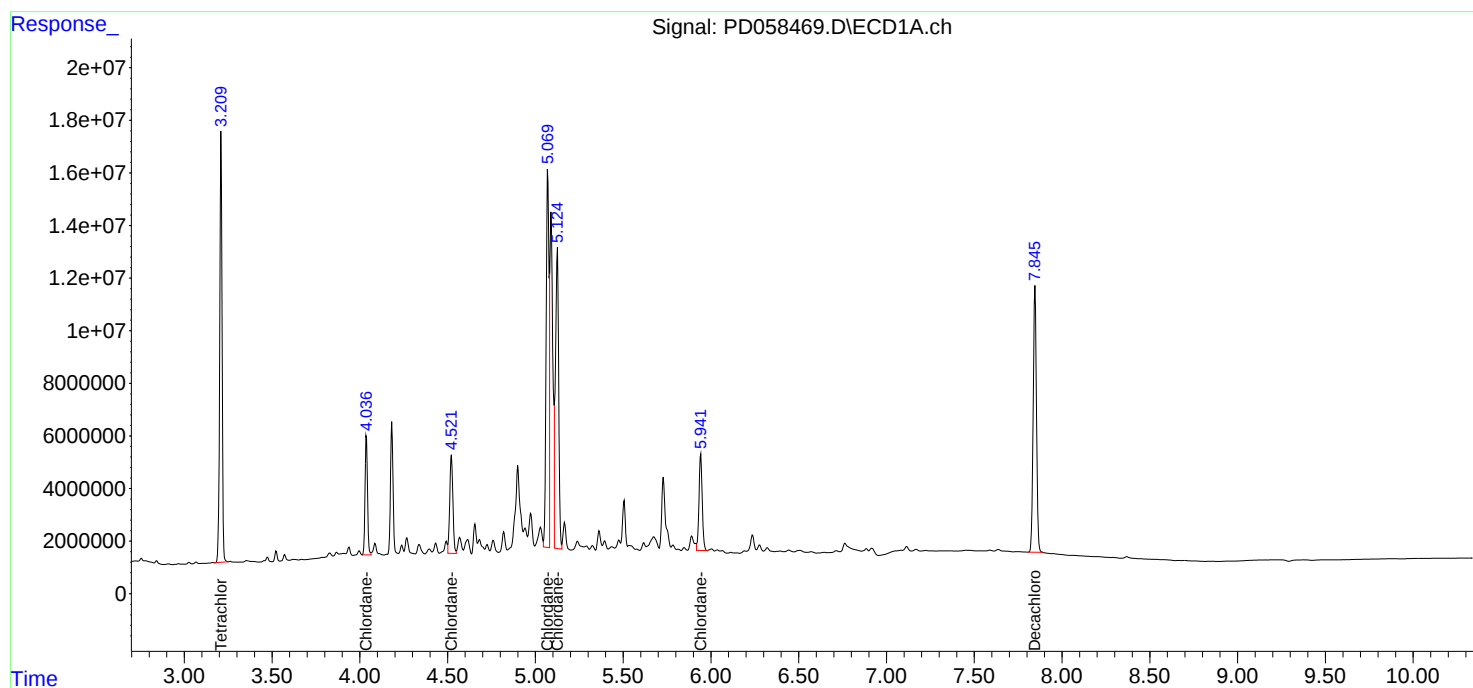


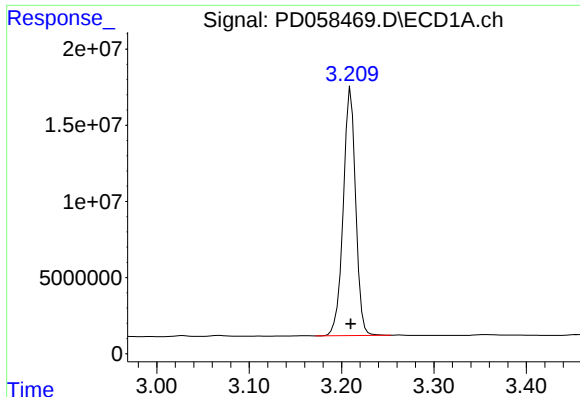

#1 Tetrachloro-m-xylene


R.T.: 3.210 min
Delta R.T.: 0.000 min
Response: 151653801
Conc: 74.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

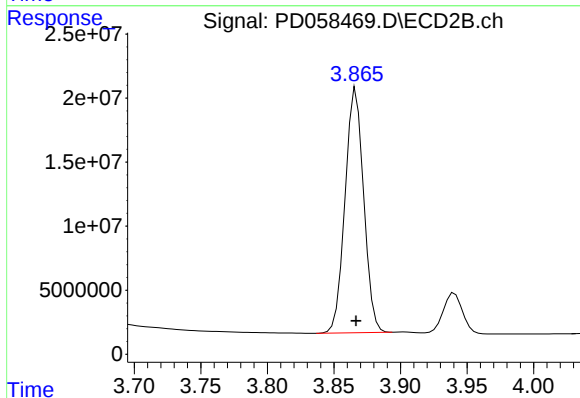


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 186212048
Conc: 74.28 ng/ml

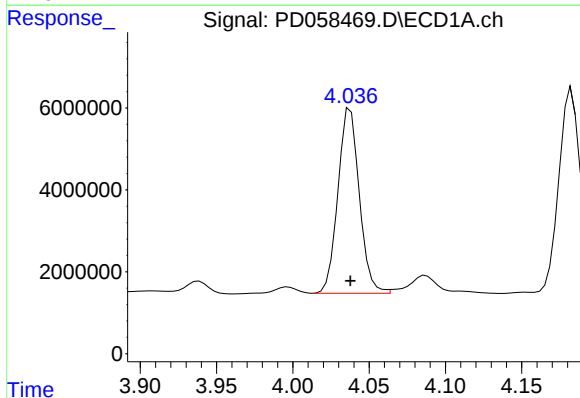


#23 Chlordane-1

R.T.: 4.038 min
Delta R.T.: 0.000 min
Response: 44013616
Conc: 750.17 ng/ml

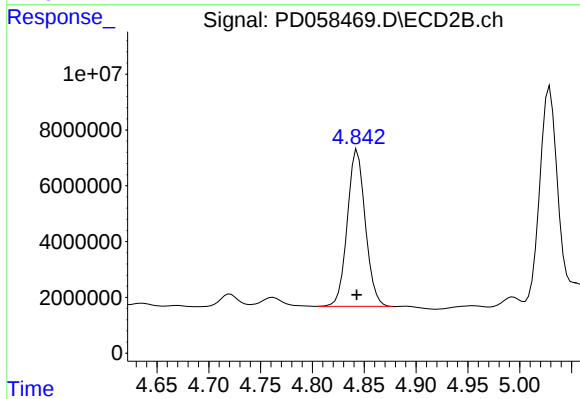

#23 Chlordane-1


R.T.: 4.843 min
Delta R.T.: 0.000 min
Response: 67832733
Conc: 752.33 ng/ml

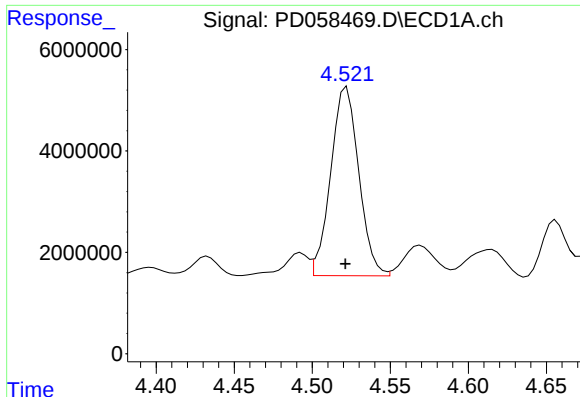

#24 Chlordane-2


R.T.: 4.522 min
Delta R.T.: 0.000 min
Response: 46670487
Conc: 714.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

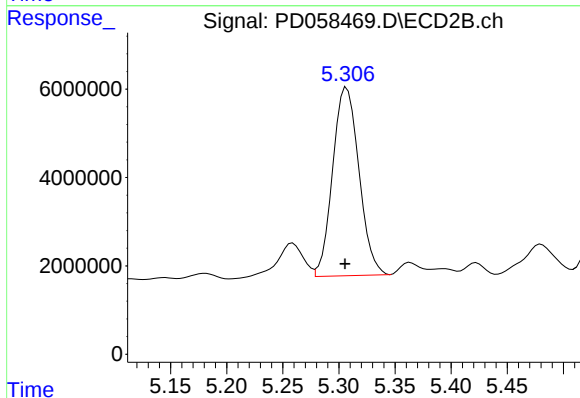


#24 Chlordane-2

R.T.: 5.307 min
Delta R.T.: 0.001 min
Response: 69566224
Conc: 730.62 ng/ml

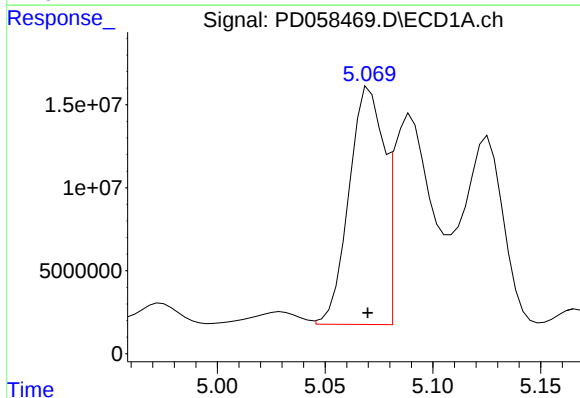


#25 Chlordane-3

R.T.: 5.071 min
Delta R.T.: 0.000 min
Response: 159431357
Conc: 752.86 ng/ml

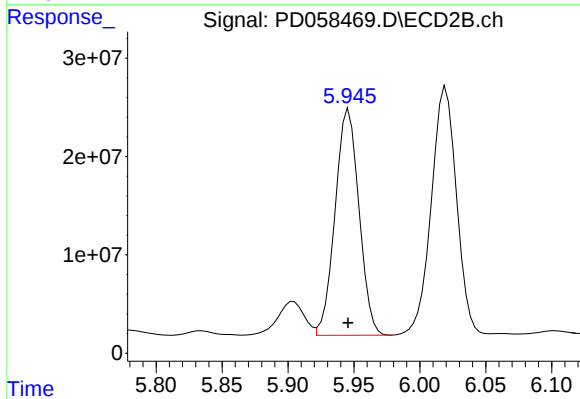

#25 Chlordane-3


R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 289636035
Conc: 758.24 ng/ml

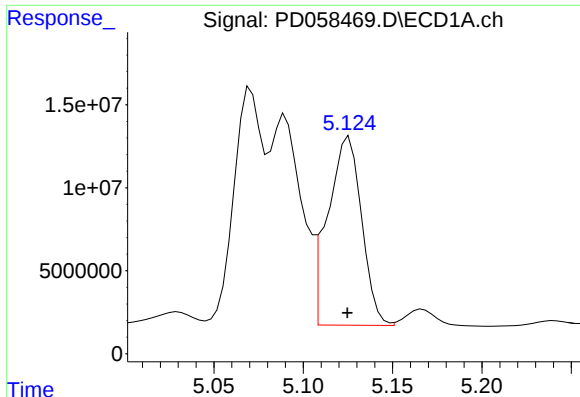

#26 Chlordane-4


R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 149781966
Conc: 775.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

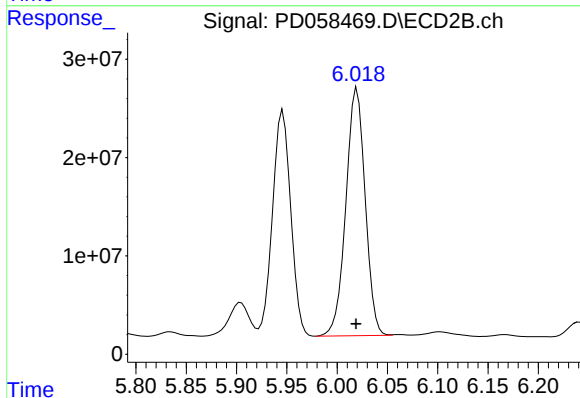


#26 Chlordane-4

R.T.: 6.020 min
Delta R.T.: 0.000 min
Response: 335334059
Conc: 752.29 ng/ml

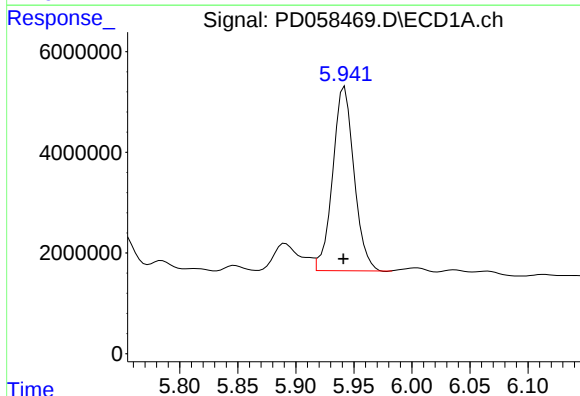


#27 Chlordane-5

R.T.: 5.942 min
Delta R.T.: 0.001 min
Response: 46667832
Conc: 735.59 ng/ml

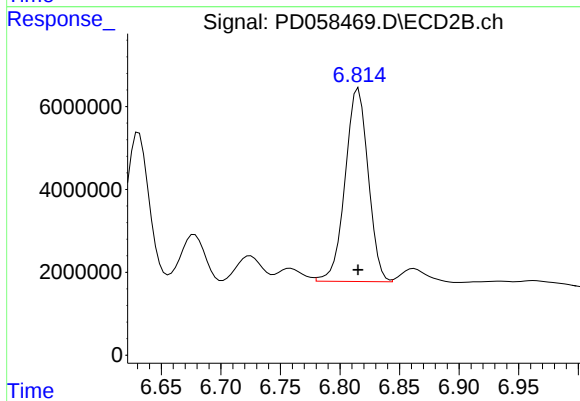

#27 Chlordane-5


R.T.: 6.816 min
Delta R.T.: 0.000 min
Response: 62884147
Conc: 770.99 ng/ml

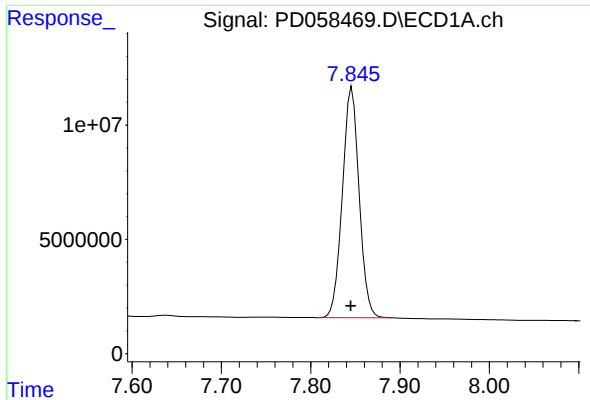

#28 Decachlorobiphenyl

R.T.: 7.846 min
Delta R.T.: 0.001 min
Response: 131084846
Conc: 73.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

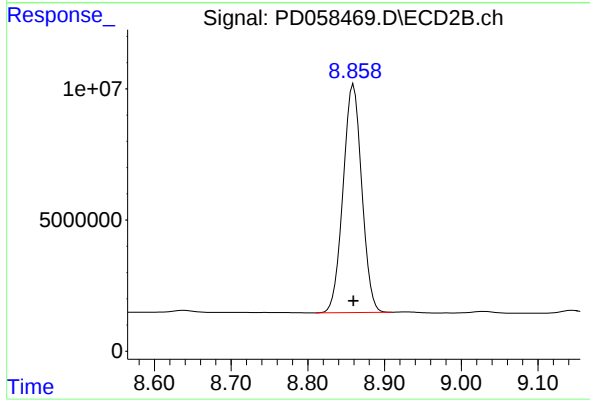

#28 Decachlorobiphenyl

R.T.: 8.860 min
Delta R.T.: 0.000 min
Response: 147964890
Conc: 71.06 ng/ml