

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070720\
 Data File : PD058470.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2020 11:46
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 12:10:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 07 12:08:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.210	3.867	101.5E6	125.3E6	50.000	50.000
28)	SA Decachlor...	7.845	8.859	88876618	104.1E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.038	4.843	29335724	45081560	500.000	500.000
24)	Chlordane-2	4.521	5.306	32654625	47607460	500.000	500.000
25)	Chlordane-3	5.070	5.946	105.9E6	191.0E6	500.000	500.000
26)	Chlordane-4	5.125	6.019	96629833	222.9E6	500.000	500.000
27)	Chlordane-5	5.941	6.815	31721551	40781267	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070720\
Data File : PD058470.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2020 11:46
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 12:10:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Tue Jul 07 12:08:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

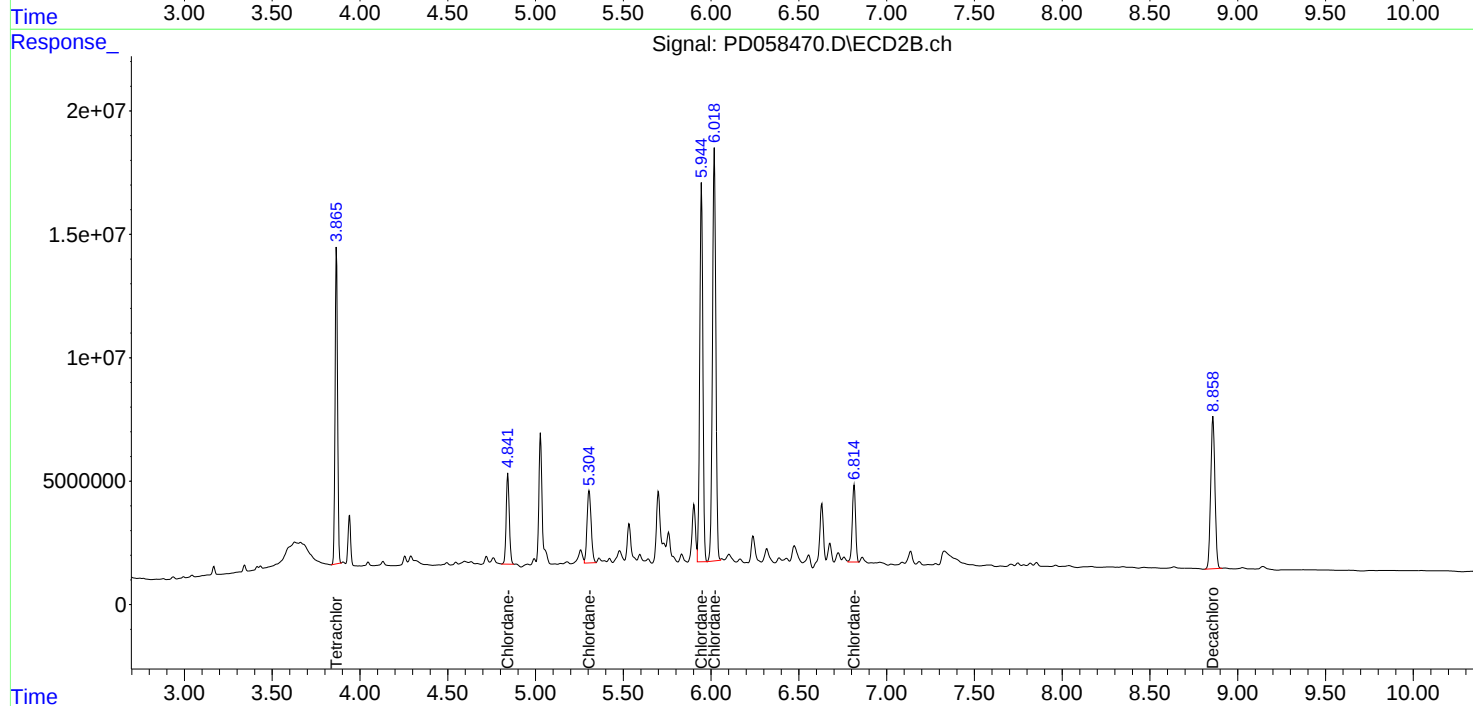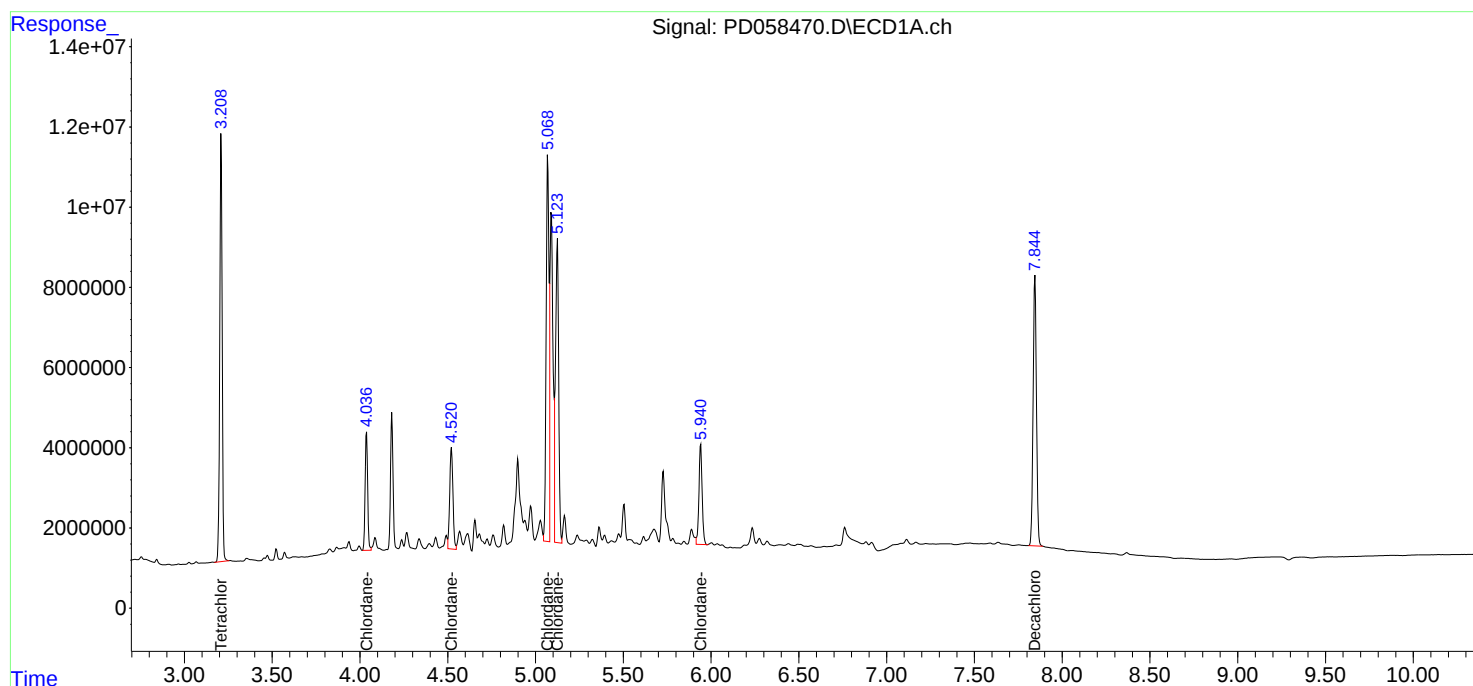


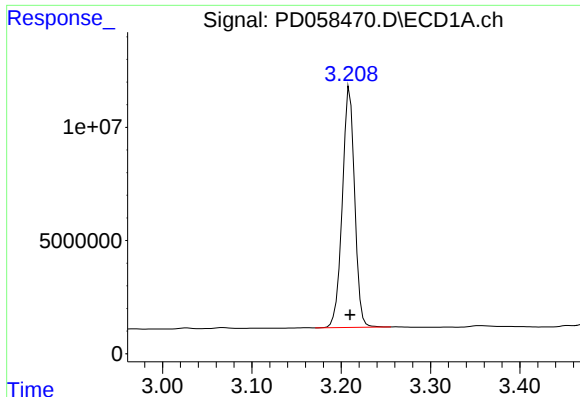

#1 Tetrachloro-m-xylene


R.T.: 3.210 min
Delta R.T.: 0.000 min
Response: 101514435
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

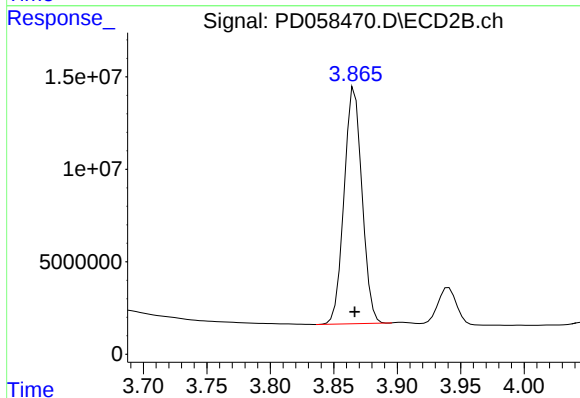


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 125344401
Conc: 50.00 ng/ml

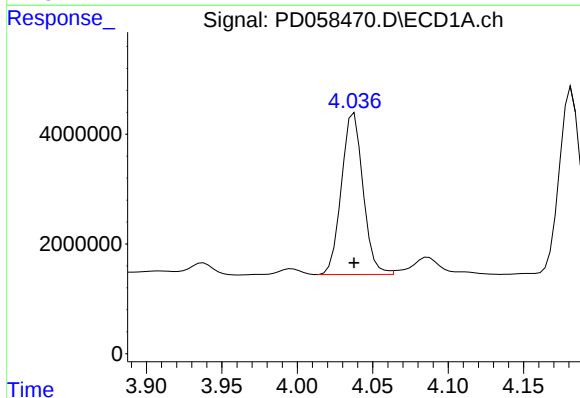


#23 Chlordane-1

R.T.: 4.038 min
Delta R.T.: 0.000 min
Response: 29335724
Conc: 500.00 ng/ml

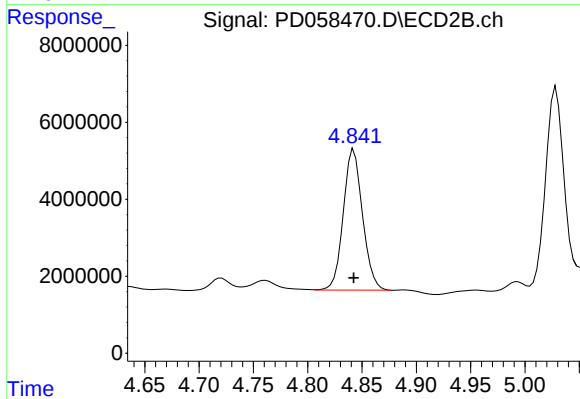

#23 Chlordane-1


R.T.: 4.843 min
Delta R.T.: 0.000 min
Response: 45081560
Conc: 500.00 ng/ml

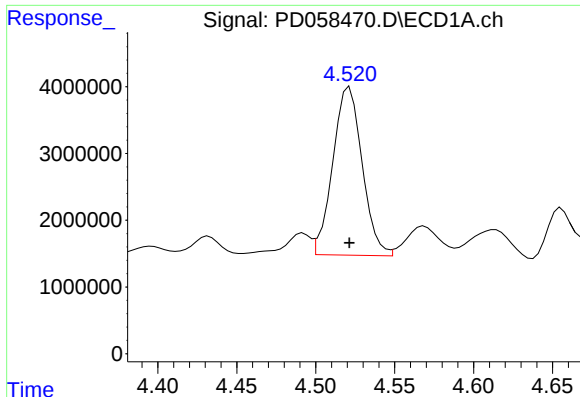

#24 Chlordane-2


R.T.: 4.521 min
Delta R.T.: 0.000 min
Response: 32654625
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

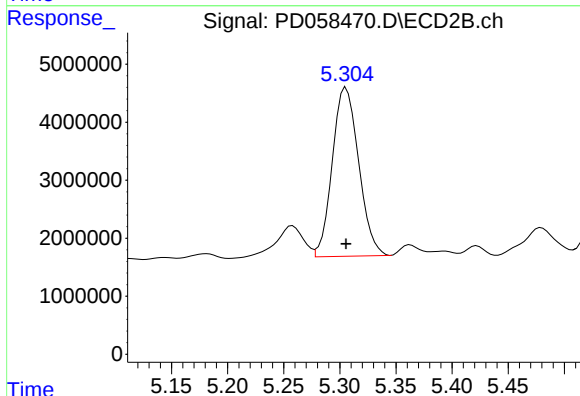


#24 Chlordane-2

R.T.: 5.306 min
Delta R.T.: 0.000 min
Response: 47607460
Conc: 500.00 ng/ml

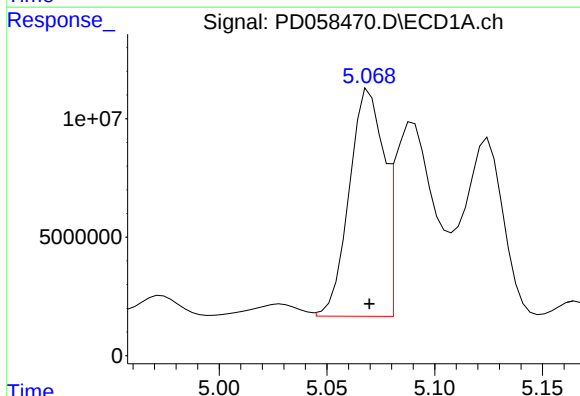


#25 Chlordane-3

R.T.: 5.070 min
Delta R.T.: 0.000 min
Response: 105883125
Conc: 500.00 ng/ml

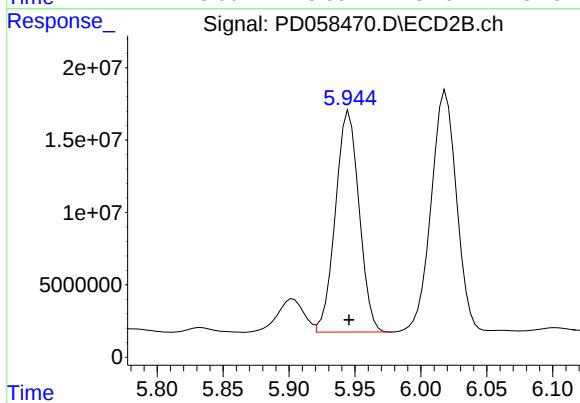

#25 Chlordane-3


R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 190992587
Conc: 500.00 ng/ml

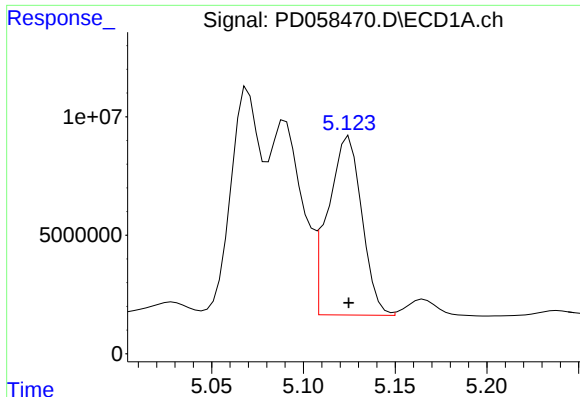

#26 Chlordane-4


R.T.: 5.125 min
Delta R.T.: 0.000 min
Response: 96629833
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

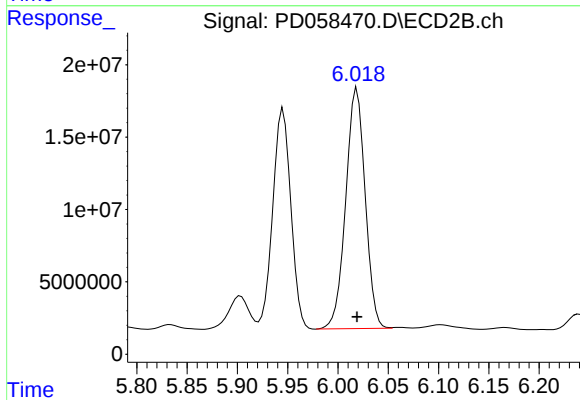


#26 Chlordane-4

R.T.: 6.019 min
Delta R.T.: 0.000 min
Response: 222876755
Conc: 500.00 ng/ml

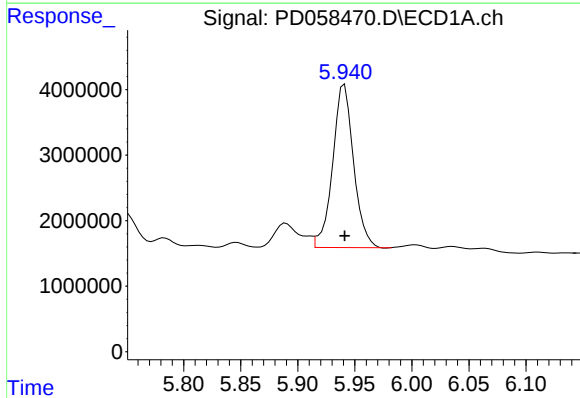


#27 Chlordane-5

R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 31721551
Conc: 500.00 ng/ml

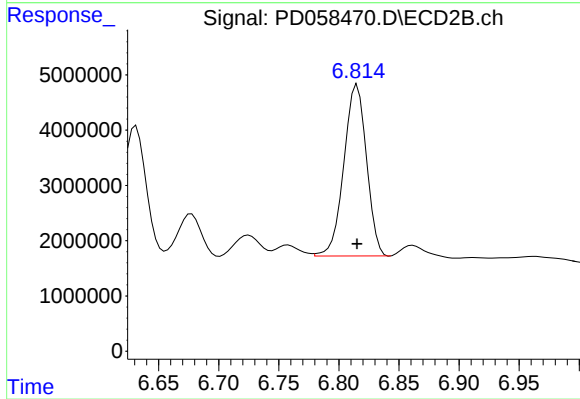

#27 Chlordane-5


R.T.: 6.815 min
Delta R.T.: 0.000 min
Response: 40781267
Conc: 500.00 ng/ml

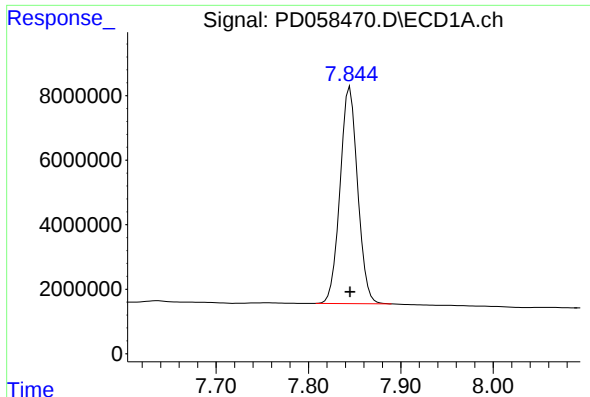

#28 Decachlorobiphenyl

R.T.: 7.845 min
Delta R.T.: 0.000 min
Response: 88876618
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

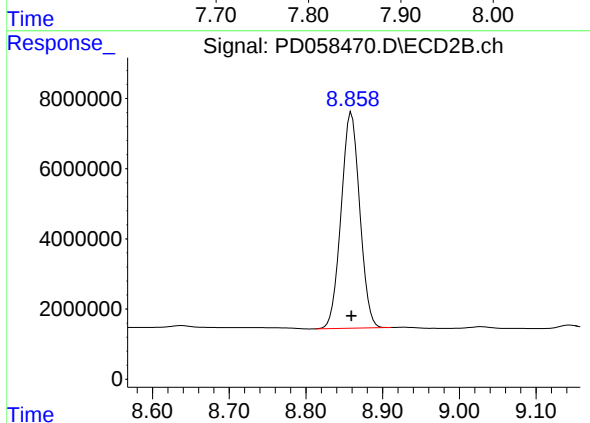

#28 Decachlorobiphenyl

R.T.: 8.859 min
Delta R.T.: 0.000 min
Response: 104118730
Conc: 50.00 ng/ml