

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070720\
 Data File : PD058471.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2020 12:01
 Operator : AJ\MA
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 12:27:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 07 12:08:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.210	3.866	48669446	61062191	23.972	24.358
28)	SA Decachlor...	7.846	8.860	44459757	53781783	25.012	25.827
Target Compounds							
23)	Chlordane-1	4.037	4.843	14318189	22110532	244.040	245.228
24)	Chlordane-2	4.522	5.306	16444721	24564804	251.798	257.993
25)	Chlordane-3	5.070	5.946	51015701	91170426	240.906	238.675
26)	Chlordane-4	5.125	6.019	47062018	107.1E6	243.517	240.191
27)	Chlordane-5	5.941	6.815	15690520	19523574	247.316	239.369



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070720\
Data File : PD058471.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2020 12:01
Operator : AJ\MA
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 12:27:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Tue Jul 07 12:08:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

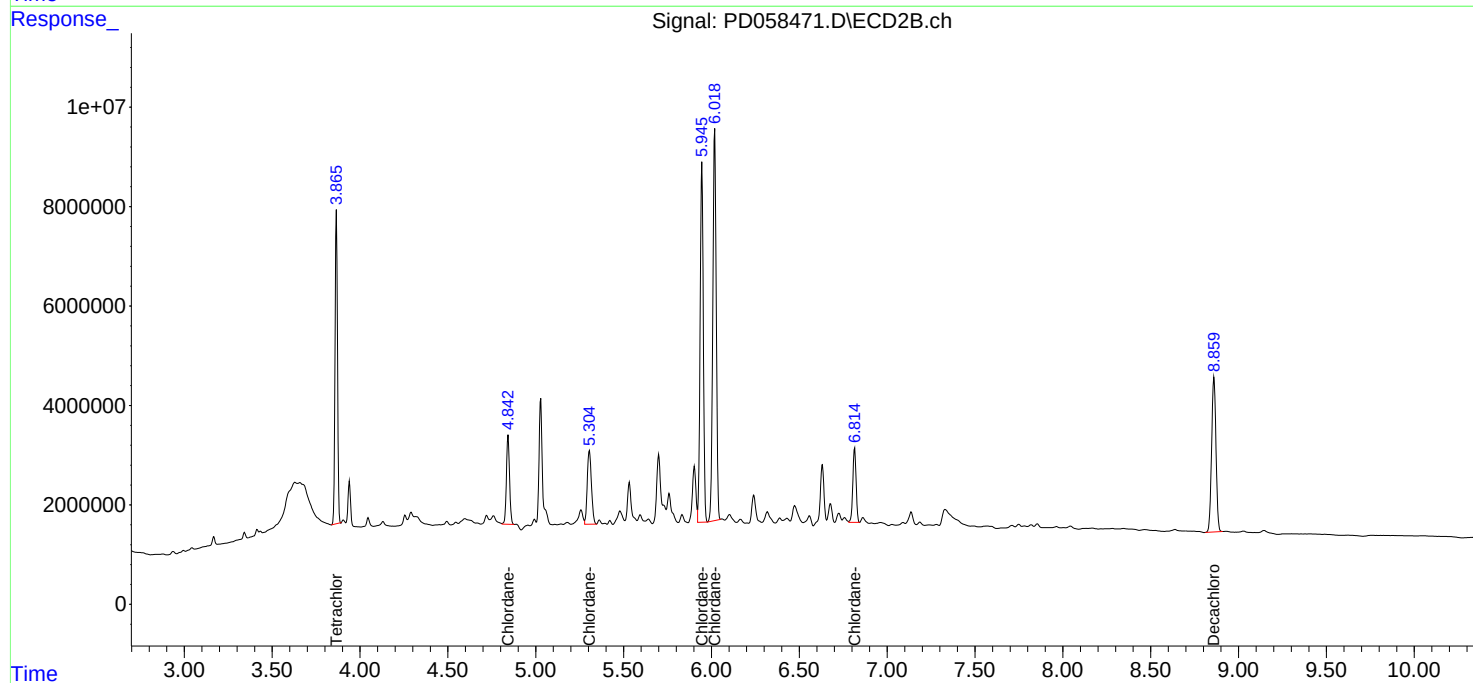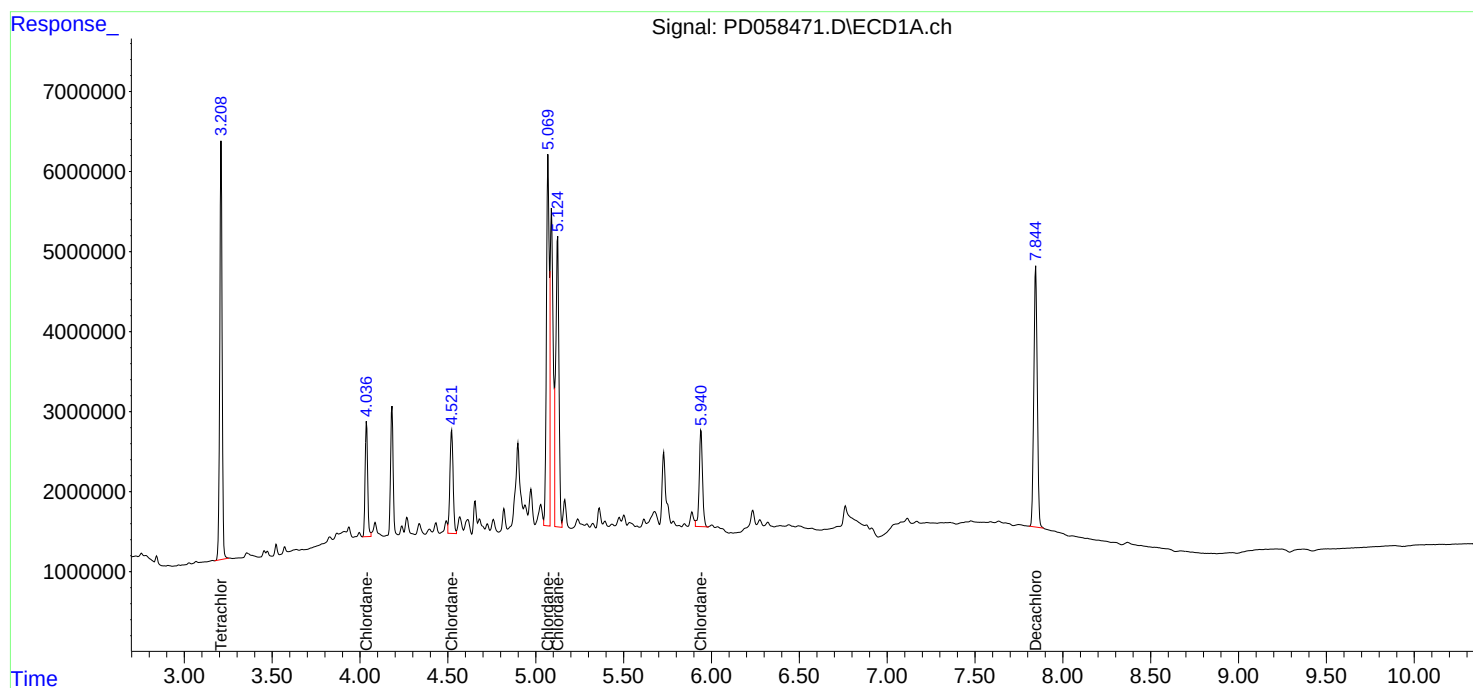


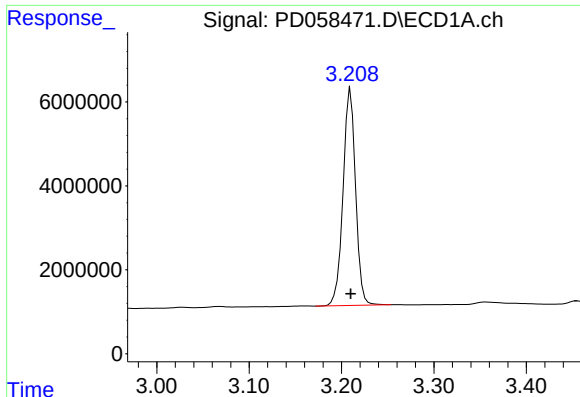

#1 Tetrachloro-m-xylene


R.T.: 3.210 min
Delta R.T.: 0.000 min
Response: 48669446
Conc: 23.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

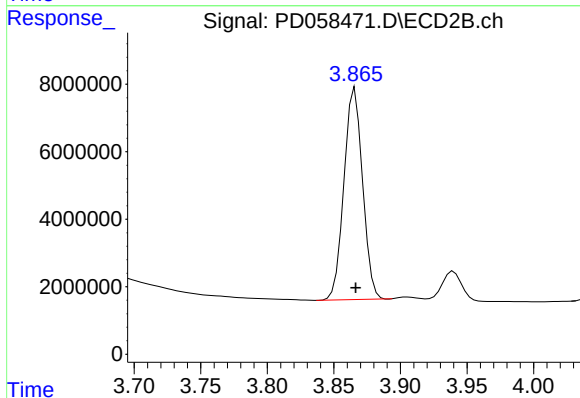


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 61062191
Conc: 24.36 ng/ml

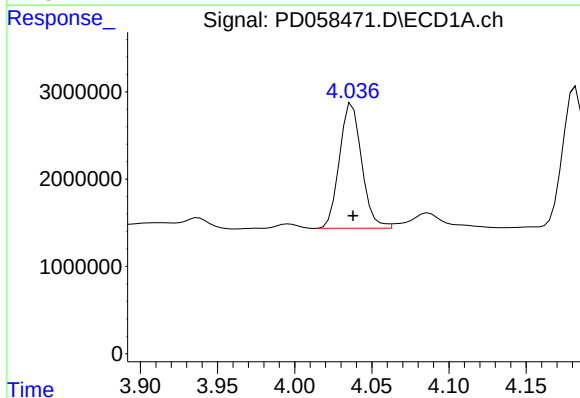


#23 Chlordane-1

R.T.: 4.037 min
Delta R.T.: 0.000 min
Response: 14318189
Conc: 244.04 ng/ml

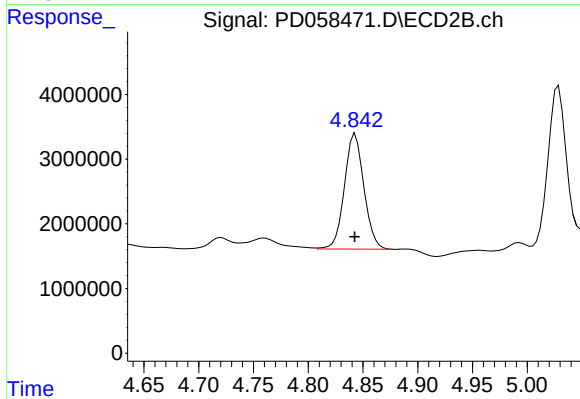

#23 Chlordane-1


R.T.: 4.843 min
Delta R.T.: 0.000 min
Response: 22110532
Conc: 245.23 ng/ml

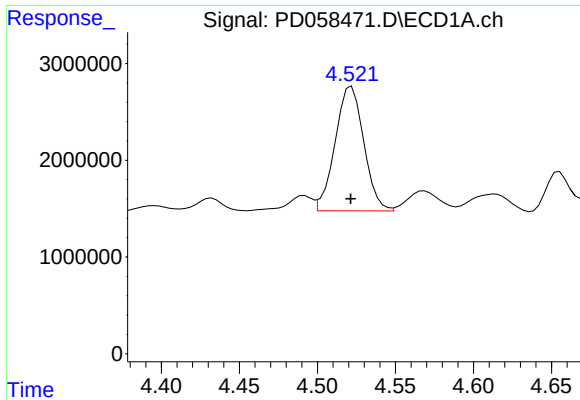

#24 Chlordane-2


R.T.: 4.522 min
Delta R.T.: 0.000 min
Response: 16444721
Conc: 251.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

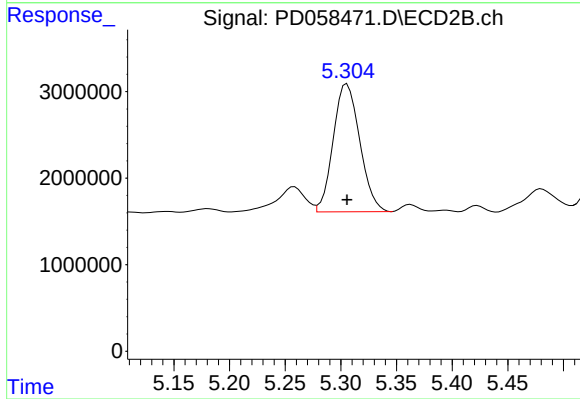


#24 Chlordane-2

R.T.: 5.306 min
Delta R.T.: 0.000 min
Response: 24564804
Conc: 257.99 ng/ml

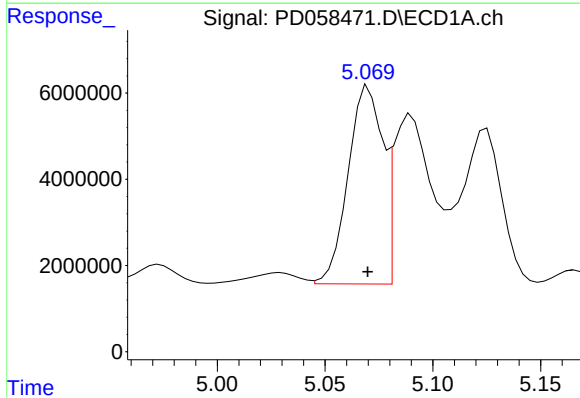


#25 Chlordane-3

R.T.: 5.070 min
Delta R.T.: 0.000 min
Response: 51015701
Conc: 240.91 ng/ml

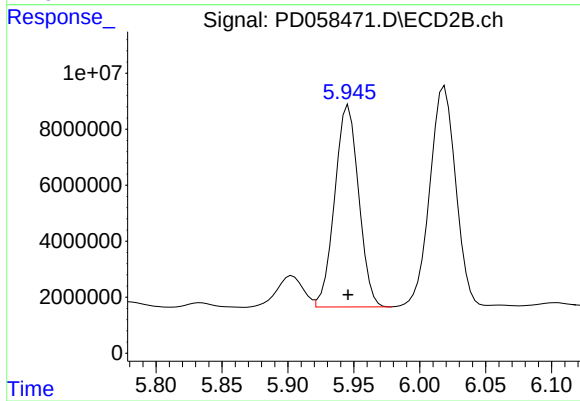

#25 Chlordane-3


R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 91170426
Conc: 238.68 ng/ml

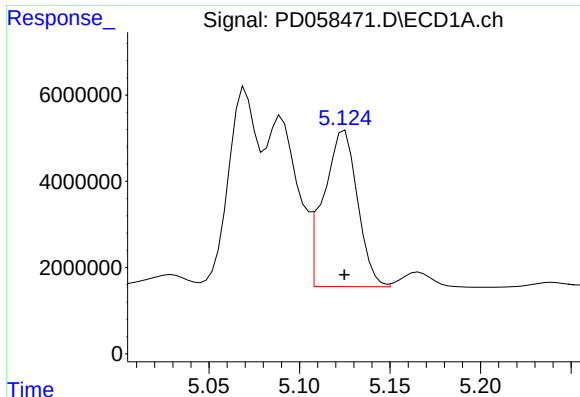

#26 Chlordane-4


R.T.: 5.125 min
Delta R.T.: 0.000 min
Response: 47062018
Conc: 243.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

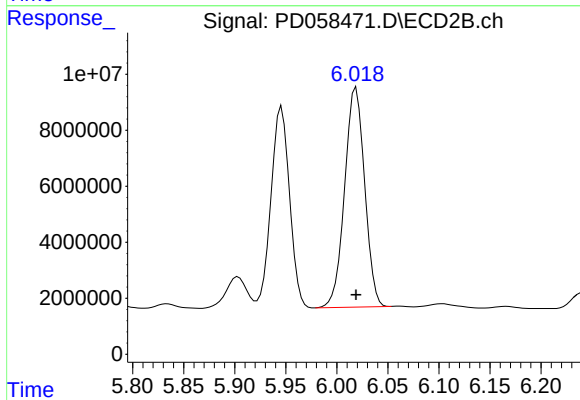


#26 Chlordane-4

R.T.: 6.019 min
Delta R.T.: 0.000 min
Response: 107065914
Conc: 240.19 ng/ml

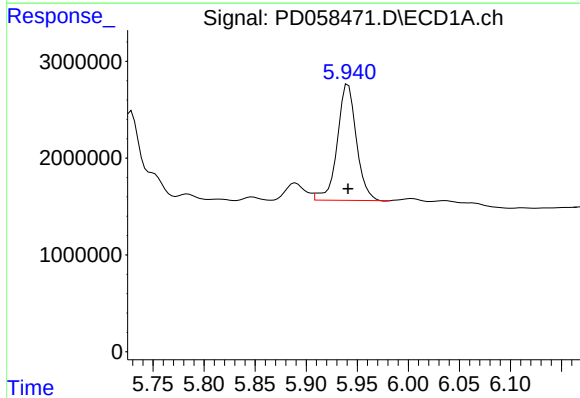


#27 Chlordane-5

R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 15690520
Conc: 247.32 ng/ml

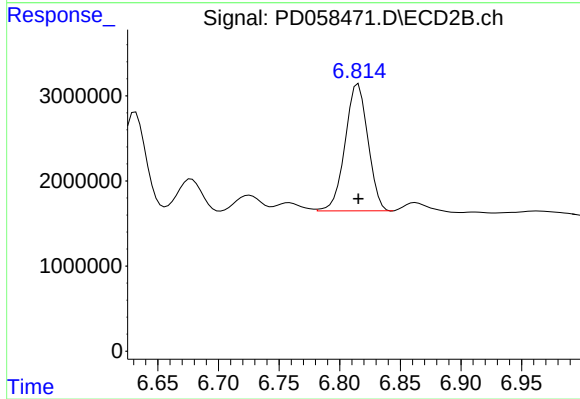

#27 Chlordane-5


R.T.: 6.815 min
Delta R.T.: 0.000 min
Response: 19523574
Conc: 239.37 ng/ml

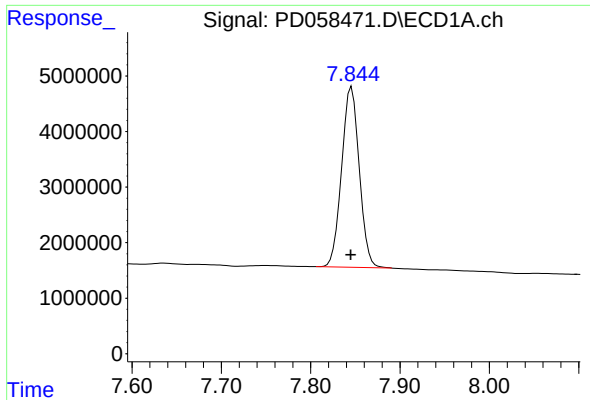

#28 Decachlorobiphenyl

R.T.: 7.846 min
Delta R.T.: 0.000 min
Response: 44459757
Conc: 25.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

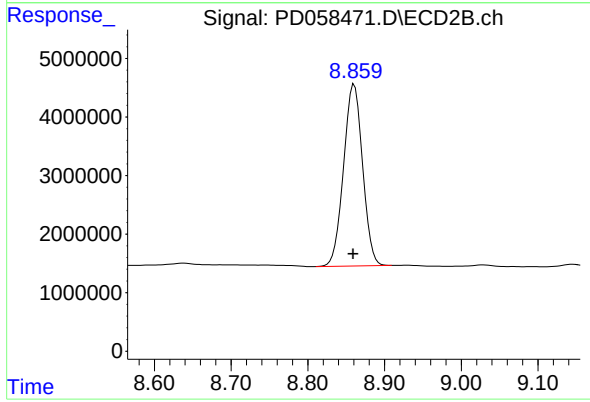

#28 Decachlorobiphenyl

R.T.: 8.860 min
Delta R.T.: 0.001 min
Response: 53781783
Conc: 25.83 ng/ml