

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070720\
 Data File : PD058479.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2020 13:58
 Operator : AJ\MA
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD070720

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 14:11:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 07 12:46:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.210	3.866	103.7E6	128.8E6	56.901	52.126
28)	SA Decachlor...	7.844	8.861	90516430	103.5E6	50.124	47.473
Target Compounds							
23)	Chlordane-1	4.038	4.842	30194913	45971240	517.454	516.525
24)	Chlordane-2	4.522	5.305	34368857	49623586	531.691	502.333
25)	Chlordane-3	5.070	5.946	109.6E6	197.0E6	535.426	529.769
26)	Chlordane-4	5.125	6.019	100.1E6	228.5E6	524.576	525.396
27)	Chlordane-5	5.941	6.816	34204299	41975260	556.601	526.806



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070720\
Data File : PD058479.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2020 13:58
Operator : AJ\MA
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD070720

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 14:11:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Tue Jul 07 12:46:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

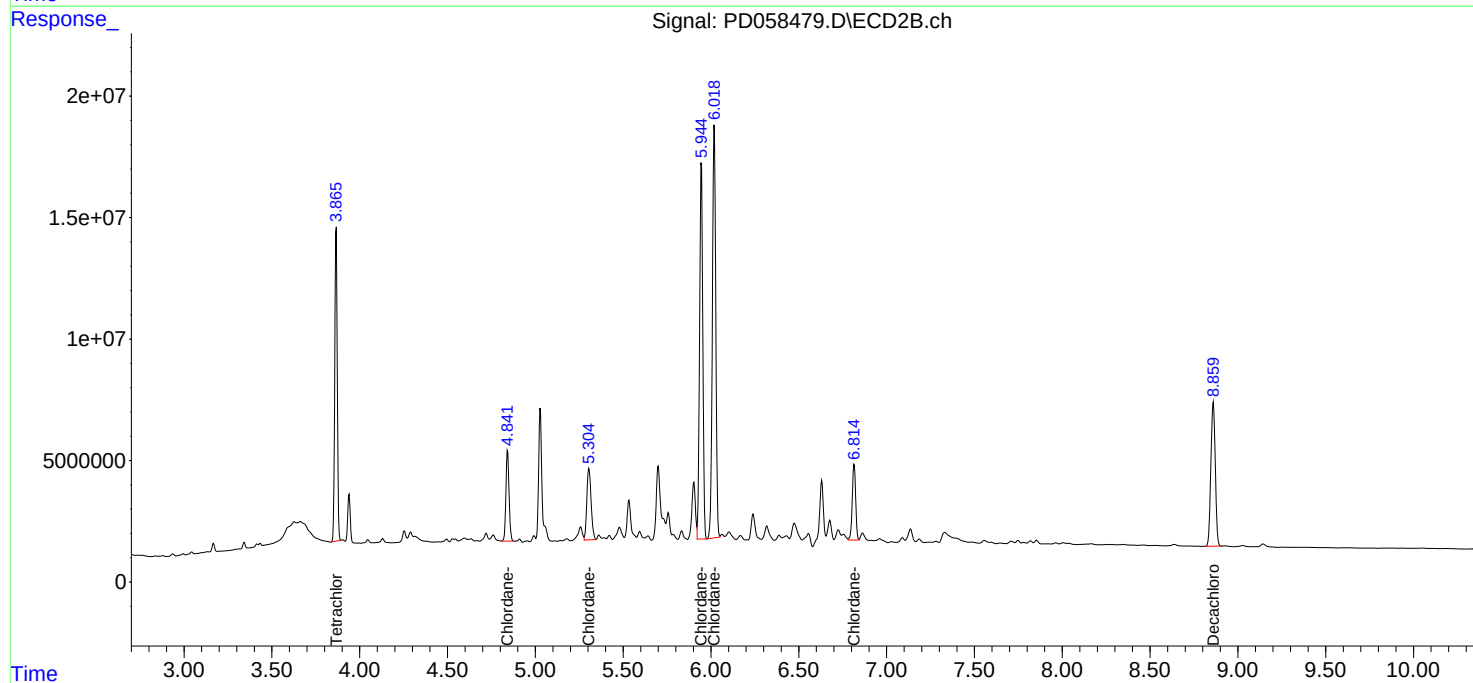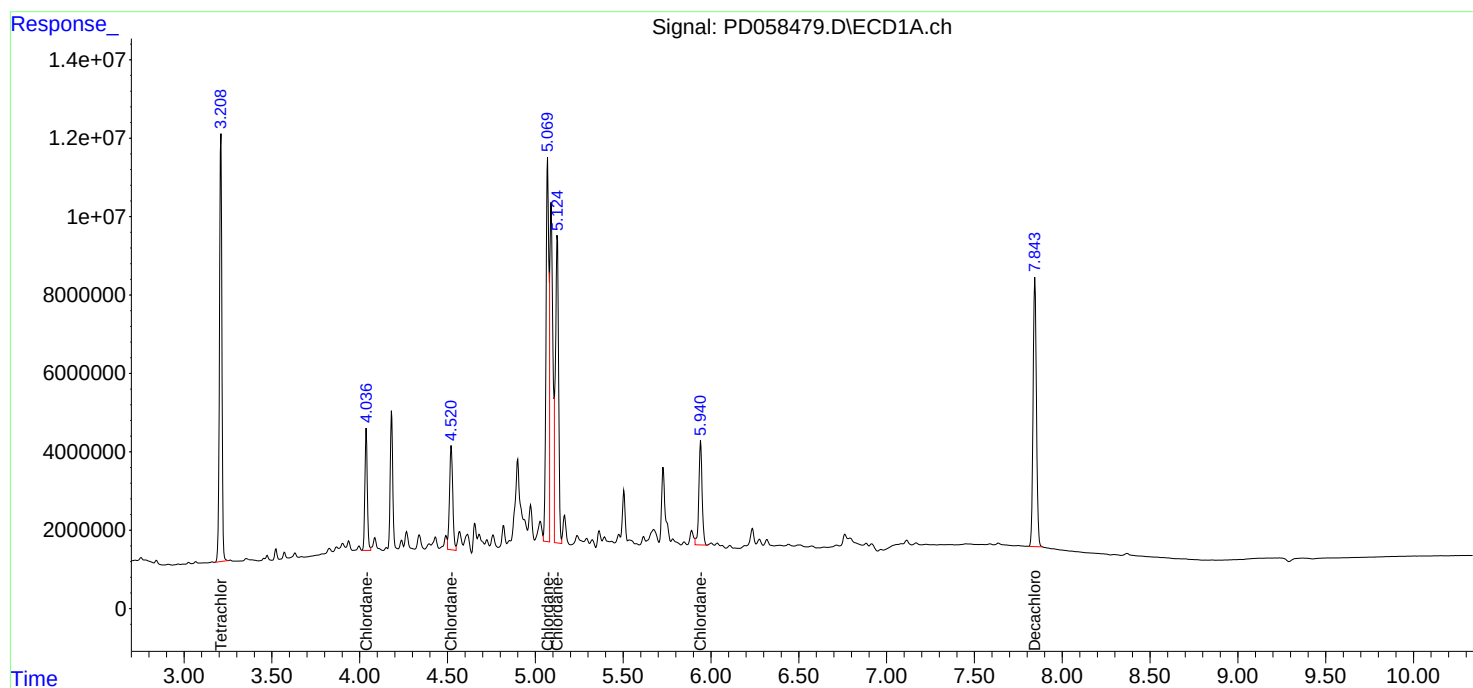


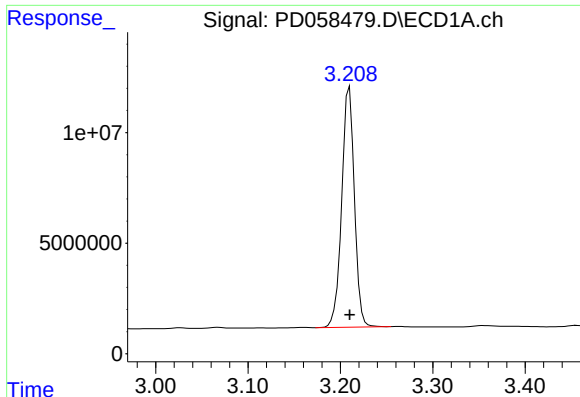

#1 Tetrachloro-m-xylene


R.T.: 3.210 min
Delta R.T.: 0.000 min
Response: 103747606
Conc: 56.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD070720

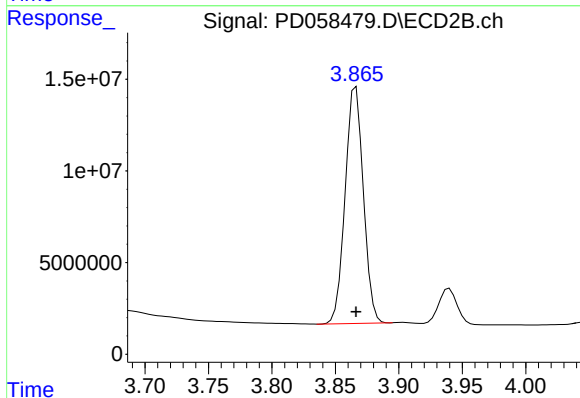


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 128792348
Conc: 52.13 ng/ml

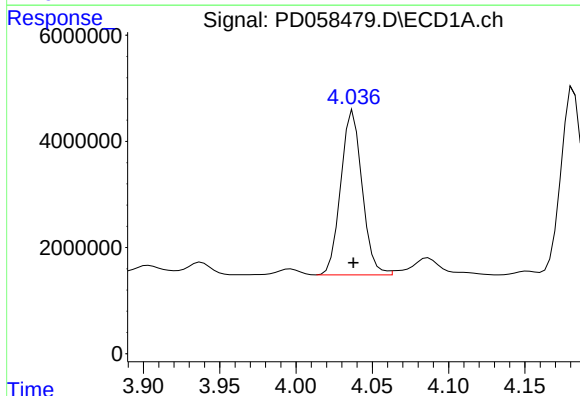


#23 Chlordane-1

R.T.: 4.038 min
Delta R.T.: 0.000 min
Response: 30194913
Conc: 517.45 ng/ml

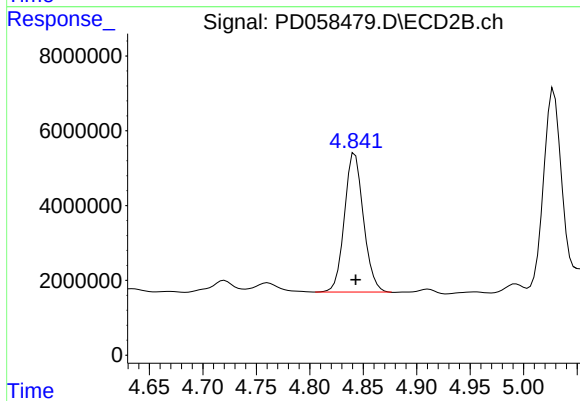

#23 Chlordane-1


R.T.: 4.842 min
Delta R.T.: 0.000 min
Response: 45971240
Conc: 516.52 ng/ml

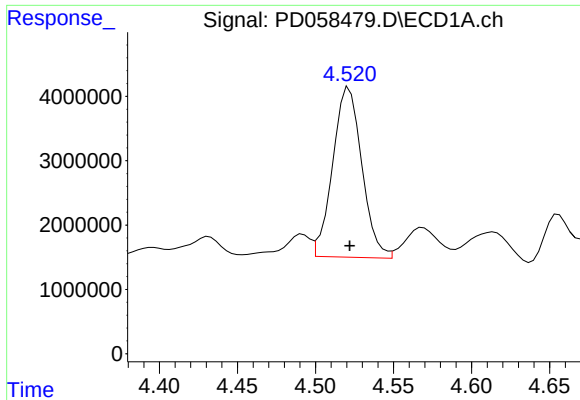

#24 Chlordane-2


R.T.: 4.522 min
Delta R.T.: 0.000 min
Response: 34368857
Conc: 531.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD070720

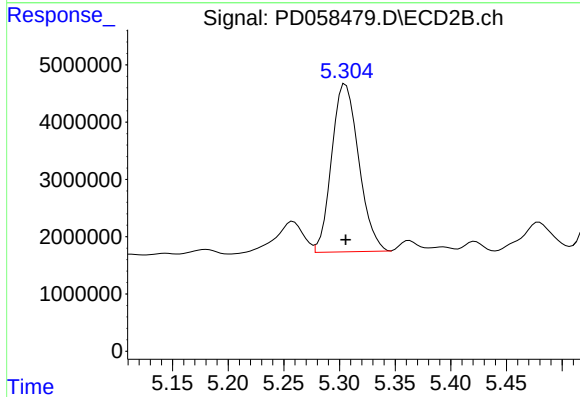


#24 Chlordane-2

R.T.: 5.305 min
Delta R.T.: 0.000 min
Response: 49623586
Conc: 502.33 ng/ml

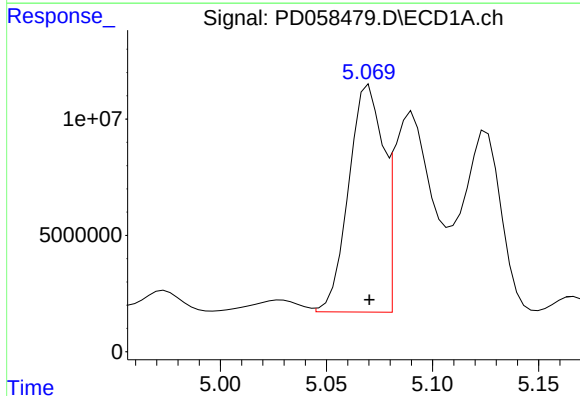


#25 Chlordane-3

R.T.: 5.070 min
Delta R.T.: 0.000 min
Response: 109598106
Conc: 535.43 ng/ml

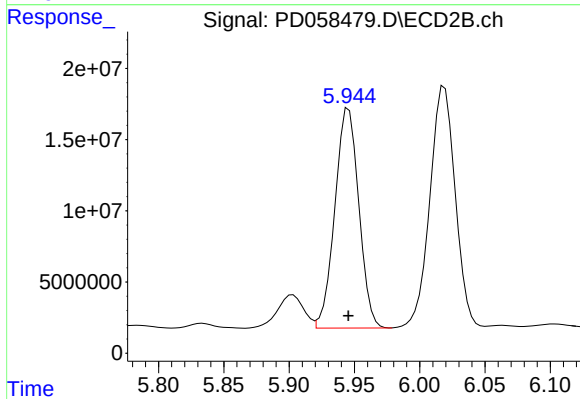

#25 Chlordane-3


R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 197045356
Conc: 529.77 ng/ml

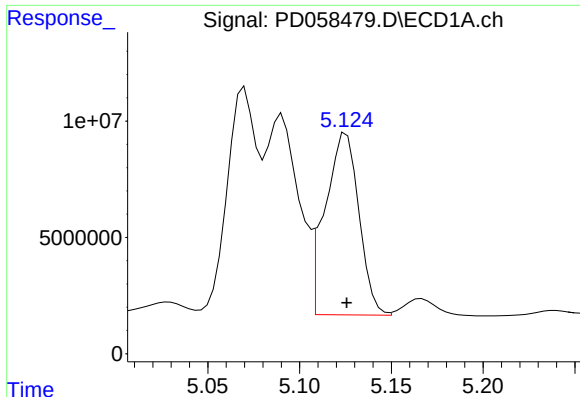

#26 Chlordane-4


R.T.: 5.125 min
Delta R.T.: 0.000 min
Response: 100104021
Conc: 524.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD070720

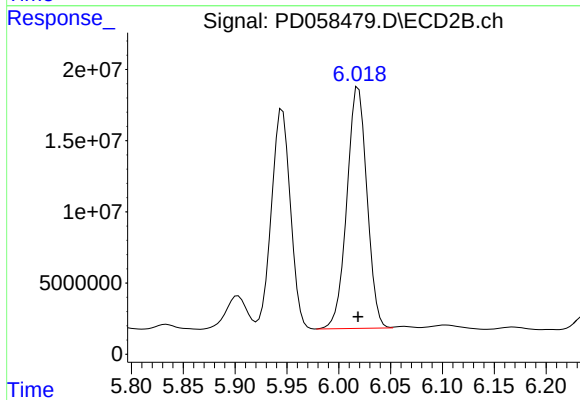


#26 Chlordane-4

R.T.: 6.019 min
Delta R.T.: 0.000 min
Response: 228547567
Conc: 525.40 ng/ml

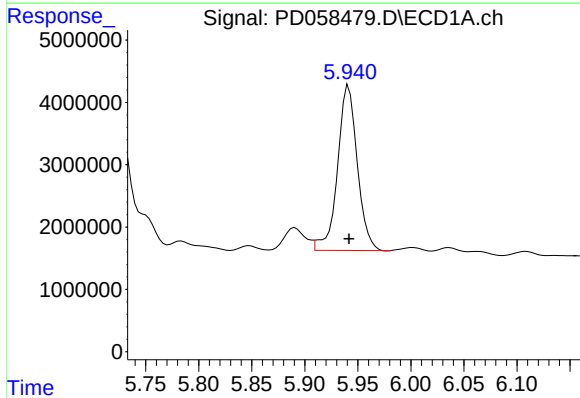


#27 Chlordane-5

R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 34204299
Conc: 556.60 ng/ml

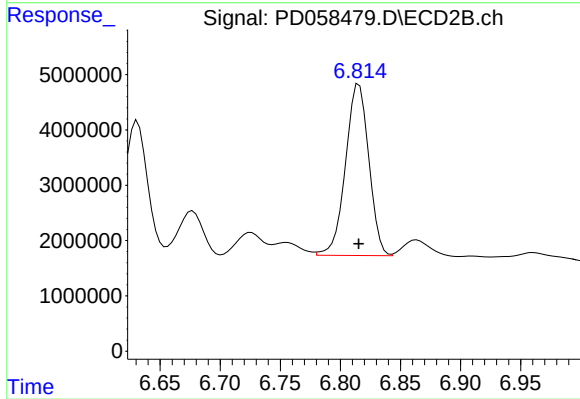

#27 Chlordane-5


R.T.: 6.816 min
Delta R.T.: 0.000 min
Response: 41975260
Conc: 526.81 ng/ml

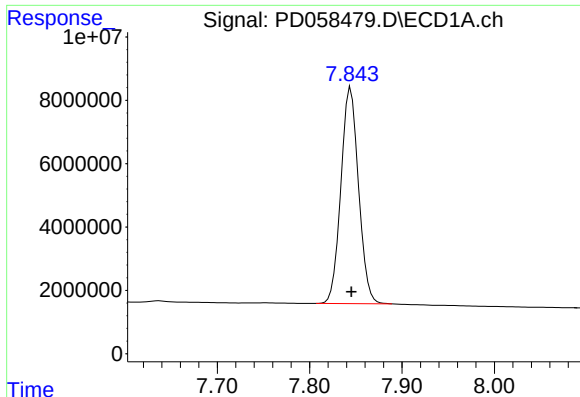

#28 Decachlorobiphenyl

R.T.: 7.844 min
Delta R.T.: 0.000 min
Response: 90516430
Conc: 50.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD070720

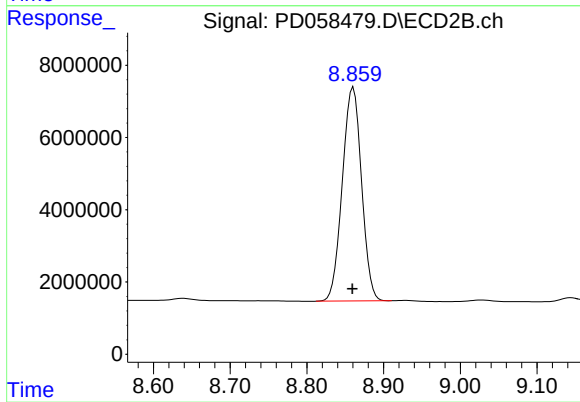

#28 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.001 min
Response: 103503930
Conc: 47.47 ng/ml