

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070721\
Data File : PD064159.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2021 03:04
Operator : AR\AJ
Sample : M2910-05
Misc :
ALS Vial : 54 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
C0AW4

Manual Integrations
APPROVED

mohammad
7/8/2021 2:01:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 04:36:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070621CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 08 02:29:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

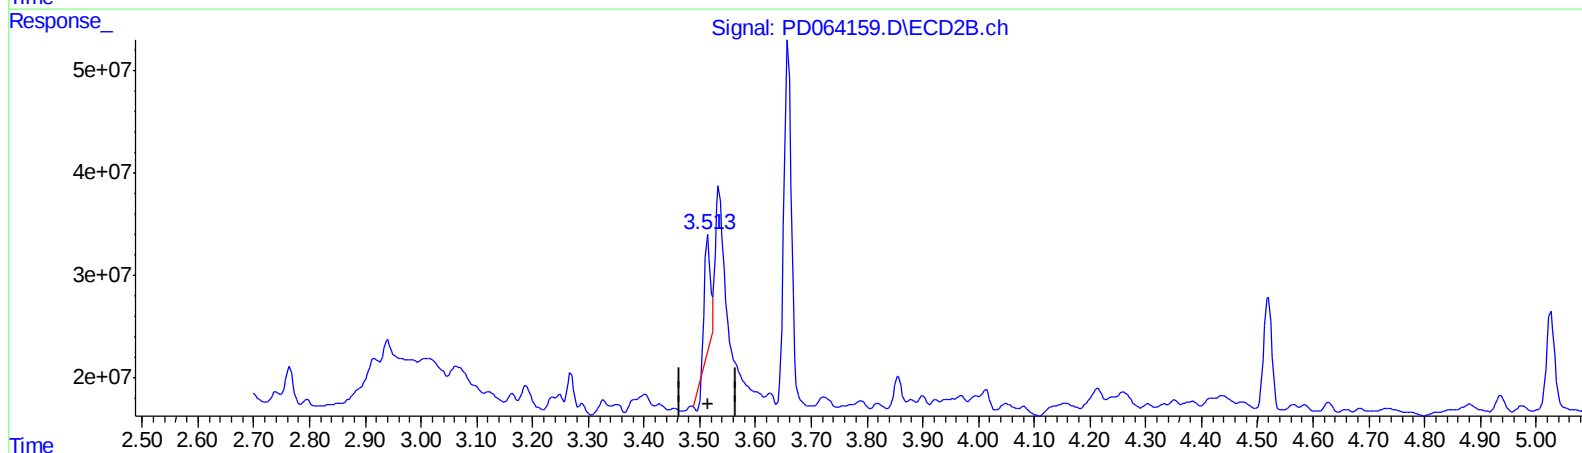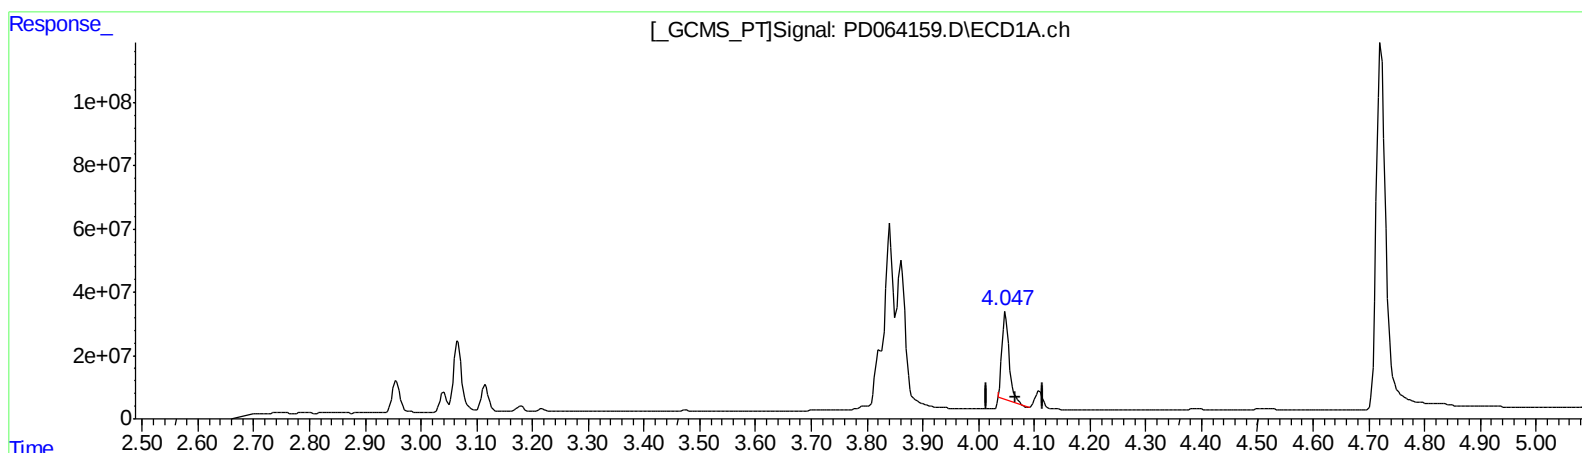

QEdit

(1) Tetrachloro-m-xylene (SA)

4.049min 185.003 ng/ml

response 259801479

(1) Tetrachloro-m-xylene #2 (SA)

3.515min 7.289 ng/ml

response 59103531

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070721\
 Data File : PD064159.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2021 03:04
 Operator : AR\AJ
 Sample : M2910-05
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AW4

Manual Integrations
 APPROVED

mohammad
 7/8/2021 2:01:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 04:36:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070621CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 08 02:29:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.047	3.513	325.7E6	138.4E6	231.939m	17.067m#
27) SA Decachlor...	9.243	8.260	34010043	125.9E6	25.652	24.813

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AJ
 07/13/21