

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070723\
 Data File : PD076377.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2023 16:30
 Operator : AR\AJ
 Sample : 03516-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BERGENFIELD-COMP-2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/07/2023
 Supervised By :Ankita Jodhani 07/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 21:42:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070423.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 05 05:21:22 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.543	2.764	32505137	16536500	9.921m	10.410m
28) SA Decachlor...	9.085	7.909	31753068	12354295	8.931	9.817

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070723\
Data File : PD076377.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2023 16:30
Operator : AR\AJ
Sample : 03516-04
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BERGENFIELD-COMP-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/07/2023
Supervised By : Ankita Jodhani 07/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 21:42:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070423.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 05:21:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

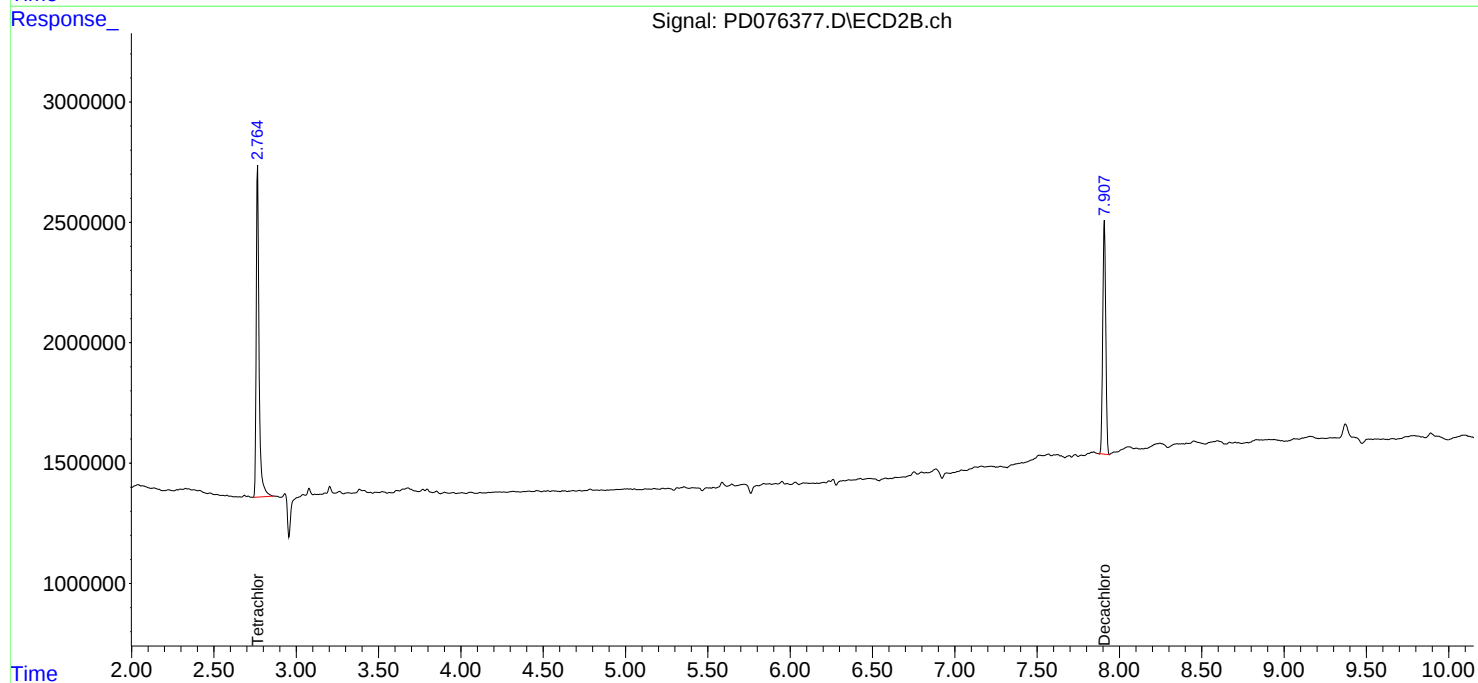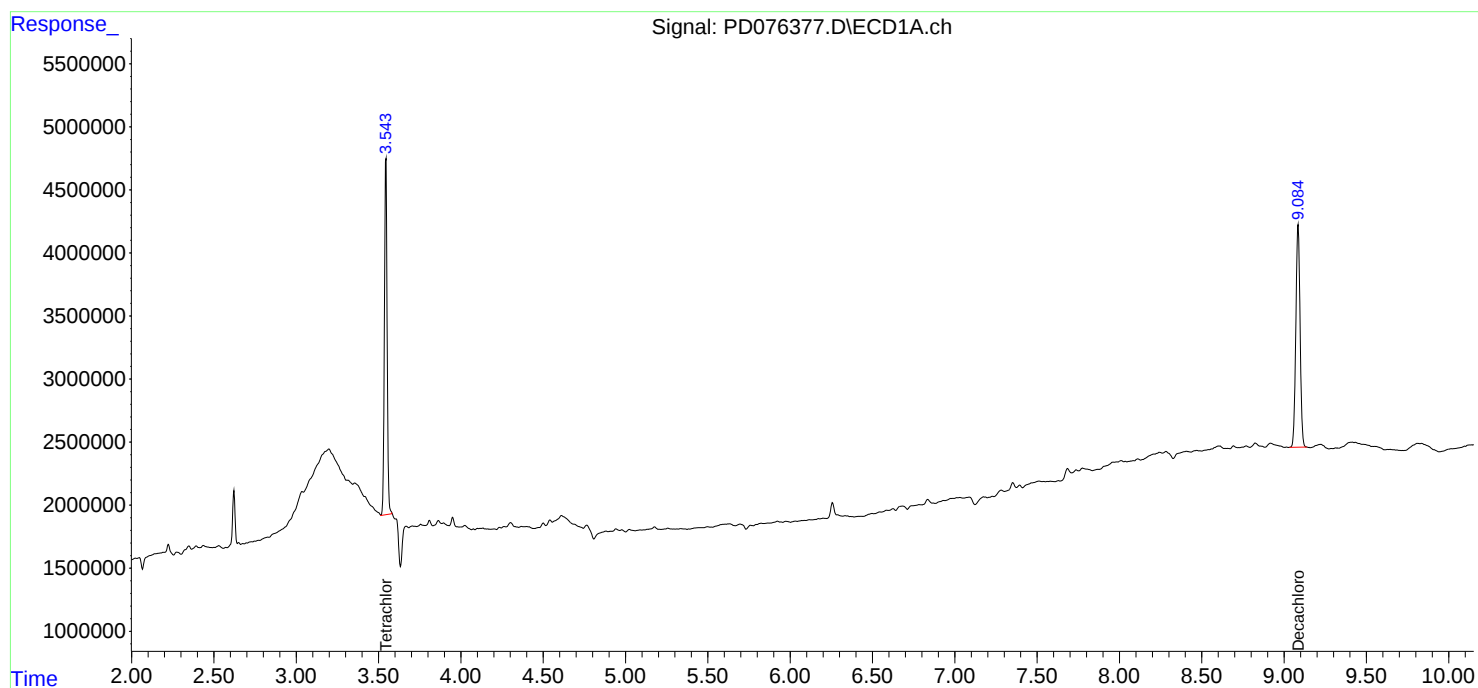

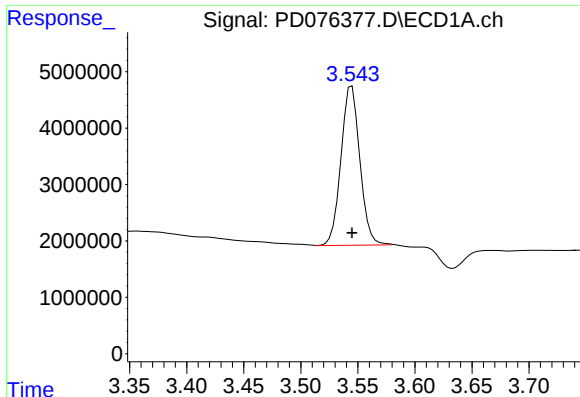


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.002 min
Response: 32505137
Conc: 9.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
BERGENFIELD-COMP-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/07/2023
Supervised By :Ankita Jodhani 07/07/2023

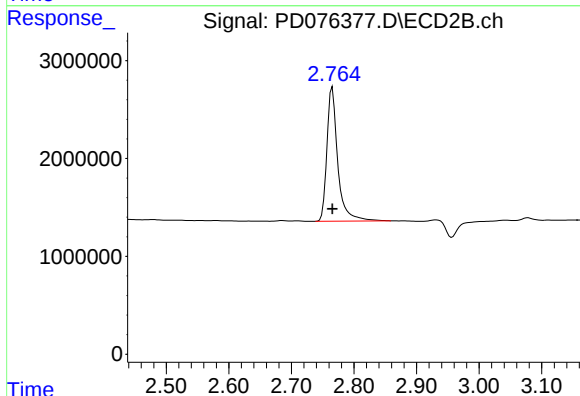


#1 Tetrachloro-m-xylene

R.T.: 2.764 min
Delta R.T.: -0.001 min
Response: 16536500
Conc: 10.41 ng/ml m

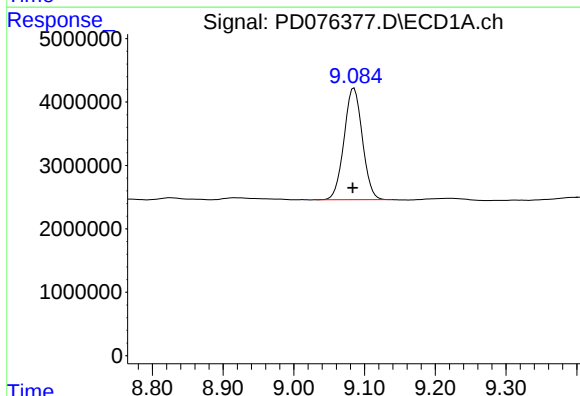

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.002 min
Response: 31753068
Conc: 8.93 ng/ml

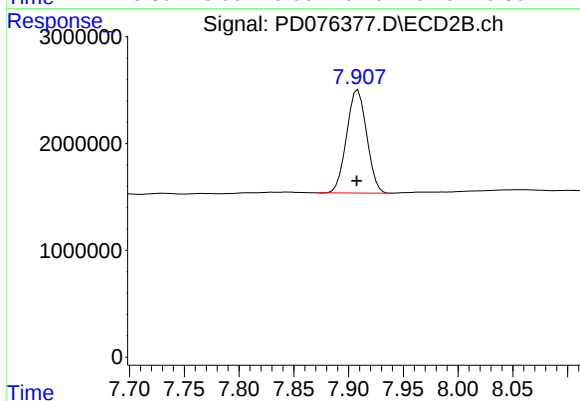

#28 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: 0.001 min
Response: 12354295
Conc: 9.82 ng/ml