

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070723\
 Data File : PD076380.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2023 17:10
 Operator : AR\AJ
 Sample : 03523-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 WALDWICK-COMP

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/07/2023
 Supervised By :Ankita Jodhani 07/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 21:45:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070423.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 05 05:21:22 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.543	2.764	41525864	20154801	12.674m	12.688m
28) SA Decachlor...	9.085	7.908	40005704	16195332	11.252	12.869

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070723\
Data File : PD076380.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2023 17:10
Operator : AR\AJ
Sample : 03523-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
WALDWICK-COMP


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/07/2023
Supervised By : Ankita Jodhani 07/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 21:45:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070423.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 05:21:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

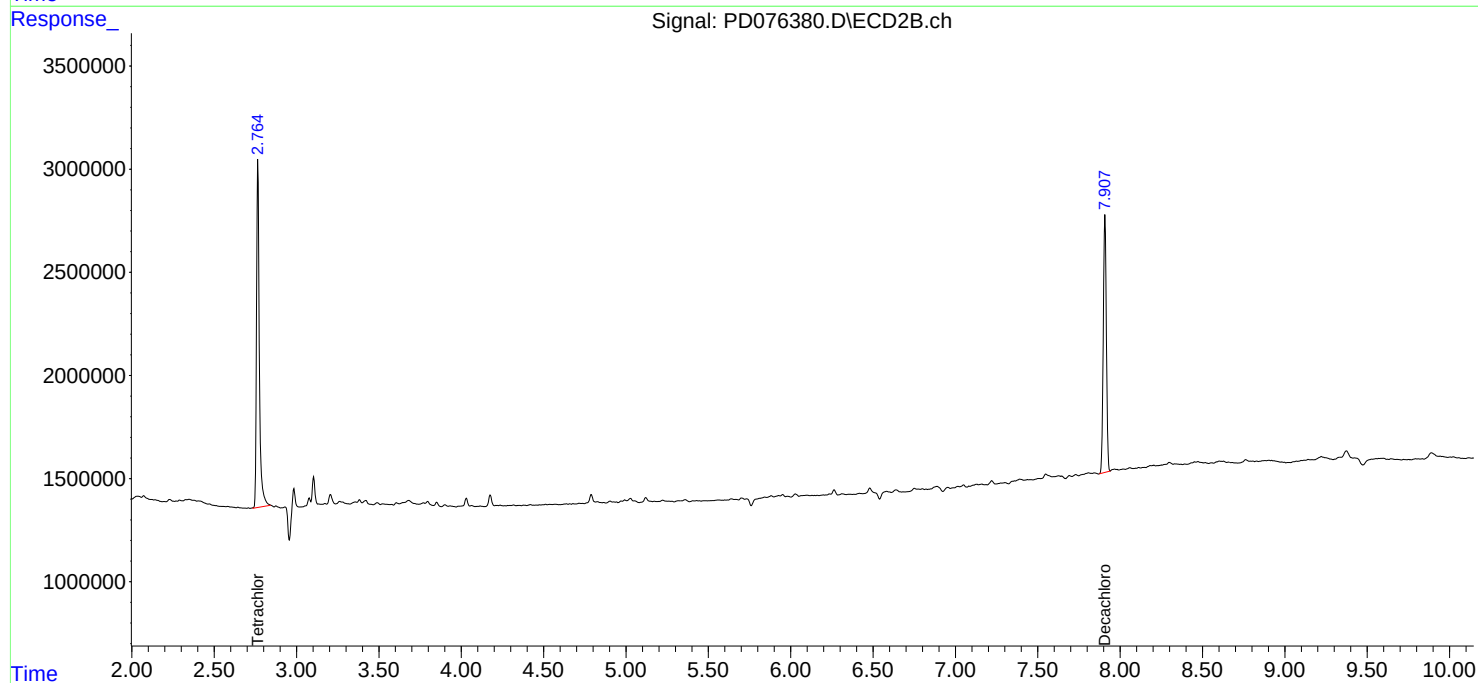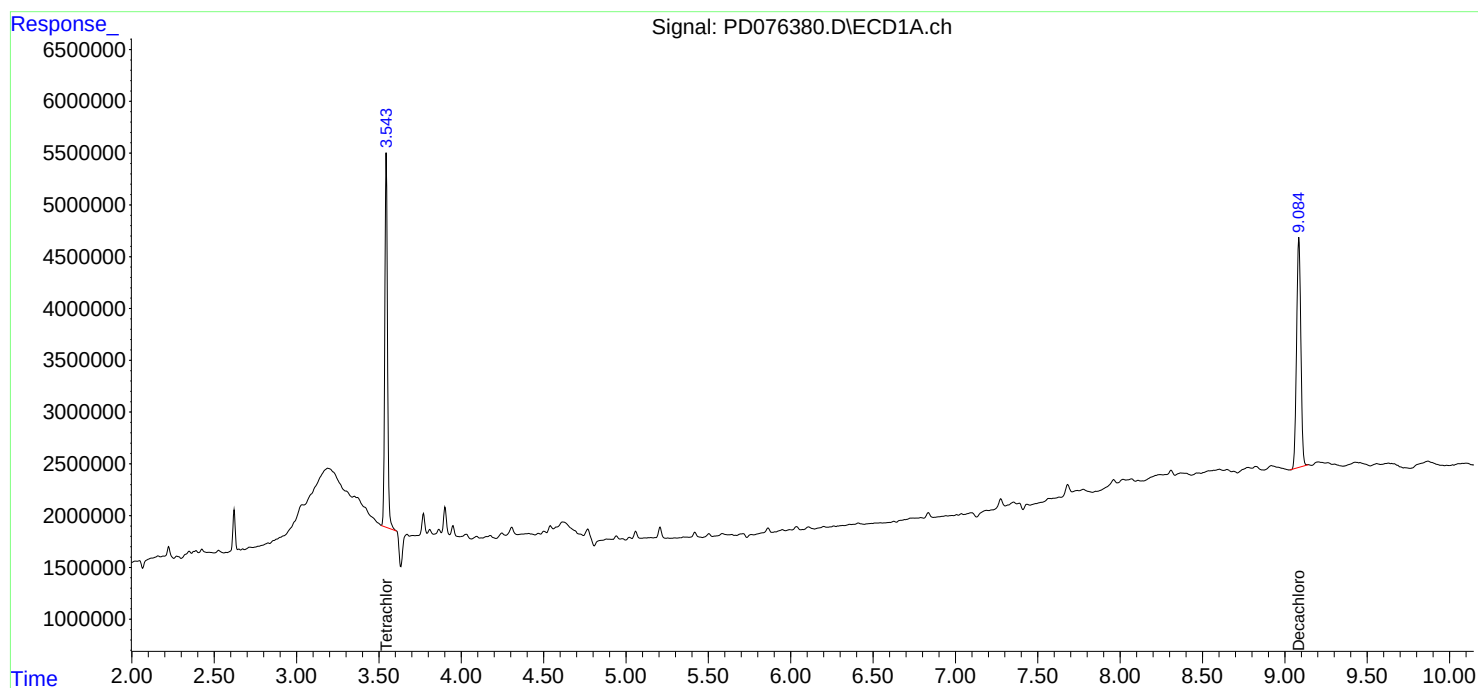

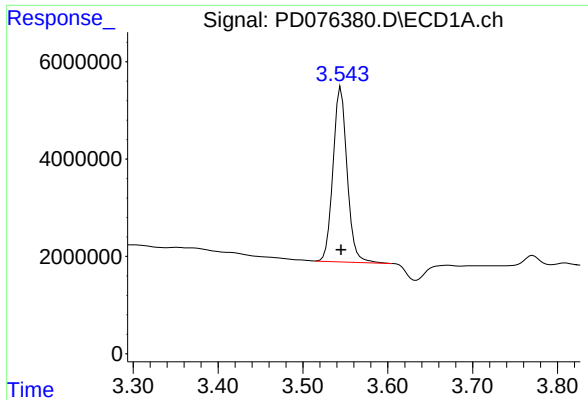


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.002 min
Response: 41525864
Conc: 12.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
WALDWICK-COMP


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/07/2023
Supervised By :Ankita Jodhani 07/07/2023

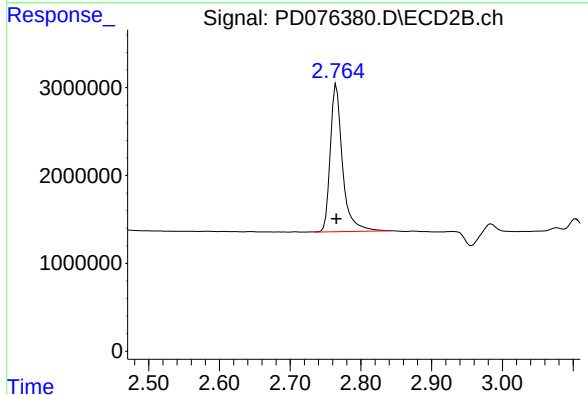


#1 Tetrachloro-m-xylene

R.T.: 2.764 min
Delta R.T.: -0.001 min
Response: 20154801
Conc: 12.69 ng/ml m

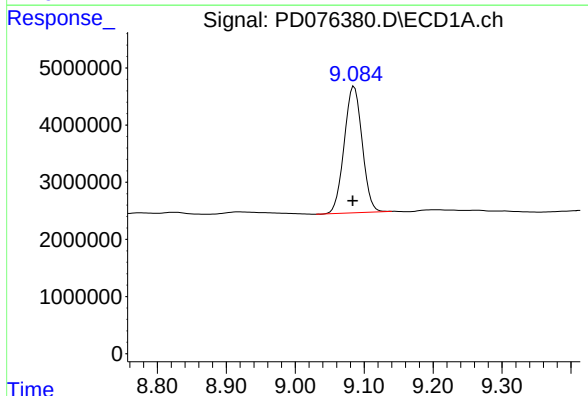

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.002 min
Response: 40005704
Conc: 11.25 ng/ml

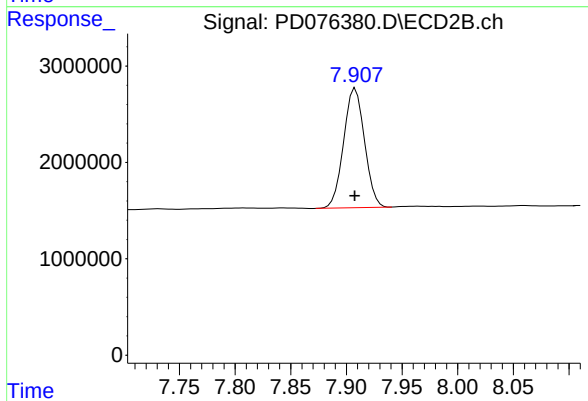

#28 Decachlorobiphenyl

R.T.: 7.908 min
Delta R.T.: 0.000 min
Response: 16195332
Conc: 12.87 ng/ml